

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
 Data File : PL042266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2018 16:49
 Operator : AJ\SJ
 Sample : MIREX-MDL-BL-W-03 (Sig #1); MIREX-MDL-BL-W-02 (Sig #2)
 Misc : FOR MIREX
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-BL-W-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:22:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	116.1E6	60737252	20.919	21.972
28)	SA Decachlor...	8.205	9.229	128.5E6	49463673	20.762	20.779

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
Data File : PL042266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2018 16:49
Operator : AJ\SJ
Sample : MIREX-MDL-BL-W-03 (Sig #1); MIREX-MDL-BL-W-02 (Sig #2)
Misc : FOR MIREX
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-BL-W-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:22:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

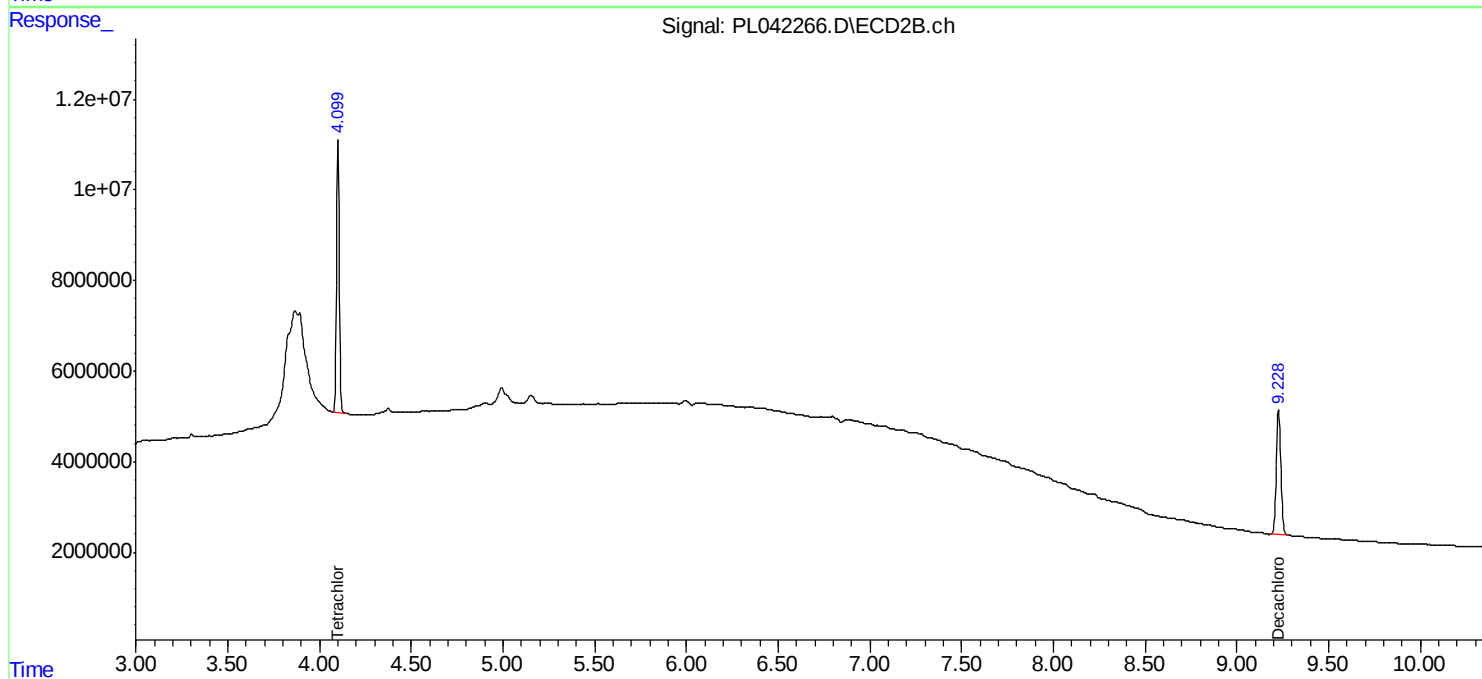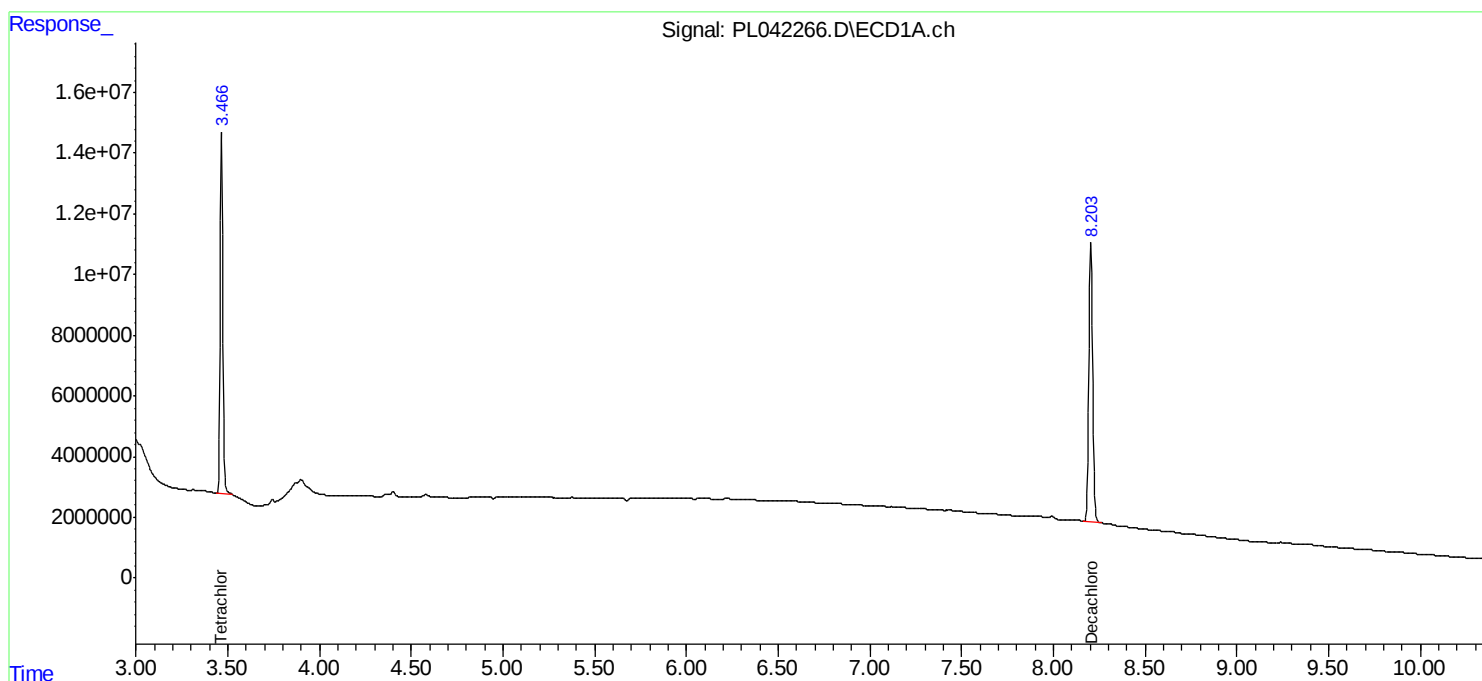


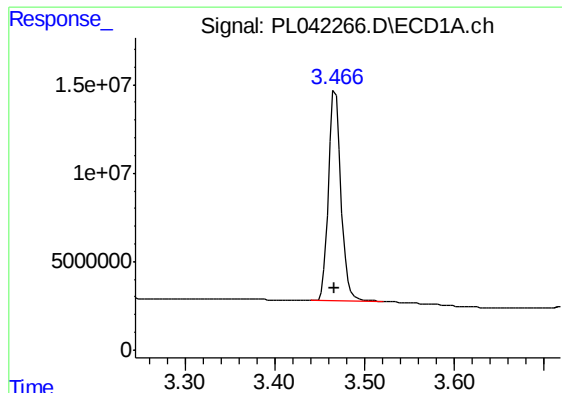

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 116110566
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-BL-W-03

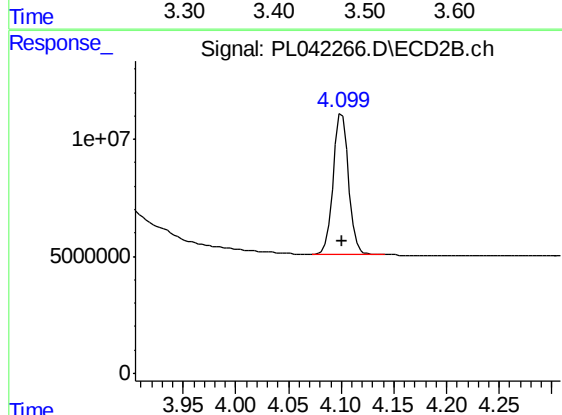


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 60737252
Conc: 21.97 ng/ml

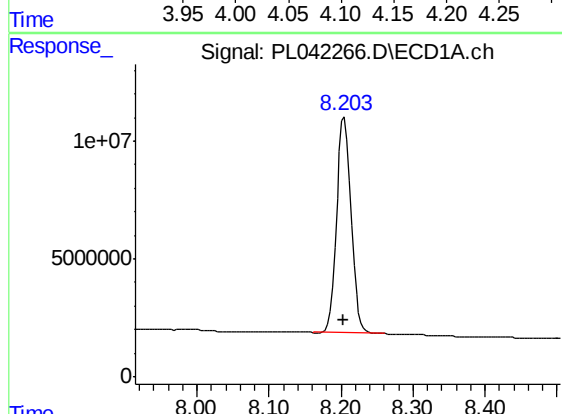

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.001 min
Response: 128482401
Conc: 20.76 ng/ml

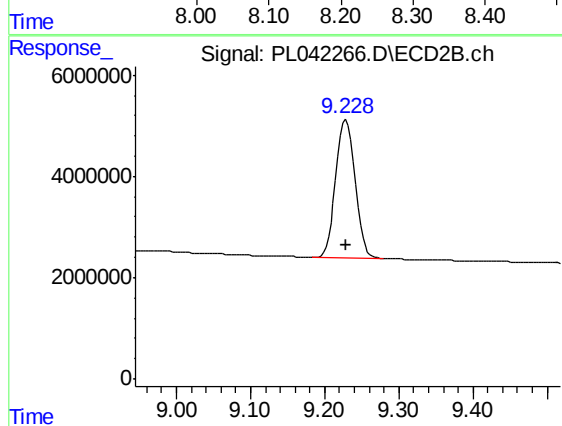

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.000 min
Response: 49463673
Conc: 20.78 ng/ml