

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
 Data File : PL042268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2018 17:17
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-07 (Sig #1); MIREX-MDL-W-05 (Sig #2)
 Misc : FOR MIREX
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-W-07

Manual Integrations
 APPROVED

Sohil
 11/19/2018 12:12:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:22:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	95883063	50679472	17.275	18.333
28)	SA Decachlor...	8.205	9.229	113.5E6	42946362	18.335	18.041
Target Compounds							
22)	Mirex	7.340	8.323	7105743	1019011	1.247	0.547m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
Data File : PL042268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2018 17:17
Operator : AJ\SJ
Sample : MIREX-MDL-W-07 (Sig #1); MIREX-MDL-W-05 (Sig #2)
Misc : FOR MIREX
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
MIREX-MDL-W-07


Manual Integrations
APPROVED

Sohil
11/19/2018 12:12:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:22:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

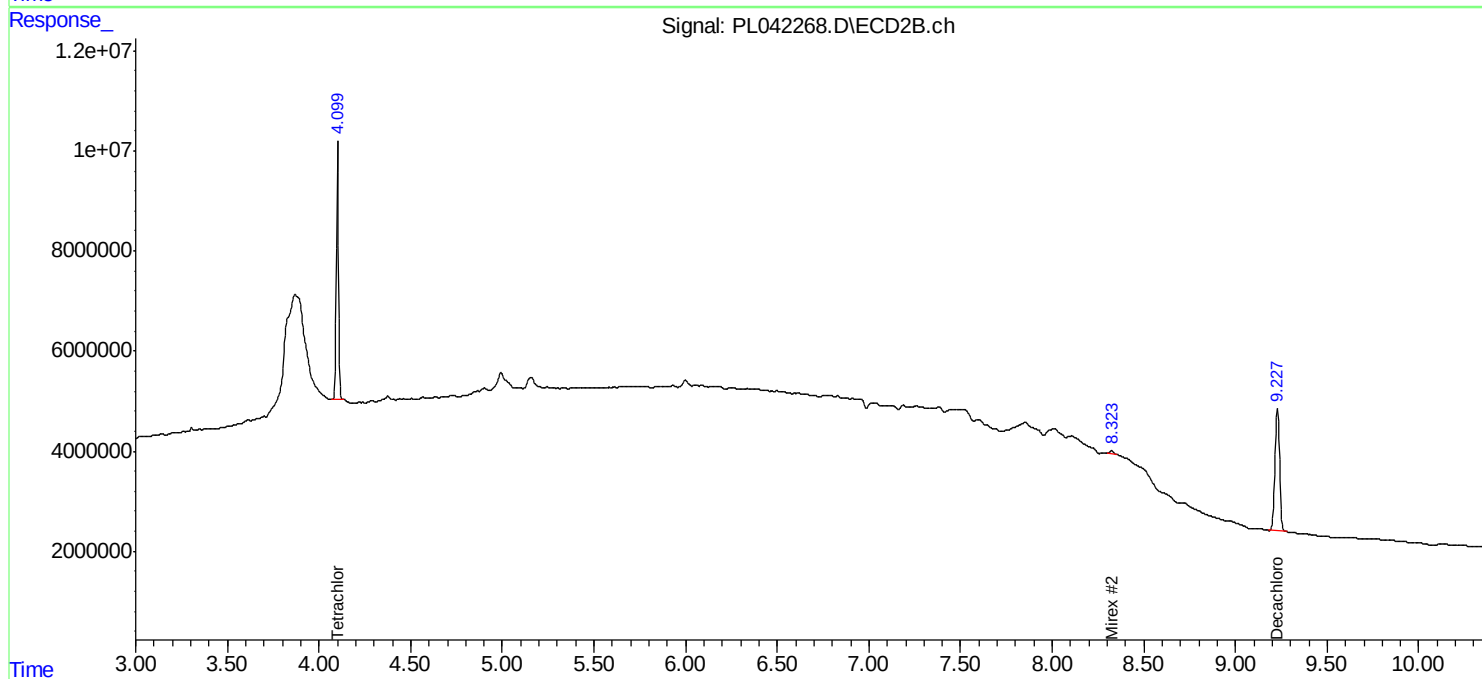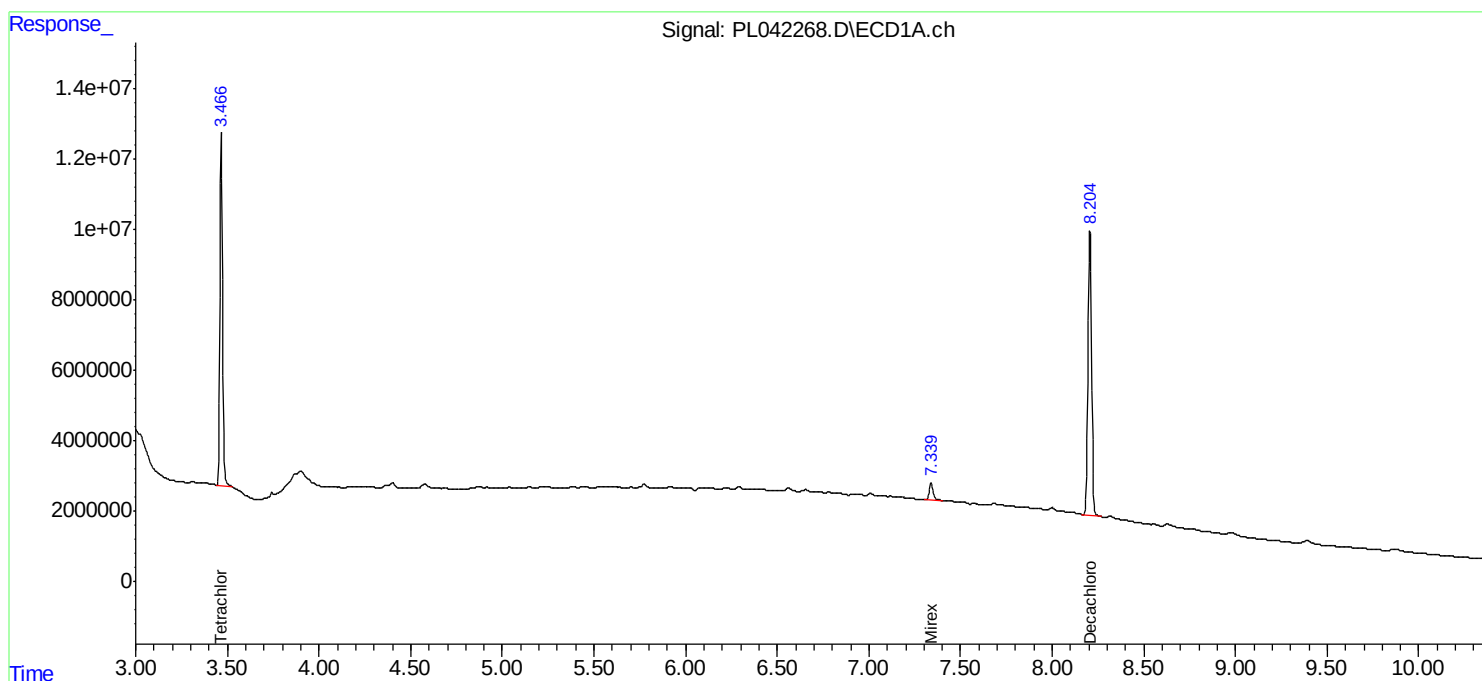

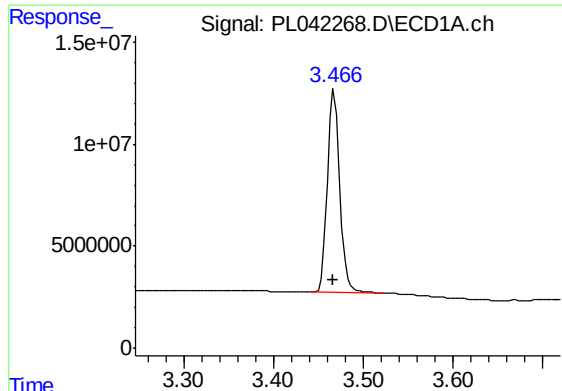


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 95883063
Conc: 17.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-07


Manual Integrations
APPROVED

Sohil
11/19/2018 12:12:15 PM

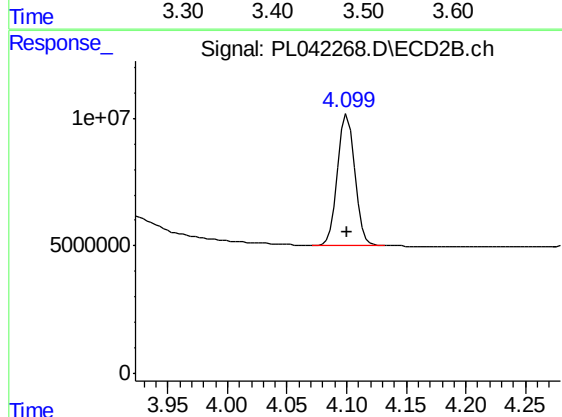


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 50679472
Conc: 18.33 ng/ml

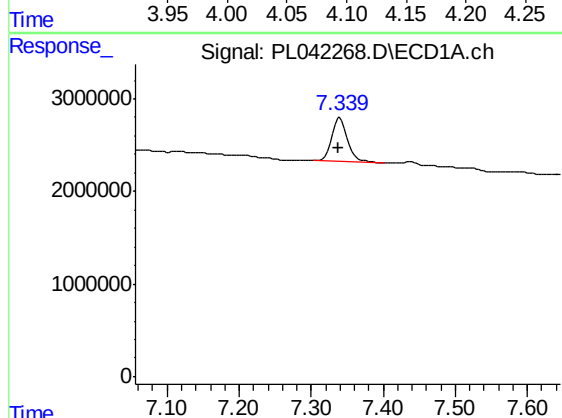


#22 Mirex

R.T.: 7.340 min
Delta R.T.: 0.003 min
Response: 7105743
Conc: 1.25 ng/ml

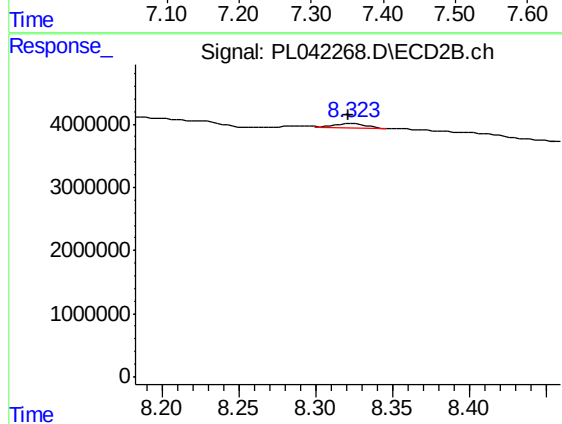

#22 Mirex

R.T.: 8.323 min
Delta R.T.: 0.001 min
Response: 1019011
Conc: 0.55 ng/ml m

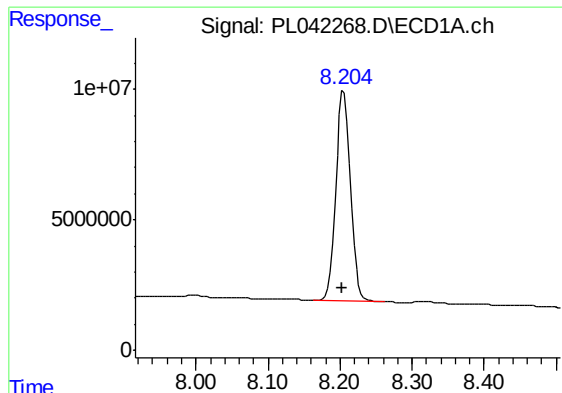


#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.002 min
Response: 113465489
Conc: 18.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-07

Manual Integrations
APPROVED

Sohil
11/19/2018 12:12:15 PM

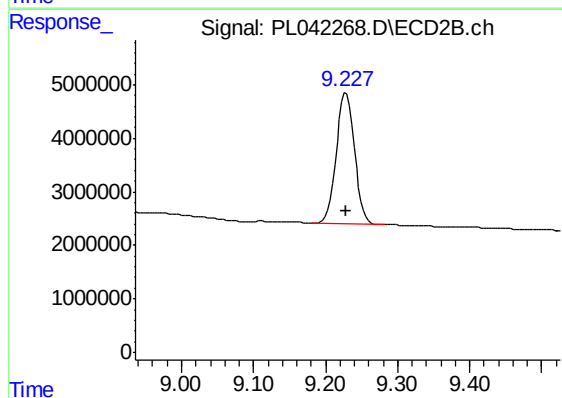

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.000 min
Response: 42946362
Conc: 18.04 ng/ml