

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111919\
 Data File : PL054457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 16:49
 Operator : SG\AJ
 Sample : K5925-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CARRIAGE-COURT

Manual Integrations
 APPROVED

Ankita
 11/20/2019 12:22:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:42:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	4.043	244.2E6	59263704	23.485	24.326
28) SA Decachlor...	8.323	9.124	179.8E6	53482790	20.309	22.120
Target Compounds						
10) B gamma-Chl...	5.498	6.155	6582516	2269069	0.513m	0.912 #
11) B alpha-Chl...	5.558	6.229	8862008	3509558	0.706	1.410 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111919\
Data File : PL054457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 16:49
Operator : SG\AJ
Sample : K5925-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CARRIAGE-COURT


Manual Integrations
APPROVED

Ankita
11/20/2019 12:22:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:42:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

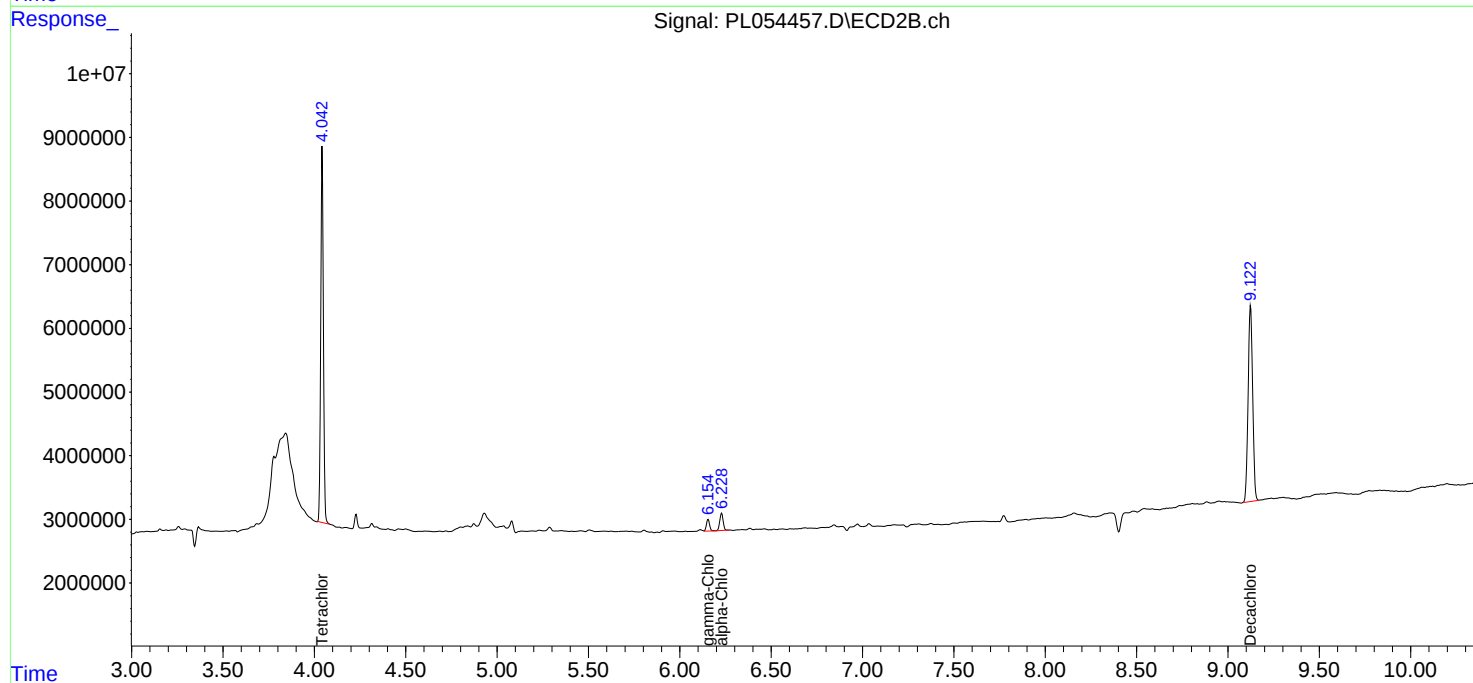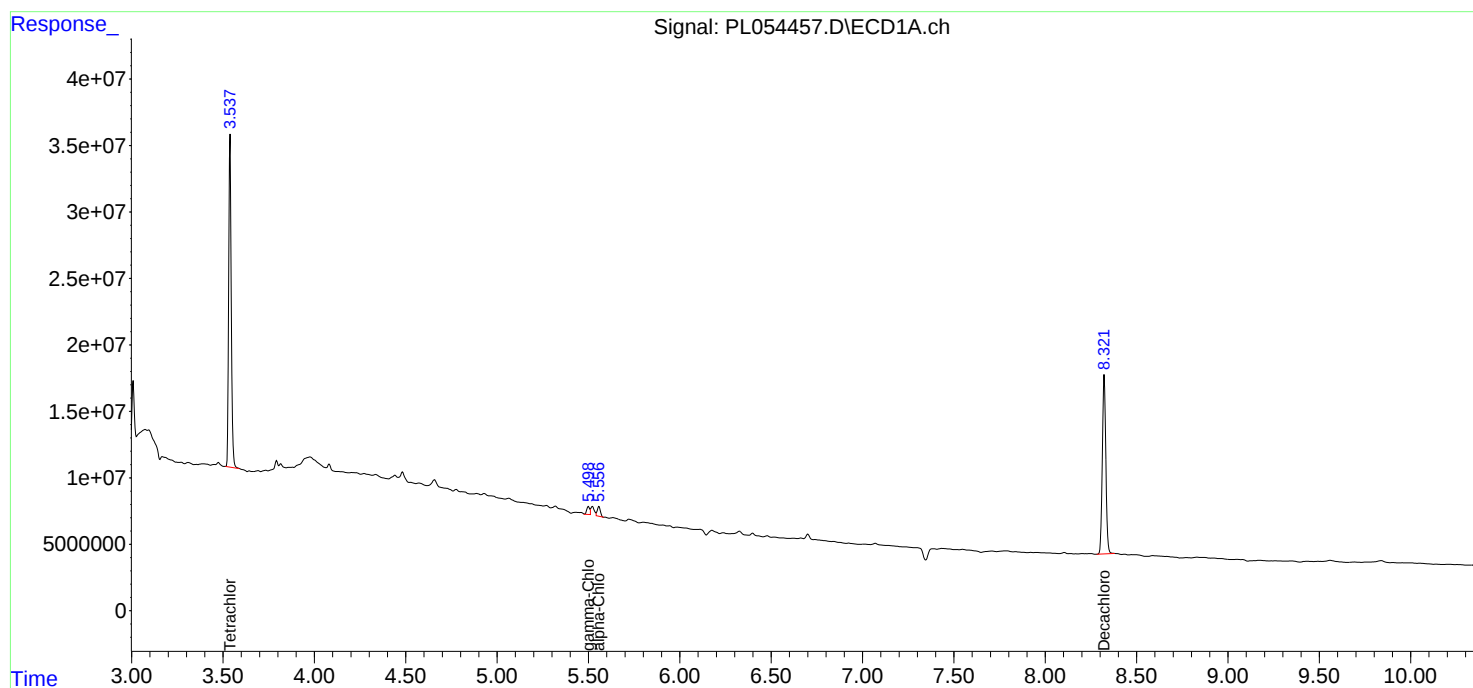

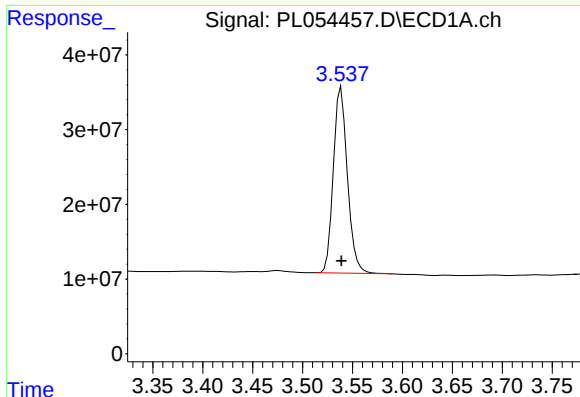


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 244178933
Conc: 23.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
CARRIAGE-COURT


Manual Integrations
APPROVED

Ankita
11/20/2019 12:22:41 PM

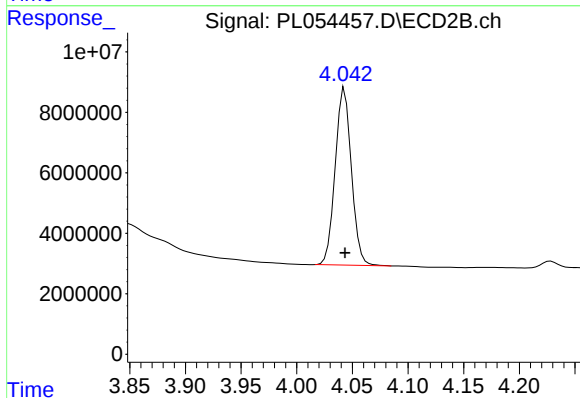


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 59263704
Conc: 24.33 ng/ml

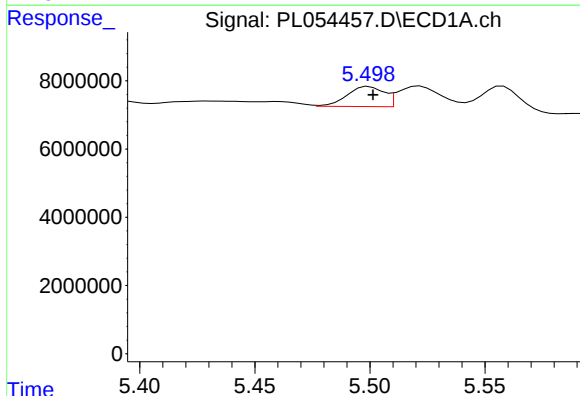


#10 gamma-Chlordane

R.T.: 5.498 min
Delta R.T.: -0.003 min
Response: 6582516
Conc: 0.51 ng/ml m

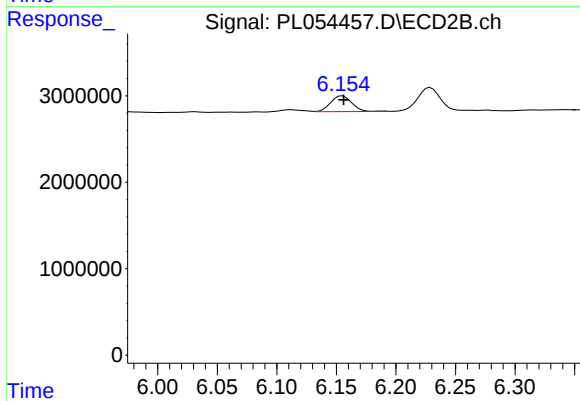

#10 gamma-Chlordane

R.T.: 6.155 min
Delta R.T.: -0.001 min
Response: 2269069
Conc: 0.91 ng/ml

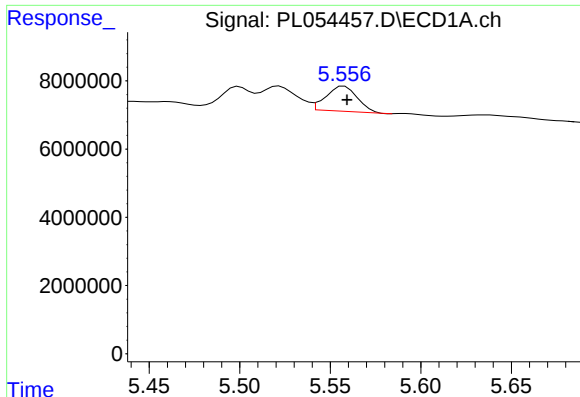


#11 alpha-Chlordane

R.T.: 5.558 min
Delta R.T.: -0.002 min
Response: 8862008
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
CARRIAGE-COURT


Manual Integrations
APPROVED

Ankita
11/20/2019 12:22:41 PM

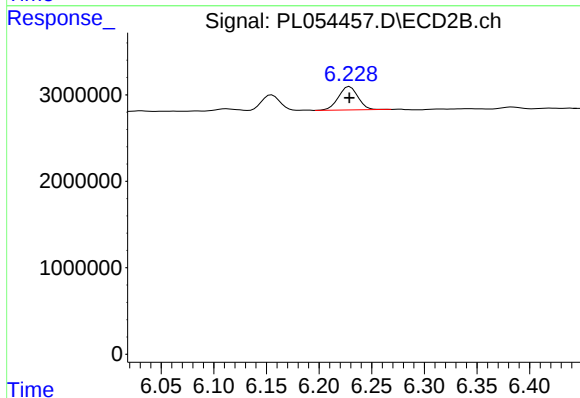


#11 alpha-Chlordane

R.T.: 6.229 min
Delta R.T.: 0.000 min
Response: 3509558
Conc: 1.41 ng/ml

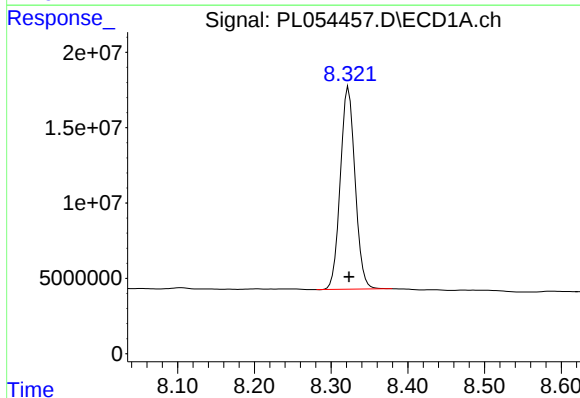

#28 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: 0.000 min
Response: 179752385
Conc: 20.31 ng/ml

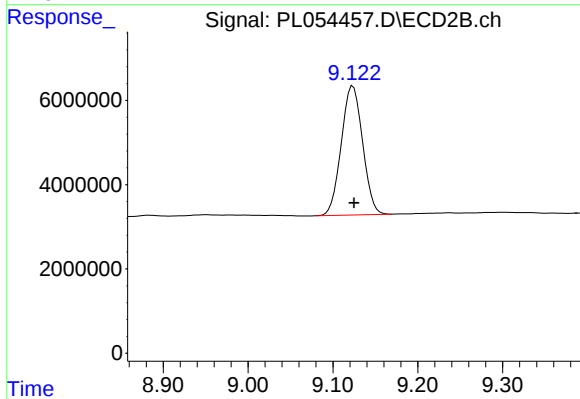

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: -0.001 min
Response: 53482790
Conc: 22.12 ng/ml