

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111920\
 Data File : PL063103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2020 13:05
 Operator : DD\AJ
 Sample : L4797-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 R-LA-2-5-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 04:48:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	34766317	59563530	20.212	20.269
28)	SA Decachlor...	8.124	8.987	28937273	34230074	18.037	16.355
Target Compounds							
2)	A alpha-BHC	3.851	0.000	1336879	0	0.524	N.D. #
7)	B delta-BHC	0.000	5.001	0	6585977	N.D.	1.882 #
8)	B Heptachlo...	0.000	5.825	0	3847709	N.D.	1.188 #
10)	B gamma-Chl...	0.000	6.065f	0	893010	N.D.	0.265 #
15)	B Endosulfa...	0.000	6.868f	0	13983602	N.D.	4.892 #
21)	B Endrin ke...	0.000	7.668	0	6094609	N.D.	2.572 #
23)	Chlordane-1	4.275	0.000	906707	0	17.589	N.D. #
25)	Chlordane-3	0.000	6.065f	0	893010	N.D.	2.211 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111920\
Data File : PL063103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2020 13:05
Operator : DD\AJ
Sample : L4797-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
R-LA-2-5-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 04:48:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

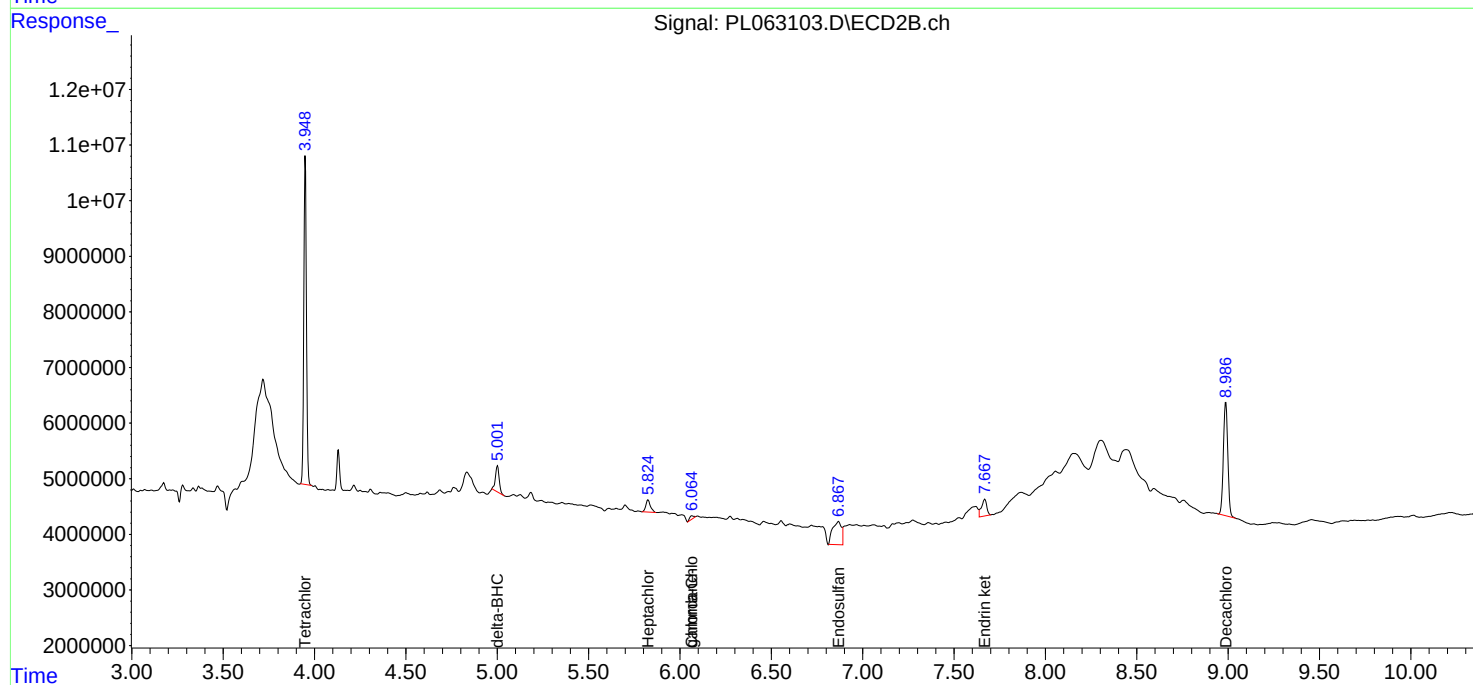


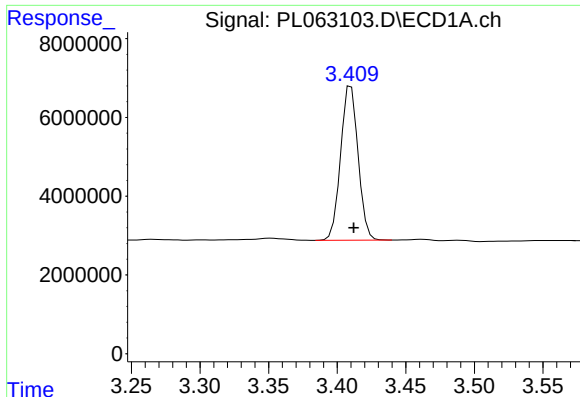

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 34766317
Conc: 20.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-LA-2-5-WC

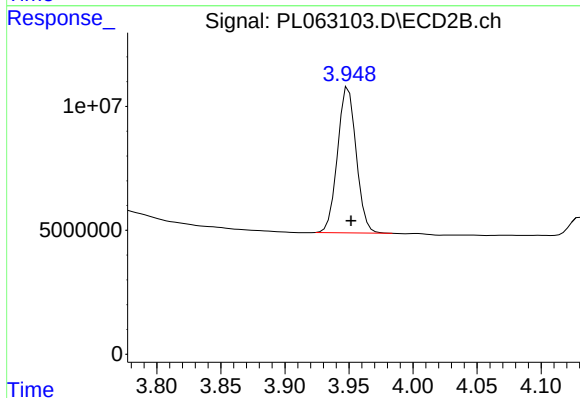


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 59563530
Conc: 20.27 ng/ml

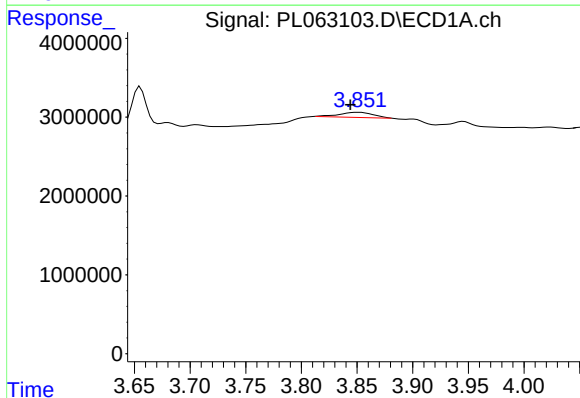


#2 alpha-BHC

R.T.: 3.851 min
Delta R.T.: 0.006 min
Response: 1336879
Conc: 0.52 ng/ml

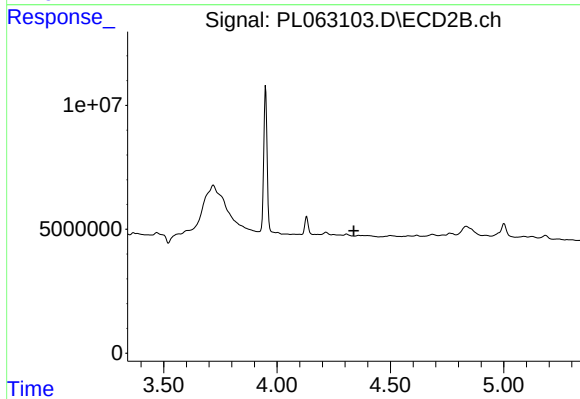

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.338 min
Response: 0
Conc: N.D.

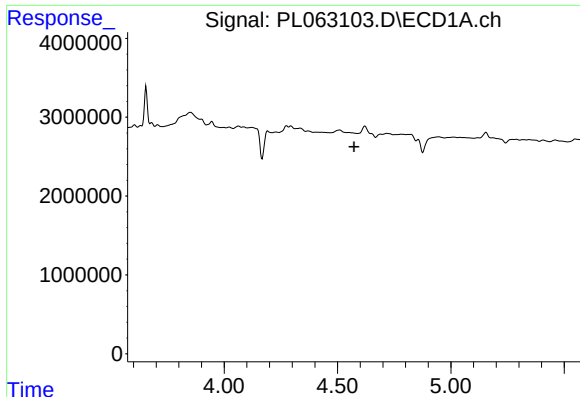

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R-LA-2-5-WC

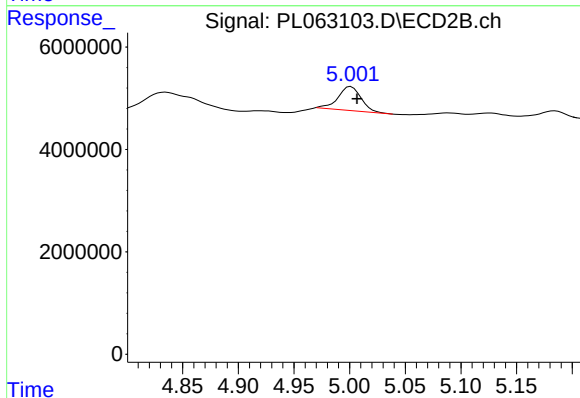


#7 delta-BHC

R.T.: 5.001 min
Delta R.T.: -0.006 min
Response: 6585977
Conc: 1.88 ng/ml

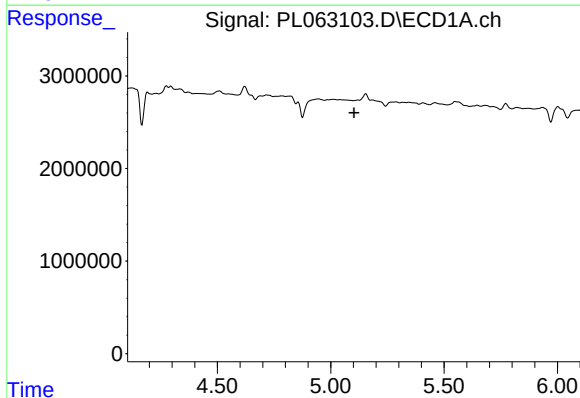


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

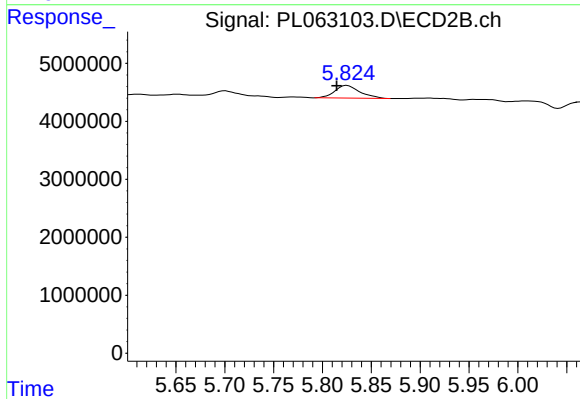

#8 Heptachlor epoxide


R.T.: 5.825 min
Delta R.T.: 0.011 min
Response: 3847709
Conc: 1.19 ng/ml

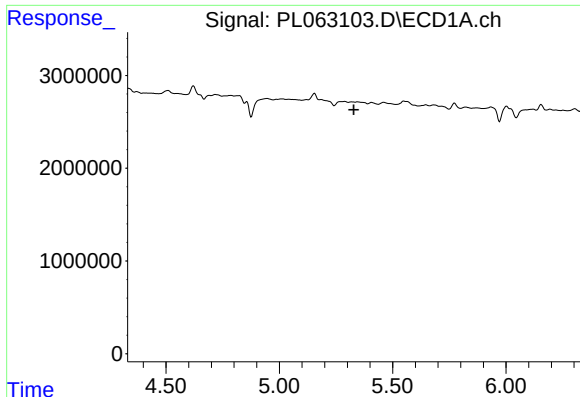

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R-LA-2-5-WC

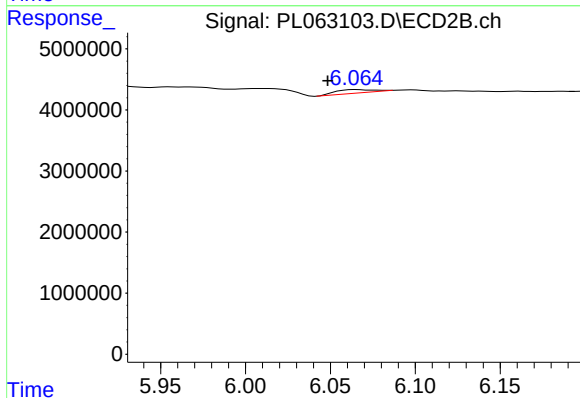


#10 gamma-Chlordane

R.T.: 6.065 min
Delta R.T.: 0.017 min
Response: 893010
Conc: 0.27 ng/ml

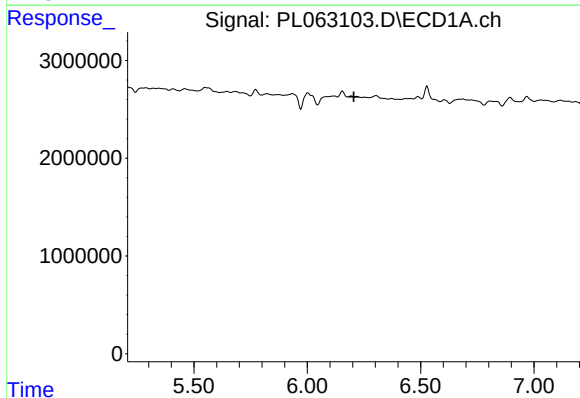


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

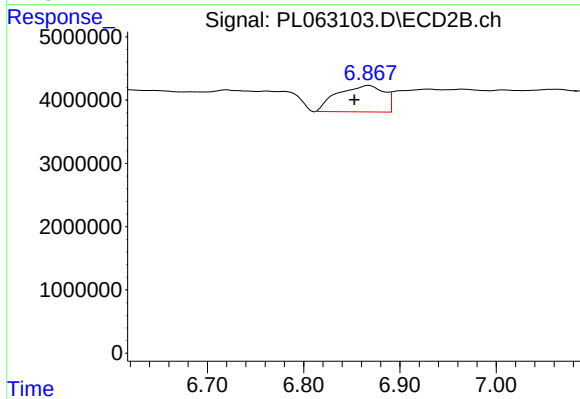

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 13983602
Conc: 4.89 ng/ml

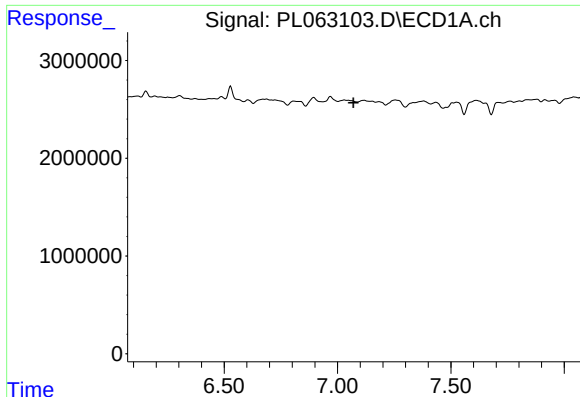

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R-LA-2-5-WC

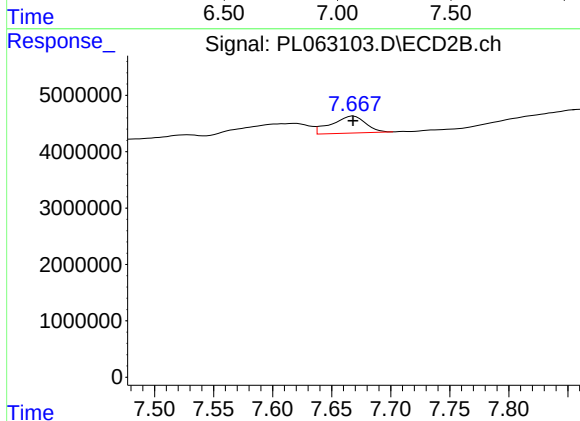


#21 Endrin ketone

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 6094609
Conc: 2.57 ng/ml

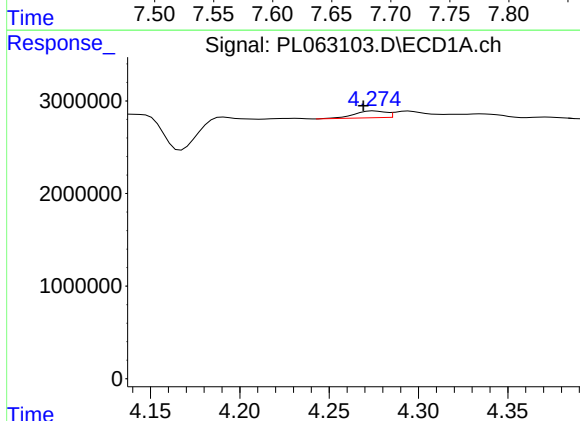


#23 Chlordane-1

R.T.: 4.275 min
Delta R.T.: 0.006 min
Response: 906707
Conc: 17.59 ng/ml

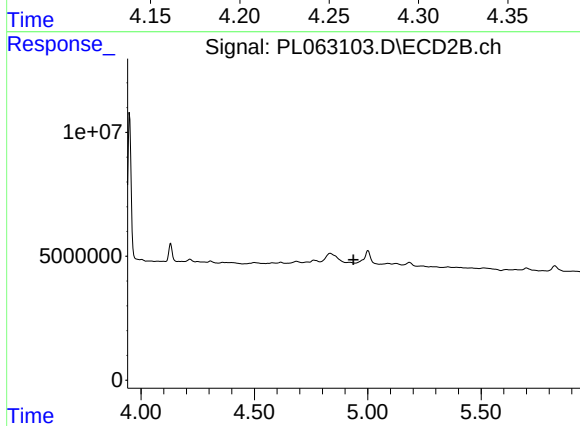

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

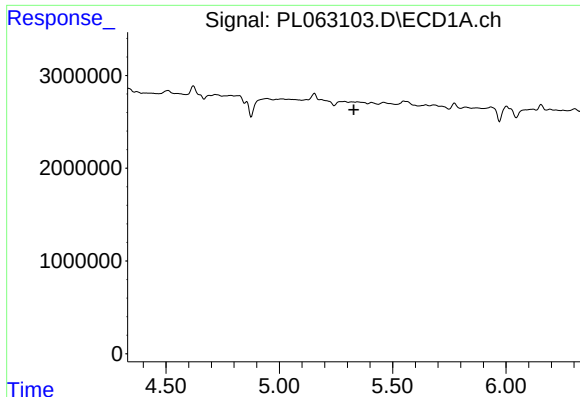

#25 Chlorodane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R-LA-2-5-WC

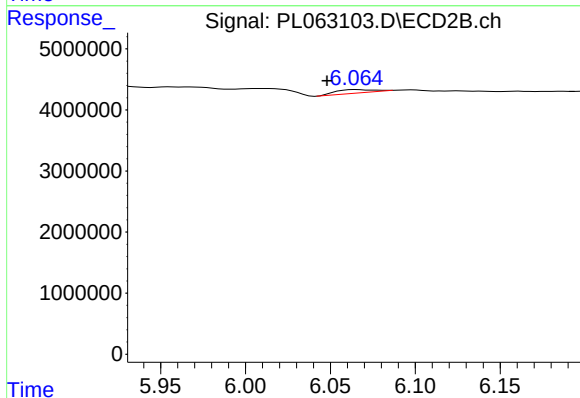


#25 Chlorodane-3

R.T.: 6.065 min
Delta R.T.: 0.017 min
Response: 893010
Conc: 2.21 ng/ml

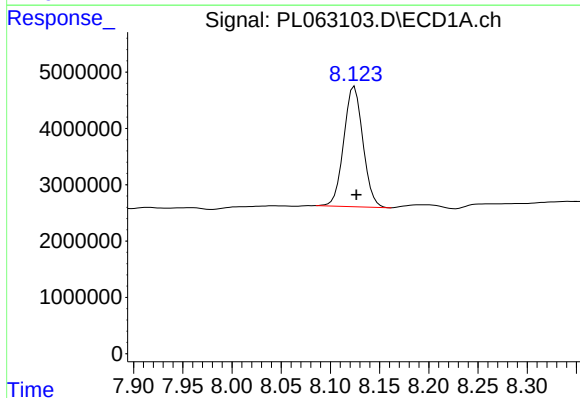

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 28937273
Conc: 18.04 ng/ml

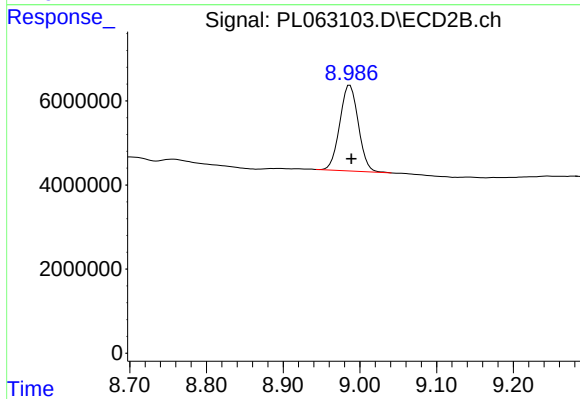

#28 Decachlorobiphenyl

R.T.: 8.987 min
Delta R.T.: -0.002 min
Response: 34230074
Conc: 16.35 ng/ml