

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111920\
 Data File : PL063114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2020 15:51
 Operator : DD\AJ
 Sample : PB133117BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 04:56:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	3.951	32614011	59361702	18.961	20.200
28)	SA Decachlor...	8.131	8.993	35619557	43796110	22.203	20.925
Target Compounds							
6)	B beta-BHC	0.000	4.798	0	10297782	N.D.	5.469 #
15)	B Endosulfa...	0.000	6.869f	0	1717688	N.D.	0.601 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111920\
Data File : PL063114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2020 15:51
Operator : DD\AJ
Sample : PB133117BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 04:56:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

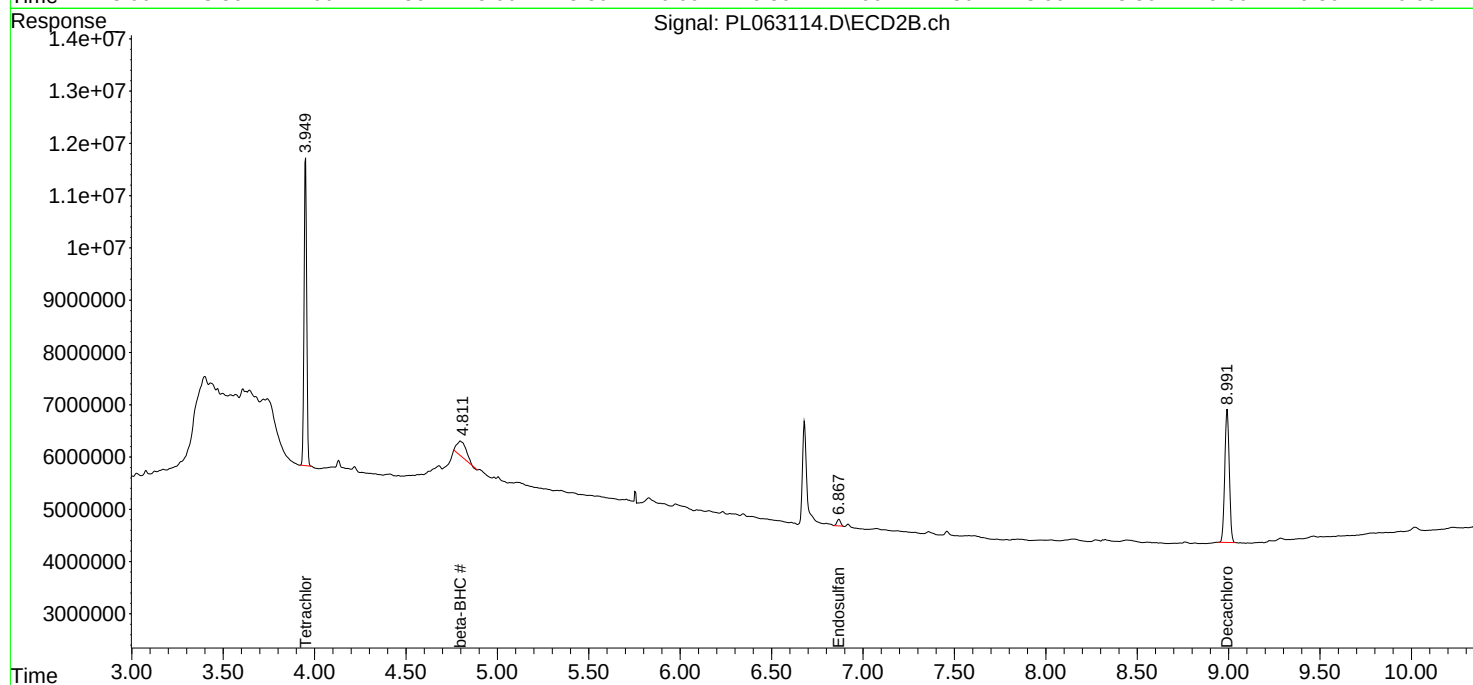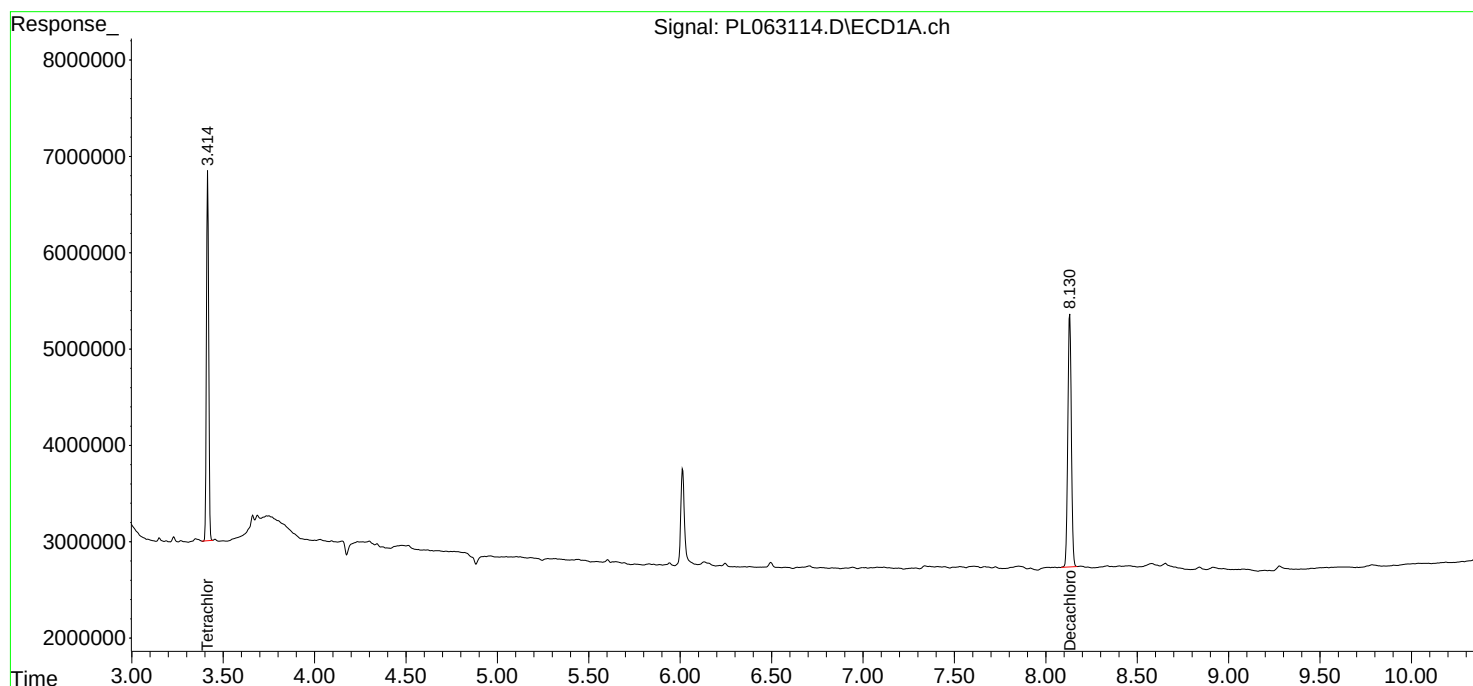


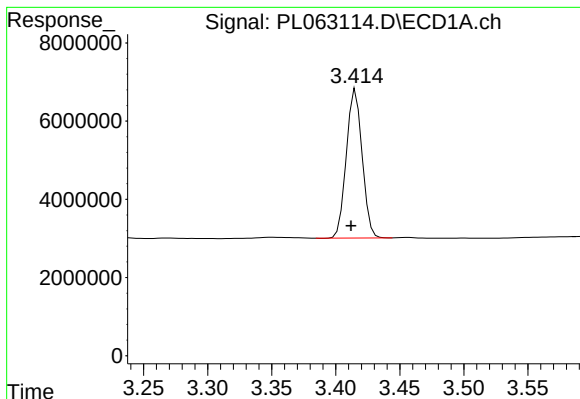

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.004 min
Response: 32614011
Conc: 18.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

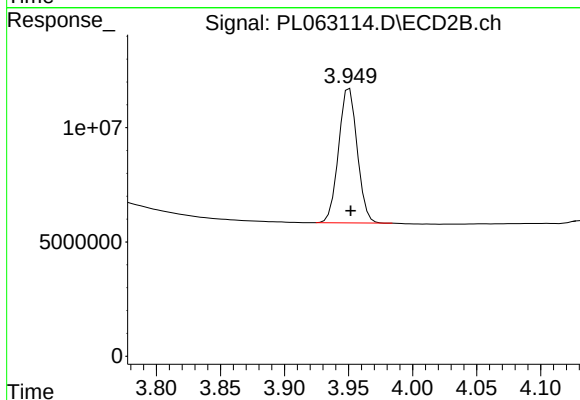


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 59361702
Conc: 20.20 ng/ml

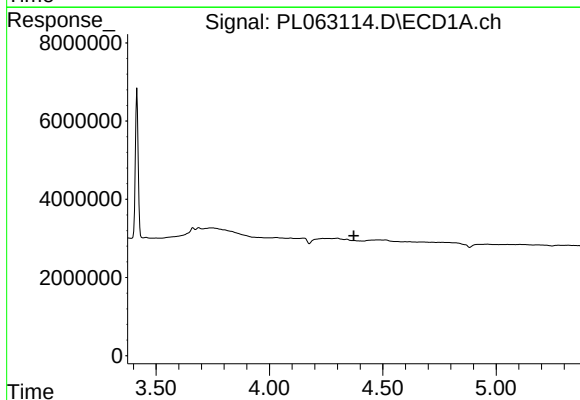


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

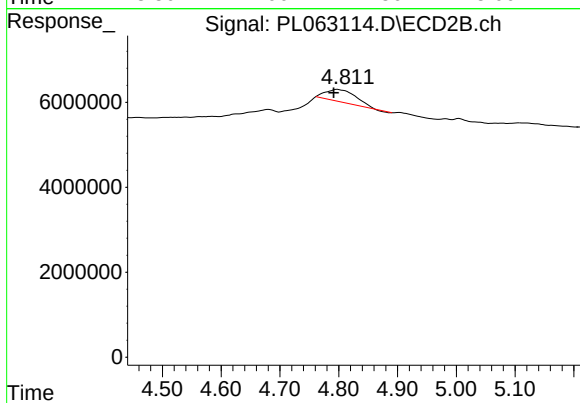

#6 beta-BHC


R.T.: 4.798 min
Delta R.T.: 0.006 min
Response: 10297782
Conc: 5.47 ng/ml

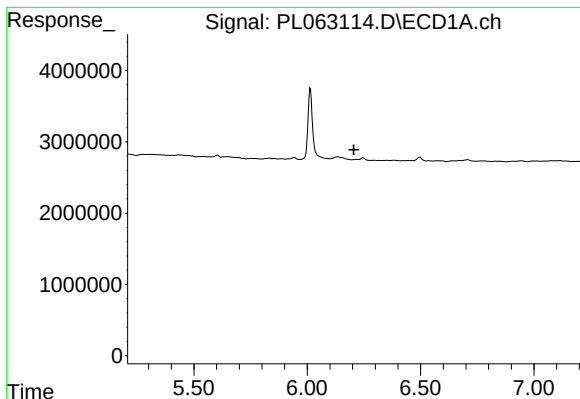

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

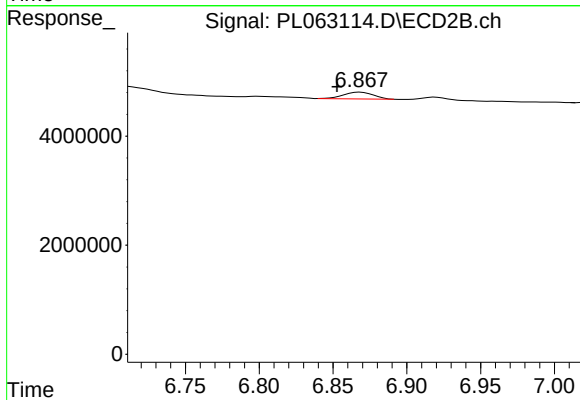


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 1717688
Conc: 0.60 ng/ml

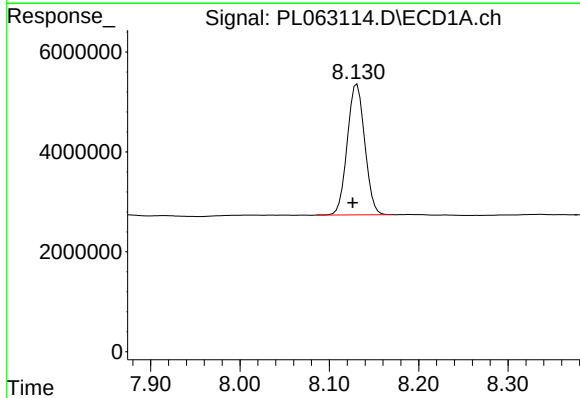

#28 Decachlorobiphenyl

R.T.: 8.131 min
Delta R.T.: 0.005 min
Response: 35619557
Conc: 22.20 ng/ml

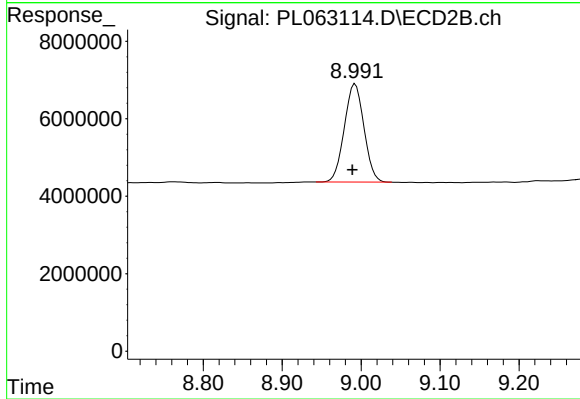

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.004 min
Response: 43796110
Conc: 20.93 ng/ml