

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111920\
 Data File : PL063117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2020 16:33
 Operator : DD\AJ
 Sample : L4776-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 04:53:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.949	35865334	59712271	20.851	20.319
28)	SA Decachlor...	8.124	8.986	40086004	47508296	24.987	22.699
Target Compounds							
7)	B delta-BHC	0.000	4.981f	0	4637069	N.D.	1.325 #
8)	B Heptachlo...	5.095	5.826	3304774	5167002	1.811	1.595
9)	A Endosulfan I	5.458f	0.000	3137356	0	1.877	N.D. #
12)	B 4,4'-DDE	0.000	6.258f	0	2429380	N.D.	0.754 #
15)	B Endosulfa...	0.000	6.864	0	4227866	N.D.	1.479 #
23)	Chlordane-1	4.259	0.000	476135	0	9.236	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111920\
Data File : PL063117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2020 16:33
Operator : DD\AJ
Sample : L4776-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 04:53:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

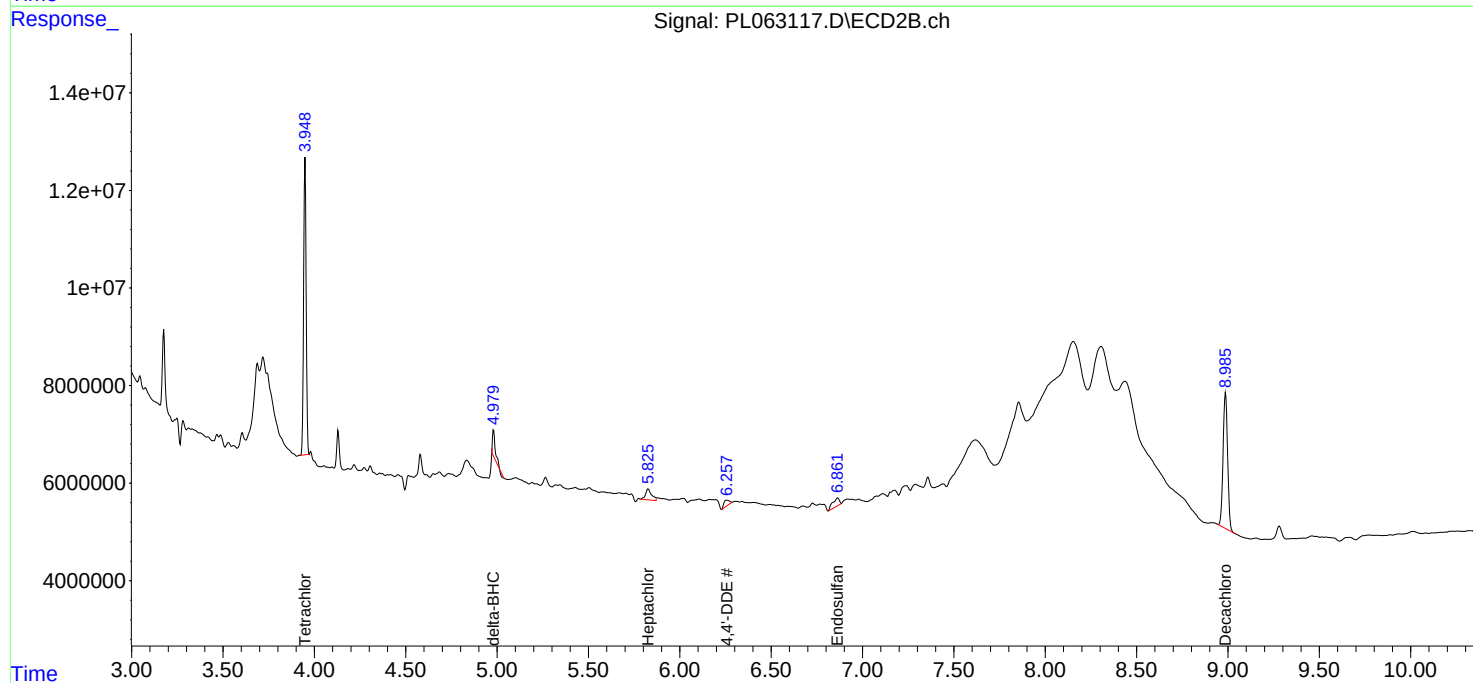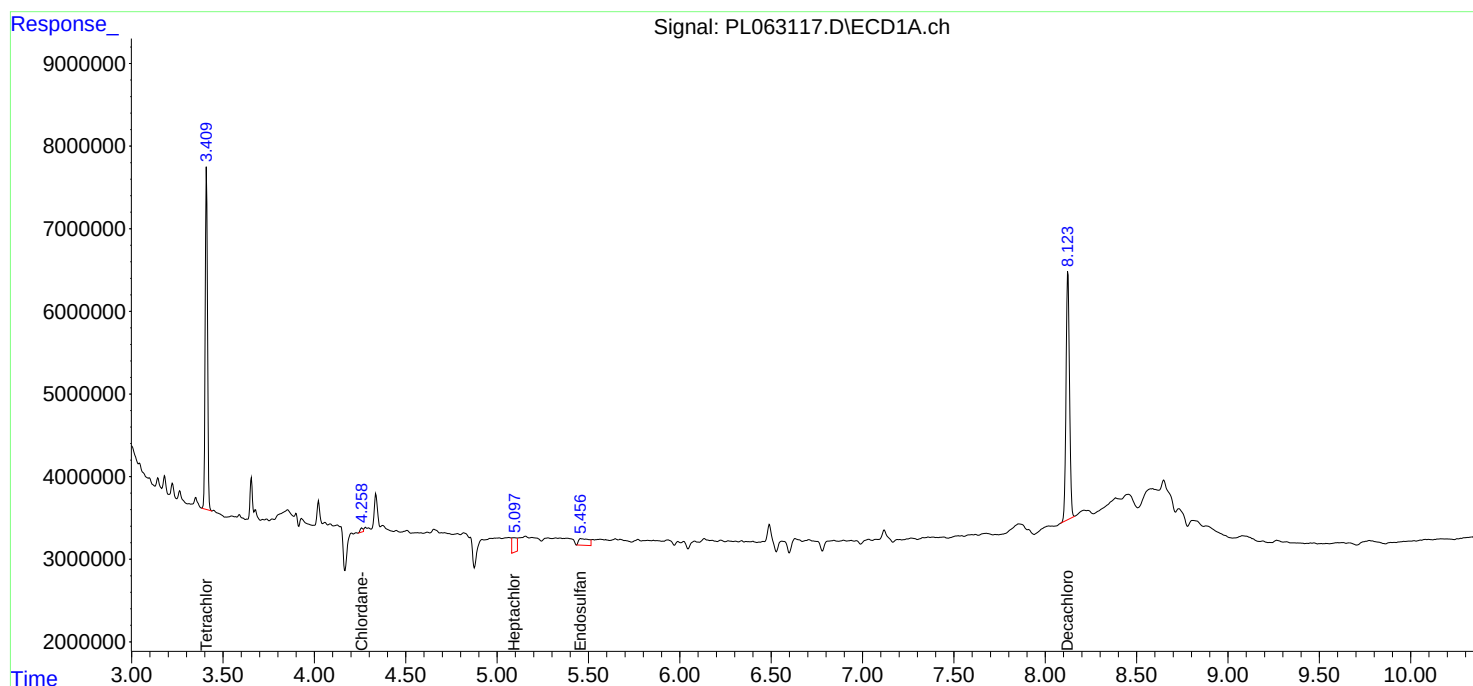


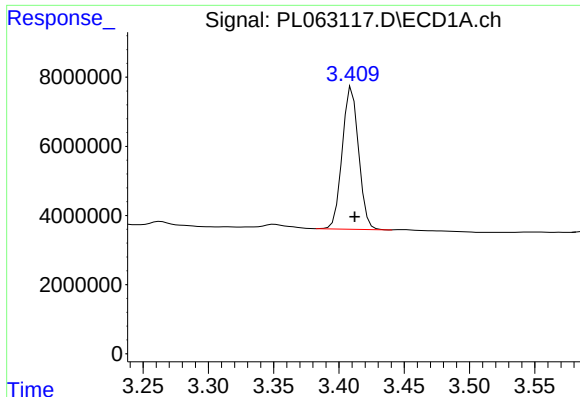

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 35865334
Conc: 20.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

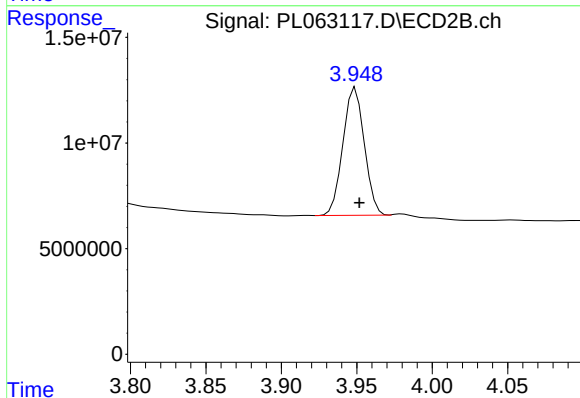


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 59712271
Conc: 20.32 ng/ml

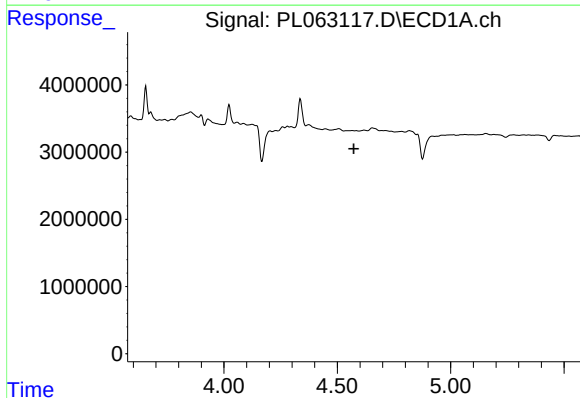


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

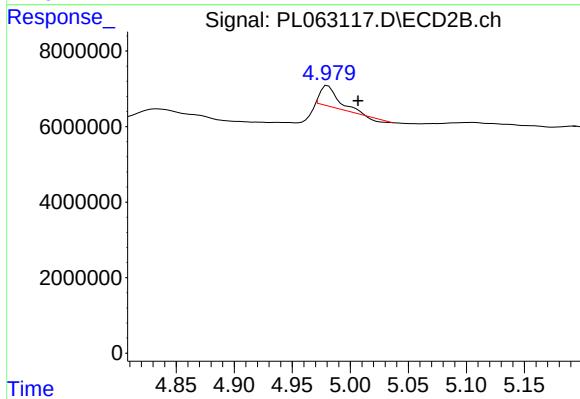

#7 delta-BHC


R.T.: 4.981 min
Delta R.T.: -0.026 min
Response: 4637069
Conc: 1.33 ng/ml

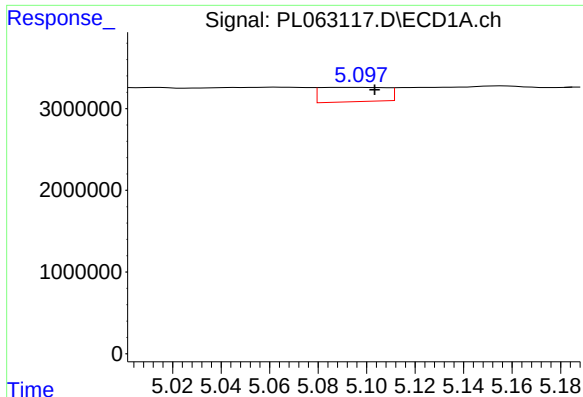

#8 Heptachlor epoxide


R.T.: 5.095 min
Delta R.T.: -0.009 min
Response: 3304774
Conc: 1.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

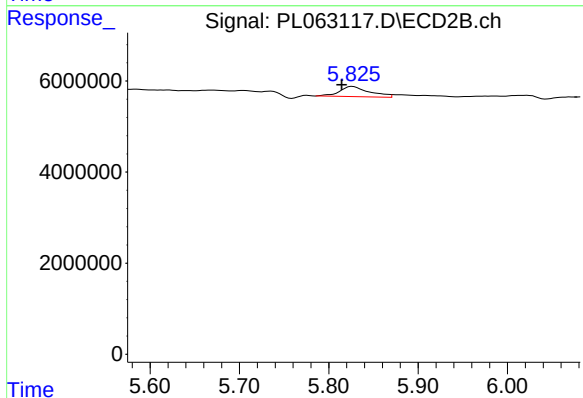


#8 Heptachlor epoxide

R.T.: 5.826 min
Delta R.T.: 0.012 min
Response: 5167002
Conc: 1.60 ng/ml

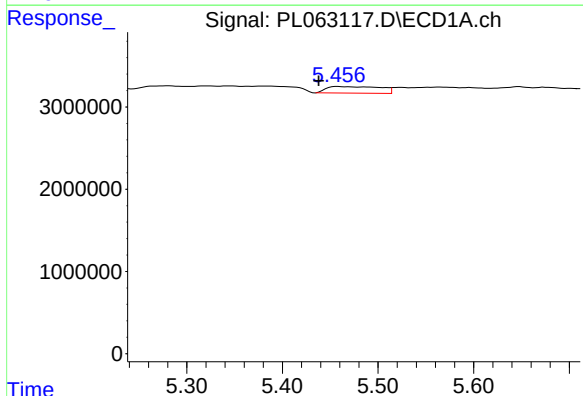


#9 Endosulfan I

R.T.: 5.458 min
Delta R.T.: 0.020 min
Response: 3137356
Conc: 1.88 ng/ml

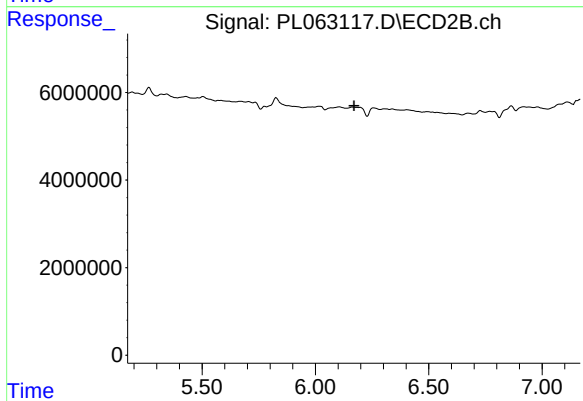

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

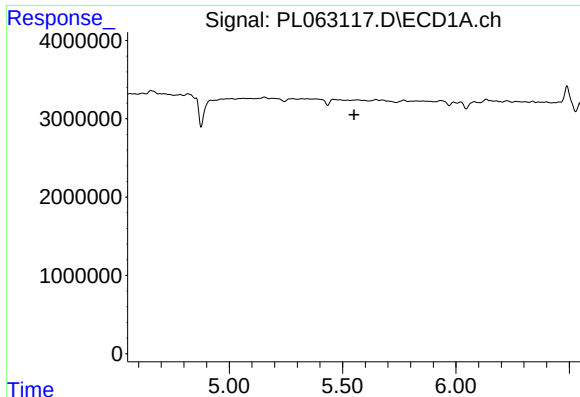

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

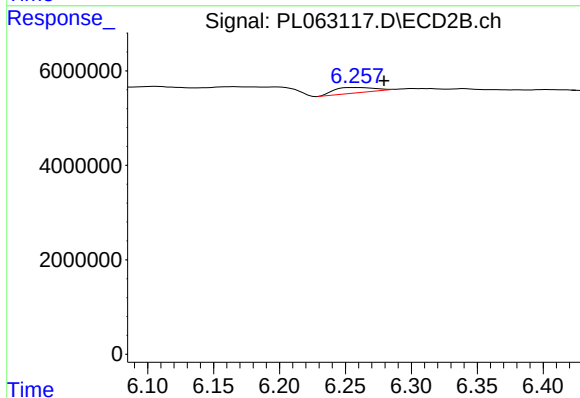


#12 4,4'-DDE

R.T.: 6.258 min
Delta R.T.: -0.022 min
Response: 2429380
Conc: 0.75 ng/ml

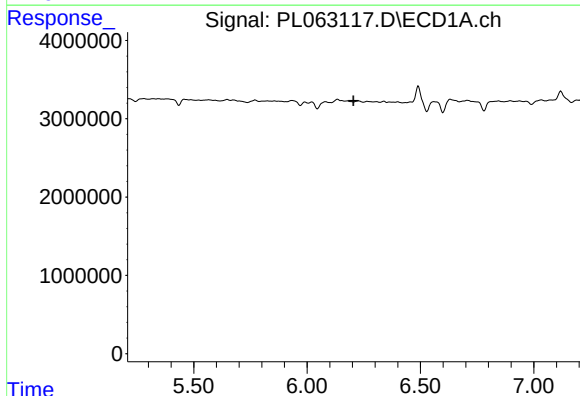


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

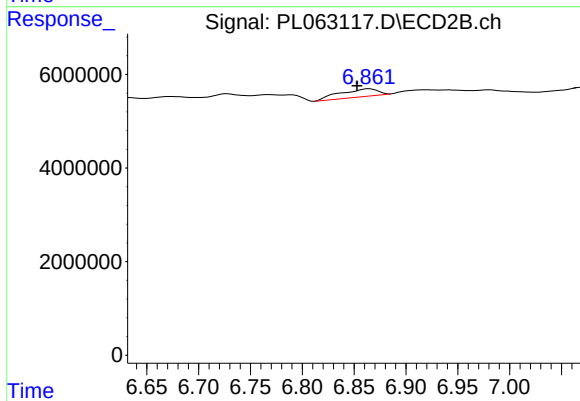

#15 Endosulfan II


R.T.: 6.864 min
Delta R.T.: 0.012 min
Response: 4227866
Conc: 1.48 ng/ml

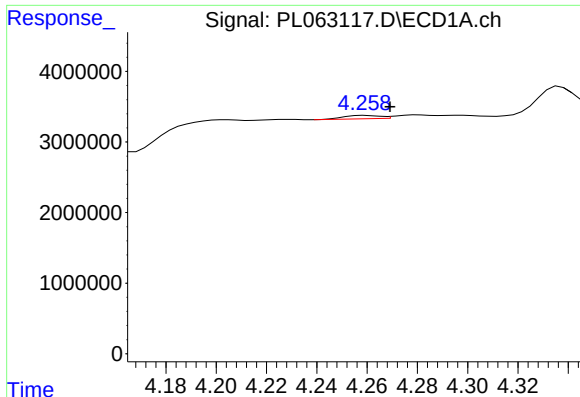

#23 Chlordane-1


R.T.: 4.259 min
Delta R.T.: -0.010 min
Response: 476135
Conc: 9.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

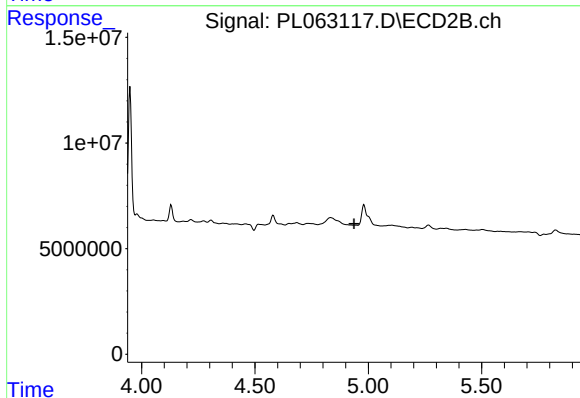


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

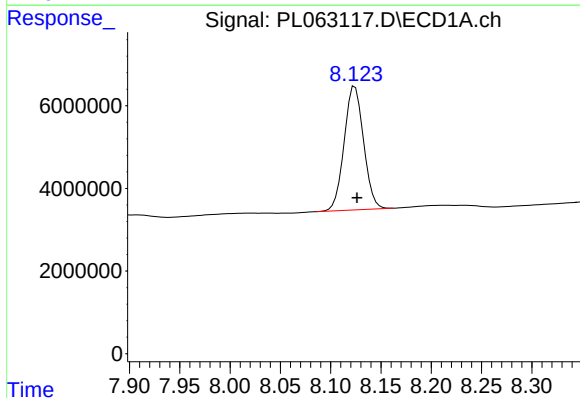

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 40086004
Conc: 24.99 ng/ml

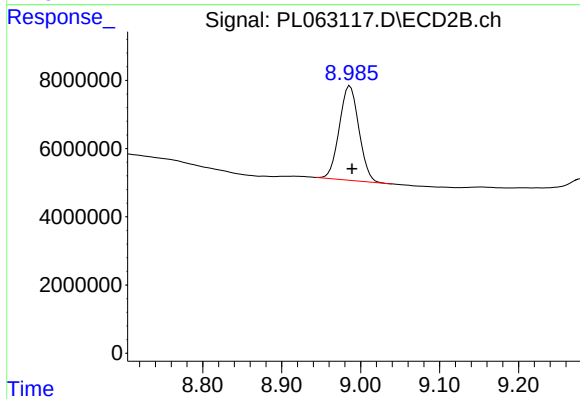

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: -0.002 min
Response: 47508296
Conc: 22.70 ng/ml