

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111921\
 Data File : PL071084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2021 16:02
 Operator : AR\AJ
 Sample : M4767-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-13-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 05:14:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.500	10102528	26363334	20.626	20.909
28)	SA Decachlor...	10.326	11.388	12418504	23926002	18.174	17.890
Target Compounds							
18)	B Endrin al...	8.510f	0.000	122874	0	0.270	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111921\
Data File : PL071084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2021 16:02
Operator : AR\AJ
Sample : M4767-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-13-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 05:14:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

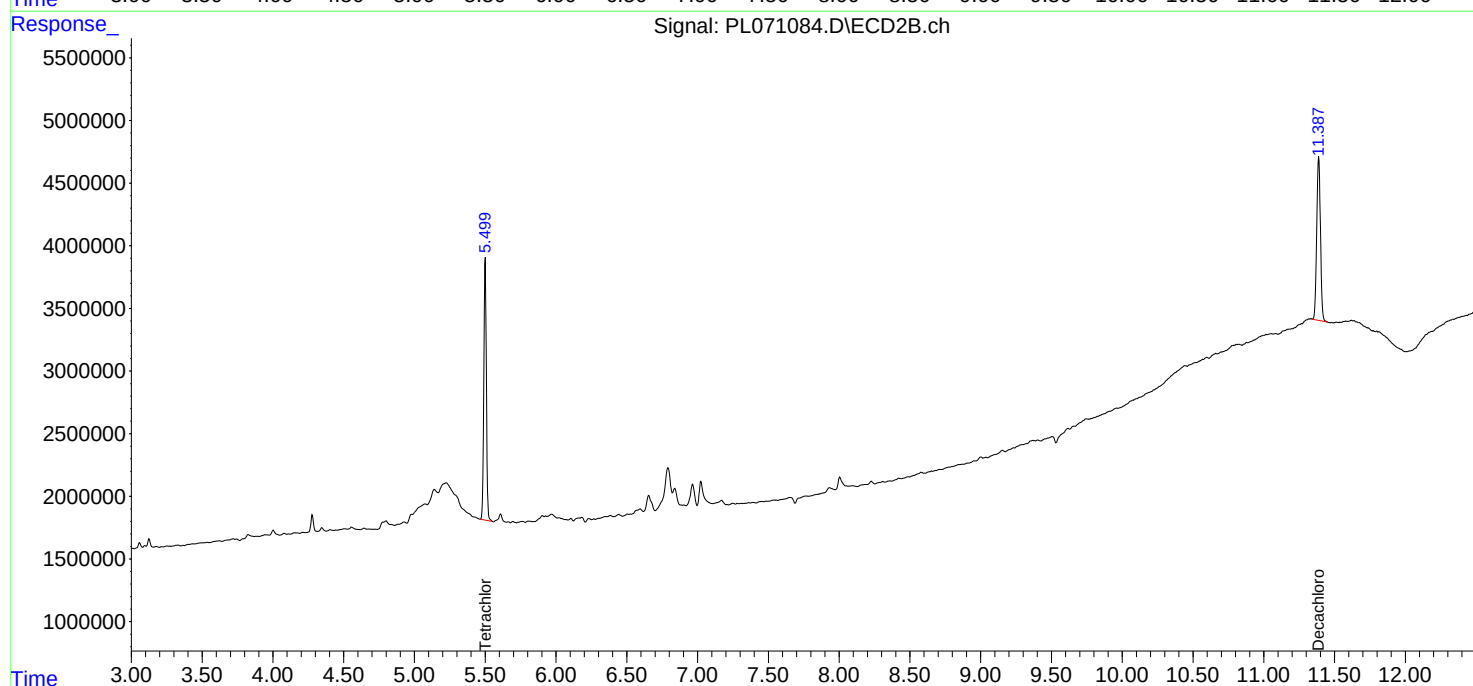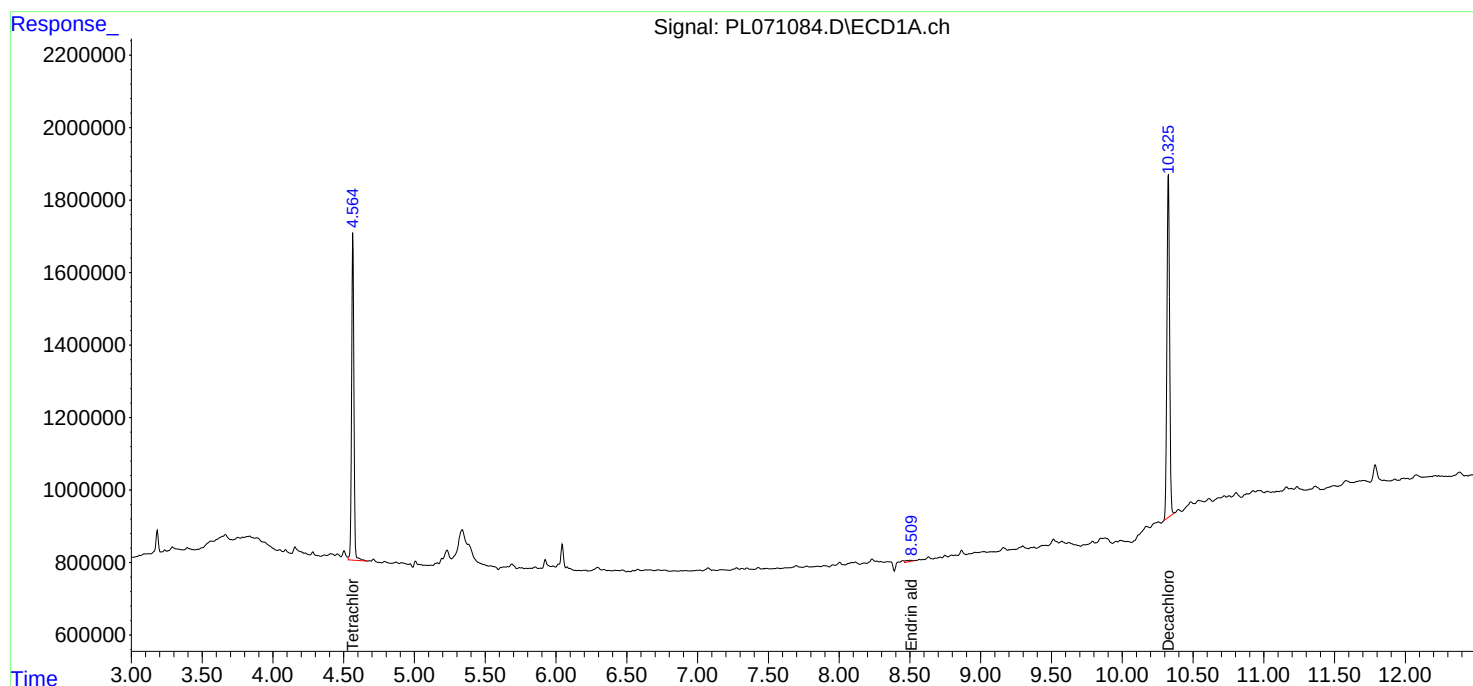


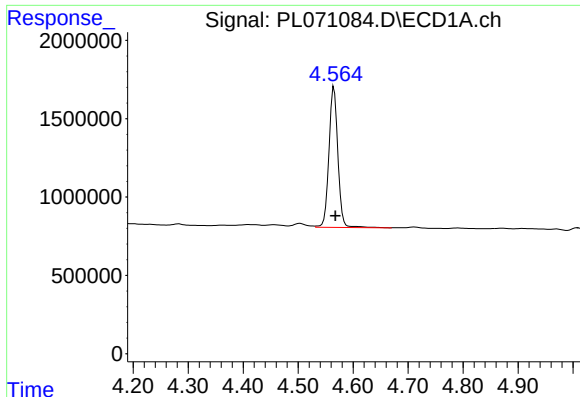

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: -0.003 min
Response: 10102528
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-COMP

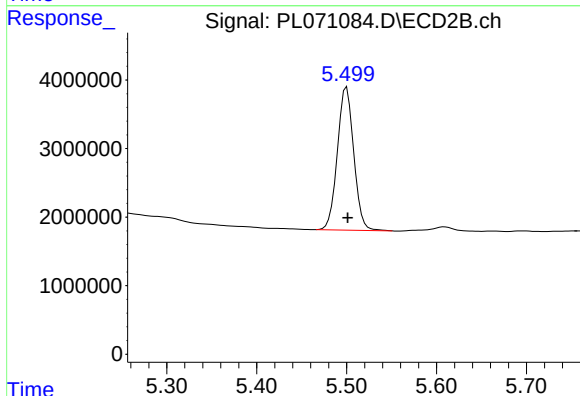


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.001 min
Response: 26363334
Conc: 20.91 ng/ml

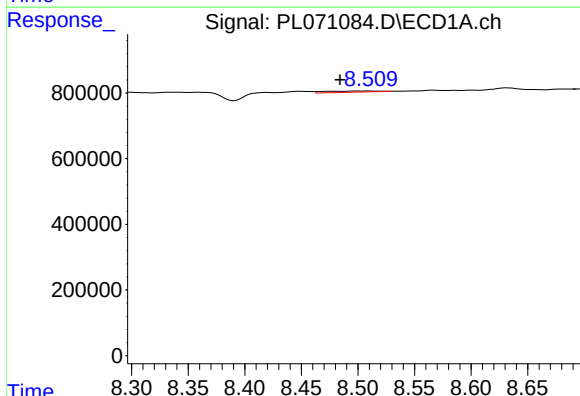


#18 Endrin aldehyde

R.T.: 8.510 min
Delta R.T.: 0.026 min
Response: 122874
Conc: 0.27 ng/ml

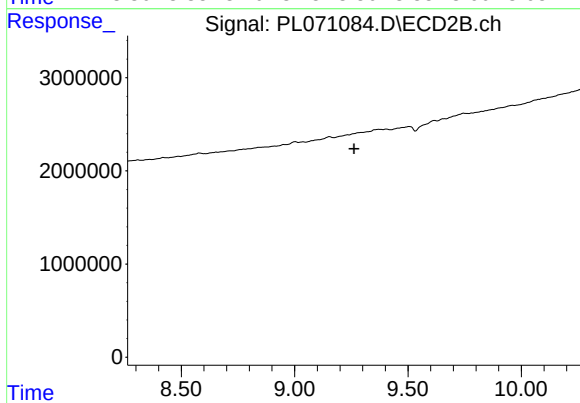

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 9.262 min
Response: 0
Conc: N.D.

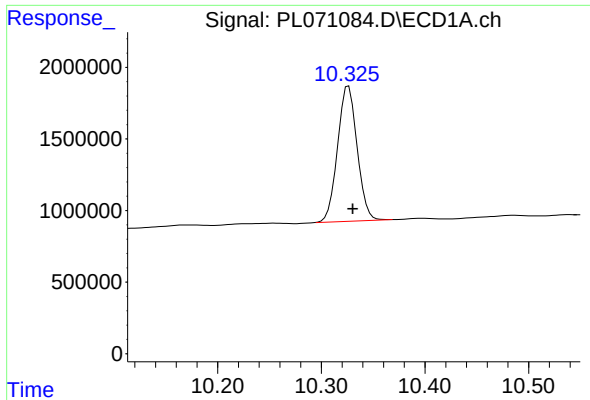

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: -0.004 min
Response: 12418504
Conc: 18.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-COMP

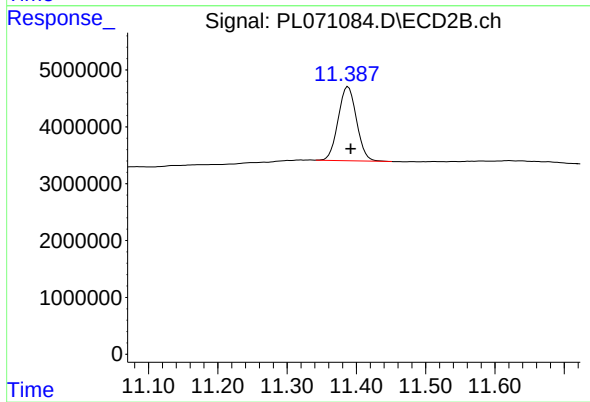

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: -0.004 min
Response: 23926002
Conc: 17.89 ng/ml