

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111921\
 Data File : PL071074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2021 13:16
 Operator : AR\AJ
 Sample : M4754-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-12-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/22/2021
 Supervised By :Ankita Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 05:12:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.501	9242537	24785766	18.870m	19.658
2)	SA Decachlor...	10.329	11.390	11181252	20661714	16.364	15.449

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111921\
Data File : PL071074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2021 13:16
Operator : AR\AJ
Sample : M4754-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-12-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/22/2021
Supervised By : Ankita Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 05:12:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

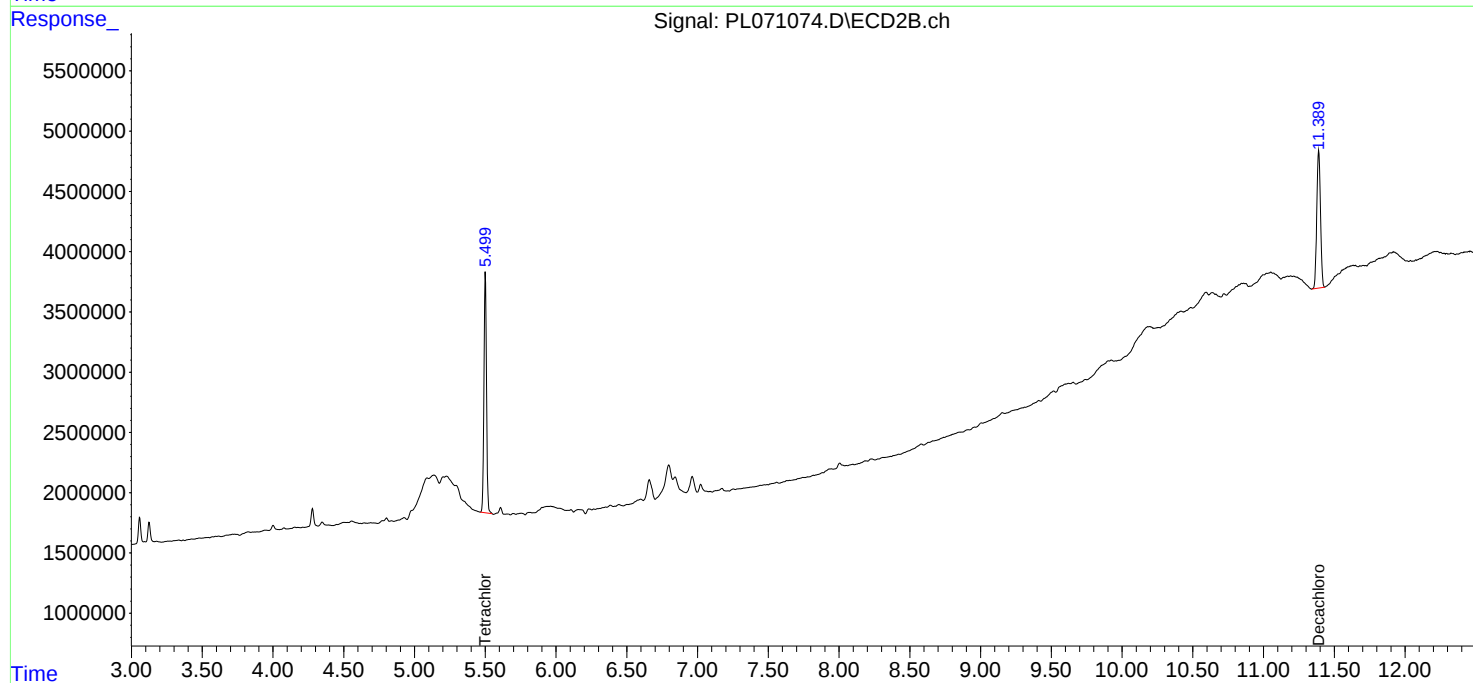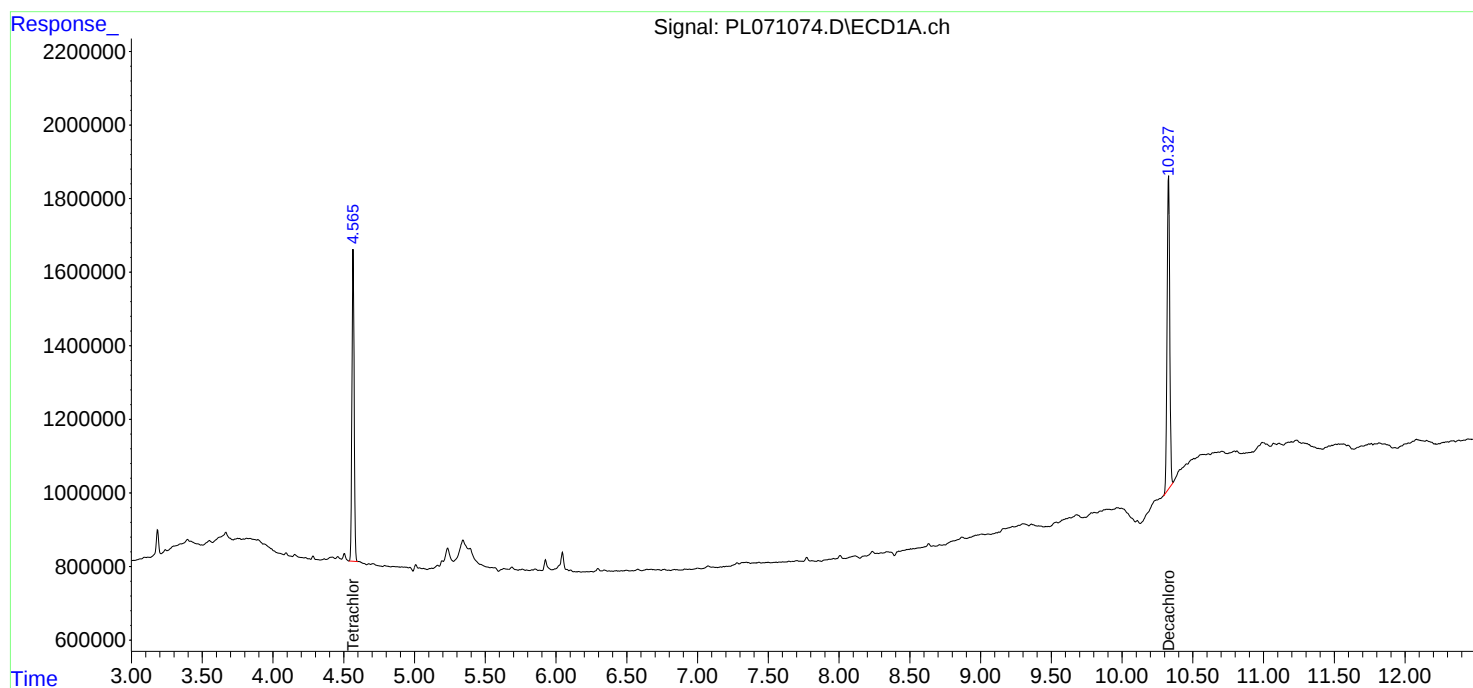

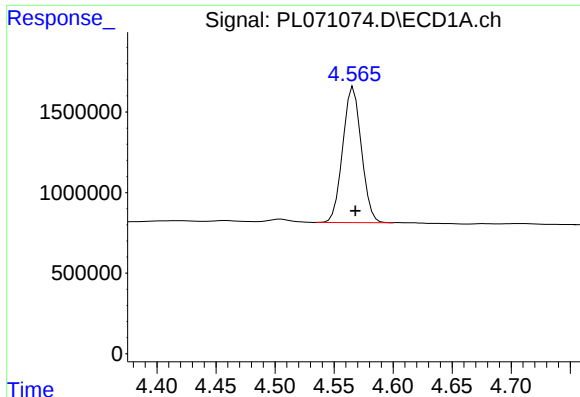


#1 Tetrachloro-m-xylene

R.T.: 4.565 min
Delta R.T.: -0.003 min
Response: 9242537
Conc: 18.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/22/2021
Supervised By :Ankita Jodhani 11/22/2021

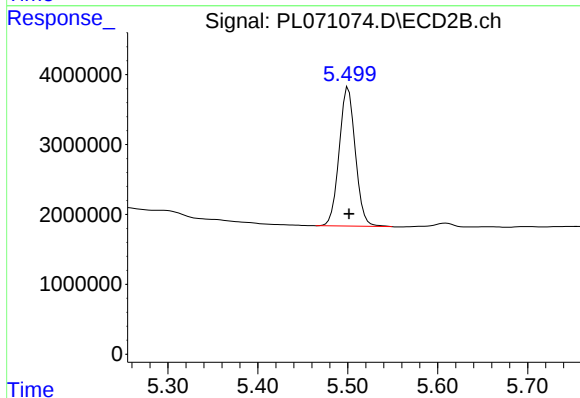


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 24785766
Conc: 19.66 ng/ml

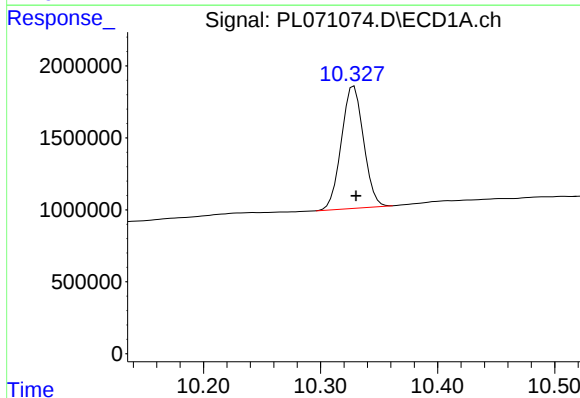

#28 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: -0.002 min
Response: 11181252
Conc: 16.36 ng/ml

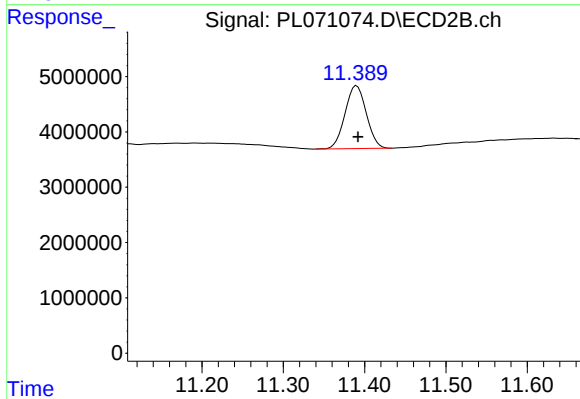

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: -0.002 min
Response: 20661714
Conc: 15.45 ng/ml