

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111924\
 Data File : PL093144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 14:57
 Operator : AR\AJ
 Sample : P4860-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PH2-BOT-005

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :Ankita Jodhani 11/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 23:04:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.534	2.773	48591948	53548701	19.832m	19.679
28) SA Decachlor...	9.054	7.913	31773803	51111175	16.510	18.727

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111924\
Data File : PL093144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 14:57
Operator : AR\AJ
Sample : P4860-10
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PH2-BOT-005


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :Ankita Jodhani 11/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 23:04:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

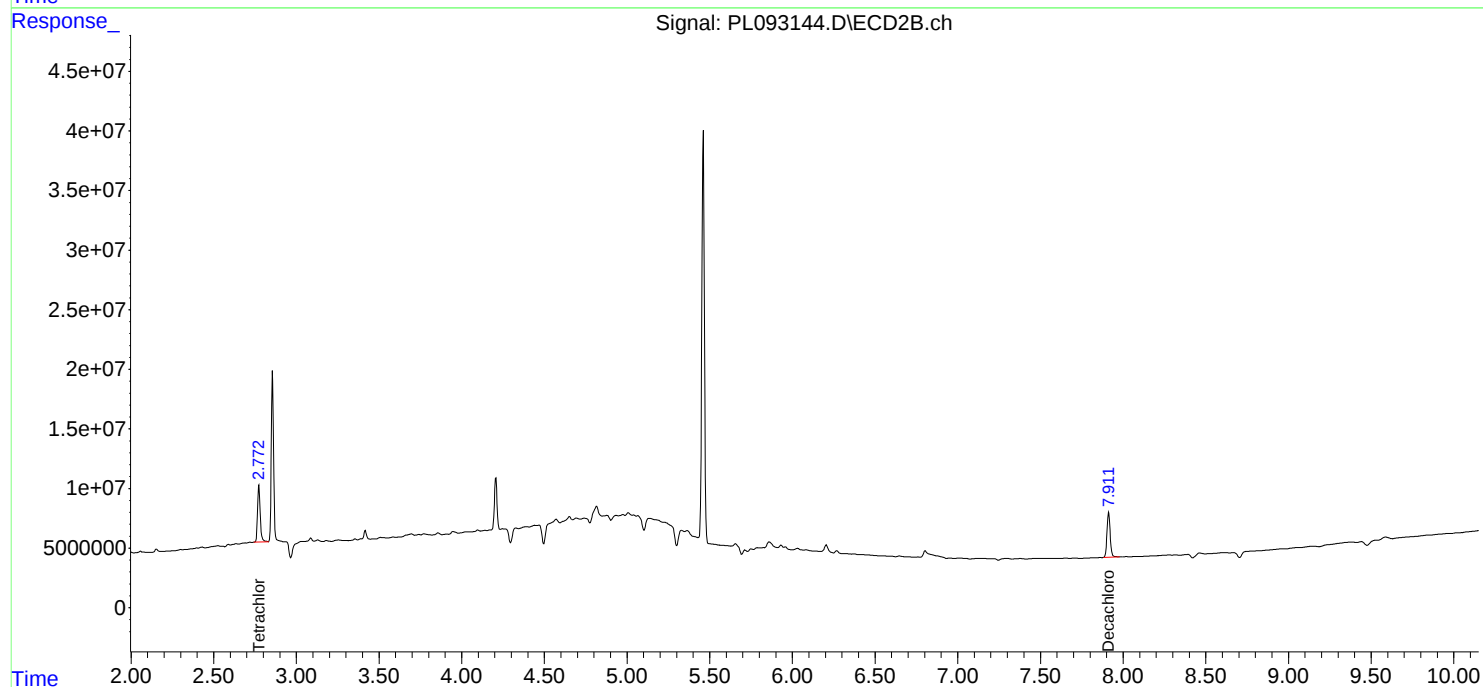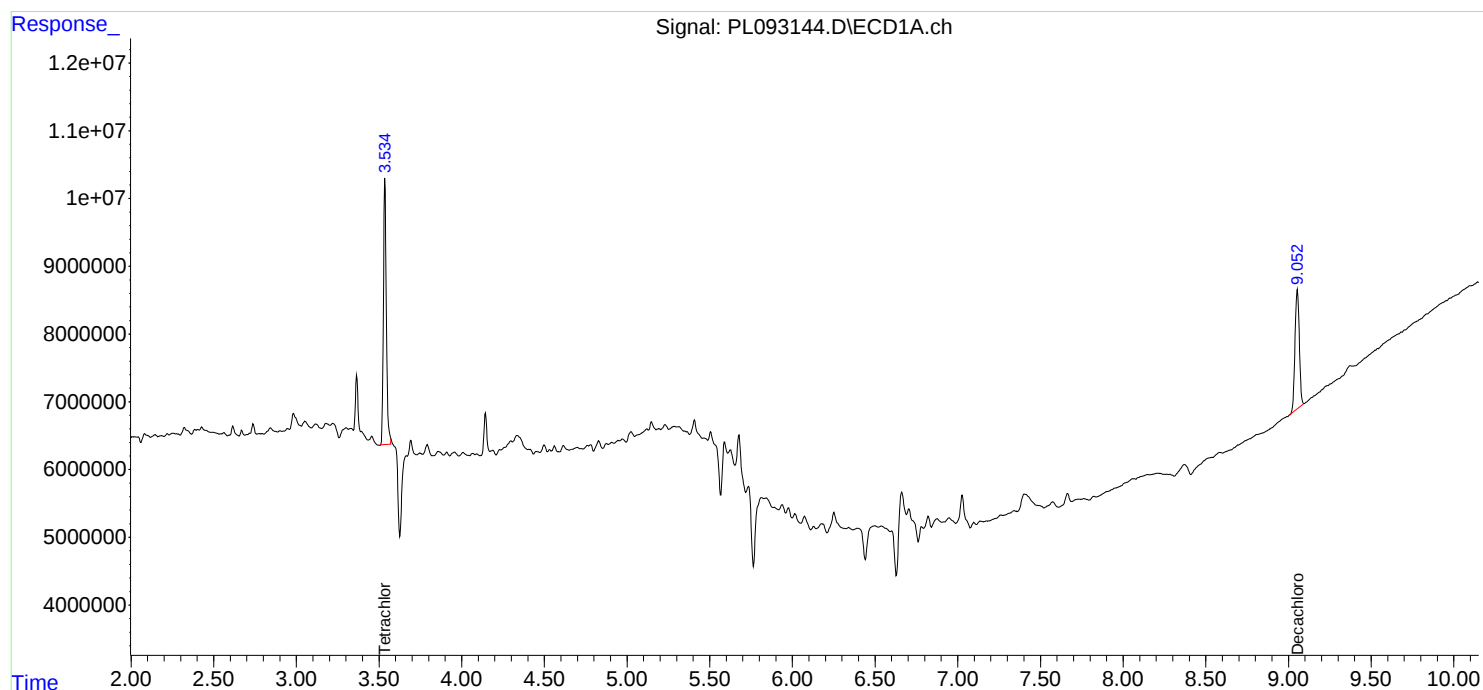

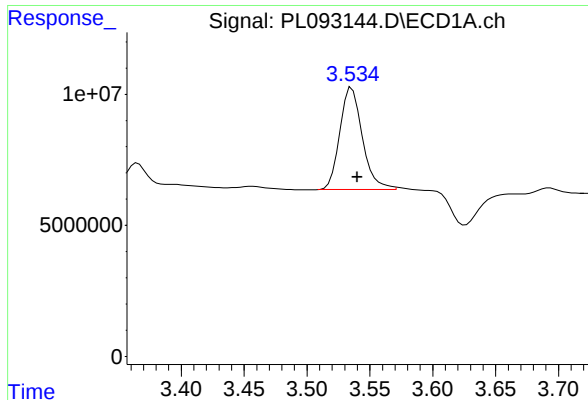


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.006 min
Response: 48591948
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PH2-BOT-005


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :Ankita Jodhani 11/20/2024

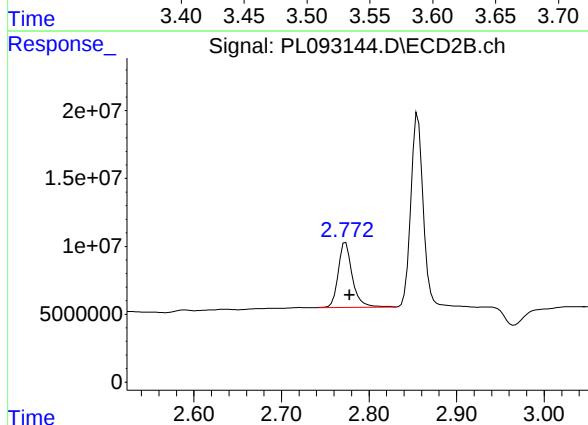


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: -0.004 min
Response: 53548701
Conc: 19.68 ng/ml

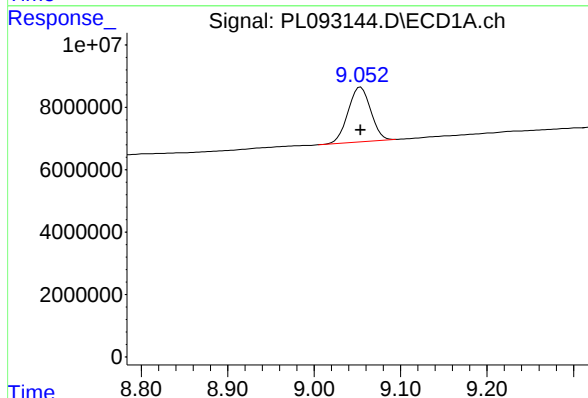

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 31773803
Conc: 16.51 ng/ml

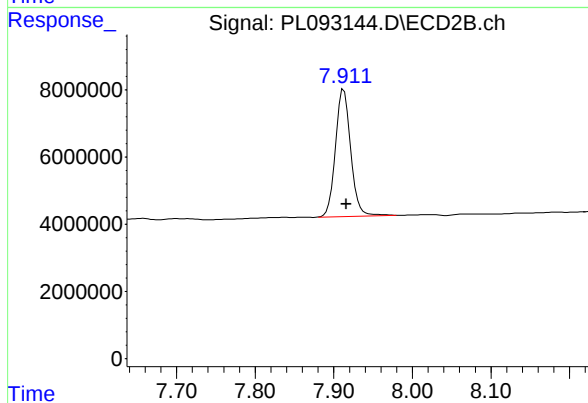

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: -0.003 min
Response: 51111175
Conc: 18.73 ng/ml