

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
 Data File : PL042271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 09:34
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:49:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) MB Aldrin	0.000	5.565f	0	2274893	N.D.	0.592 #
6) B beta-BHC	4.401f	4.904f	5671591	693534	1.601	0.440 #
7) B delta-BHC	0.000	5.161	0	3292875	N.D.	0.895 #
8) B Heptachlo...	0.000	5.992	0	7899058	N.D.	2.203 #
15) B Endosulfa...	6.230f	0.000	2835634	0	0.454	N.D. #
23) Chlordane-1	4.401	5.161	5671591	3292875	20.514	24.771
24) Chlordane-2	0.000	5.565	0	2274893	N.D.	16.314 #
27) Chlordane-5	6.230	0.000	2835634	0	9.516	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
Data File : PL042271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 09:34
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:49:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

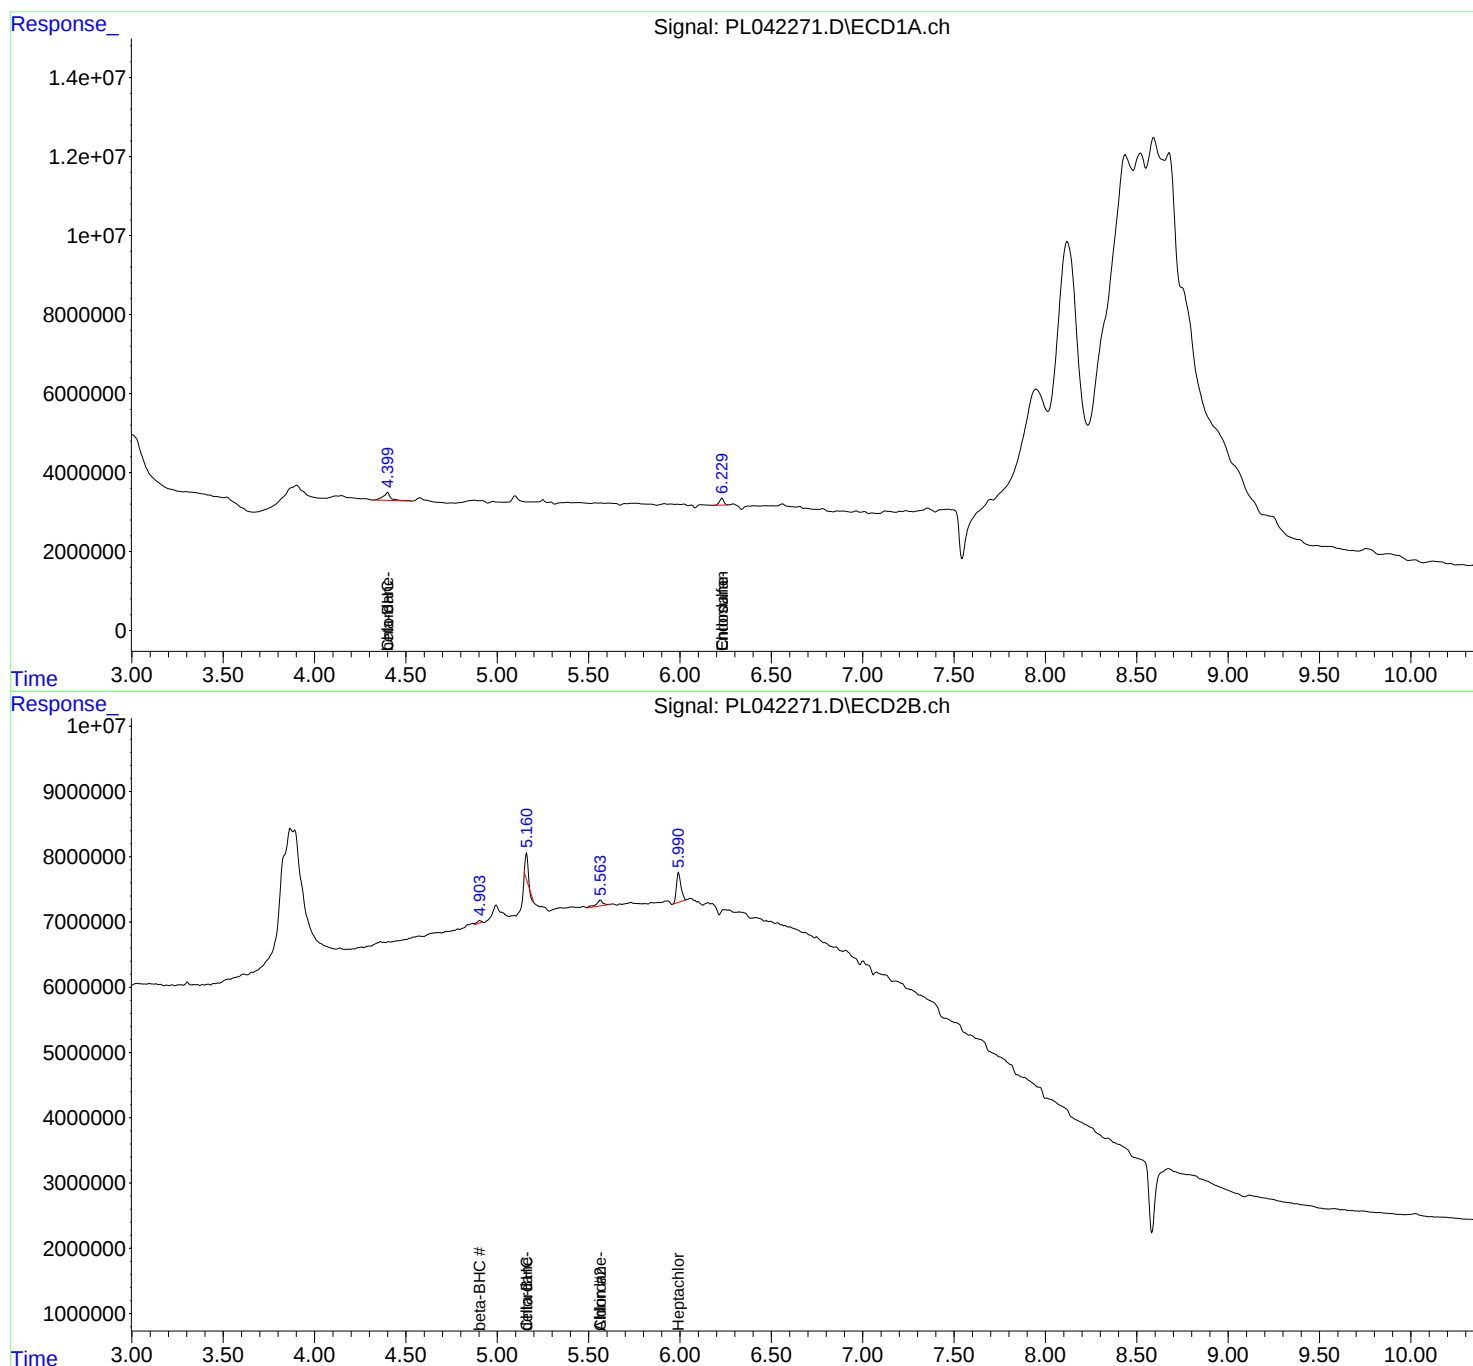


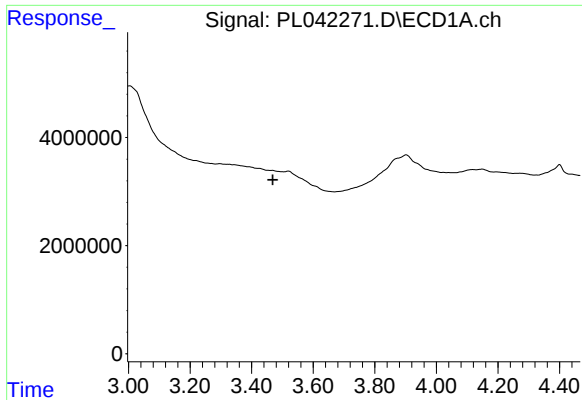

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

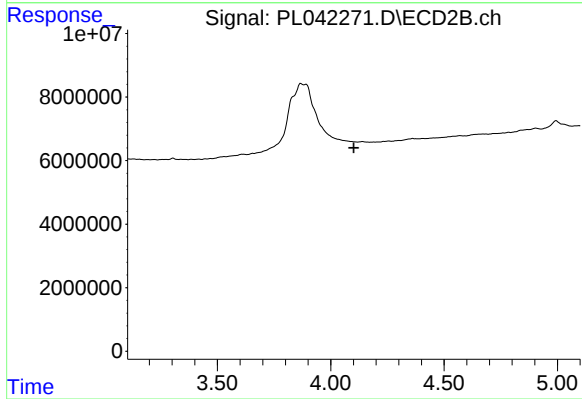


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.102 min
Response: 0
Conc: N.D.

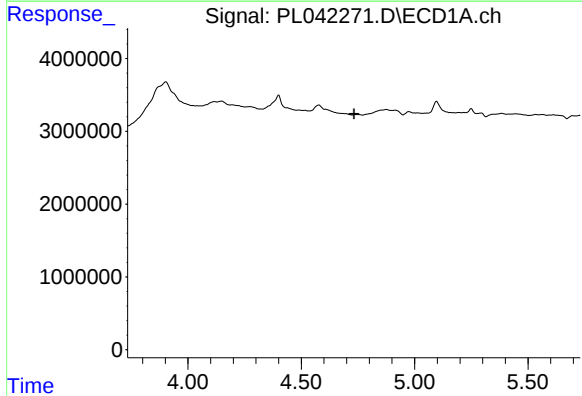


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.733 min
Response: 0
Conc: N.D.

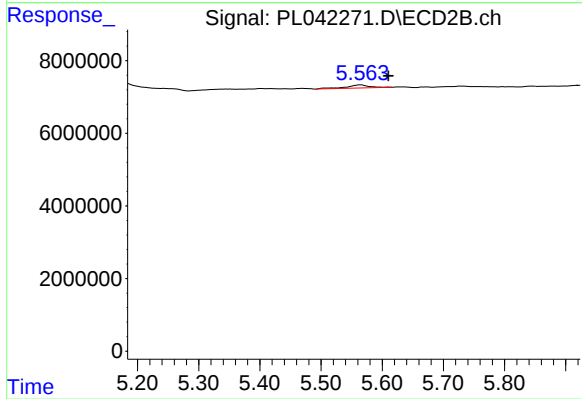

#5 Aldrin


R.T.: 5.565 min
Delta R.T.: -0.045 min
Response: 2274893
Conc: 0.59 ng/ml

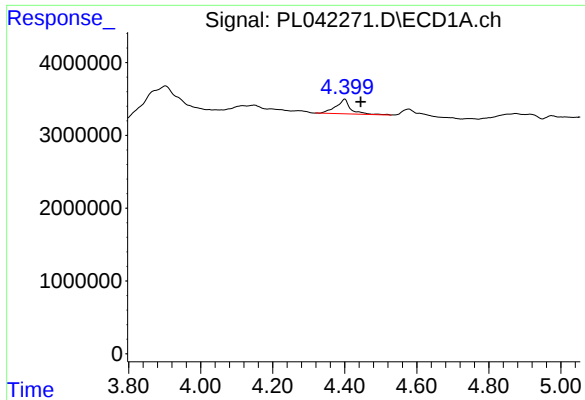

#6 beta-BHC


R.T.: 4.401 min
Delta R.T.: -0.044 min
Response: 5671591
Conc: 1.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

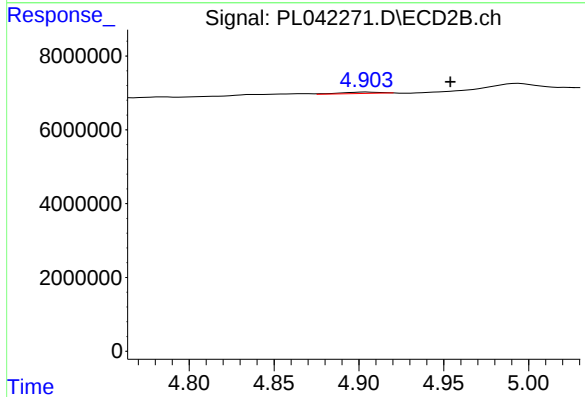


#6 beta-BHC

R.T.: 4.904 min
Delta R.T.: -0.050 min
Response: 693534
Conc: 0.44 ng/ml

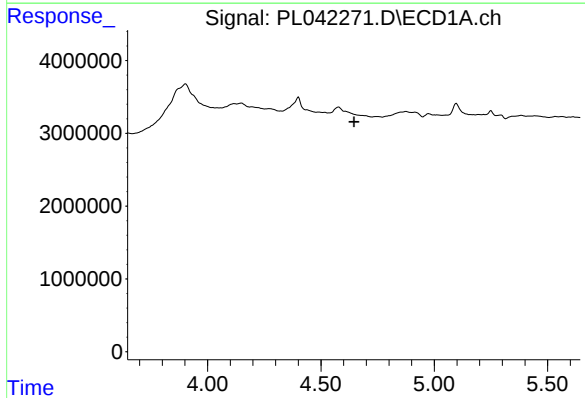


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.646 min
Response: 0
Conc: N.D.

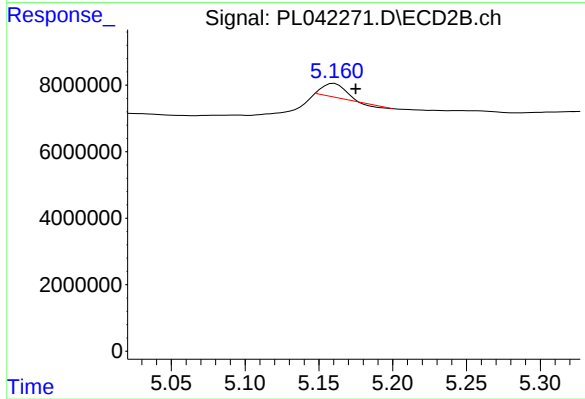

#7 delta-BHC


R.T.: 5.161 min
Delta R.T.: -0.014 min
Response: 3292875
Conc: 0.89 ng/ml

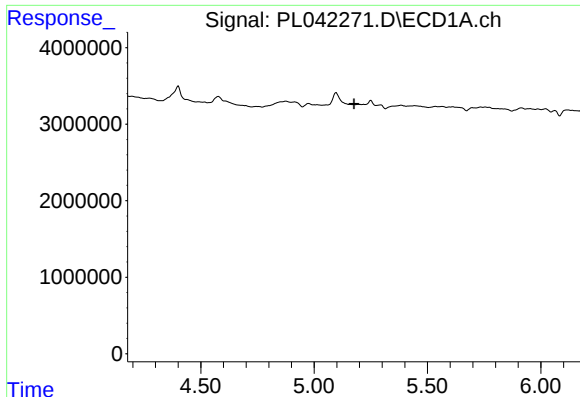

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

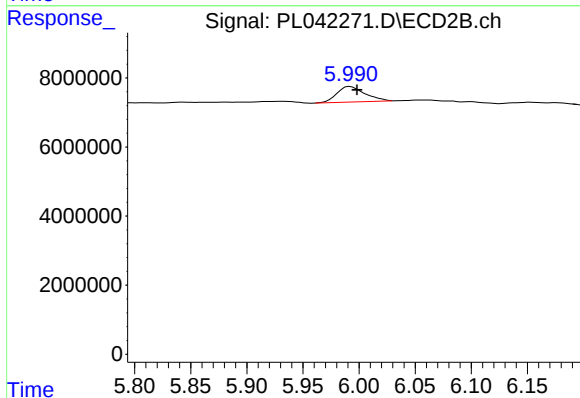


#8 Heptachlor epoxide

R.T.: 5.992 min
Delta R.T.: -0.006 min
Response: 7899058
Conc: 2.20 ng/ml

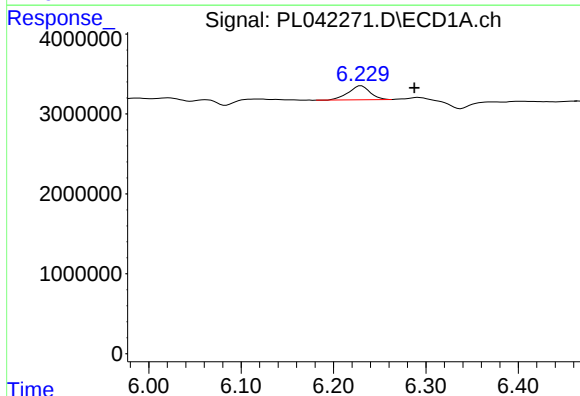


#15 Endosulfan II

R.T.: 6.230 min
Delta R.T.: -0.058 min
Response: 2835634
Conc: 0.45 ng/ml

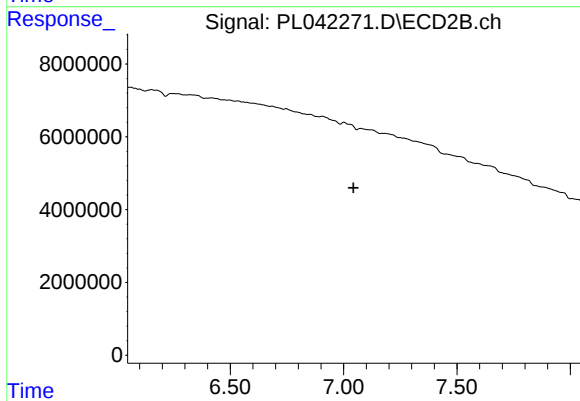

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.044 min
Response: 0
Conc: N.D.

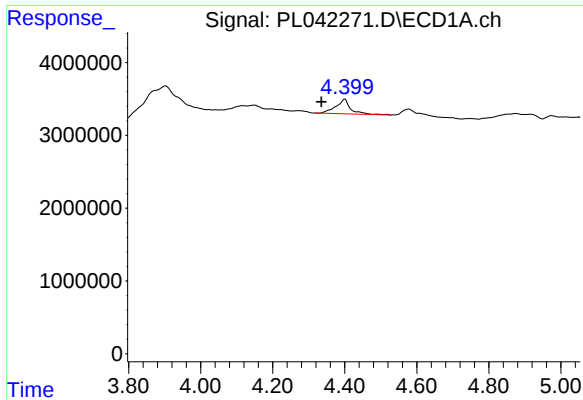

#23 Chlordane-1


R.T.: 4.401 min
Delta R.T.: 0.065 min
Response: 5671591
Conc: 20.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

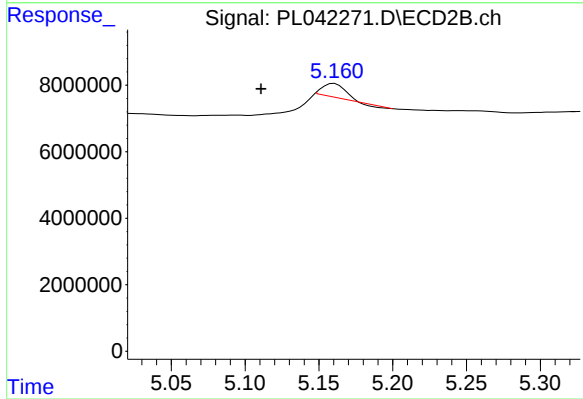


#23 Chlordane-1

R.T.: 5.161 min
Delta R.T.: 0.050 min
Response: 3292875
Conc: 24.77 ng/ml

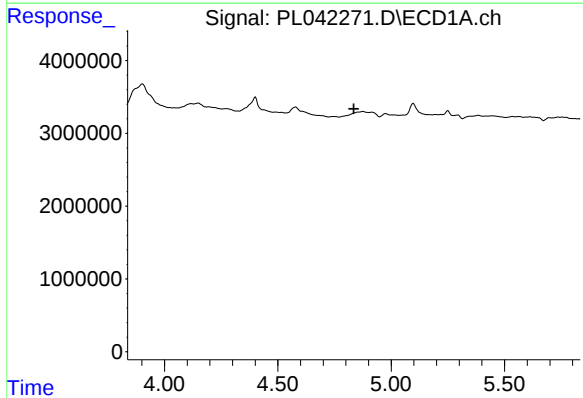


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.835 min
Response: 0
Conc: N.D.

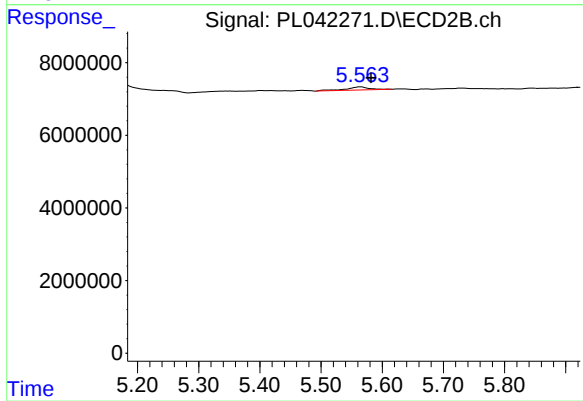

#24 Chlordane-2


R.T.: 5.565 min
Delta R.T.: -0.017 min
Response: 2274893
Conc: 16.31 ng/ml

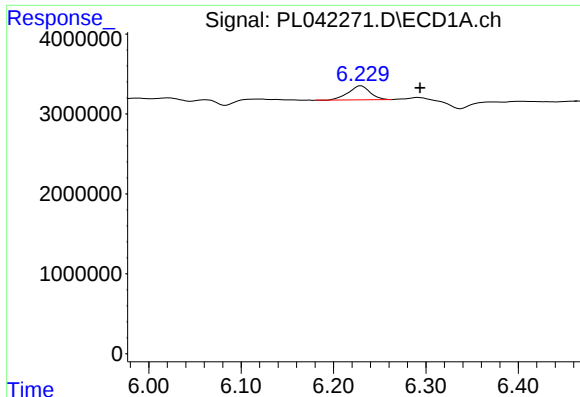

#27 Chlordane-5


R.T.: 6.230 min
Delta R.T.: -0.064 min
Response: 2835634
Conc: 9.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

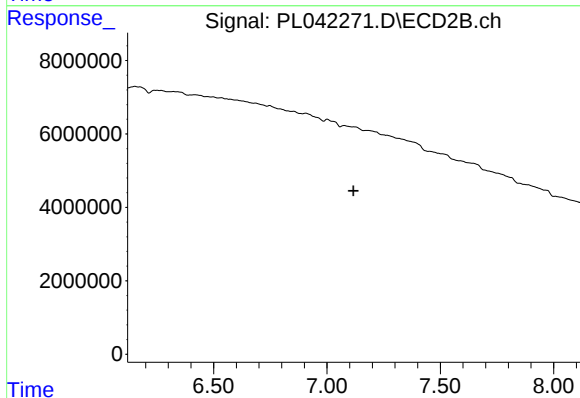


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

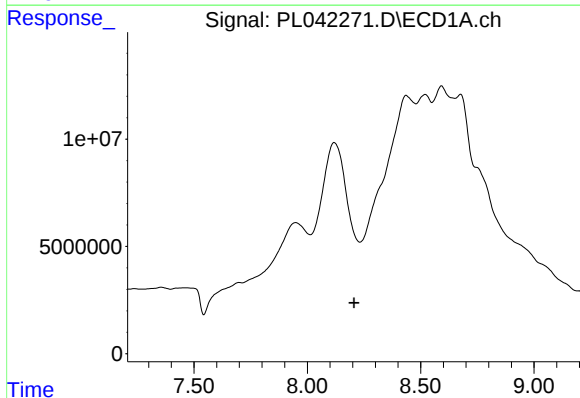

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.207 min
Response: 0
Conc: N.D.

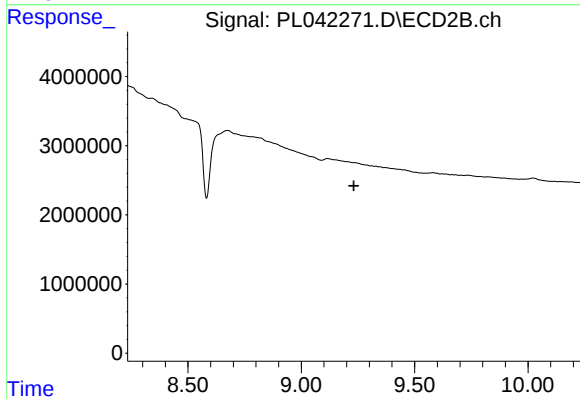

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.232 min
Response: 0
Conc: N.D.