

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
 Data File : PL042310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 21:23
 Operator : AJ\SJ
 Sample : J5964-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:53:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	110.1E6	59068643	18.716	20.538
28)	SA Decachlor...	8.207	9.233	110.0E6	44560712	17.451	18.476
Target Compounds							
3)	MA gamma-BHC...	4.199	0.000	1560879	0	0.189	N.D. #
6)	B beta-BHC	4.403f	0.000	17367571	0	4.902	N.D. #
8)	B Heptachlo...	5.239f	5.995	2770806	2570410	0.366	0.717 #
9)	A Endosulfan I	5.543	0.000	3350489	0	0.484	N.D. #
19)	B Endosulfa...	6.656	7.385	7155627	5517731	1.147	1.984 #
20)	A Methoxychlor	0.000	7.648f	0	6154409	N.D.	4.514 #
21)	B Endrin ke...	7.202f	0.000	316730	0	0.046	N.D. #
23)	Chlordane-1	4.342	0.000	1486163	0	5.375	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
Data File : PL042310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 21:23
Operator : AJ\SJ
Sample : J5964-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:53:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

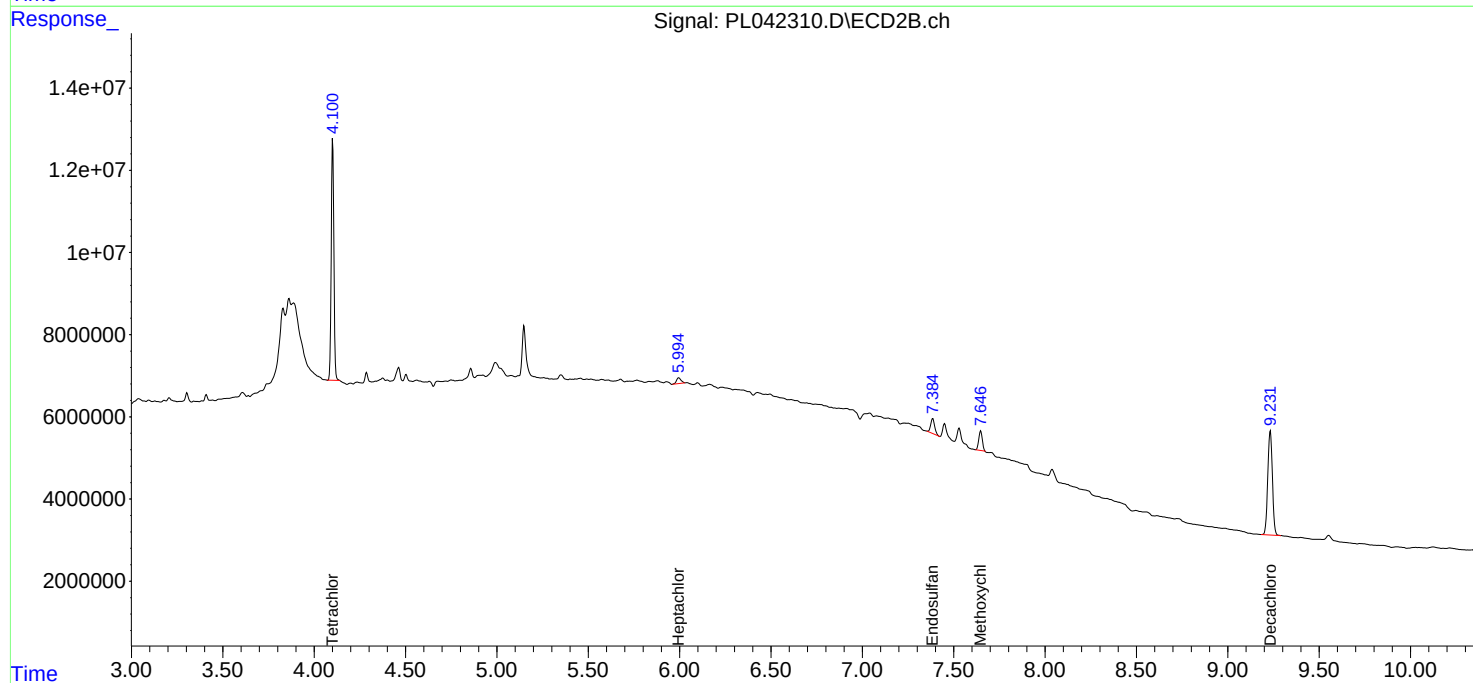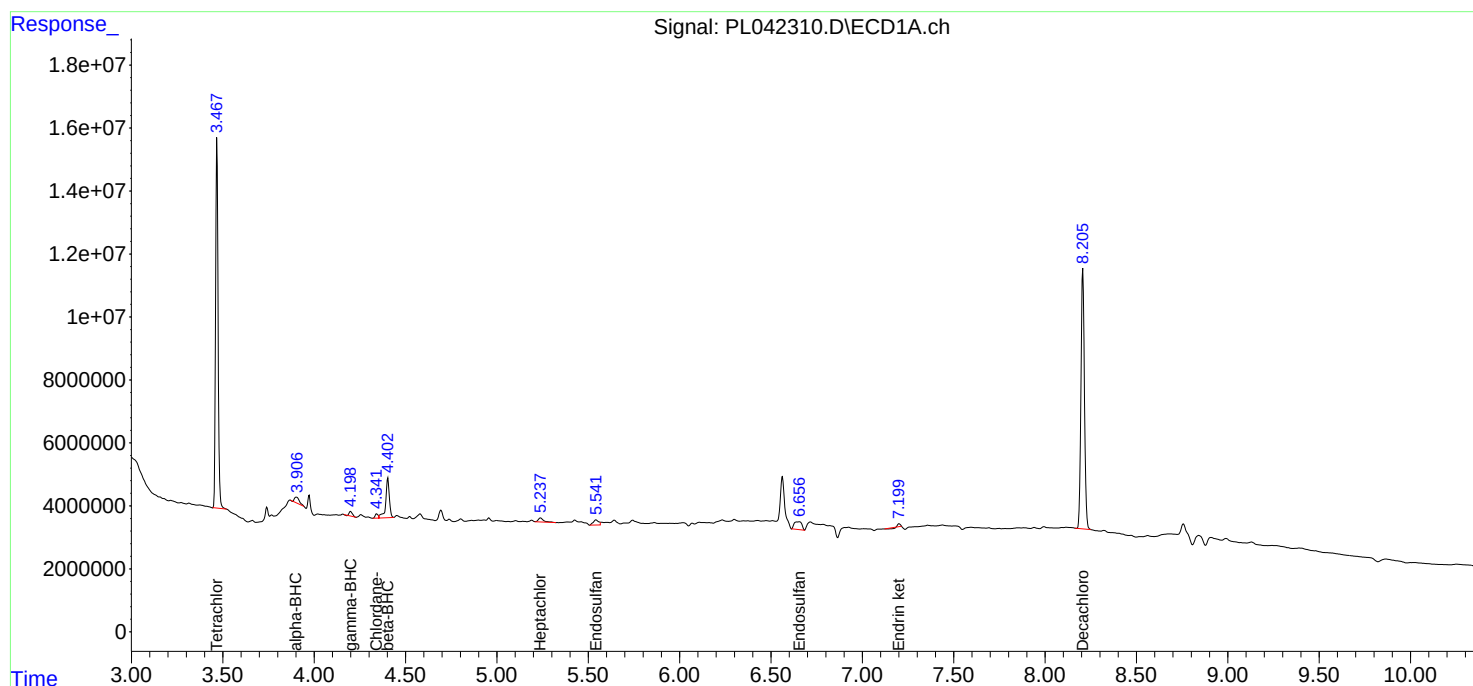


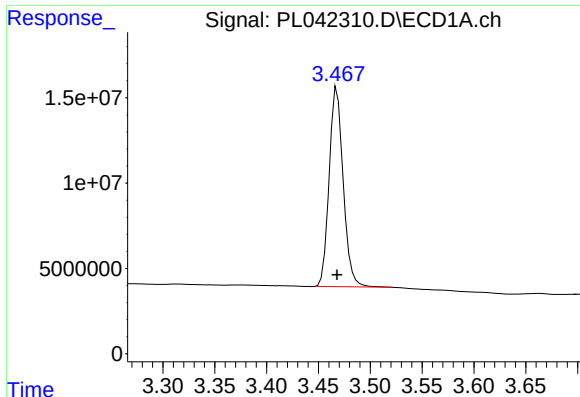

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 110113606
Conc: 18.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

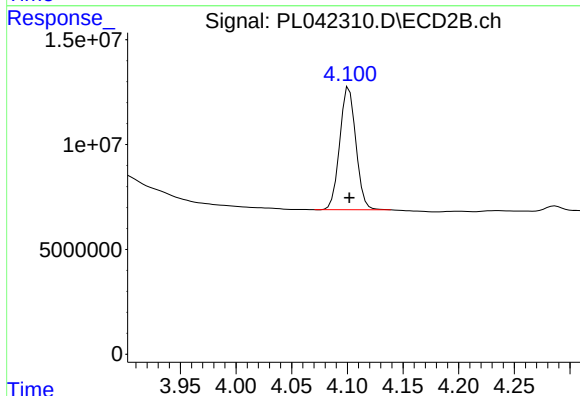


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 59068643
Conc: 20.54 ng/ml

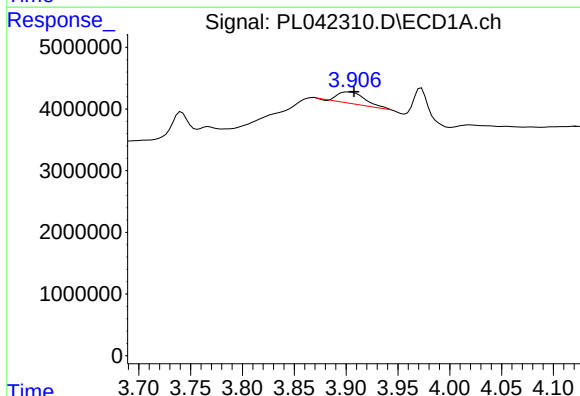


#2 alpha-BHC

R.T.: 3.902 min
Delta R.T.: -0.006 min
Response: 3227540
Conc: 0.36 ng/ml

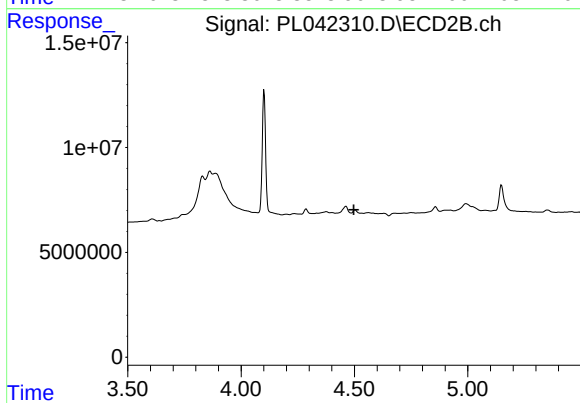

#2 alpha-BHC


R.T.: 4.503 min
Delta R.T.: 0.006 min
Response: -1794486
Conc: N.D.

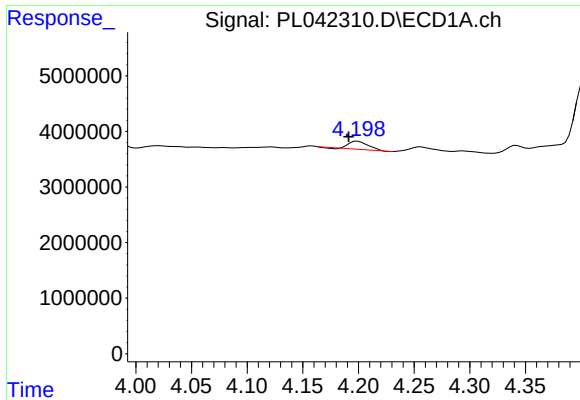

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.008 min
Response: 1560879
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

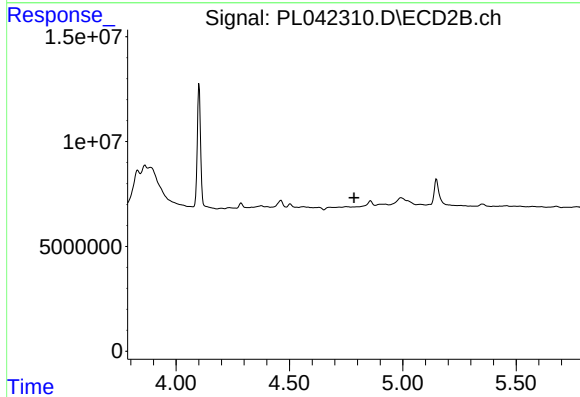


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

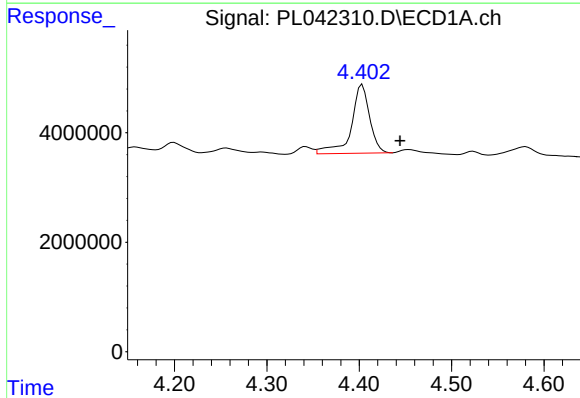


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: -0.041 min
Response: 17367571
Conc: 4.90 ng/ml

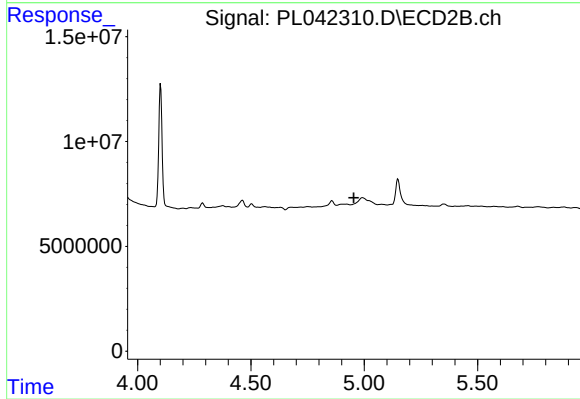

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

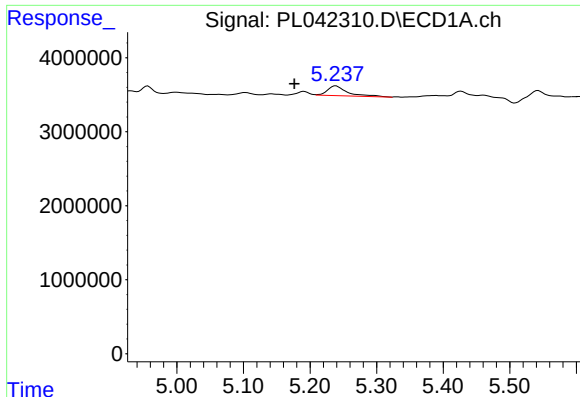

#8 Heptachlor epoxide


R.T.: 5.239 min
Delta R.T.: 0.062 min
Response: 2770806
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

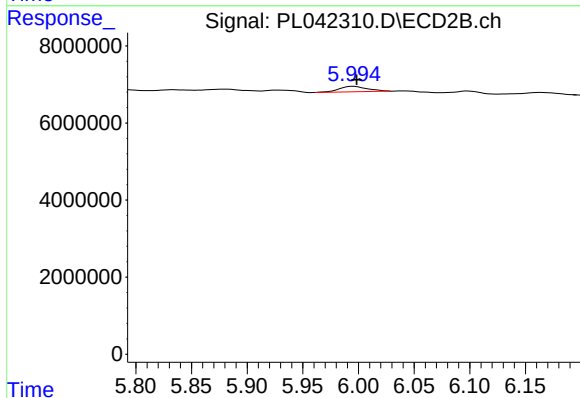


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 2570410
Conc: 0.72 ng/ml

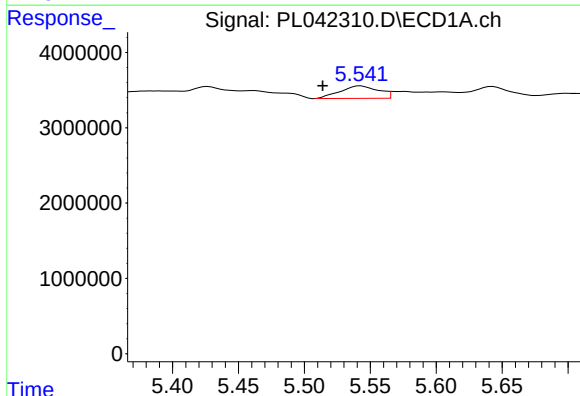


#9 Endosulfan I

R.T.: 5.543 min
Delta R.T.: 0.029 min
Response: 3350489
Conc: 0.48 ng/ml

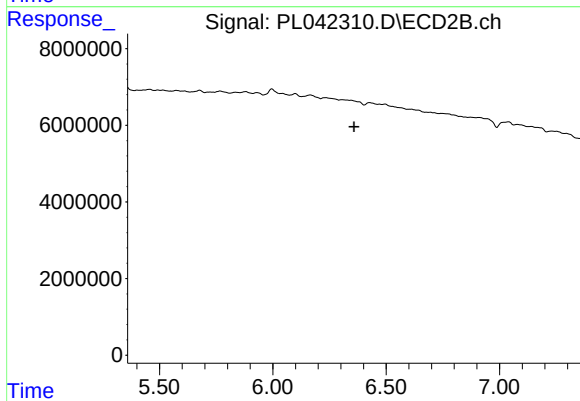

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

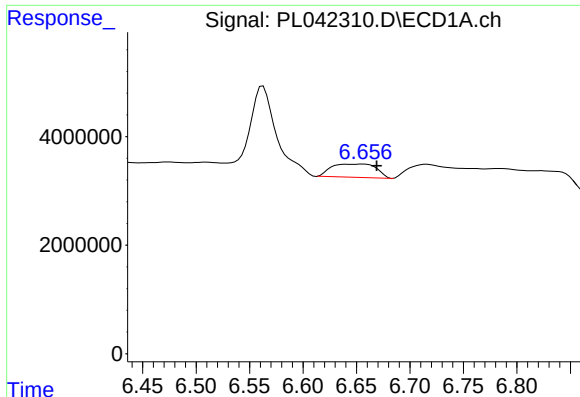

#19 Endosulfan Sulfate


R.T.: 6.656 min
Delta R.T.: -0.013 min
Response: 7155627
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

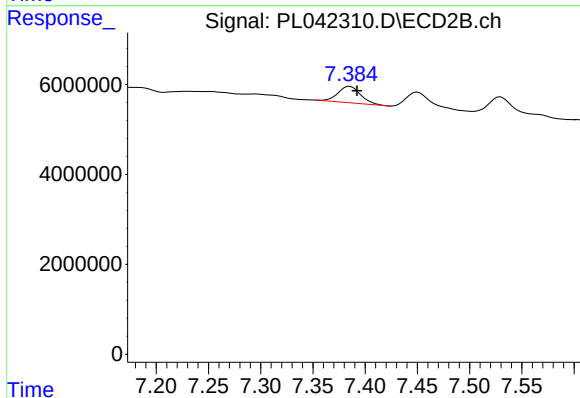


#19 Endosulfan Sulfate

R.T.: 7.385 min
Delta R.T.: -0.007 min
Response: 5517731
Conc: 1.98 ng/ml

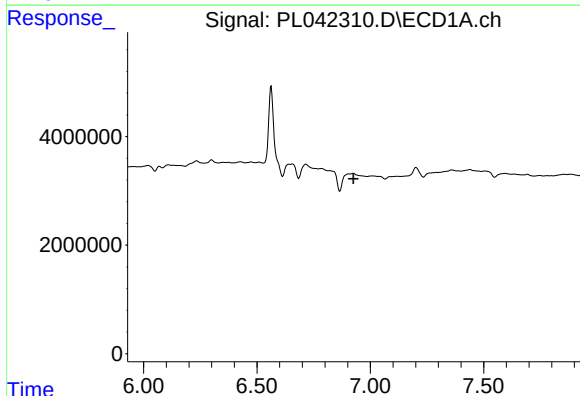


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.926 min
Response: 0
Conc: N.D.

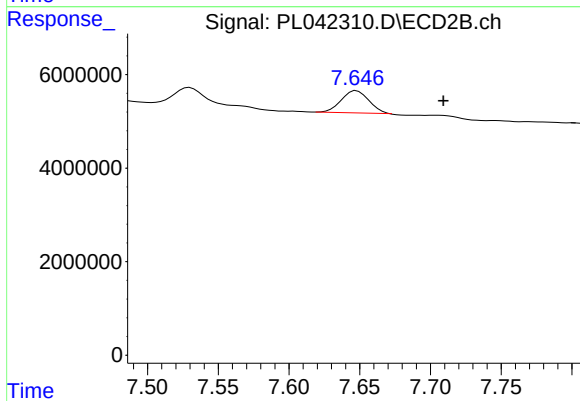

#20 Methoxychlor


R.T.: 7.648 min
Delta R.T.: -0.061 min
Response: 6154409
Conc: 4.51 ng/ml

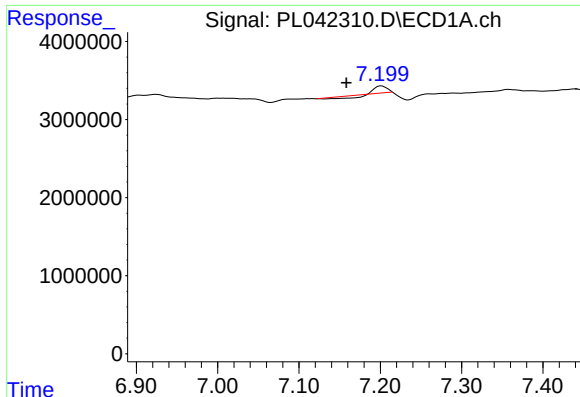

#21 Endrin ketone


R.T.: 7.202 min
Delta R.T.: 0.043 min
Response: 316730
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

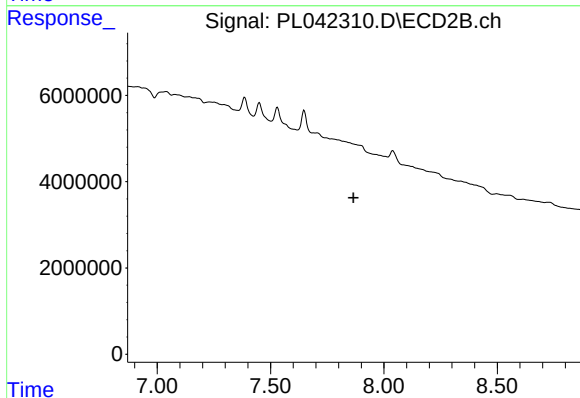


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

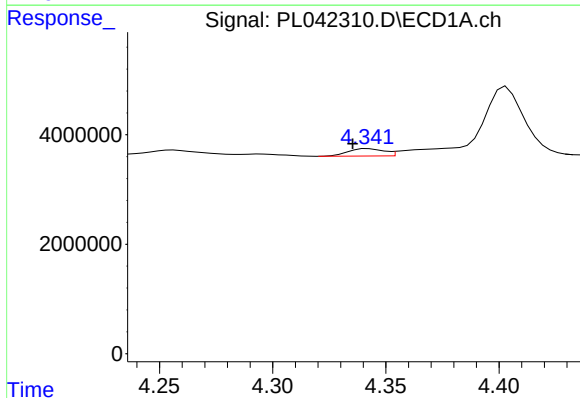


#23 Chlordane-1

R.T.: 4.342 min
Delta R.T.: 0.007 min
Response: 1486163
Conc: 5.38 ng/ml

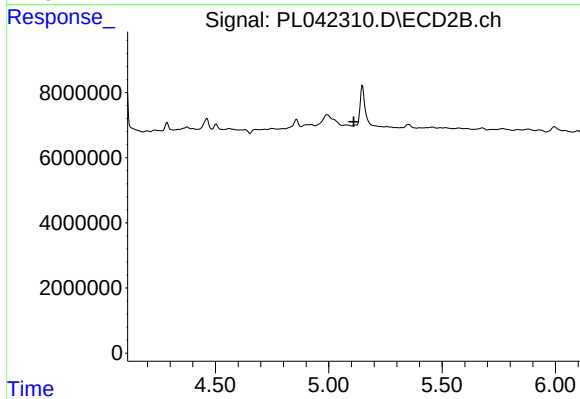

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

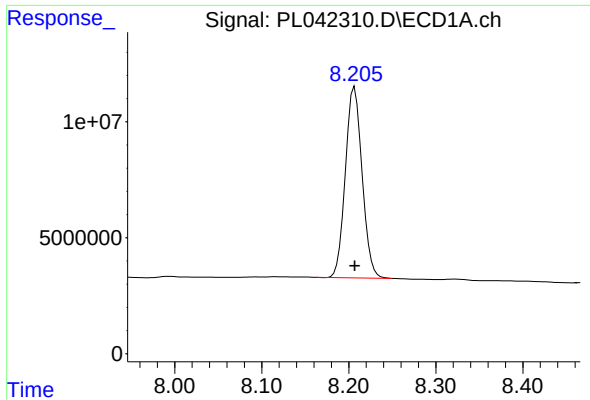

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 109979104
Conc: 17.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

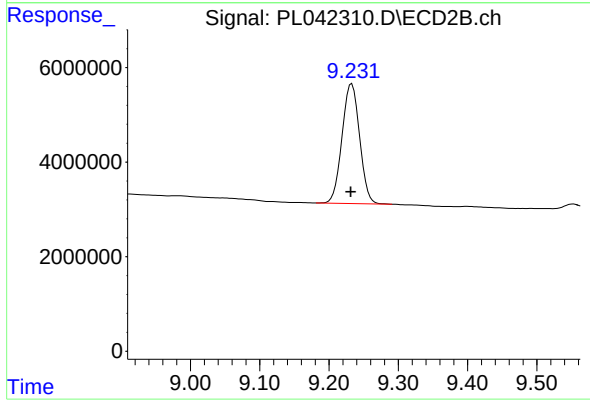

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.001 min
Response: 44560712
Conc: 18.48 ng/ml