

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
 Data File : PL042314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 22:19
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:54:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	117.1E6	60181564	19.906	20.924
28)	SA Decachlor...	8.207	9.233	122.2E6	50003458	19.384	20.732
Target Compounds							
2)	A alpha-BHC	3.901	0.000	3696756	0	0.410	N.D. #
6)	B beta-BHC	4.402f	0.000	3744858	0	1.057	N.D. #
7)	B delta-BHC	0.000	5.161	0	1248810	N.D.	0.339 #
8)	B Heptachlo...	0.000	5.994	0	4448920	N.D.	1.241 #
23)	Chlordane-1	4.366	5.161	1945507	1248810	7.037	9.394 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
Data File : PL042314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 22:19
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:54:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

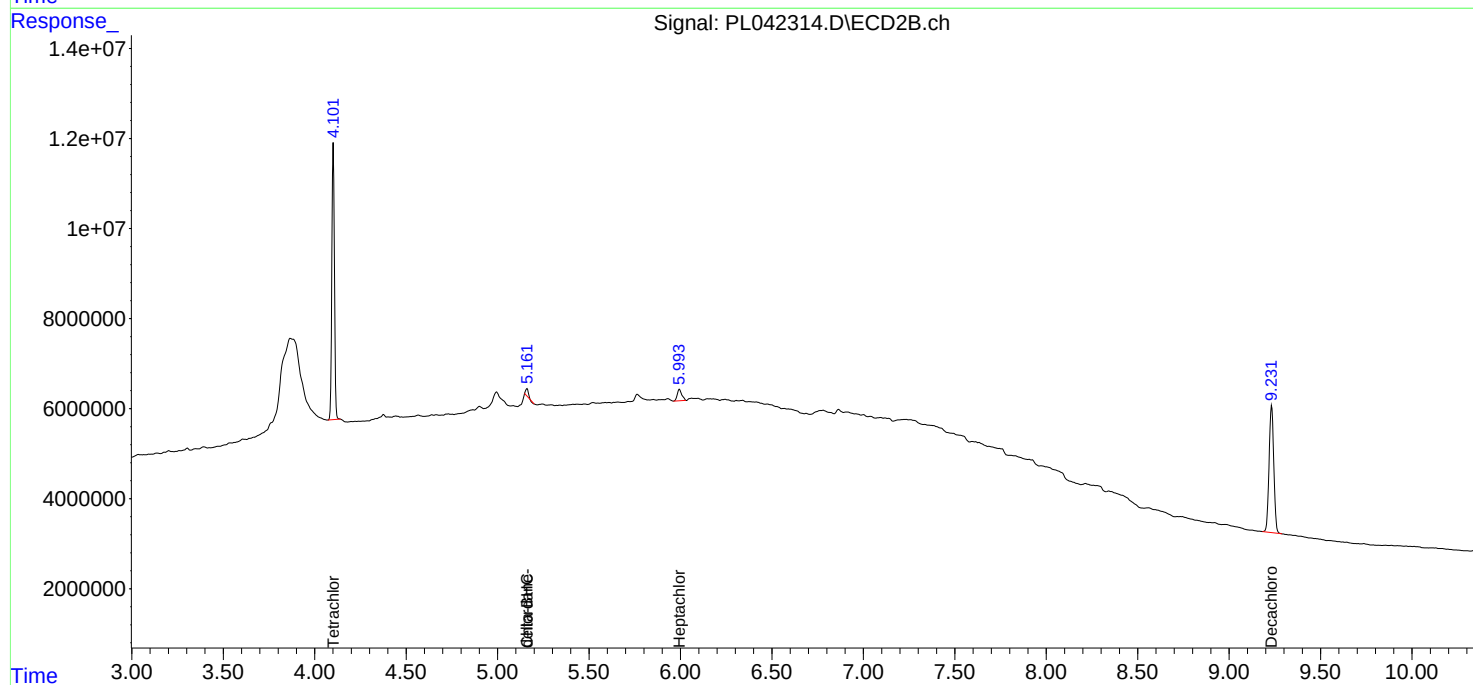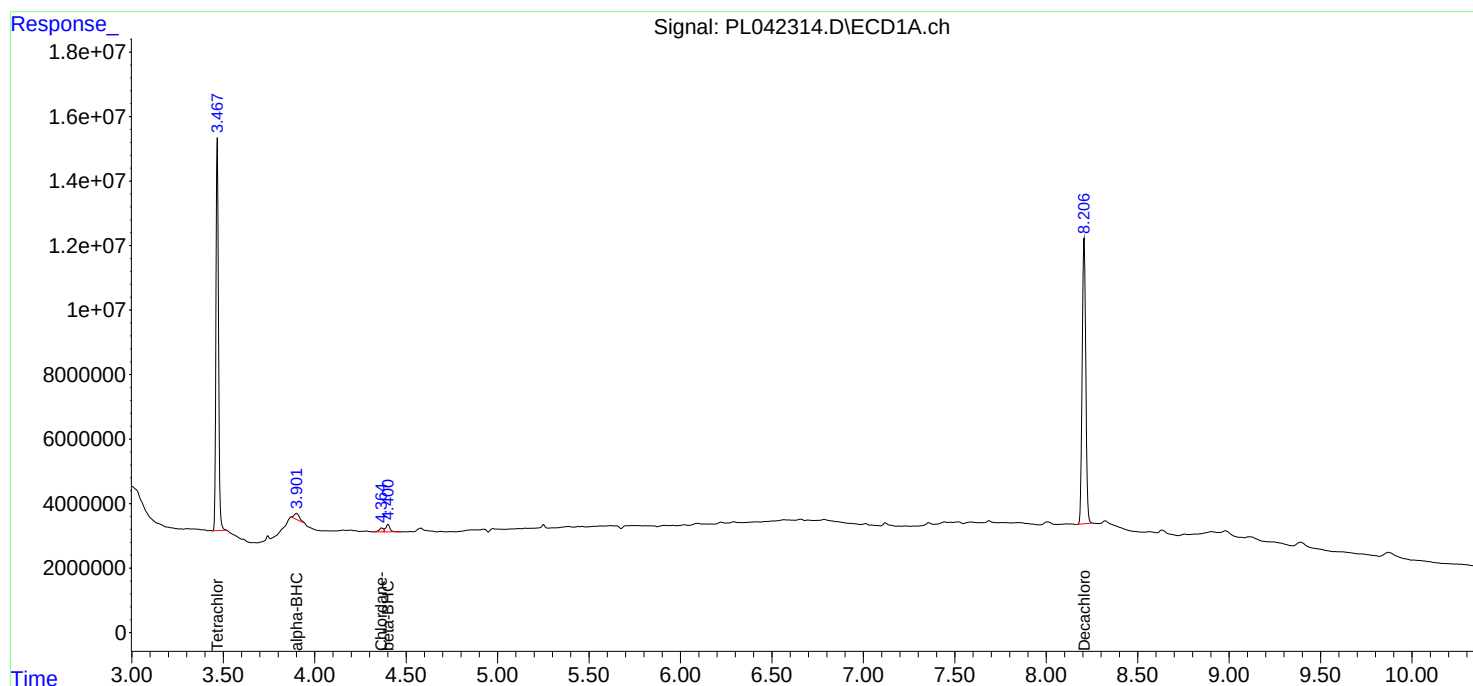


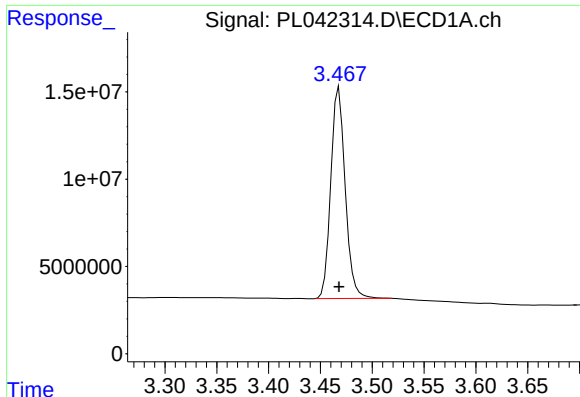

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 117114474
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

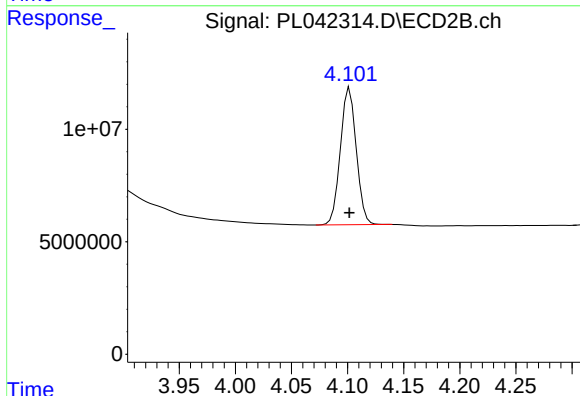


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 60181564
Conc: 20.92 ng/ml

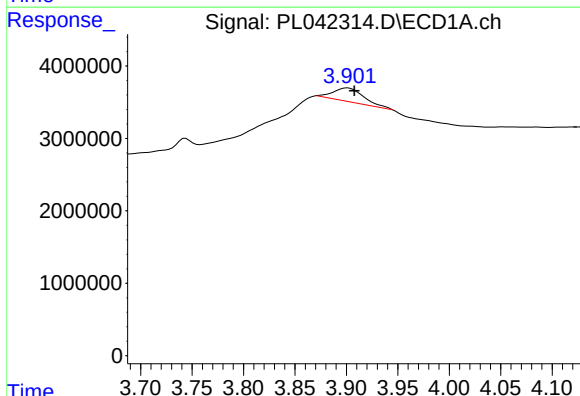


#2 alpha-BHC

R.T.: 3.901 min
Delta R.T.: -0.006 min
Response: 3696756
Conc: 0.41 ng/ml

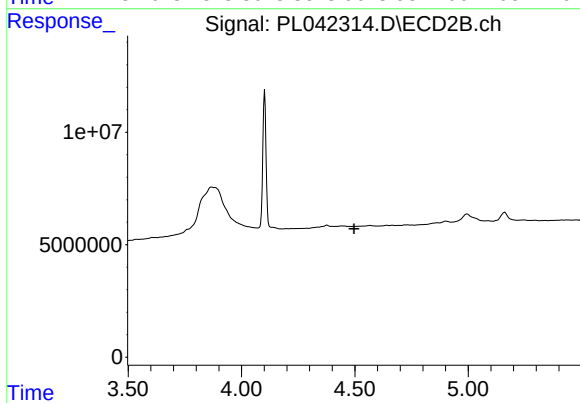

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

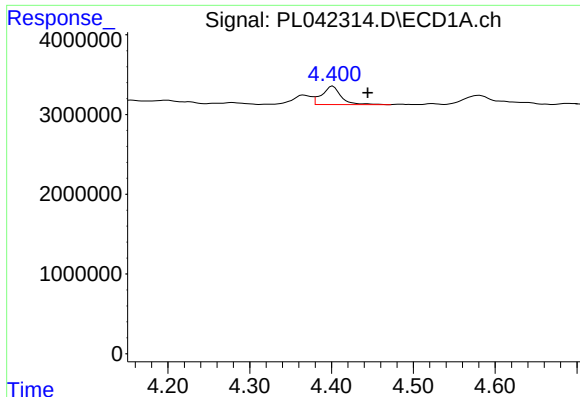

#6 beta-BHC


R.T.: 4.402 min
Delta R.T.: -0.043 min
Response: 3744858
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

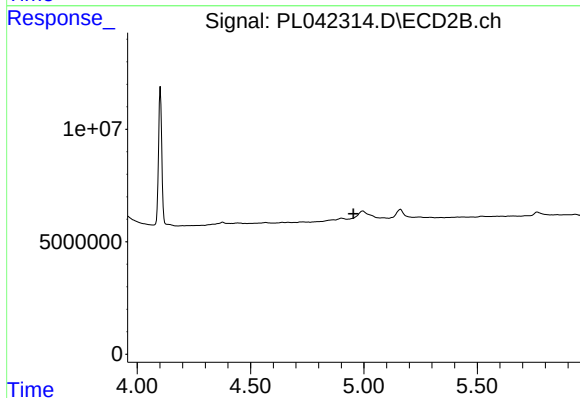


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

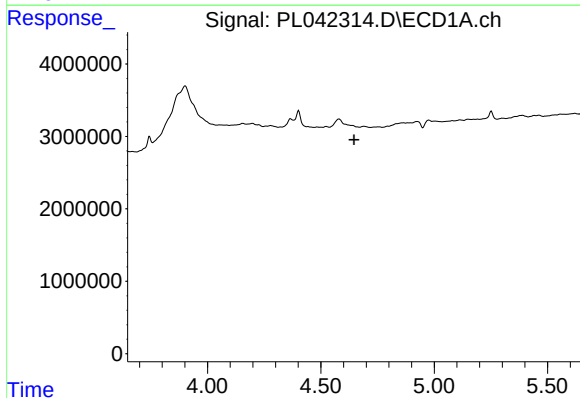


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.646 min
Response: 0
Conc: N.D.

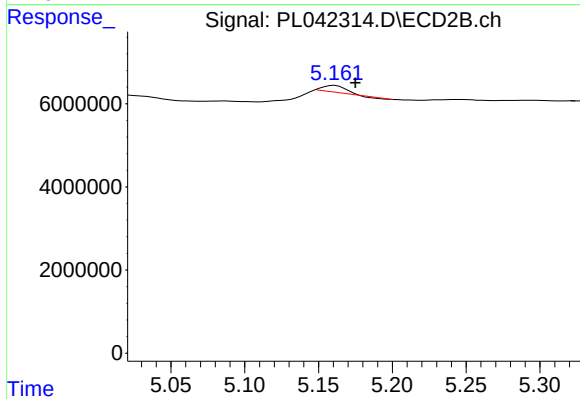

#7 delta-BHC


R.T.: 5.161 min
Delta R.T.: -0.014 min
Response: 1248810
Conc: 0.34 ng/ml

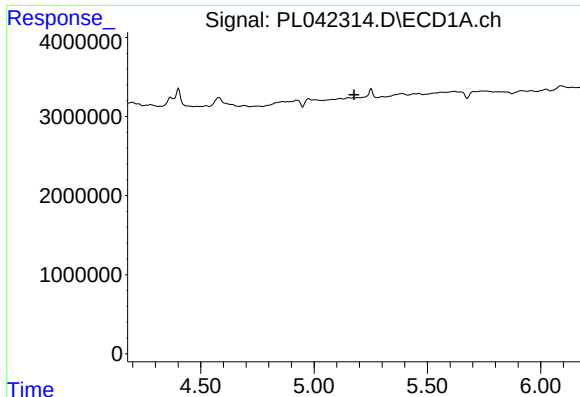

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

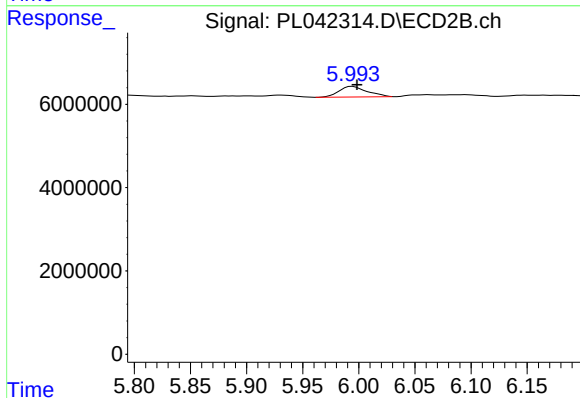


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.004 min
Response: 4448920
Conc: 1.24 ng/ml

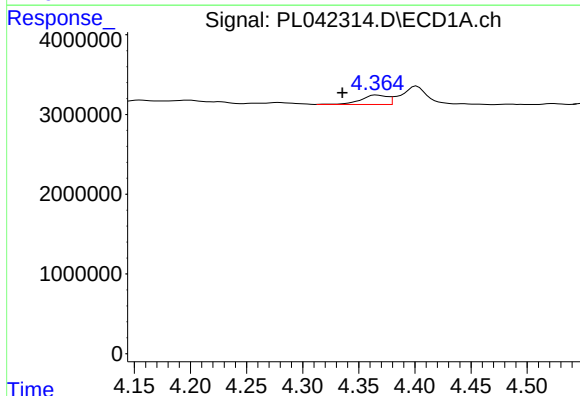


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.030 min
Response: 1945507
Conc: 7.04 ng/ml

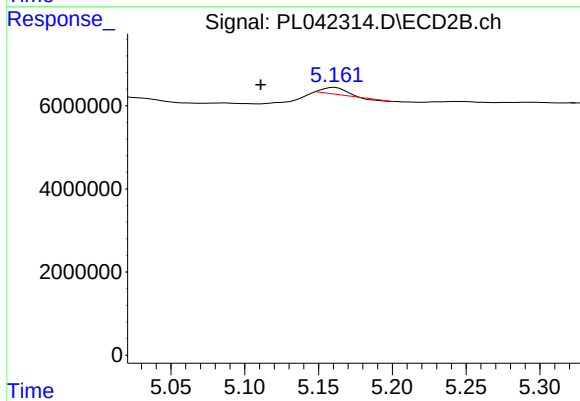

#23 Chlordane-1

R.T.: 5.161 min
Delta R.T.: 0.050 min
Response: 1248810
Conc: 9.39 ng/ml

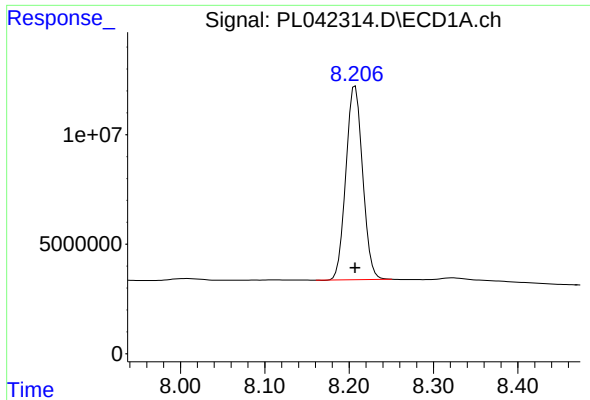

#28 Decachlorobiphenyl


R.T.: 8.207 min

Delta R.T.: 0.000 min

Response: 122160120

Conc: 19.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

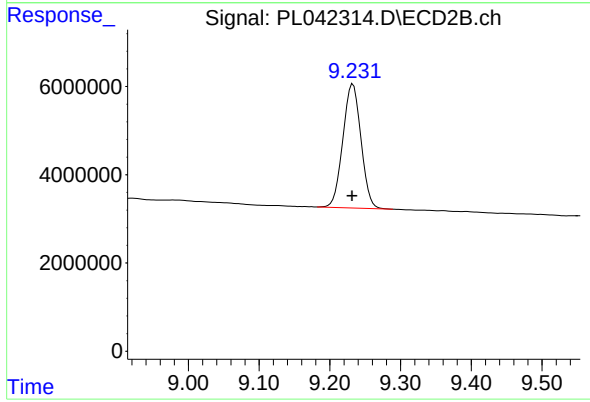

#28 Decachlorobiphenyl

R.T.: 9.233 min

Delta R.T.: 0.001 min

Response: 50003458

Conc: 20.73 ng/ml