

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
 Data File : PL042326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2018 01:23
 Operator : AJ\SJ
 Sample : J5762-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:56:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.103	103.0E6	60500754	17.513	21.035
28)	SA Decachlor...	8.207	9.234	134.8E6	53838678	21.394	22.323
Target Compounds							
2)	A alpha-BHC	3.906	0.000	3385870	0	0.375	N.D. #
3)	MA gamma-BHC...	0.000	4.833f	0	1571869	N.D.	0.398 #
6)	B beta-BHC	4.404f	0.000	16559254	0	4.674	N.D. #
8)	B Heptachlo...	5.237f	5.996	1952257	2418393	0.258	0.674 #
12)	B 4,4'-DDE	5.642	0.000	1977174	0	0.302	N.D. #
14)	MA Endrin	6.000	0.000	3977196	0	0.608	N.D. #
15)	B Endosulfa...	6.295	0.000	2233491	0	0.357	N.D. #
19)	B Endosulfa...	0.000	7.458f	0	4686020	N.D.	1.685 #
23)	Chlordane-1	4.343	0.000	1165000	0	4.214	N.D. #
27)	Chlordane-5	6.295	0.000	2233491	0	7.496	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
Data File : PL042326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2018 01:23
Operator : AJ\SJ
Sample : J5762-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:56:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

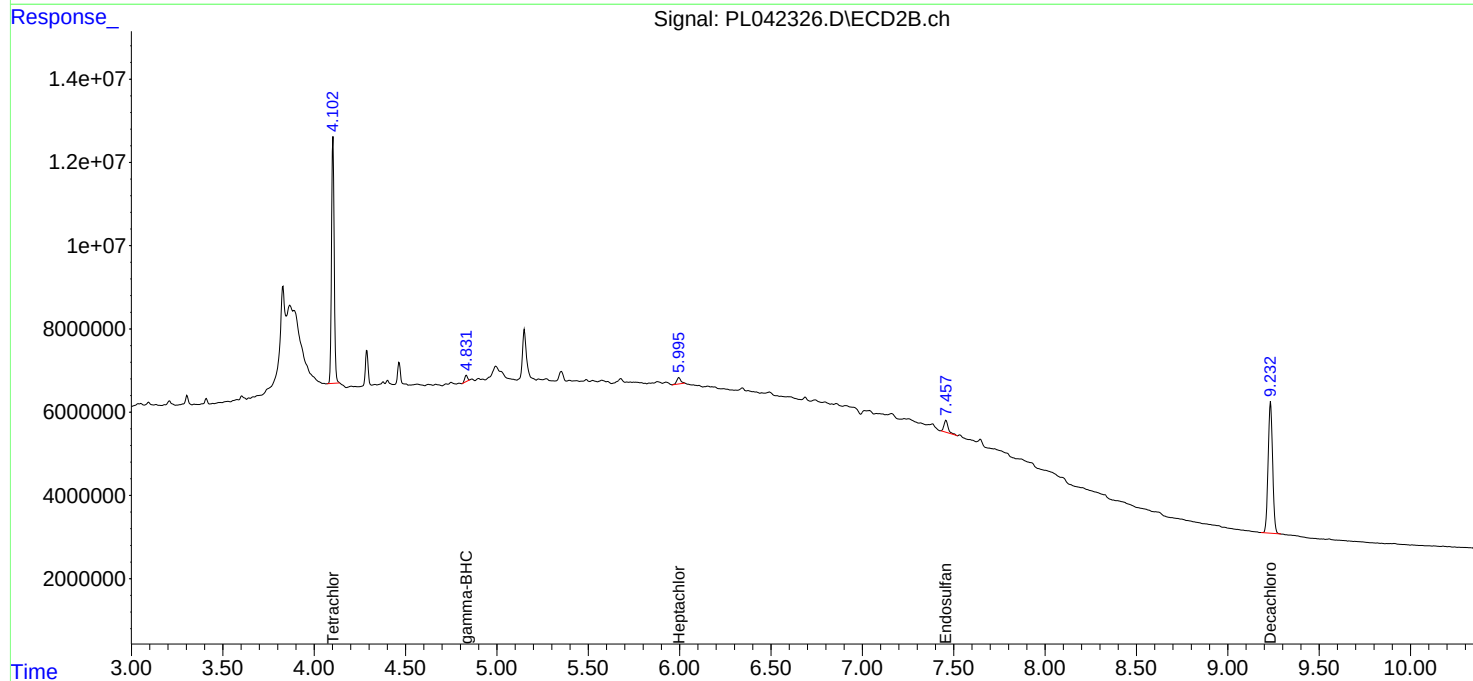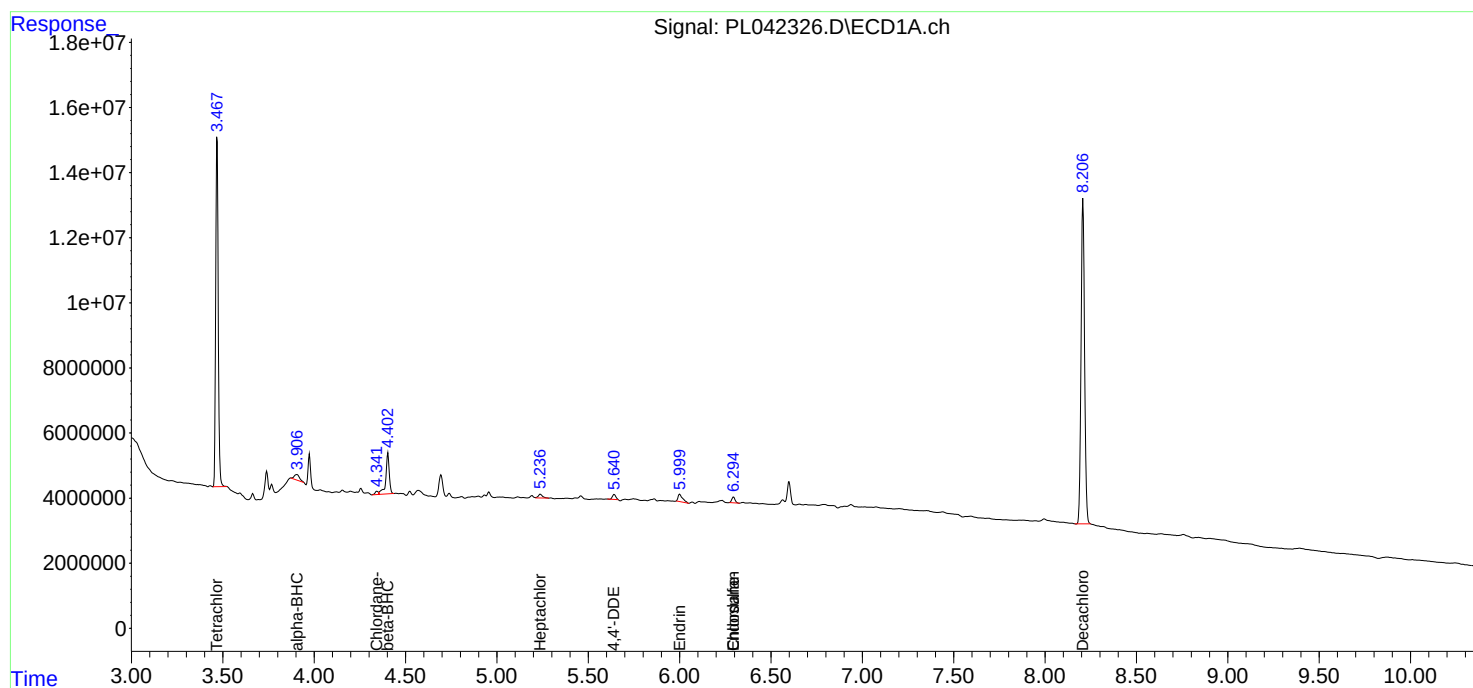


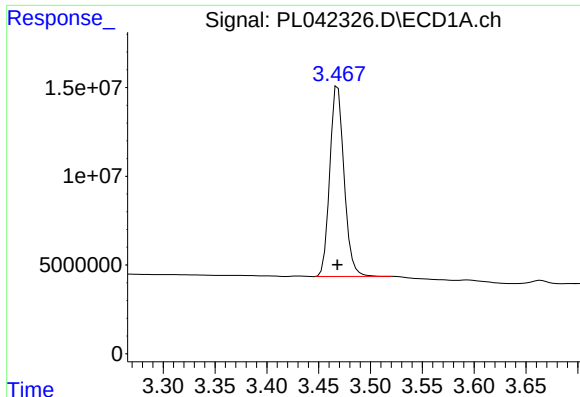

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 103039099
Conc: 17.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

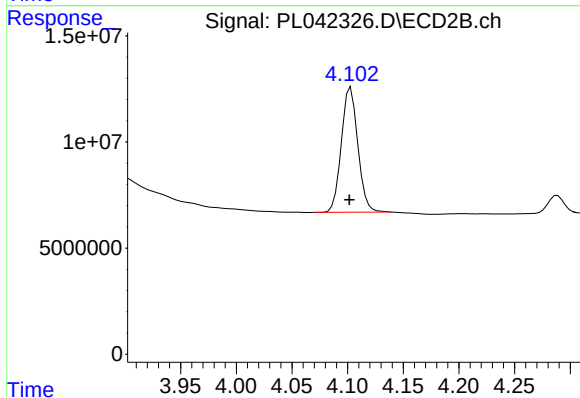


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.001 min
Response: 60500754
Conc: 21.04 ng/ml

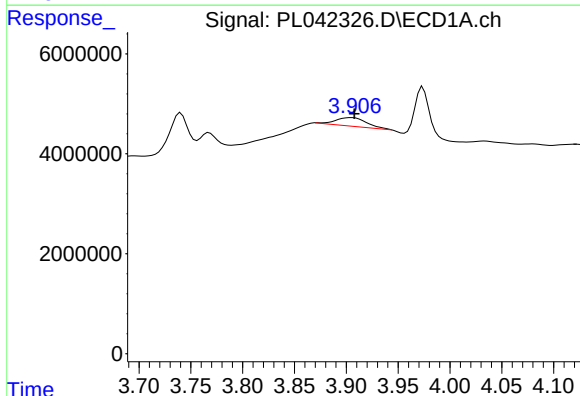


#2 alpha-BHC

R.T.: 3.906 min
Delta R.T.: -0.002 min
Response: 3385870
Conc: 0.38 ng/ml

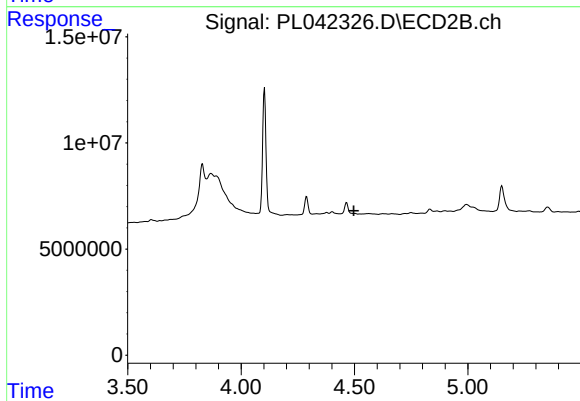

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

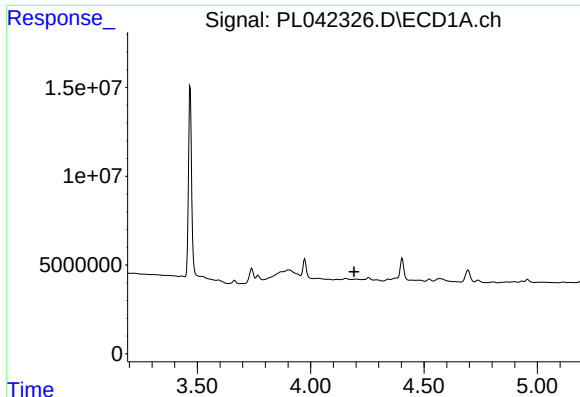

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

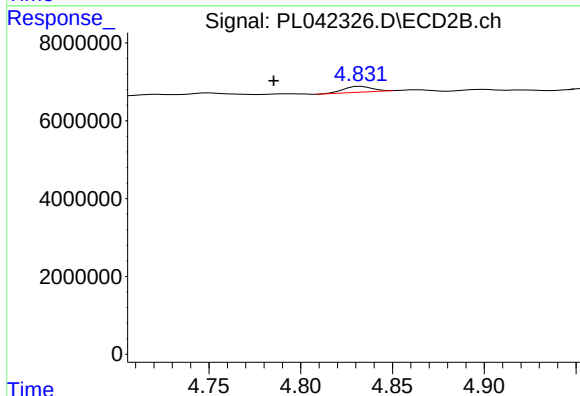


#3 gamma-BHC (Lindane)

R.T.: 4.833 min
Delta R.T.: 0.047 min
Response: 1571869
Conc: 0.40 ng/ml

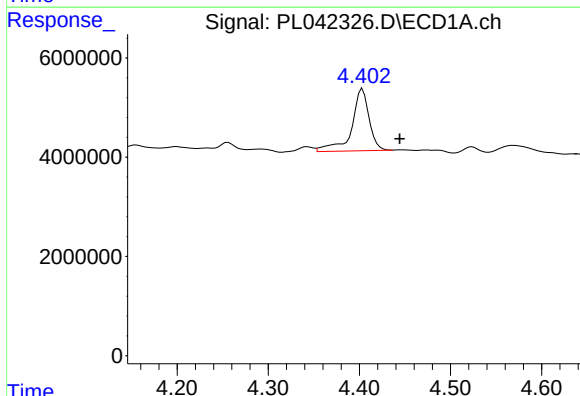


#6 beta-BHC

R.T.: 4.404 min
Delta R.T.: -0.041 min
Response: 16559254
Conc: 4.67 ng/ml

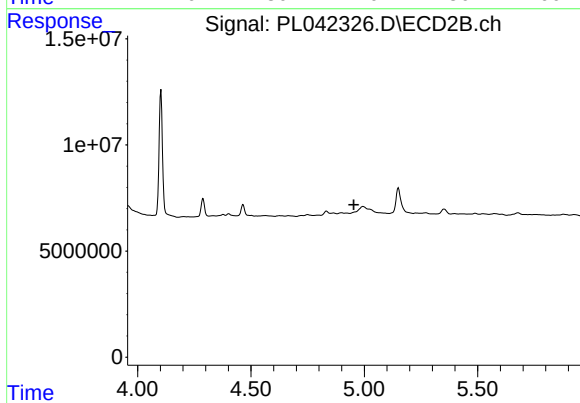

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.954 min
Response: 0
Conc: N.D.

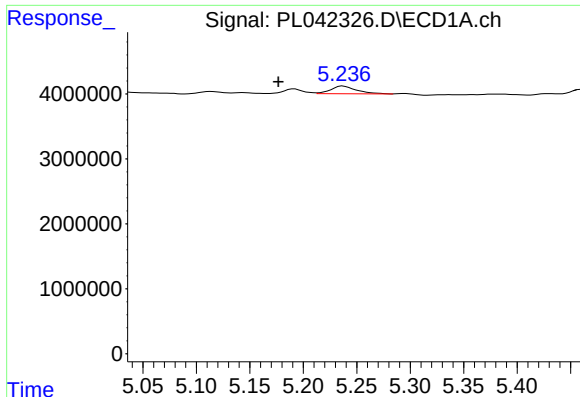

#8 Heptachlor epoxide


R.T.: 5.237 min
Delta R.T.: 0.061 min
Response: 1952257
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

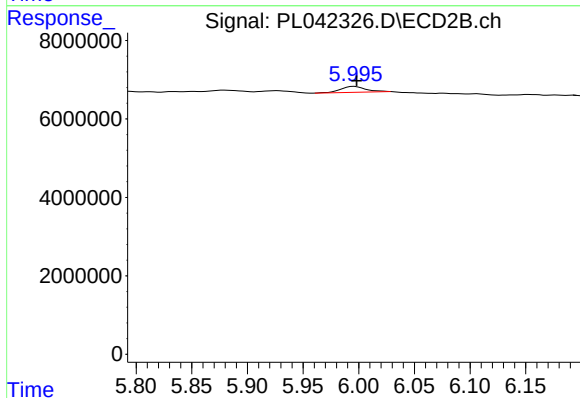


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: -0.002 min
Response: 2418393
Conc: 0.67 ng/ml

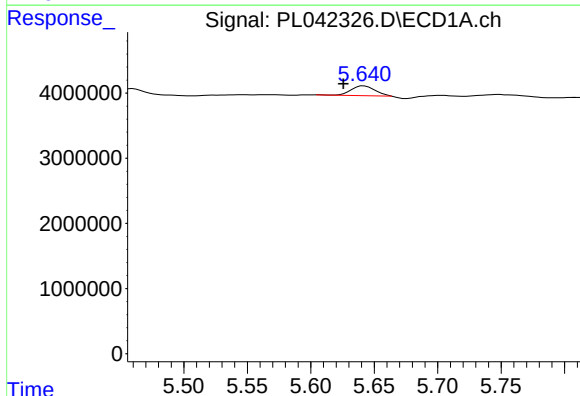


#12 4,4'-DDE

R.T.: 5.642 min
Delta R.T.: 0.016 min
Response: 1977174
Conc: 0.30 ng/ml

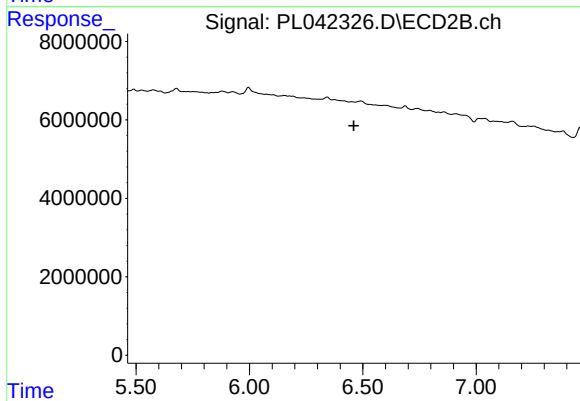

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.461 min
Response: 0
Conc: N.D.

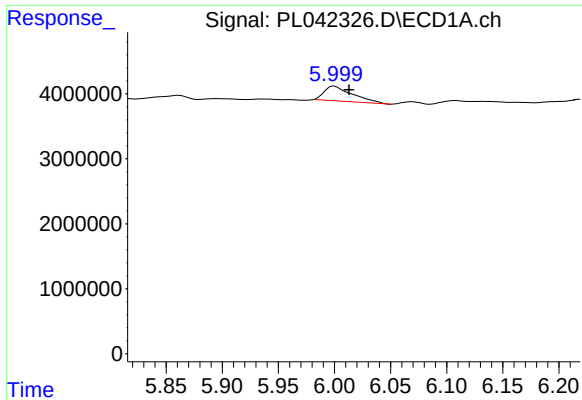

#14 Endrin


R.T.: 6.000 min
Delta R.T.: -0.013 min
Response: 3977196
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

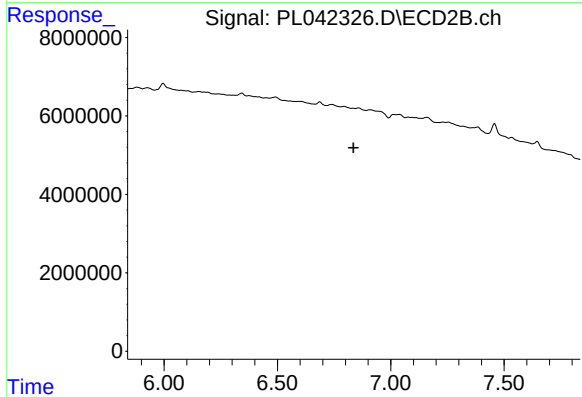


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

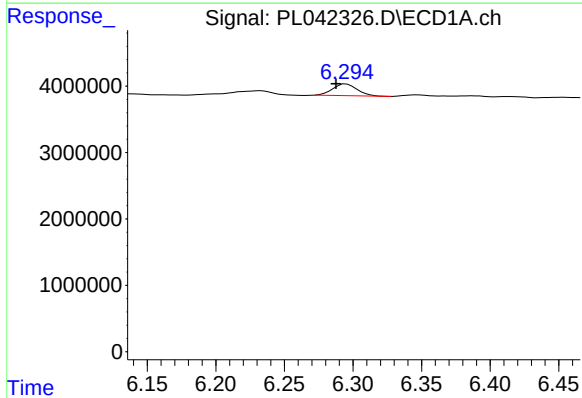


#15 Endosulfan II

R.T.: 6.295 min
Delta R.T.: 0.007 min
Response: 2233491
Conc: 0.36 ng/ml

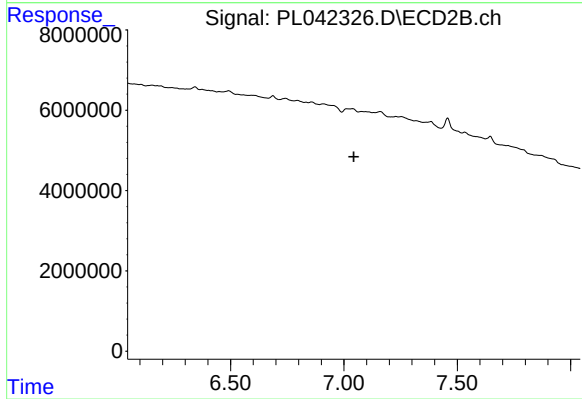

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

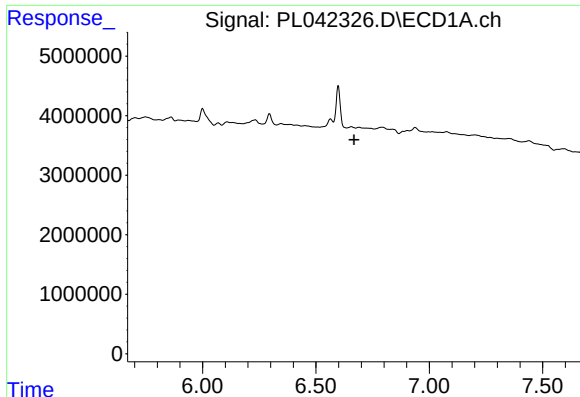

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

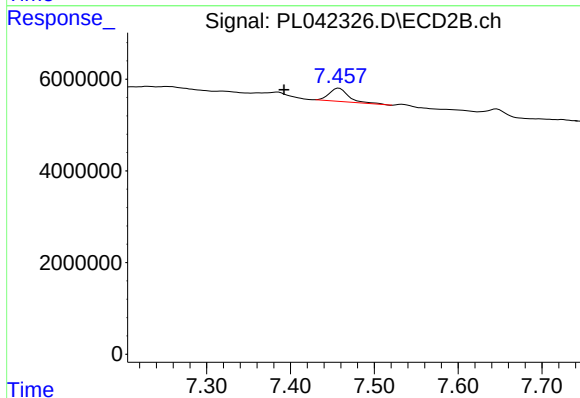


#19 Endosulfan Sulfate

R.T.: 7.458 min
Delta R.T.: 0.066 min
Response: 4686020
Conc: 1.68 ng/ml

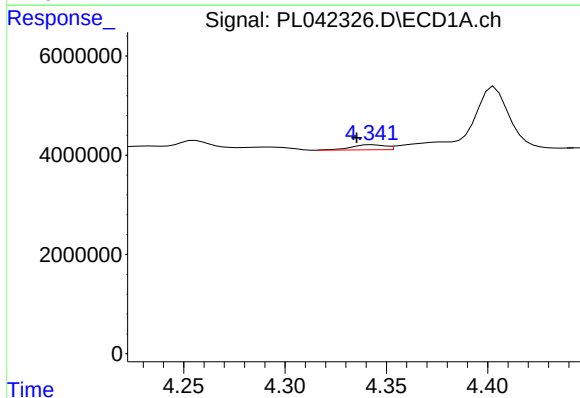


#23 Chlordane-1

R.T.: 4.343 min
Delta R.T.: 0.008 min
Response: 1165000
Conc: 4.21 ng/ml

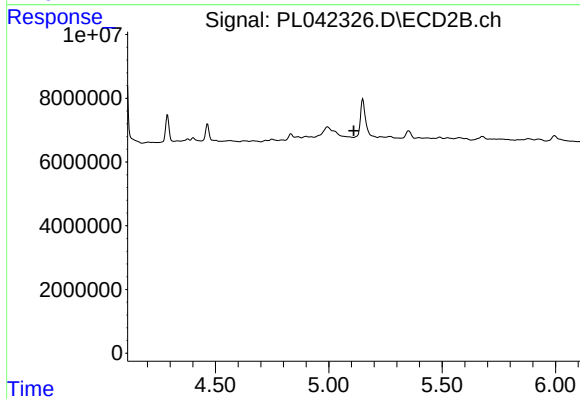

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.111 min
Response: 0
Conc: N.D.

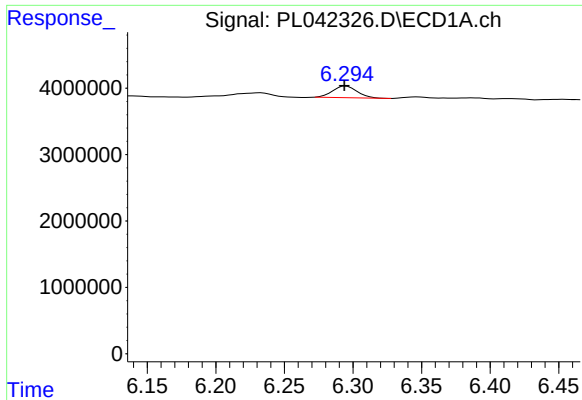

#27 Chlordane-5


R.T.: 6.295 min
Delta R.T.: 0.001 min
Response: 2233491
Conc: 7.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

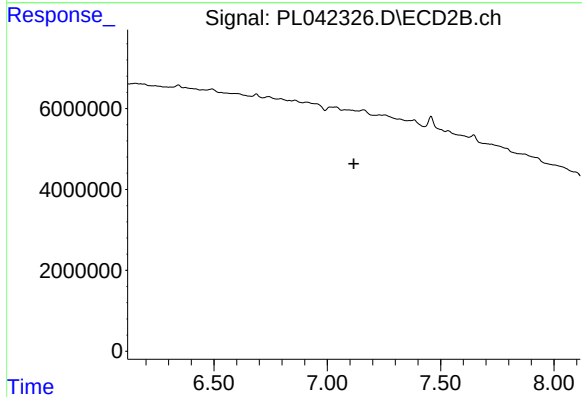


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

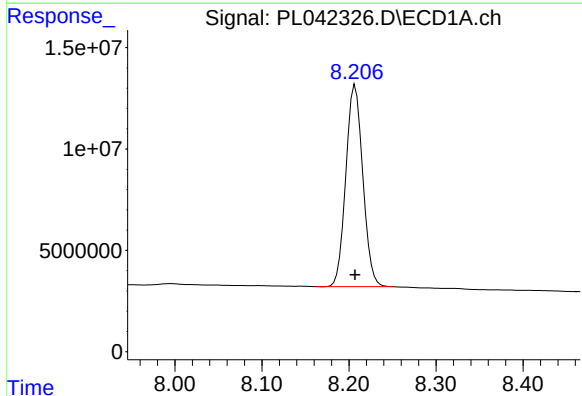

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 134828787
Conc: 21.39 ng/ml

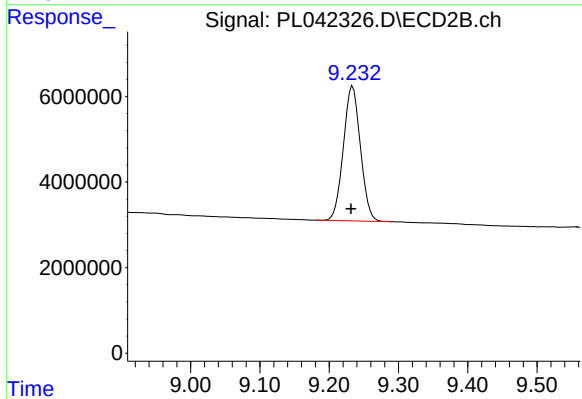

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.002 min
Response: 53838678
Conc: 22.32 ng/ml