

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
 Data File : PL042328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2018 01:51
 Operator : AJ\SJ
 Sample : J5975-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:56:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	90643961	46614206	15.407	16.207
28)	SA Decachlor...	8.207	9.234	109.1E6	43813122	17.306	18.166
Target Compounds							
2)	A alpha-BHC	3.897	0.000	3964676	0	0.439	N.D. #
6)	B beta-BHC	4.403f	0.000	13795296	0	3.894	N.D. #
8)	B Heptachlo...	0.000	5.993	0	12522334	N.D.	3.492 #
10)	B gamma-Chl...	0.000	6.195f	0	845117	N.D.	0.248 #
17)	MA 4,4'-DDT	6.394	0.000	541997	0	0.097	N.D. #
18)	B Endrin al...	6.394f	0.000	541997	0	0.104	N.D. #
23)	Chlordane-1	4.403	0.000	13795296	0	49.897	N.D. #
24)	Chlordane-2	4.904	5.516	13367929	2335904	47.569	16.752 #
25)	Chlordane-3	0.000	6.195	0	845117	N.D.	1.798 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
Data File : PL042328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2018 01:51
Operator : AJ\SJ
Sample : J5975-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:56:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

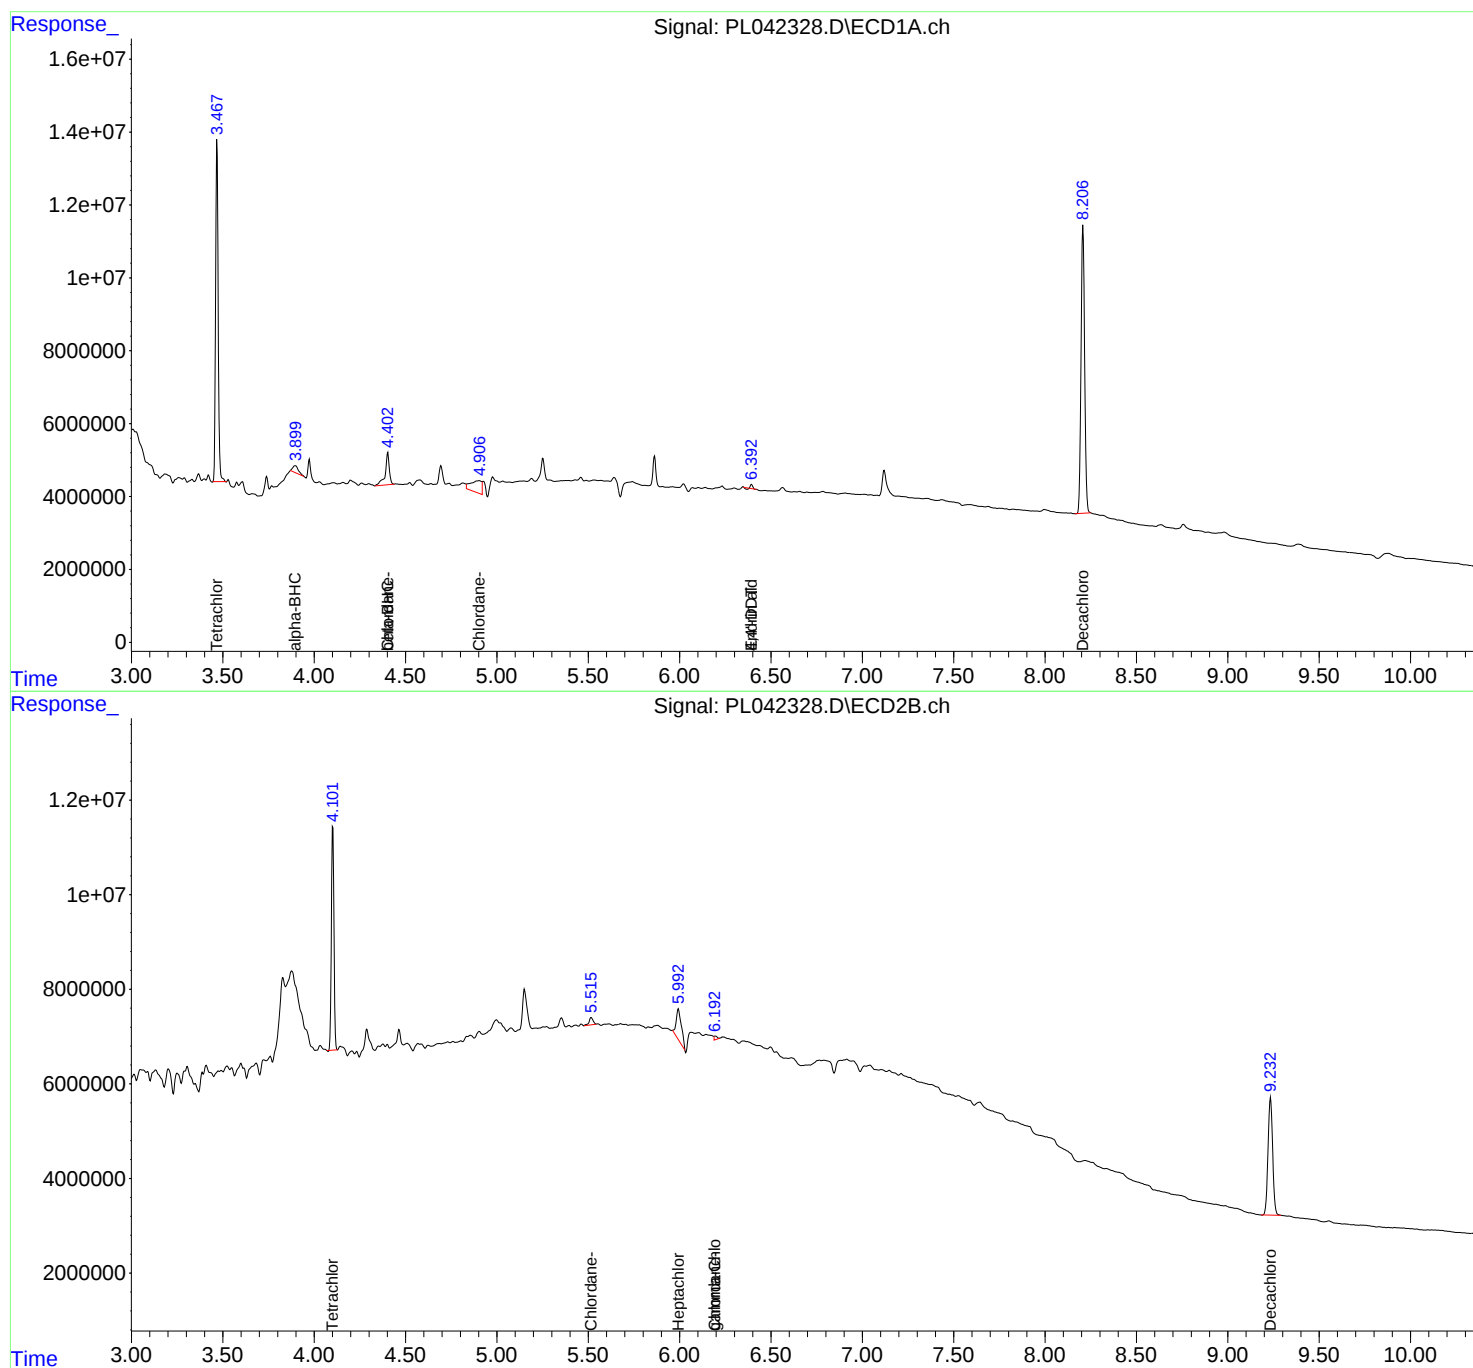


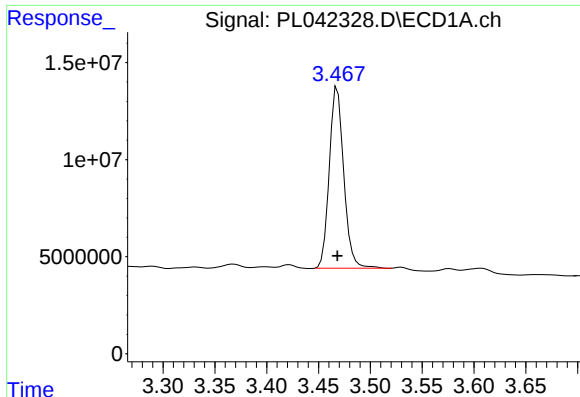

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 90643961
Conc: 15.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

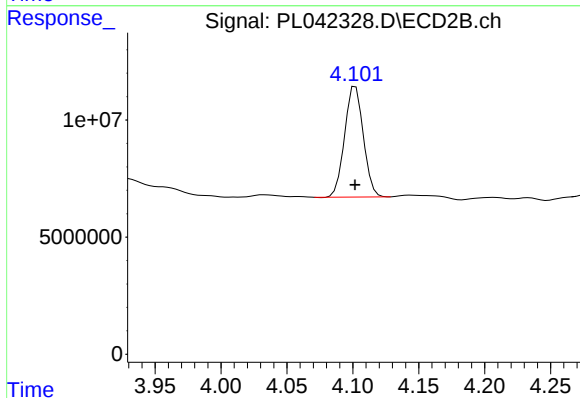


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 46614206
Conc: 16.21 ng/ml

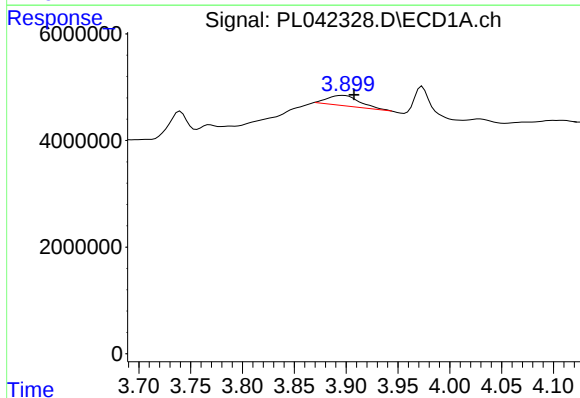


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: -0.011 min
Response: 3964676
Conc: 0.44 ng/ml

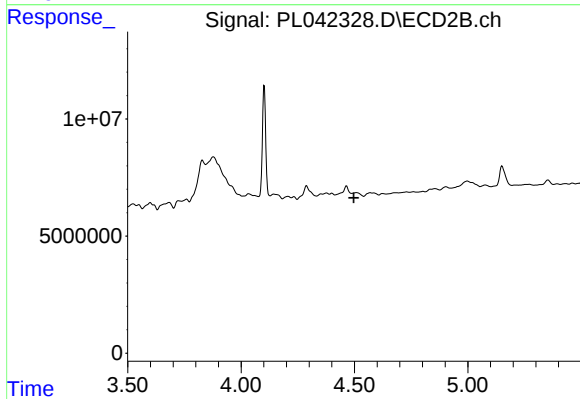

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

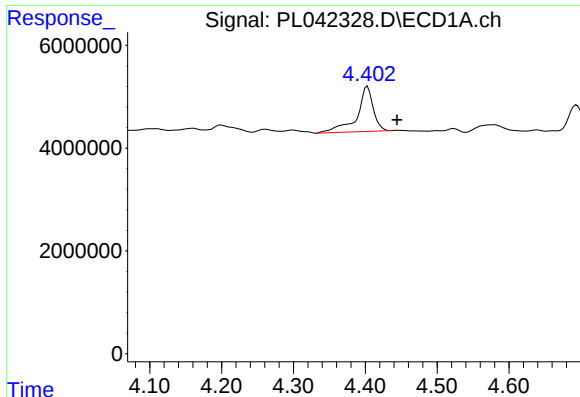

#6 beta-BHC


R.T.: 4.403 min
Delta R.T.: -0.041 min
Response: 13795296
Conc: 3.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

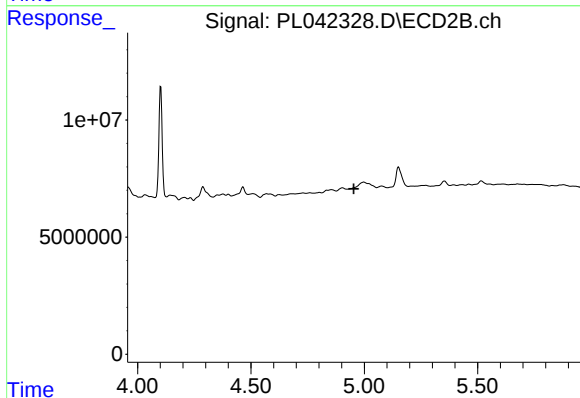


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

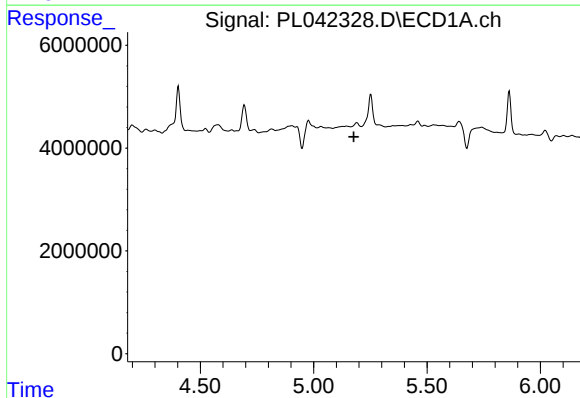


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

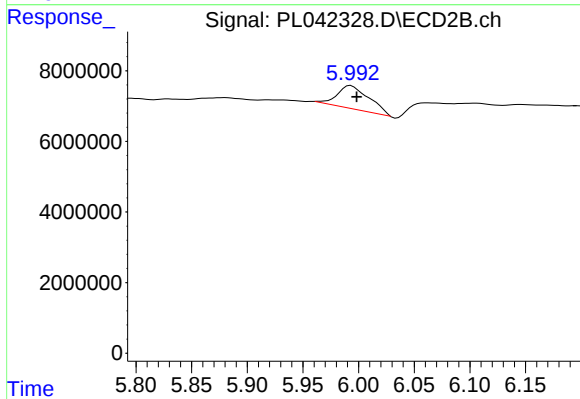

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.005 min
Response: 12522334
Conc: 3.49 ng/ml

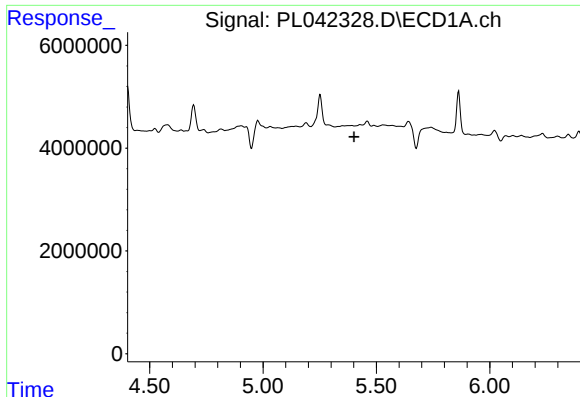

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

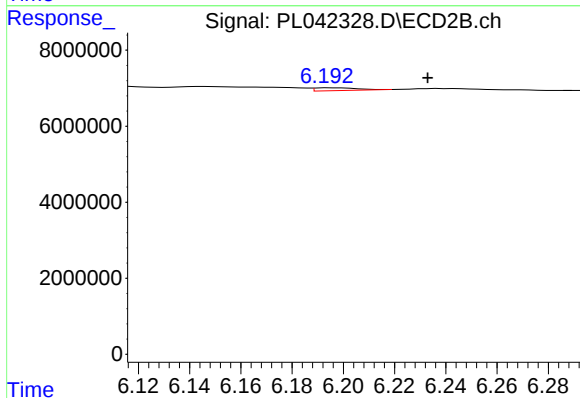


#10 gamma-Chlordane

R.T.: 6.195 min
Delta R.T.: -0.038 min
Response: 845117
Conc: 0.25 ng/ml

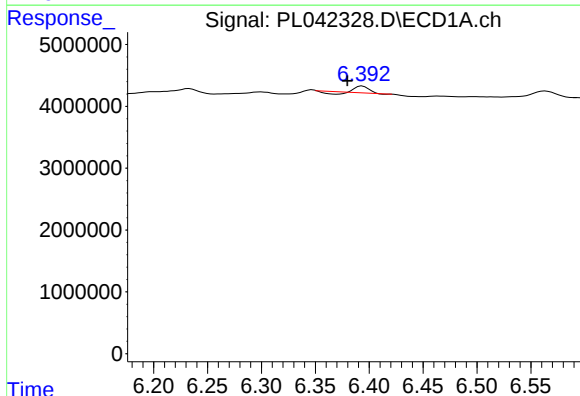


#17 4,4'-DDT

R.T.: 6.394 min
Delta R.T.: 0.014 min
Response: 541997
Conc: 0.10 ng/ml

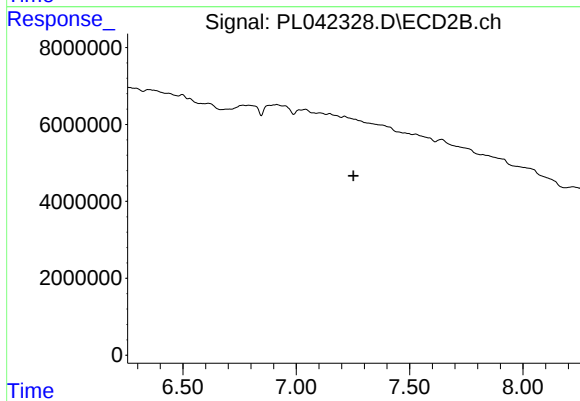

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

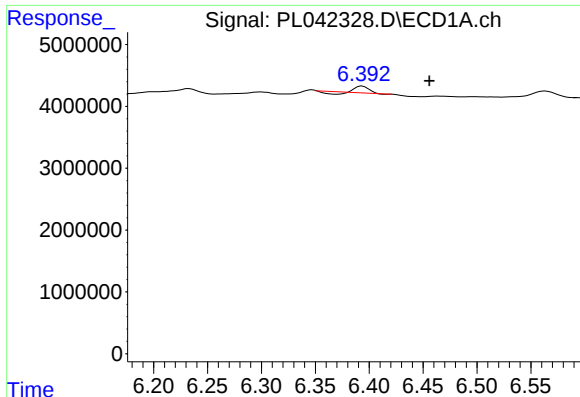

#18 Endrin aldehyde


R.T.: 6.394 min
Delta R.T.: -0.062 min
Response: 541997
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

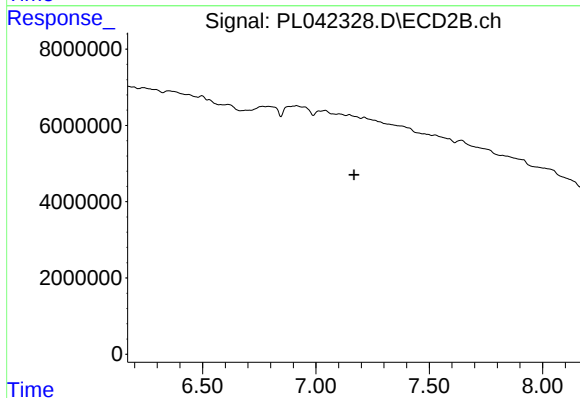


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.169 min
Response: 0
Conc: N.D.

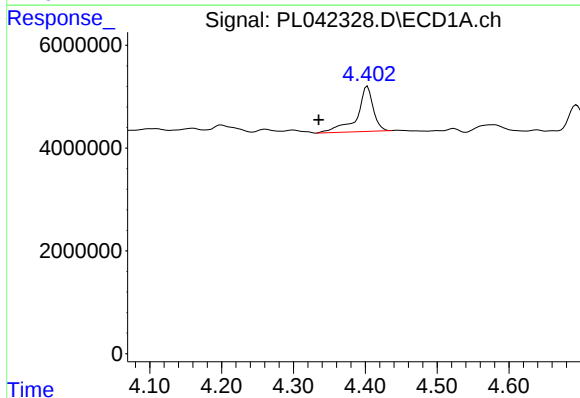


#23 Chlordane-1

R.T.: 4.403 min
Delta R.T.: 0.068 min
Response: 13795296
Conc: 49.90 ng/ml

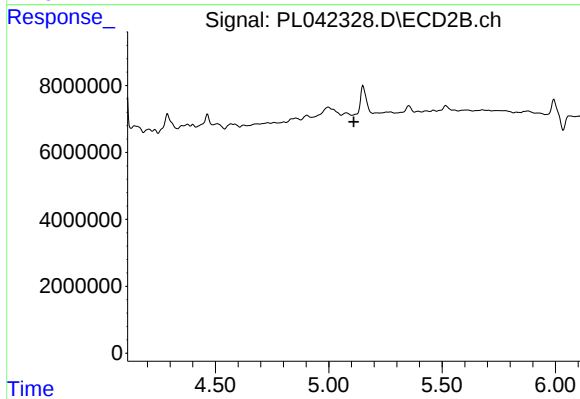

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

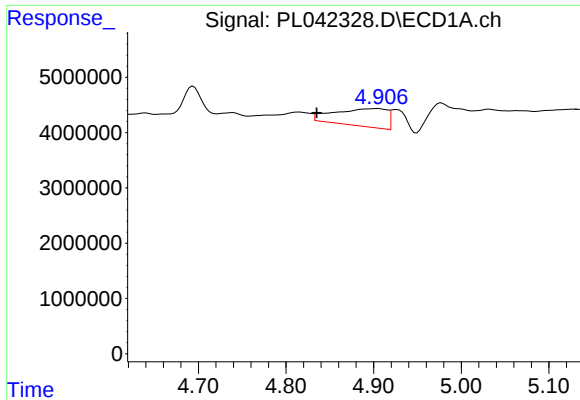

#24 Chlordane-2


R.T.: 4.904 min
Delta R.T.: 0.069 min
Response: 13367929
Conc: 47.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

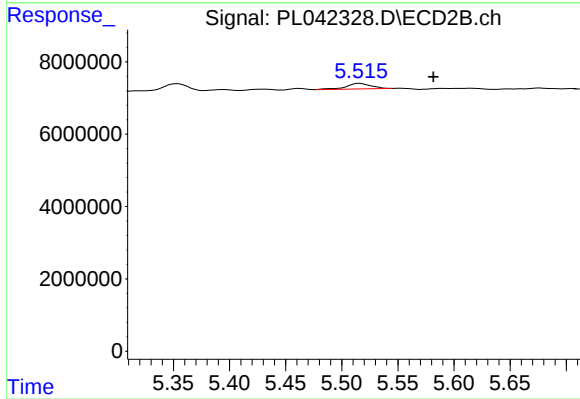


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: -0.065 min
Response: 2335904
Conc: 16.75 ng/ml

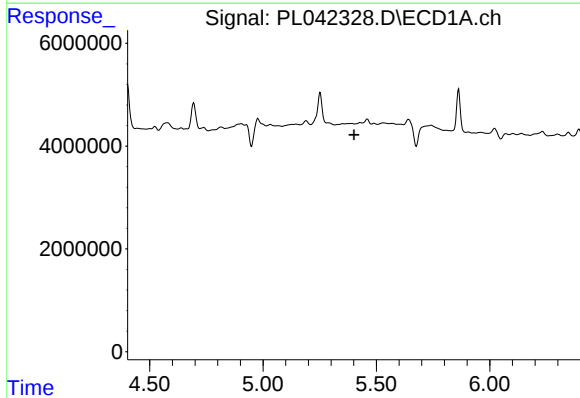


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

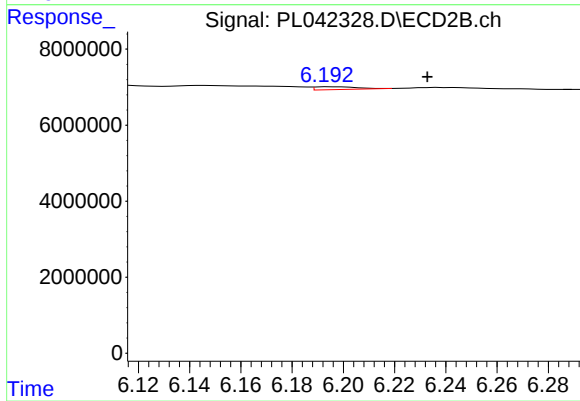

#25 Chlordane-3

R.T.: 6.195 min
Delta R.T.: -0.037 min
Response: 845117
Conc: 1.80 ng/ml

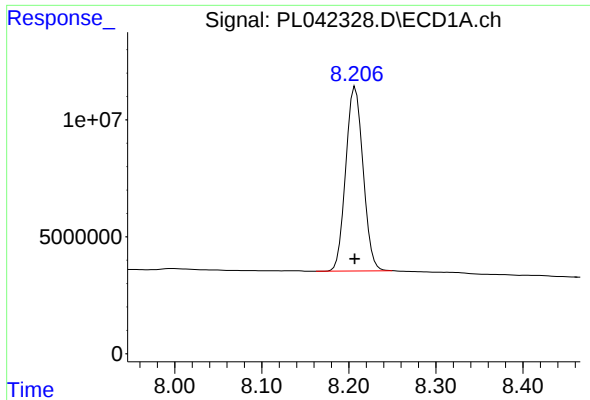

#28 Decachlorobiphenyl


R.T.: 8.207 min

Delta R.T.: 0.000 min

Response: 109061800

Conc: 17.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

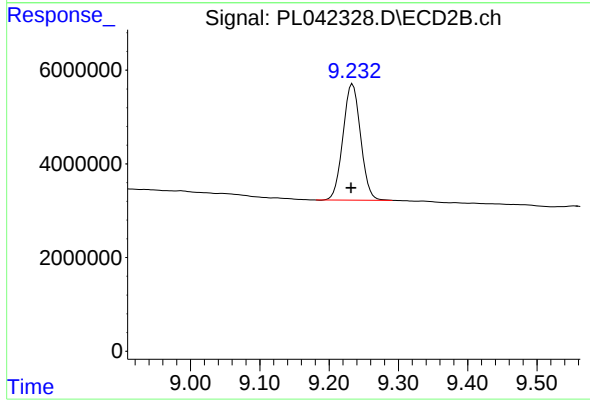

#28 Decachlorobiphenyl

R.T.: 9.234 min

Delta R.T.: 0.002 min

Response: 43813122

Conc: 18.17 ng/ml