

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
 Data File : PL042280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 11:41
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:28:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:27:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	609.5E6	286.7E6	50.000	50.000
28)	SA Decachlor...	8.207	9.232	578.3E6	230.9E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.335	5.111	138.2E6	66466181	500.000	500.000
24)	Chlordane-2	4.835	5.582	140.5E6	69722040	500.000	500.000
25)	Chlordane-3	5.402	6.233	438.3E6	235.0E6	500.000	500.000
26)	Chlordane-4	5.459	6.308	379.5E6	273.6E6	500.000	500.000
27)	Chlordane-5	6.294	7.117	149.0E6	48097715	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
Data File : PL042280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 11:41
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:28:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:27:55 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

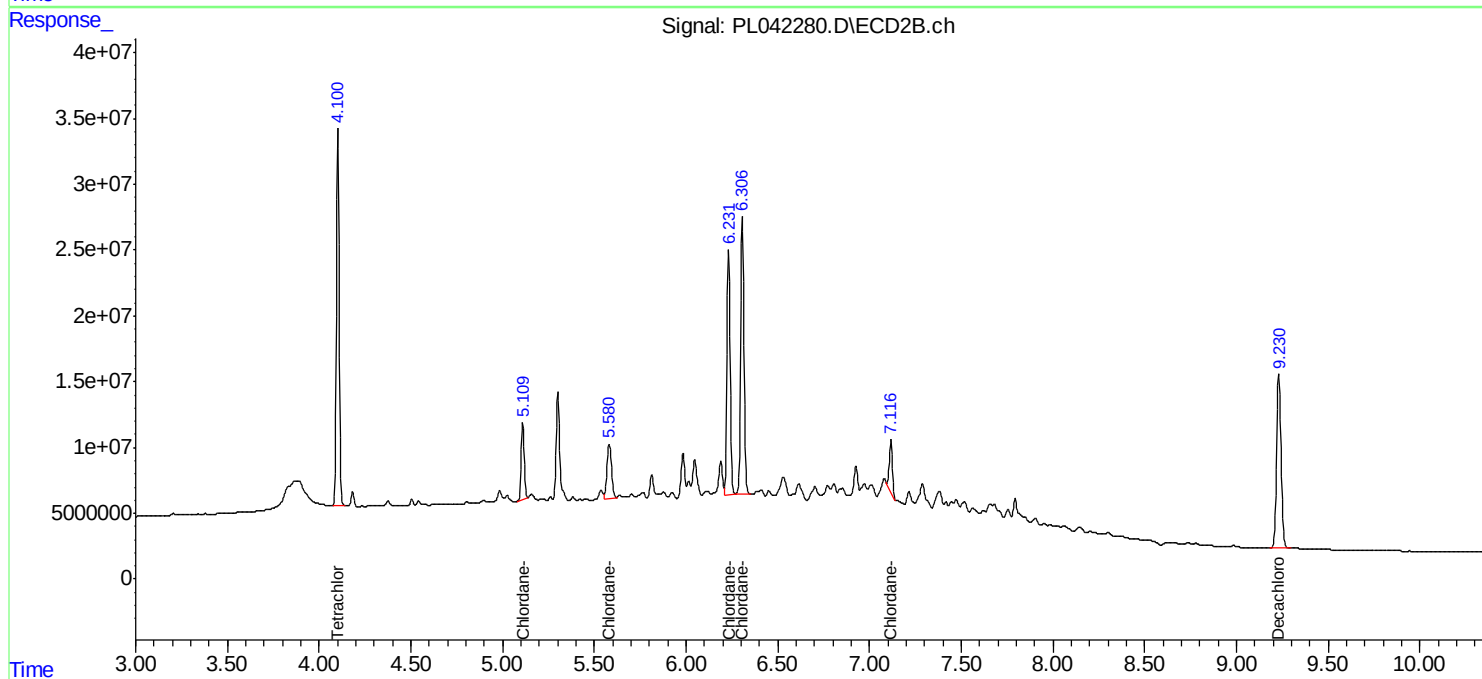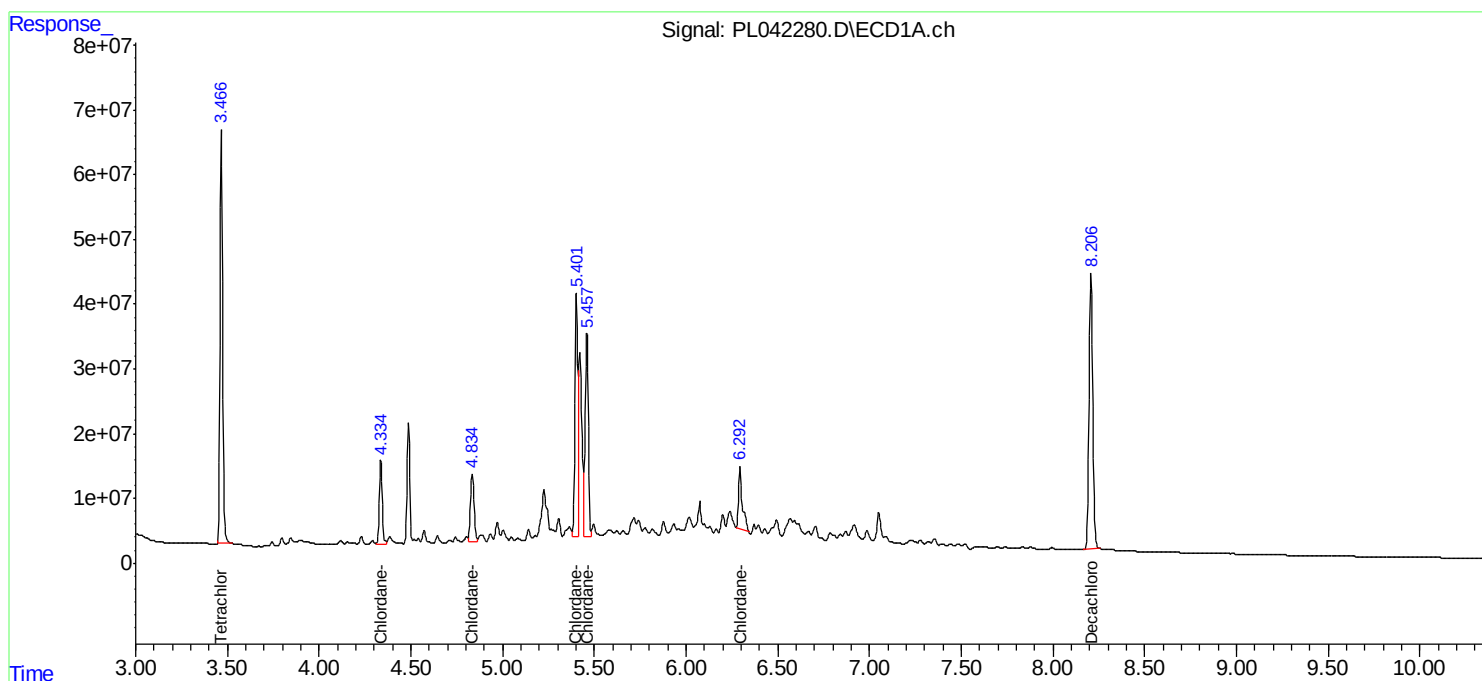


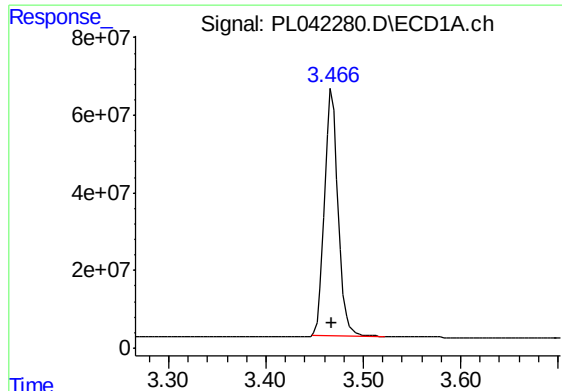

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 609506647
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

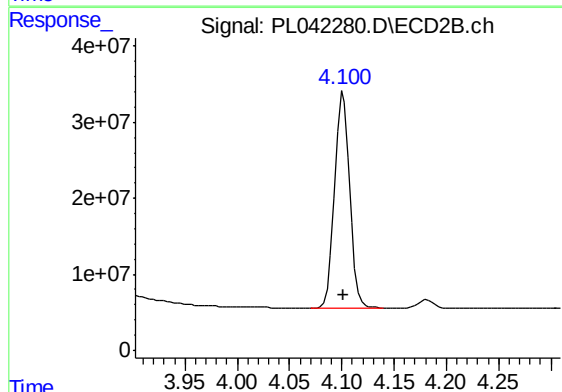


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 286653985
Conc: 50.00 ng/ml

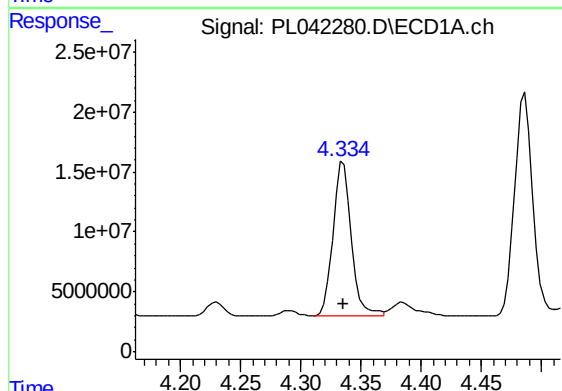


#23 Chlordane-1

R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 138236525
Conc: 500.00 ng/ml

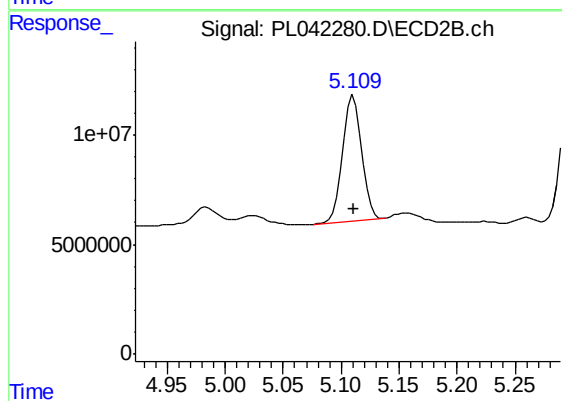

#23 Chlordane-1


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 66466181
Conc: 500.00 ng/ml

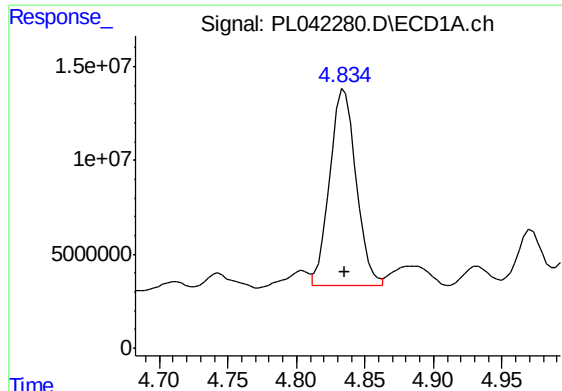

#24 Chlordane-2


R.T.: 4.835 min
Delta R.T.: 0.000 min
Response: 140511577
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

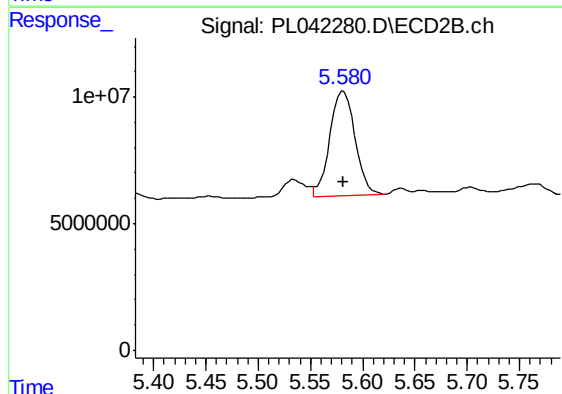


#24 Chlordane-2

R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 69722040
Conc: 500.00 ng/ml

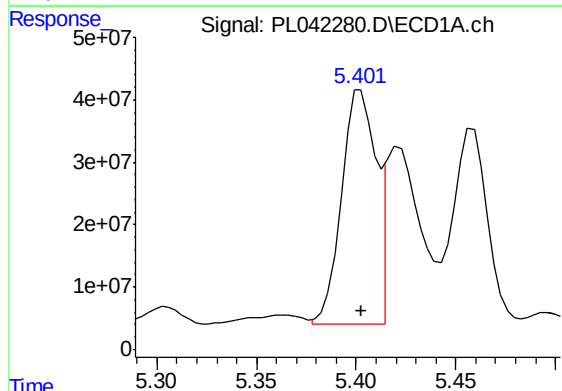


#25 Chlordane-3

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 438294936
Conc: 500.00 ng/ml

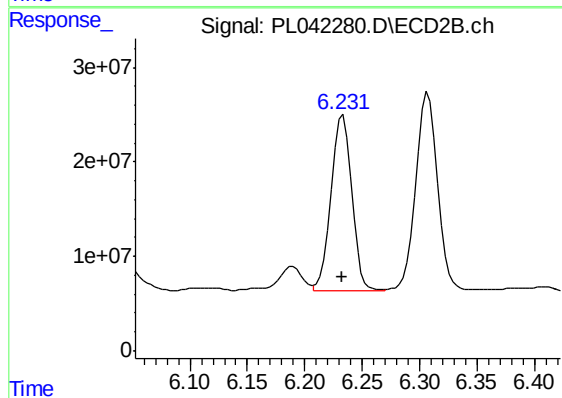

#25 Chlordane-3


R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 234962676
Conc: 500.00 ng/ml

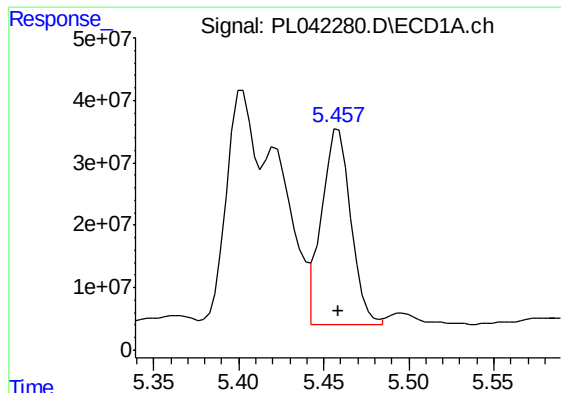

#26 Chlordane-4


R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 379460173
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

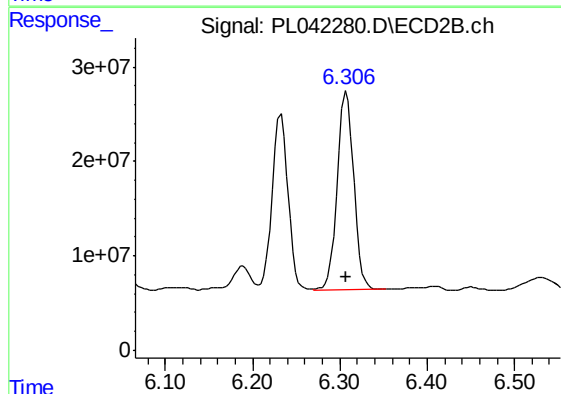


#26 Chlordane-4

R.T.: 6.308 min
Delta R.T.: 0.000 min
Response: 273577934
Conc: 500.00 ng/ml

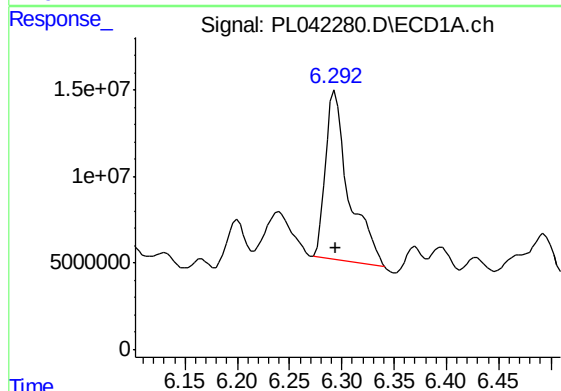


#27 Chlordane-5

R.T.: 6.294 min
Delta R.T.: 0.000 min
Response: 148986074
Conc: 500.00 ng/ml

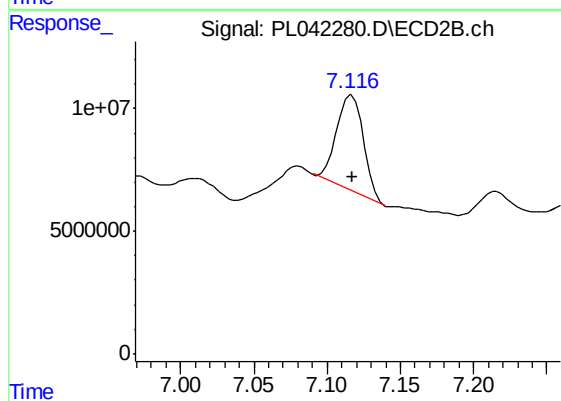

#27 Chlordane-5


R.T.: 7.117 min
Delta R.T.: 0.000 min
Response: 48097715
Conc: 500.00 ng/ml

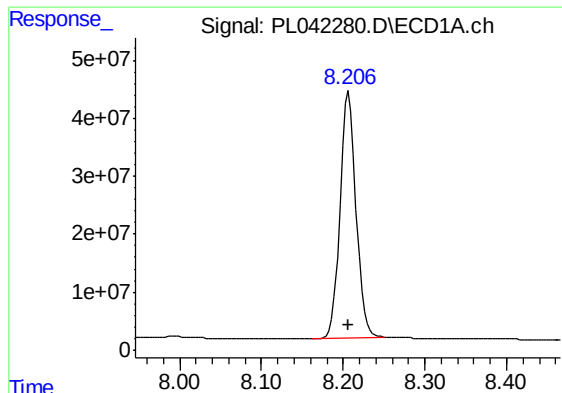

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 578324716
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

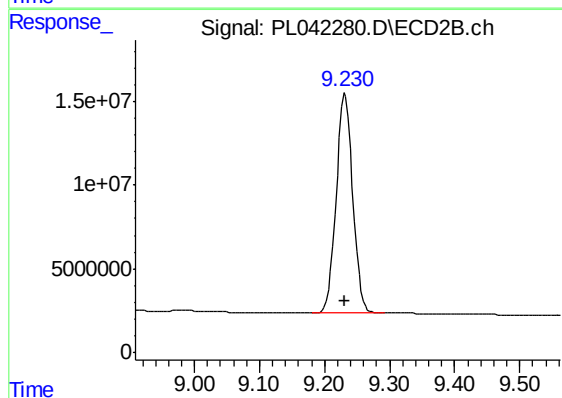

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 230868326
Conc: 50.00 ng/ml