

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
 Data File : PL042321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2018 00:12
 Operator : AJ\SJ
 Sample : J5980-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TS

Manual Integrations
 APPROVED

Sohil
 11/20/2018 12:21:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:55:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	103.0E6	49717608	17.506	17.286
28)	SA Decachlor...	8.209	9.234	109.1E6	44021587	17.304	18.252
Target Compounds							
13)	MA Dieldrin	5.757	6.617	124.9E6	59482256	16.971	17.870m
14)	MA Endrin	6.017	6.840	12356527	3583087	1.889m	1.301m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112018\
Data File : PL042321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2018 00:12
Operator : AJ\SJ
Sample : J5980-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TS


Manual Integrations
APPROVED

Sohil
11/20/2018 12:21:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:55:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

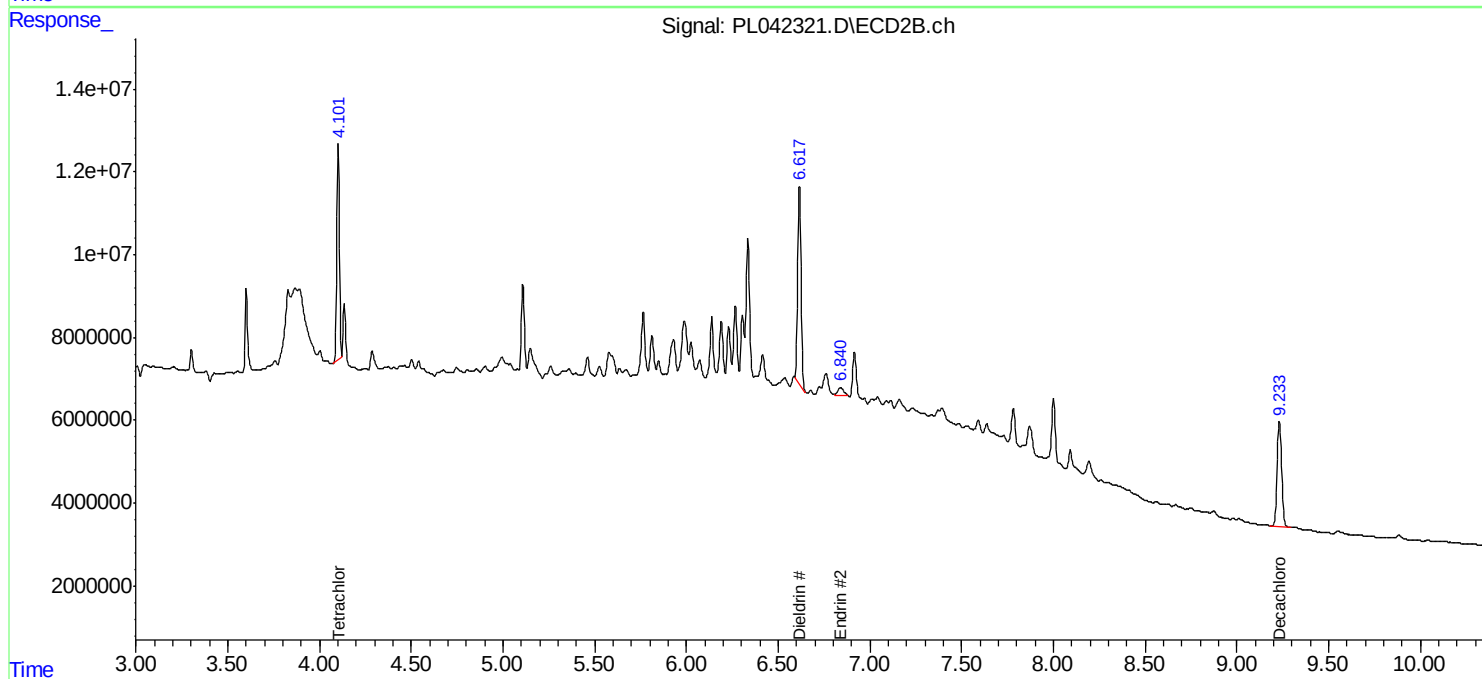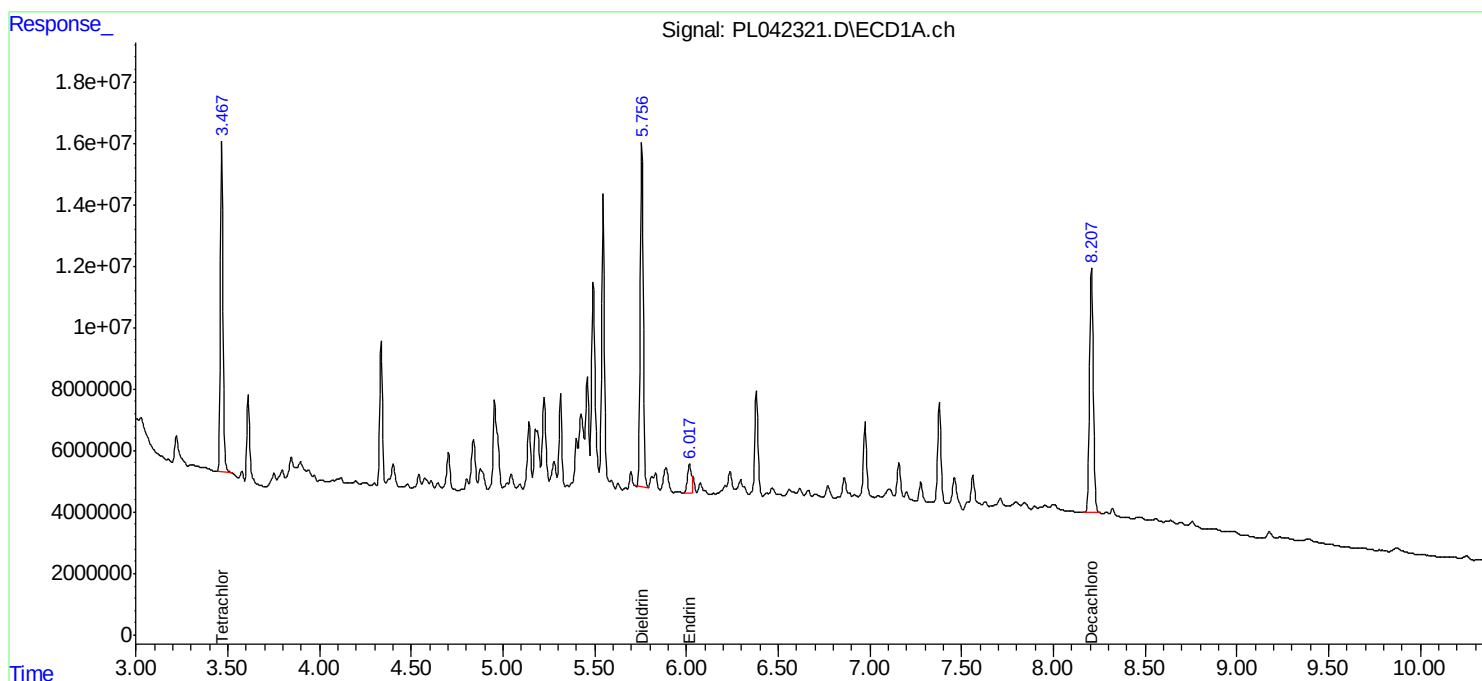

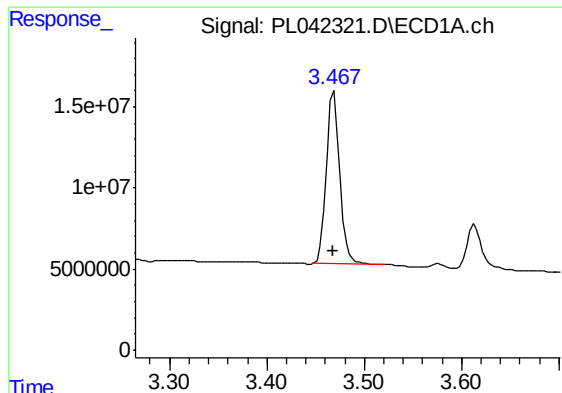


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 102994167
Conc: 17.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TS


Manual Integrations
APPROVED

Sohil
11/20/2018 12:21:22 PM

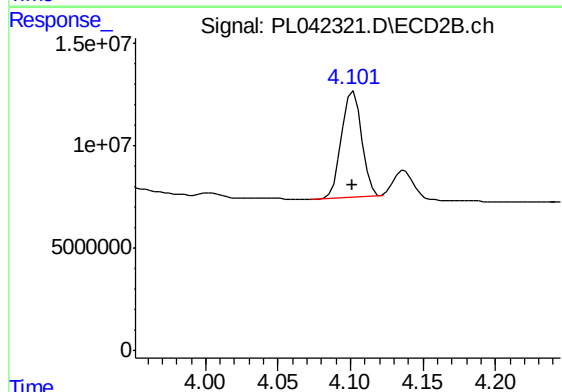


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 49717608
Conc: 17.29 ng/ml

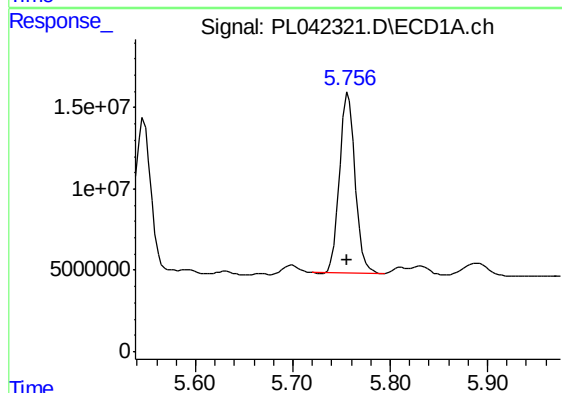


#13 Dieldrin

R.T.: 5.757 min
Delta R.T.: 0.000 min
Response: 124852314
Conc: 16.97 ng/ml

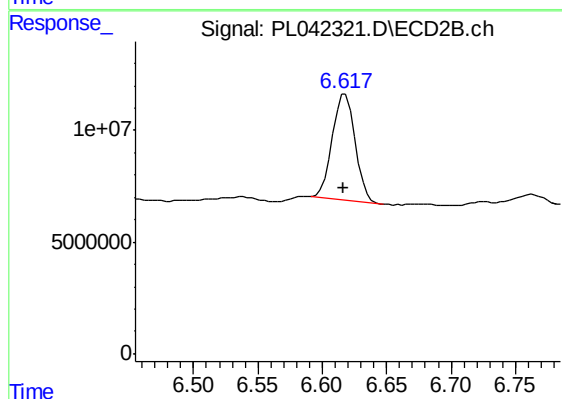

#13 Dieldrin

R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 59482256
Conc: 17.87 ng/ml m

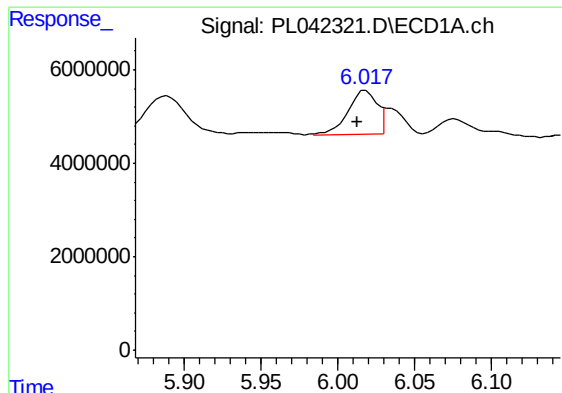


#14 Endrin

R.T.: 6.017 min
Delta R.T.: 0.004 min
Response: 12356527
Conc: 1.89 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TS


Manual Integrations
APPROVED

Sohil
11/20/2018 12:21:22 PM

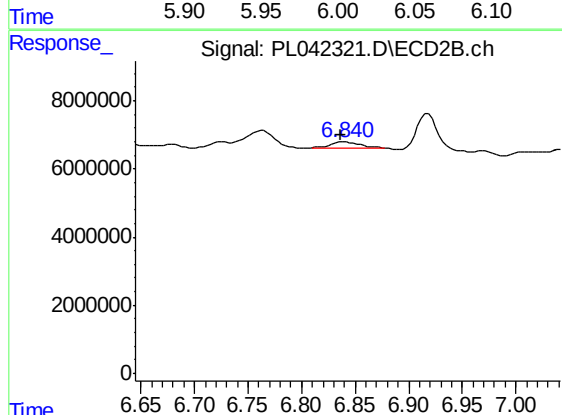


#14 Endrin

R.T.: 6.840 min
Delta R.T.: 0.003 min
Response: 3583087
Conc: 1.30 ng/ml m

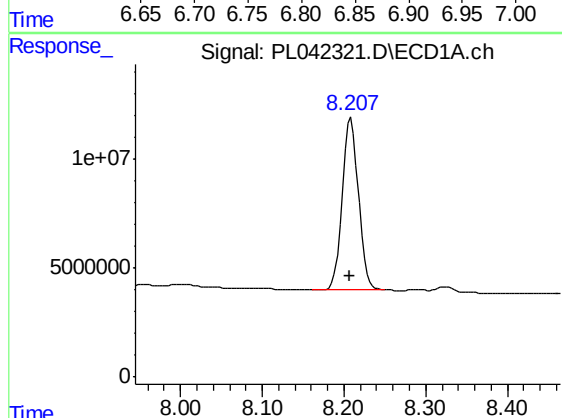

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.002 min
Response: 109050209
Conc: 17.30 ng/ml

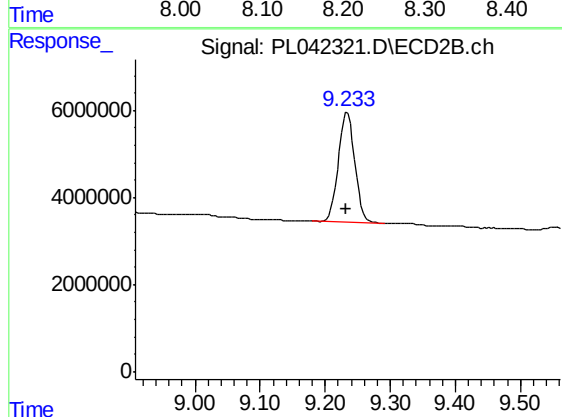

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.002 min
Response: 44021587
Conc: 18.25 ng/ml