

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112019\
 Data File : PL054502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2019 20:38
 Operator : SG\AJ
 Sample : K5938-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-277

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:08:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.043	202.2E6	52152223	19.450	21.407
28)	SA Decachlor...	8.320	9.121	180.3E6	53630944	20.371	22.182
Target Compounds							
7)	B delta-BHC	0.000	5.081f	0	1699397	N.D.	0.675 #
23)	Chlordane-1	4.426	0.000	716480	0	1.845	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112019\
Data File : PL054502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2019 20:38
Operator : SG\AJ
Sample : K5938-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ETGI-277

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:08:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

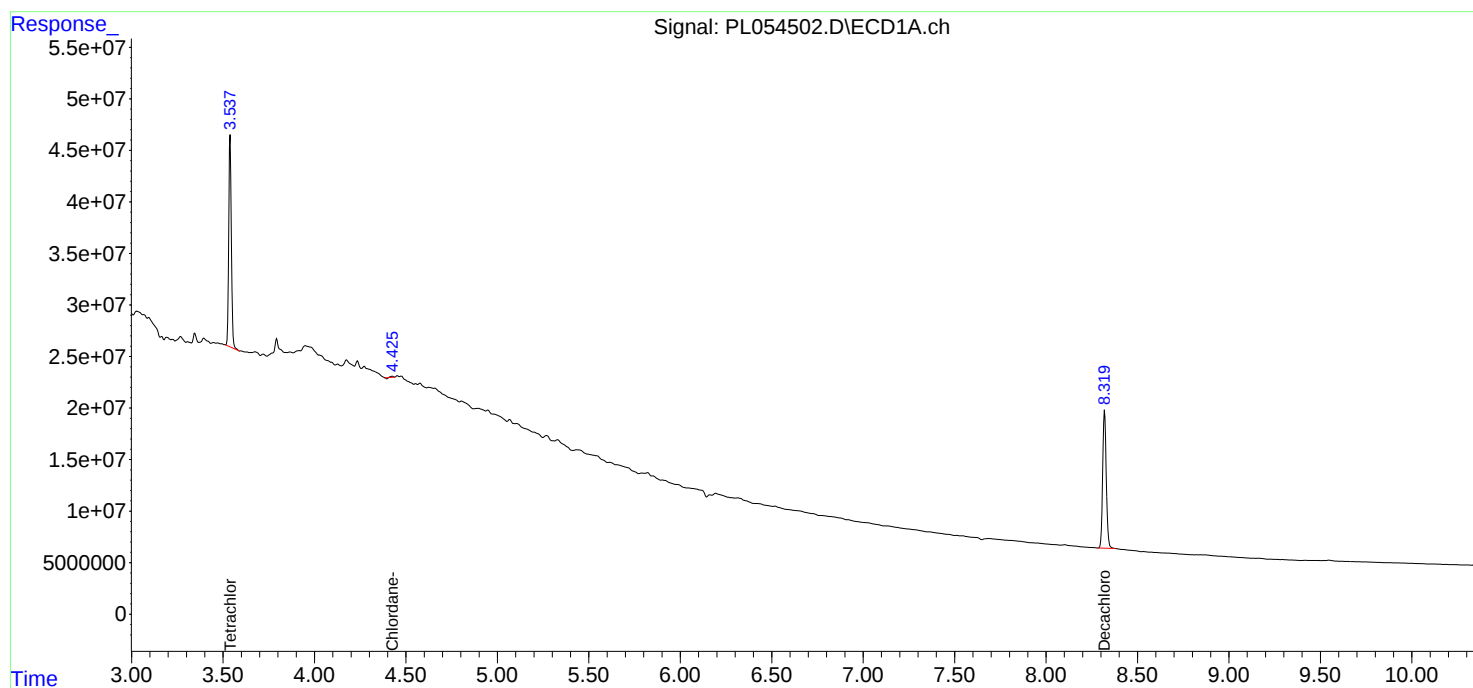


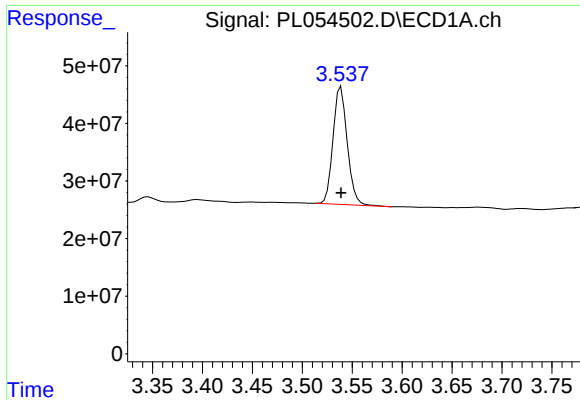

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 202224880
Conc: 19.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-277

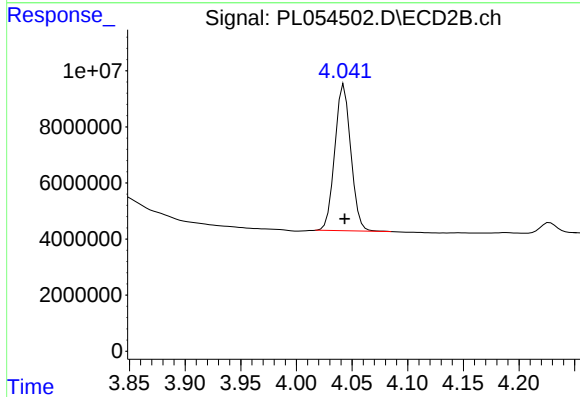


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 52152223
Conc: 21.41 ng/ml

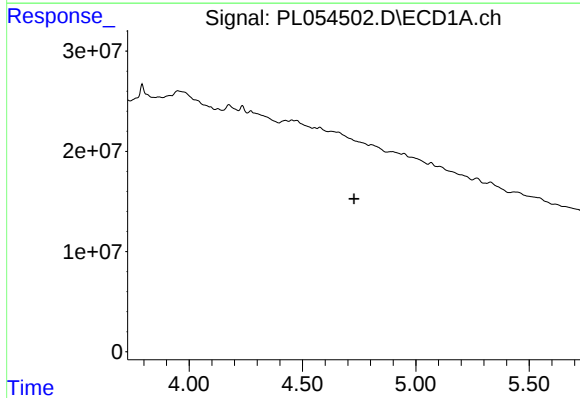


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.728 min
Response: 0
Conc: N.D.

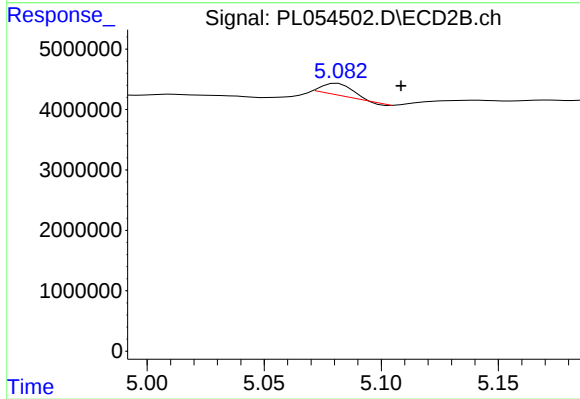

#7 delta-BHC


R.T.: 5.081 min
Delta R.T.: -0.027 min
Response: 1699397
Conc: 0.67 ng/ml

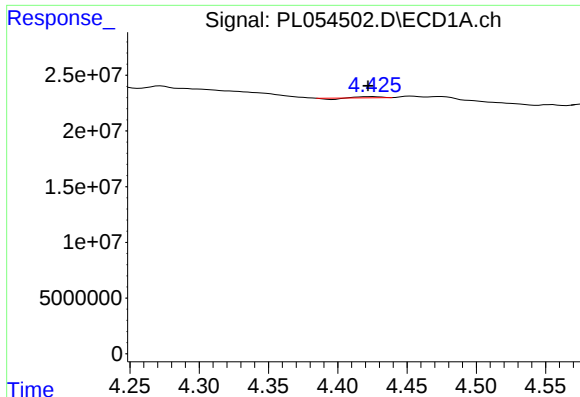

#23 Chlordane-1


R.T.: 4.426 min
Delta R.T.: 0.004 min
Response: 716480
Conc: 1.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-277

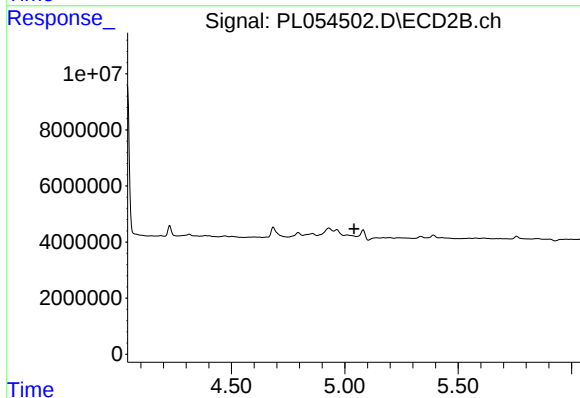


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.041 min
Response: 0
Conc: N.D.

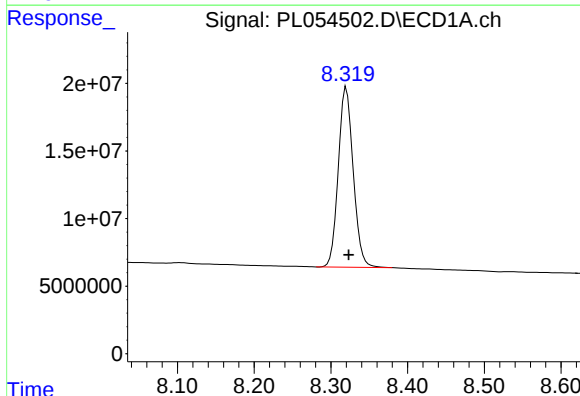

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.003 min
Response: 180305366
Conc: 20.37 ng/ml

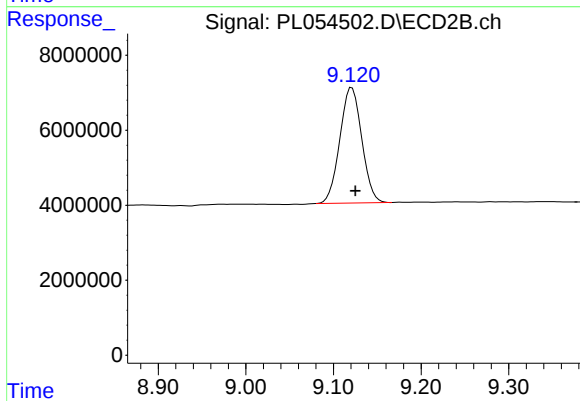

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.004 min
Response: 53630944
Conc: 22.18 ng/ml