

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112020\
 Data File : PL063125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2020 08:48
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 18:32:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
13) MA	Dieldrin	0.000	6.449f	0	4761513	N.D. 1.488 #
17) MA	4,4'-DDT	6.295	7.078	4178885	5442998	3.131 2.424
18) B	Endrin al...	6.388f	0.000	3295477	0	2.269 N.D. #
20) A	Methoxychlor	6.854	7.534	1738986	5647112	2.019 4.571 #
21) B	Endrin ke...	7.056f	0.000	2693204	0	1.494 N.D. #
22)	Mirex	0.000	8.137f	0	4310715	N.D. 2.530 #
23)	Chlordane-1	4.264	0.000	296997	0	5.761 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112020\
Data File : PL063125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2020 08:48
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 18:32:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

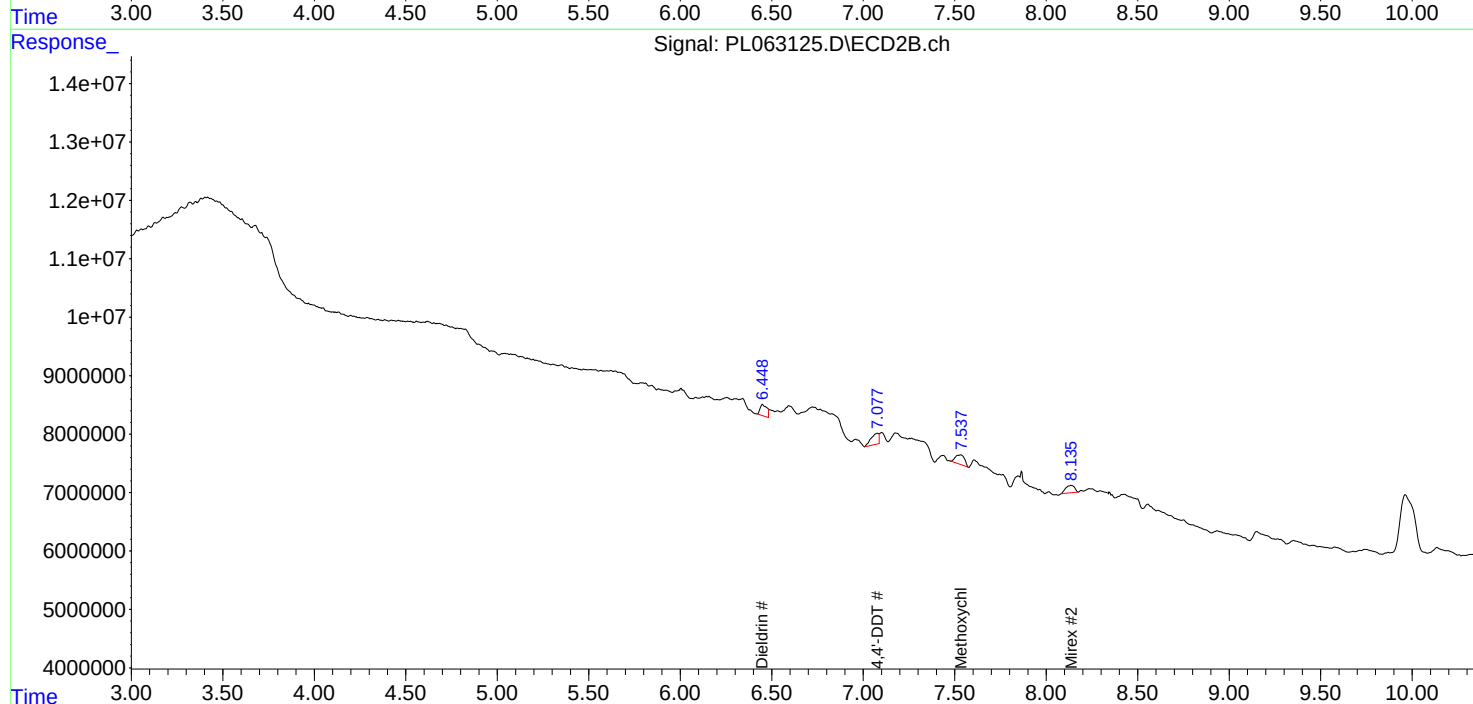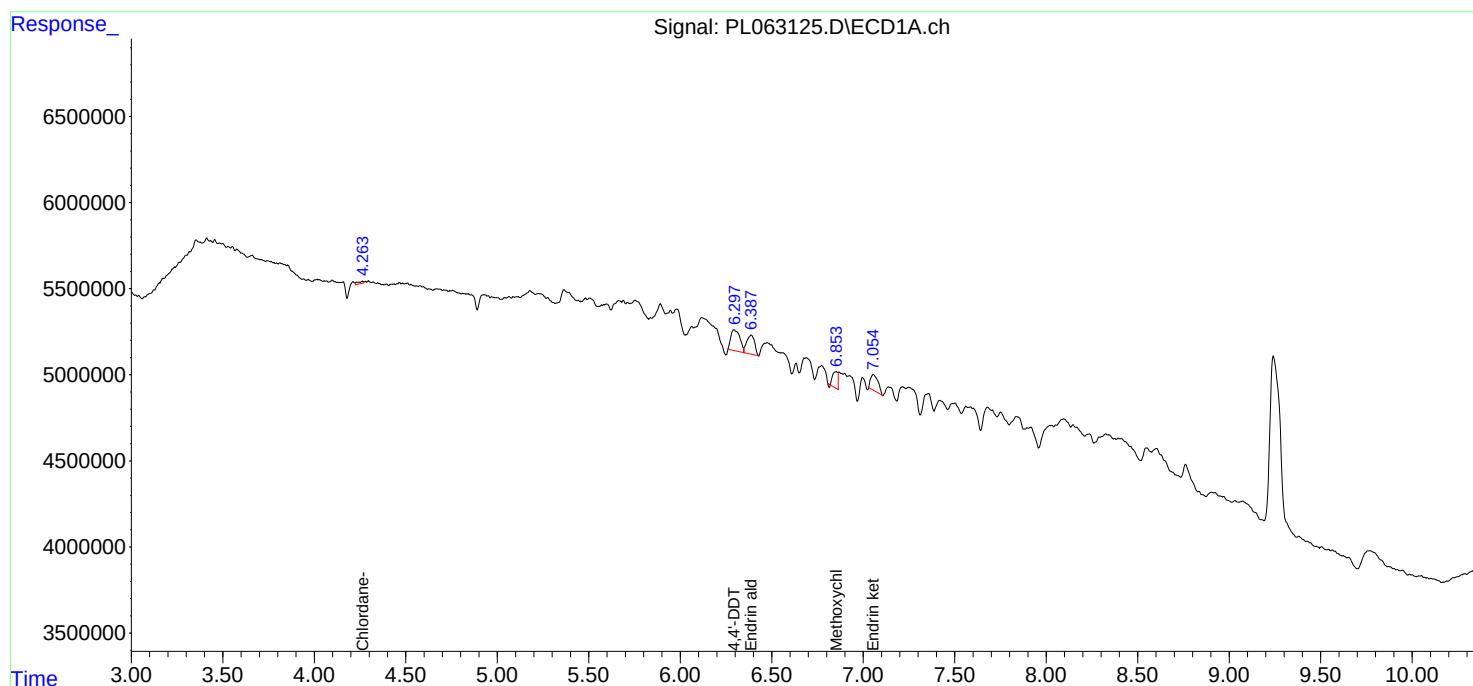


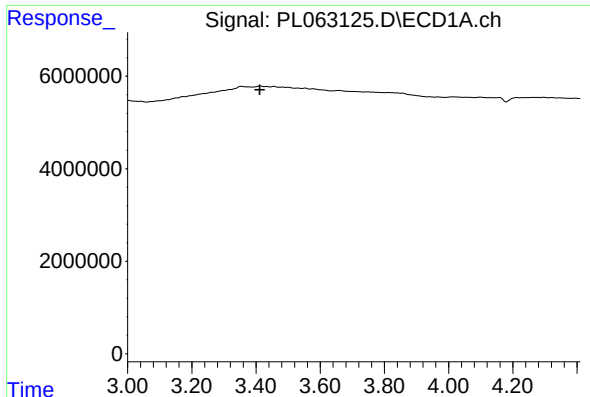

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

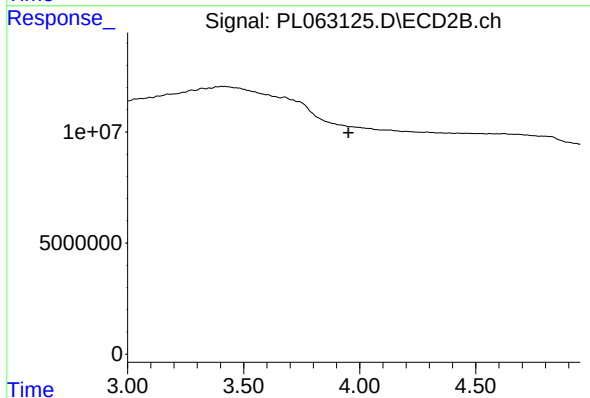


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

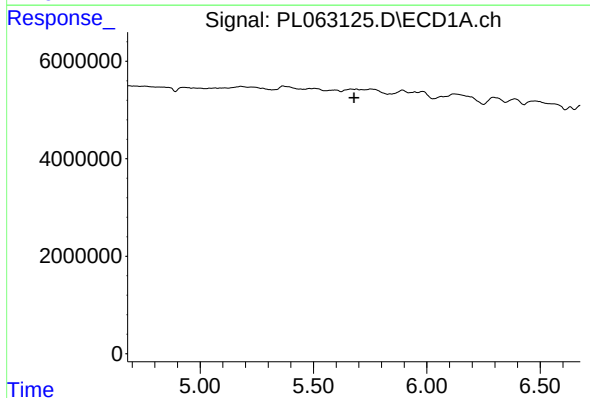


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.679 min
Response: 0
Conc: N.D.

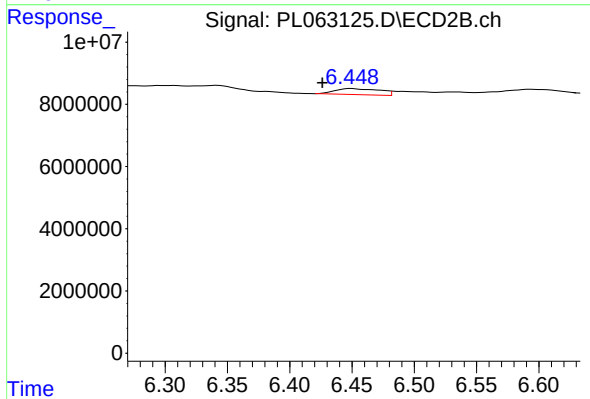

#13 Dieldrin


R.T.: 6.449 min
Delta R.T.: 0.023 min
Response: 4761513
Conc: 1.49 ng/ml

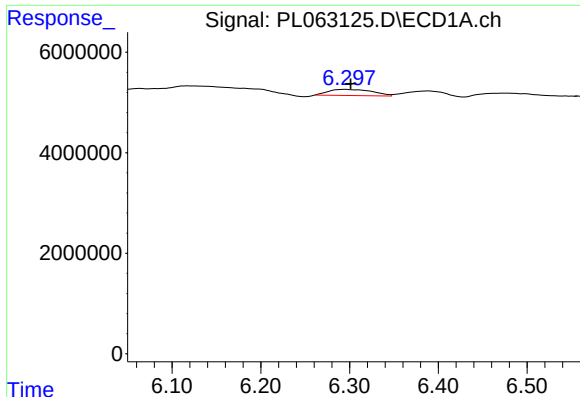

#17 4,4'-DDT


R.T.: 6.295 min
Delta R.T.: -0.006 min
Response: 4178885
Conc: 3.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

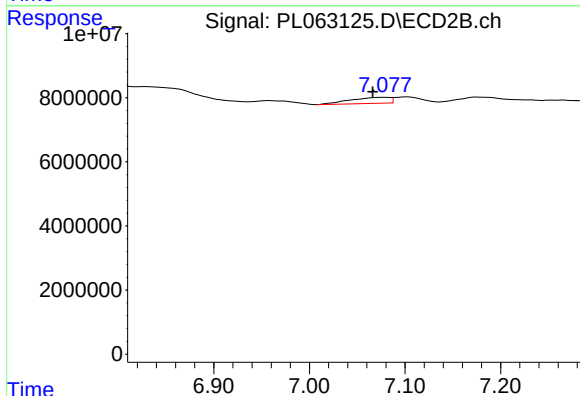


#17 4,4'-DDT

R.T.: 7.078 min
Delta R.T.: 0.012 min
Response: 5442998
Conc: 2.42 ng/ml

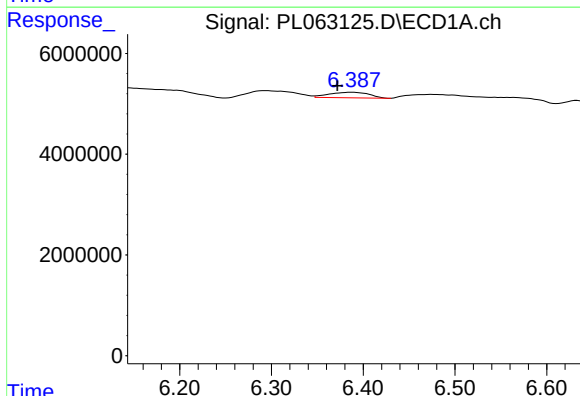


#18 Endrin aldehyde

R.T.: 6.388 min
Delta R.T.: 0.016 min
Response: 3295477
Conc: 2.27 ng/ml

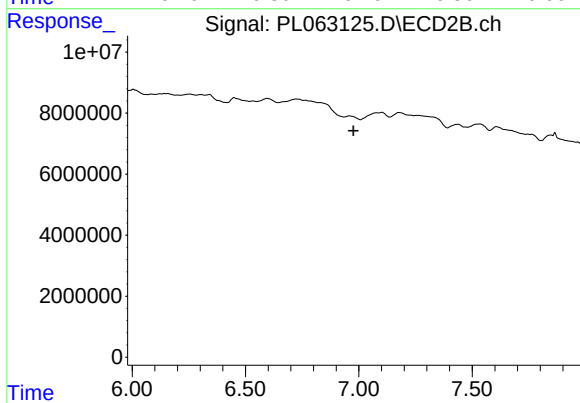

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

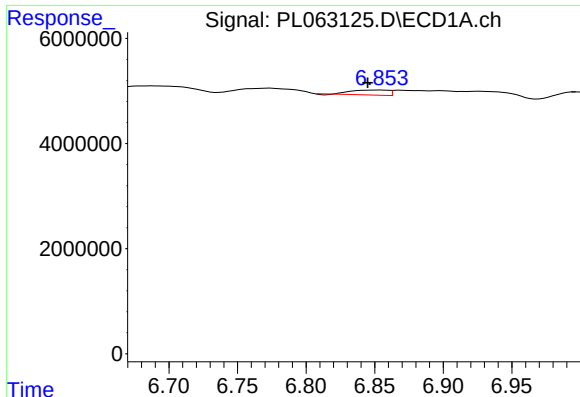

#20 Methoxychlor


R.T.: 6.854 min
Delta R.T.: 0.009 min
Response: 1738986
Conc: 2.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

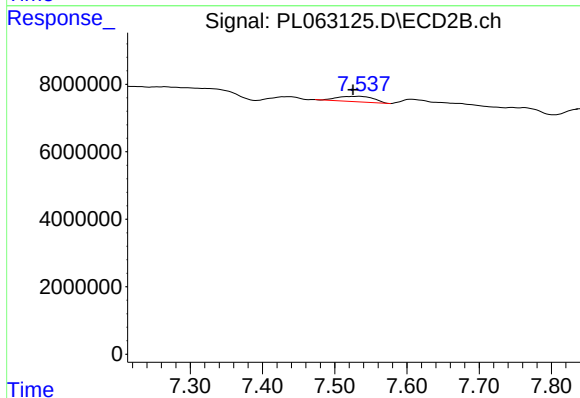


#20 Methoxychlor

R.T.: 7.534 min
Delta R.T.: 0.009 min
Response: 5647112
Conc: 4.57 ng/ml

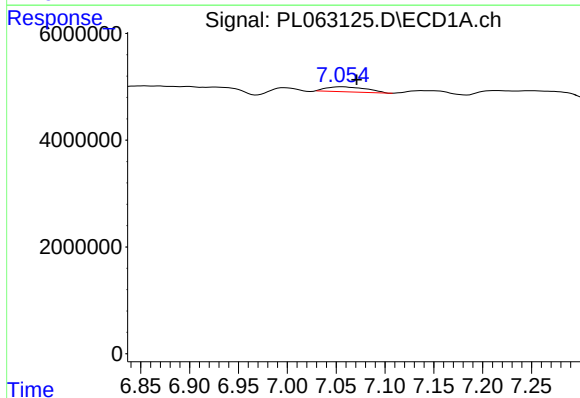


#21 Endrin ketone

R.T.: 7.056 min
Delta R.T.: -0.015 min
Response: 2693204
Conc: 1.49 ng/ml

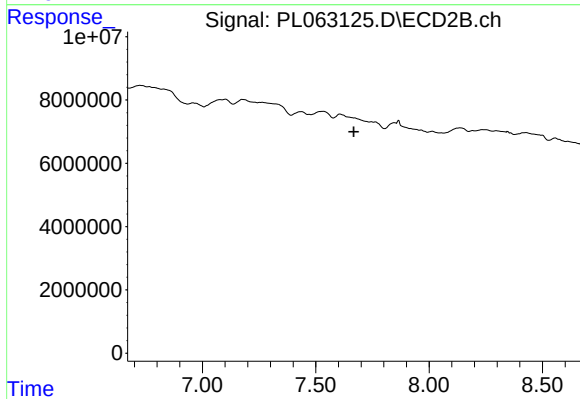

#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.668 min
Response: 0
Conc: N.D.

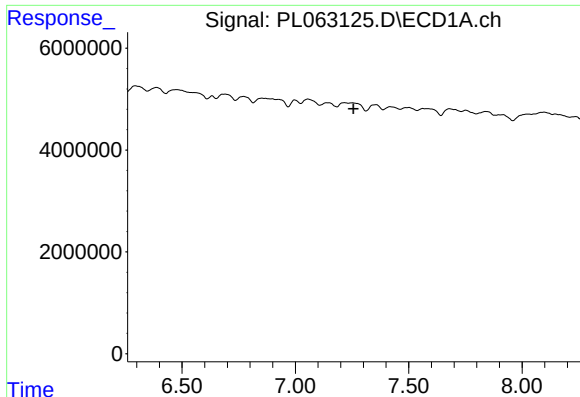

#22 Mirex


R.T.: 0.000 min

Exp R.T. : 7.257 min

Response: 0

Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

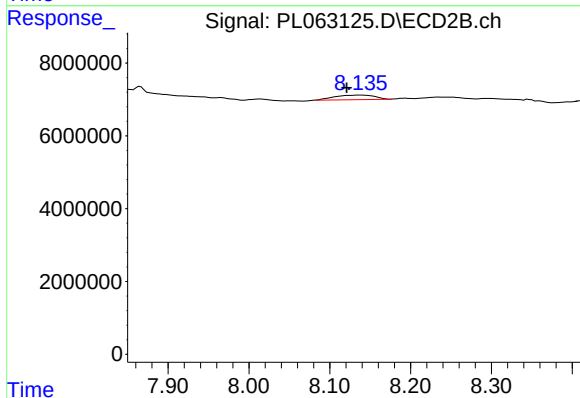


#22 Mirex

R.T.: 8.137 min

Delta R.T.: 0.016 min

Response: 4310715

Conc: 2.53 ng/ml

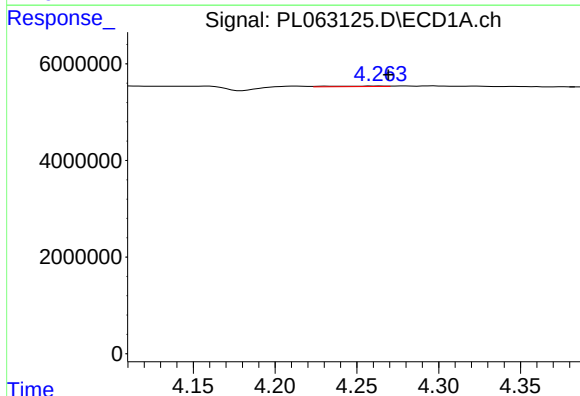


#23 Chlordane-1

R.T.: 4.264 min

Delta R.T.: -0.005 min

Response: 296997

Conc: 5.76 ng/ml

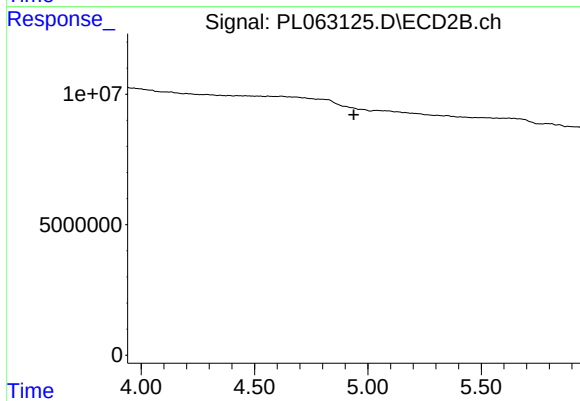


#23 Chlordane-1

R.T.: 0.000 min

Exp R.T. : 4.938 min

Response: 0


Conc: N.D.

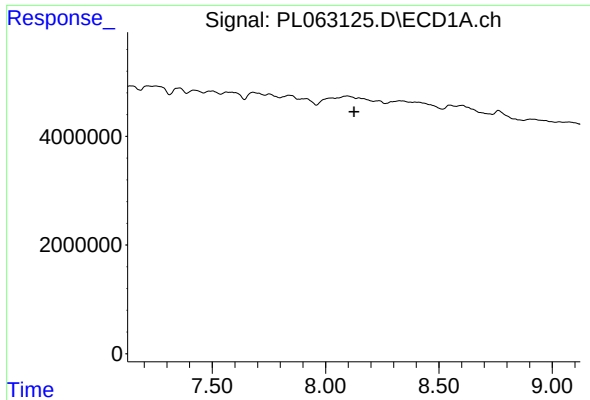

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

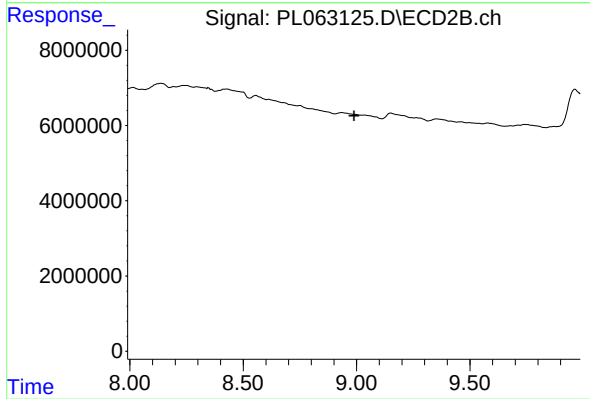

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.989 min
Response: 0
Conc: N.D.