

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112020\
 Data File : PL063132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2020 13:04
 Operator : DD\AJ
 Sample : L4800-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KENS-B1-111820-0-1

Manual Integrations
 APPROVED

mohammad
 11/23/2020 12:00:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 18:33:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.408	3.950	39726913	63603009	23.096m	21.643
28) SA Decachlor...	8.124	8.987	27059548	34562170	16.867	16.514

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112020\
Data File : PL063132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2020 13:04
Operator : DD\AJ
Sample : L4800-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
KENS-B1-111820-0-1


Manual Integrations
APPROVED

mohammad
11/23/2020 12:00:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 18:33:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

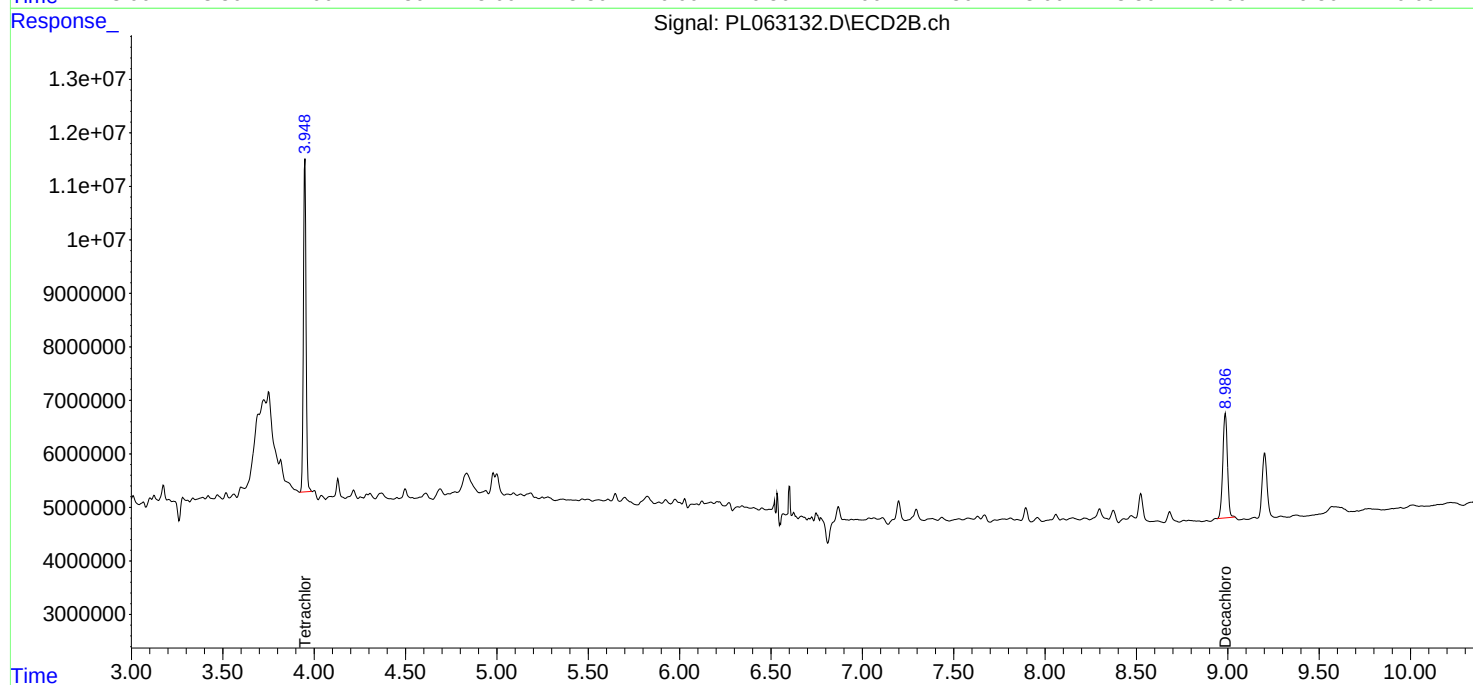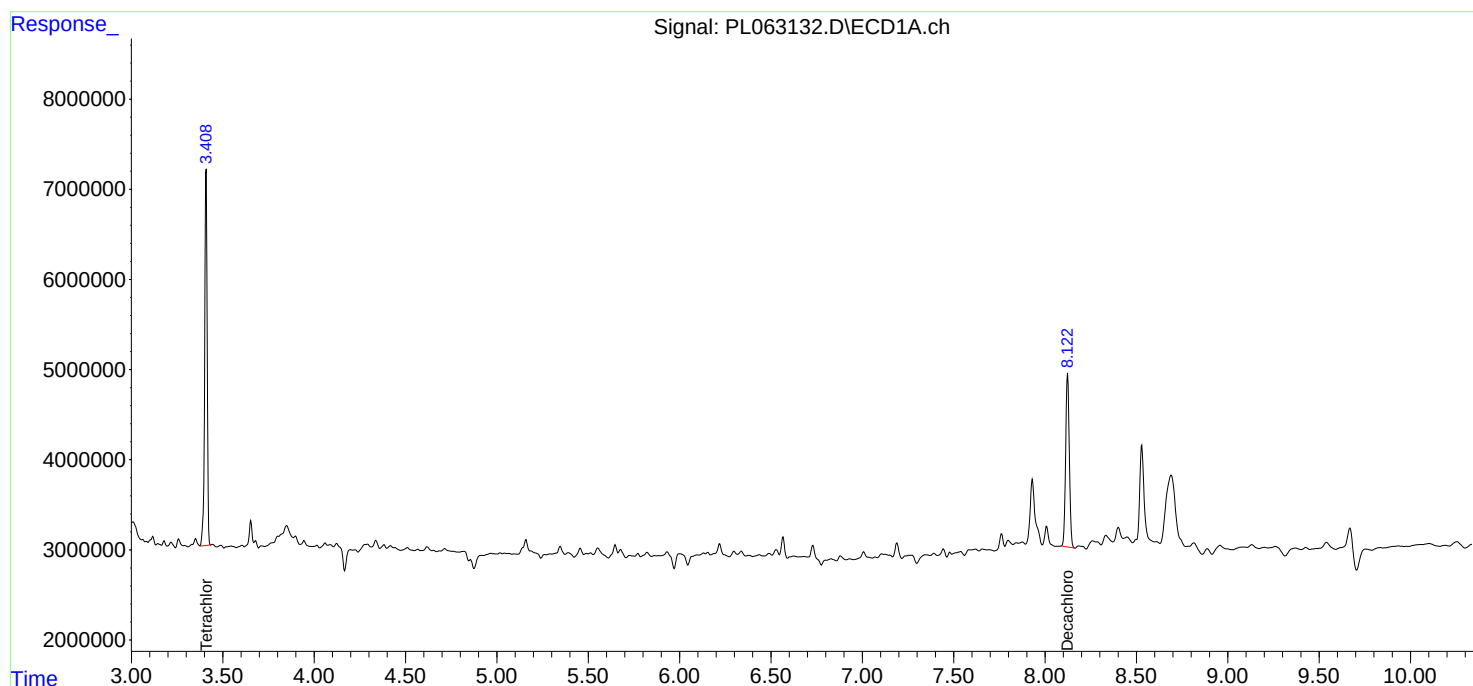

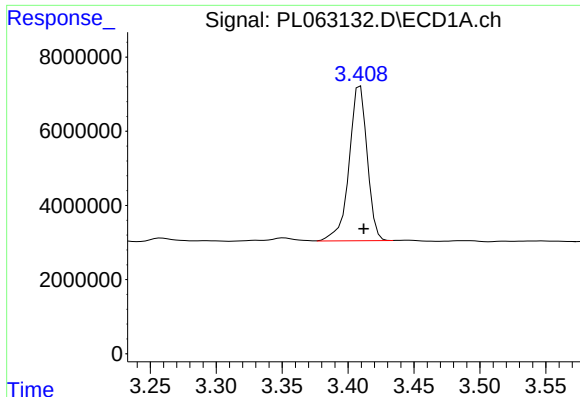


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: -0.004 min
Response: 39726913
Conc: 23.10 ng/ml m

Instrument :
ECD_L
ClientSampleId :
KENS-B1-111820-0-1


Manual Integrations
APPROVED

mohammad
11/23/2020 12:00:37 PM

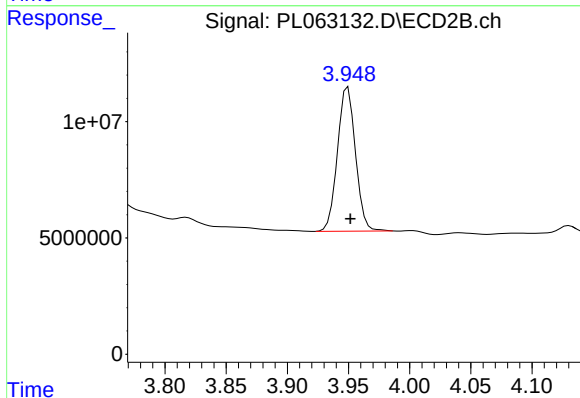


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 63603009
Conc: 21.64 ng/ml

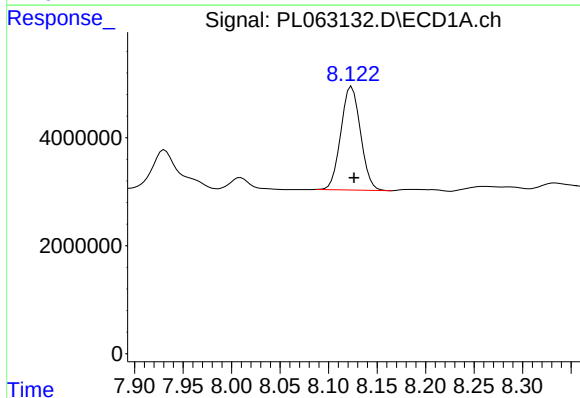

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 27059548
Conc: 16.87 ng/ml

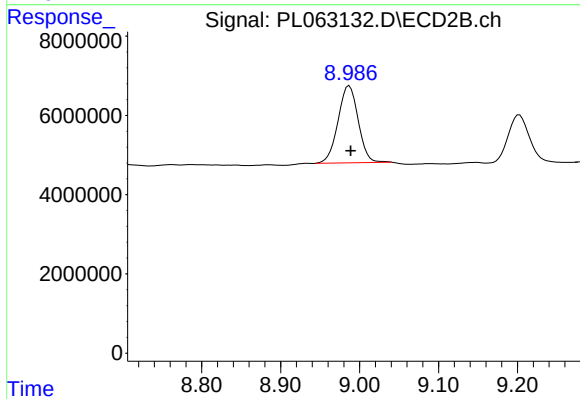

#28 Decachlorobiphenyl

R.T.: 8.987 min
Delta R.T.: -0.002 min
Response: 34562170
Conc: 16.51 ng/ml