

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112020\
 Data File : PL063136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2020 14:01
 Operator : DD\AJ
 Sample : L4809-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MS-CON-B

Manual Integrations
 APPROVED

mohammad
 11/23/2020 12:00:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 18:34:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	33903059	59671682	19.710	20.305
28)	SA Decachlor...	8.125	8.989	35709426	42575437	22.259	20.342
Target Compounds							
12)	B 4,4'-DDE	5.548	6.276	684198	2186164	0.414	0.679 #
17)	MA 4,4'-DDT	6.296	7.055	1909825	777910	1.431	0.346m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112020\
Data File : PL063136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2020 14:01
Operator : DD\AJ
Sample : L4809-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
MS-CON-B


Manual Integrations
APPROVED

mohammad
11/23/2020 12:00:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 18:34:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

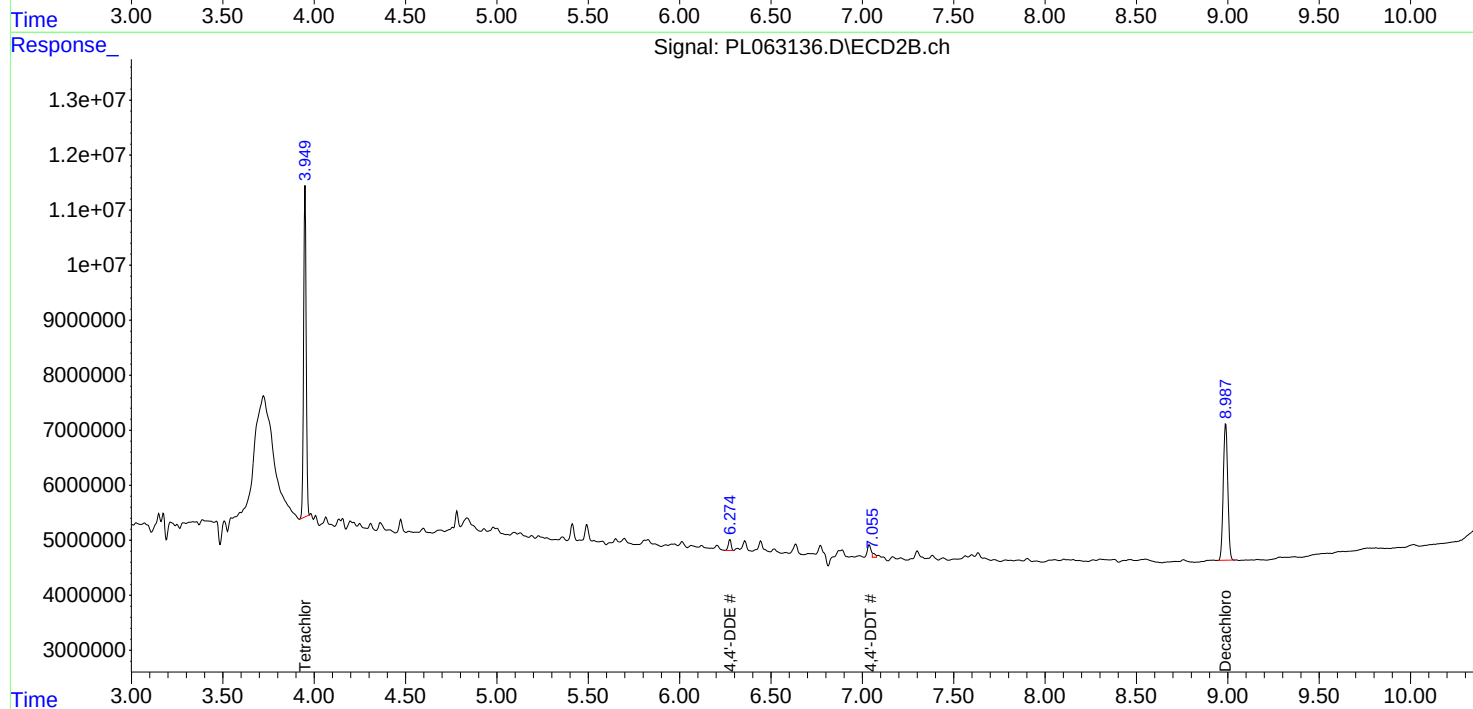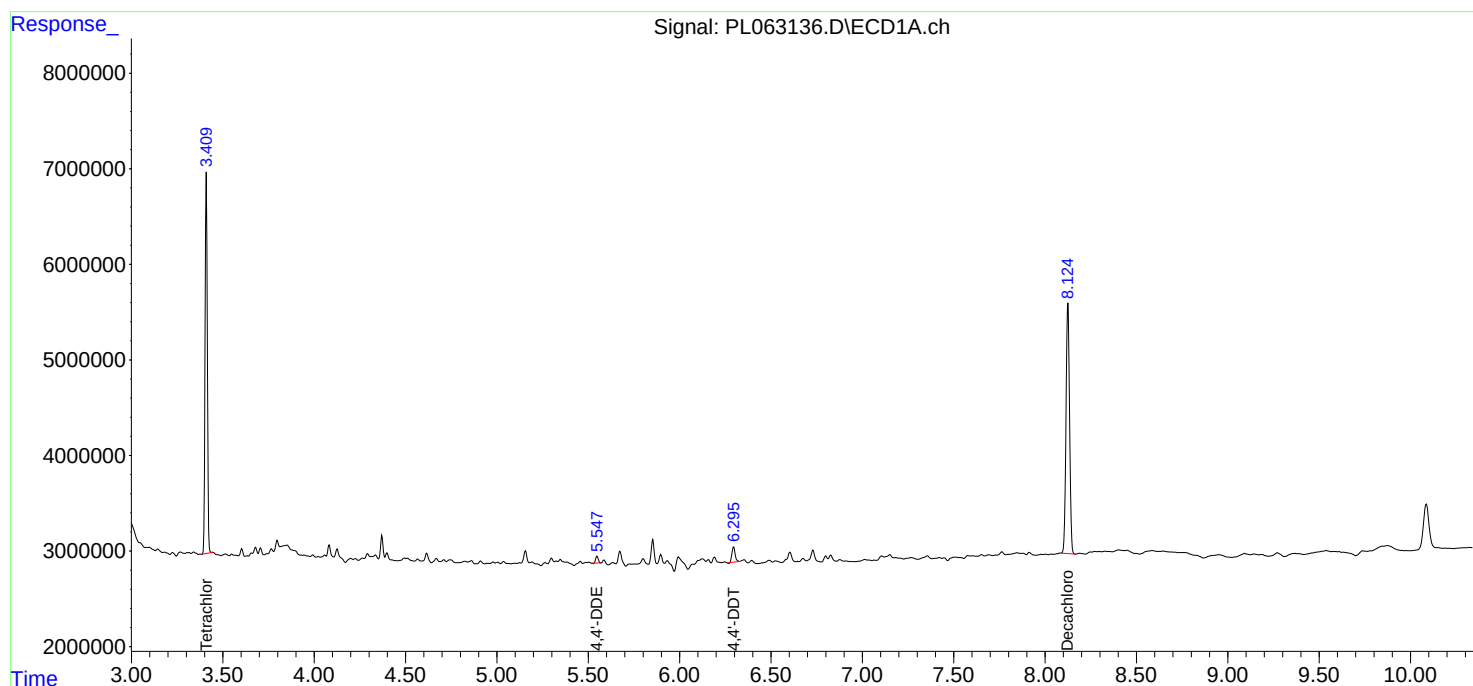

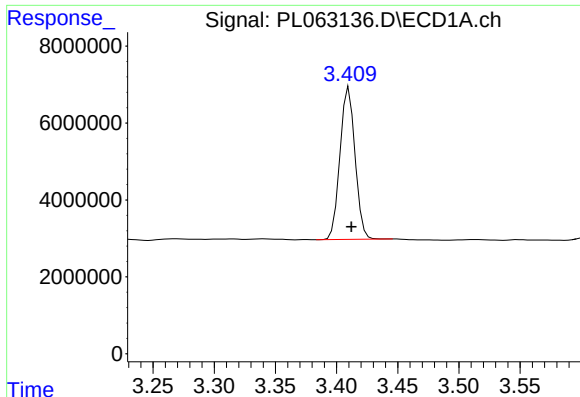


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 33903059
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
MS-CON-B


Manual Integrations
APPROVED

mohammad
11/23/2020 12:00:43 PM

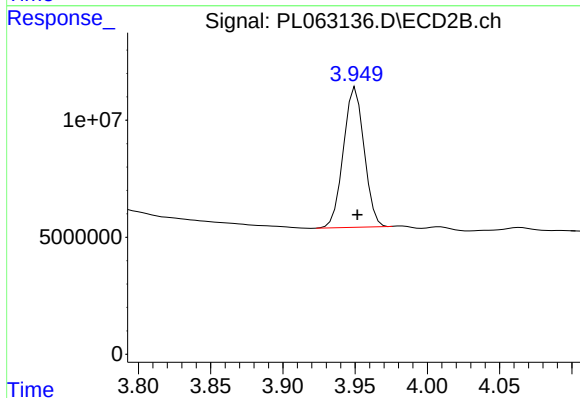


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.001 min
Response: 59671682
Conc: 20.31 ng/ml

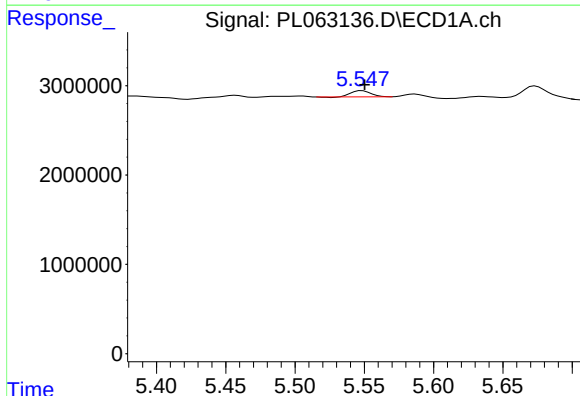


#12 4,4'-DDE

R.T.: 5.548 min
Delta R.T.: -0.002 min
Response: 684198
Conc: 0.41 ng/ml

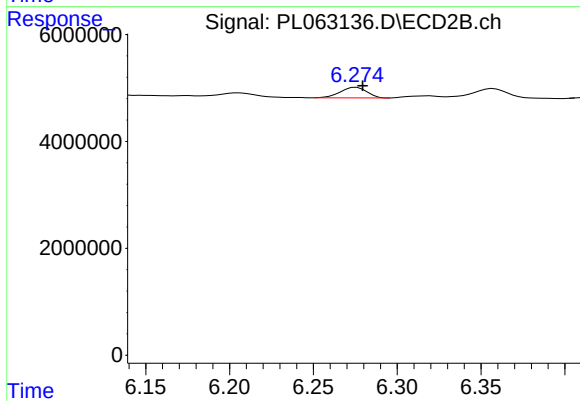

#12 4,4'-DDE

R.T.: 6.276 min
Delta R.T.: -0.004 min
Response: 2186164
Conc: 0.68 ng/ml

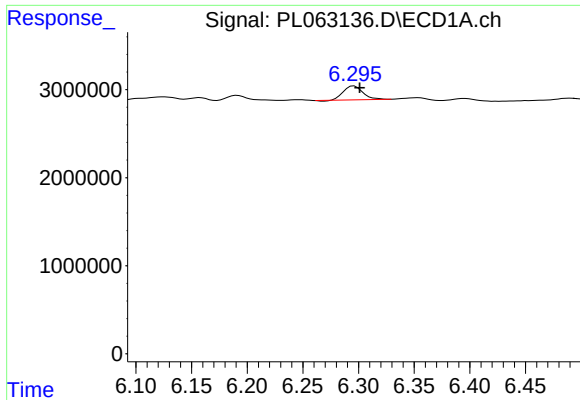


#17 4,4'-DDT

R.T.: 6.296 min
Delta R.T.: -0.005 min
Response: 1909825
Conc: 1.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
MS-CON-B


Manual Integrations
APPROVED

mohammad
11/23/2020 12:00:43 PM

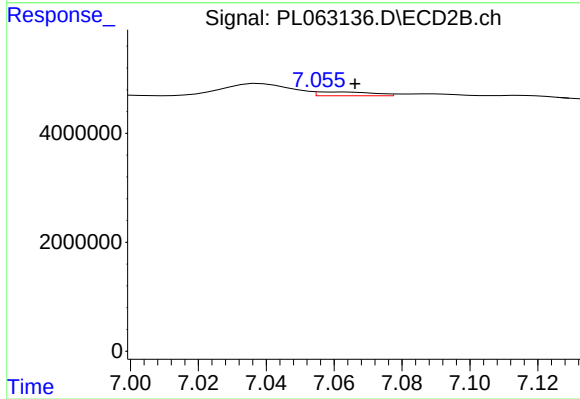


#17 4,4'-DDT

R.T.: 7.055 min
Delta R.T.: -0.012 min
Response: 777910
Conc: 0.35 ng/ml m

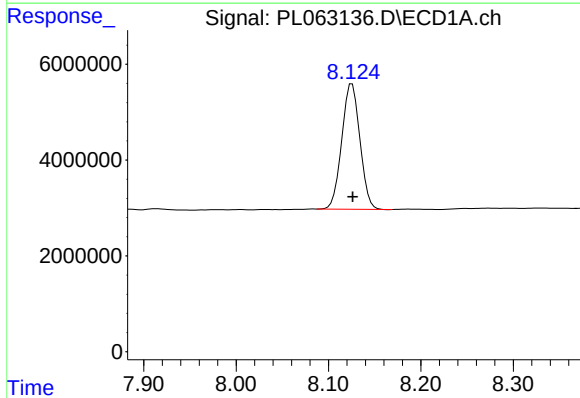

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 35709426
Conc: 22.26 ng/ml

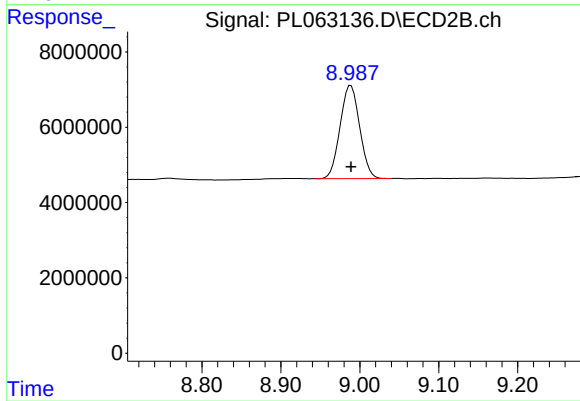

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 42575437
Conc: 20.34 ng/ml