

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112023\
 Data File : PL086746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 10:37
 Operator : AR\AJ
 Sample : 05434-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2023
 Supervised By :Ankita Jodhani 11/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 20:14:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.358	2.617	30509120	8951145	9.396	9.091
28) SA Decachlor...	8.856	7.768	26775079	12383467	9.147	10.255
Target Compounds						
12) B 4,4'-DDE	6.018	5.074	7428462	2023786	2.142m	1.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112023\
Data File : PL086746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 10:37
Operator : AR\AJ
Sample : 05434-11
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 20:14:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

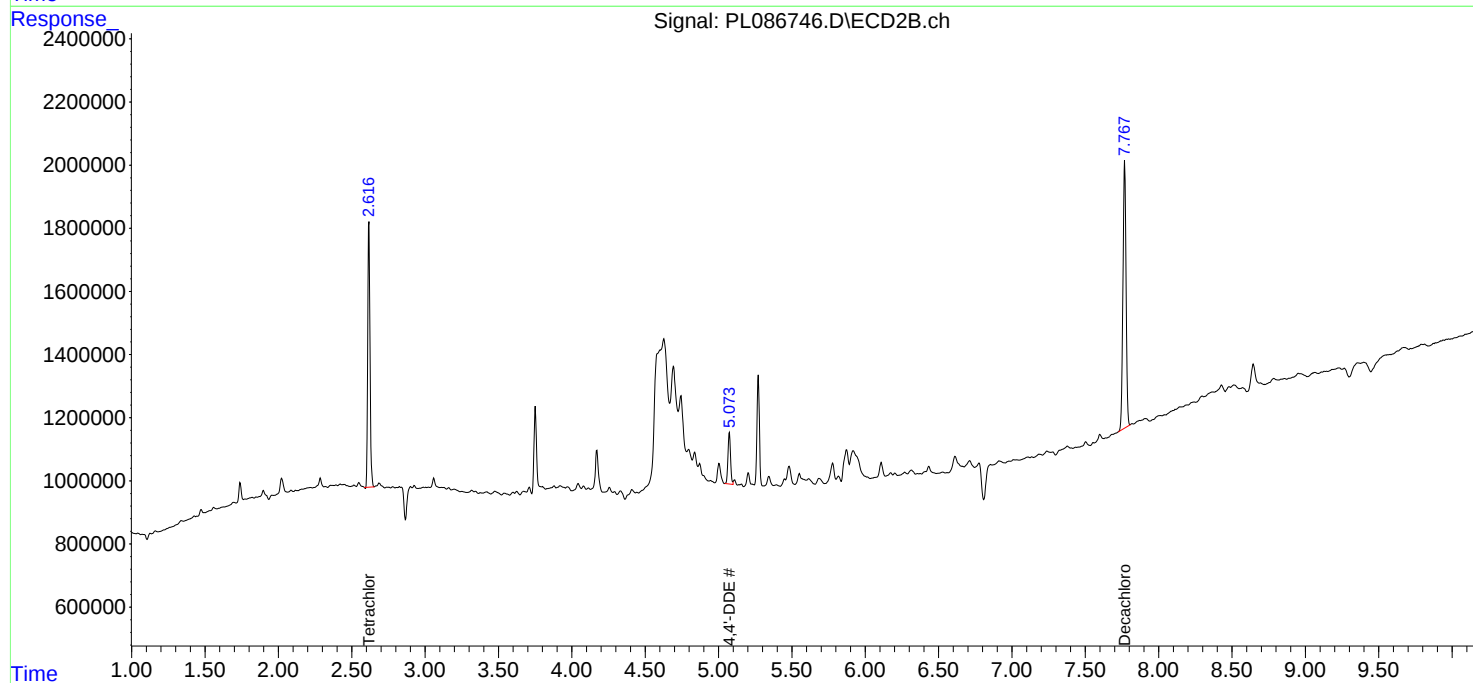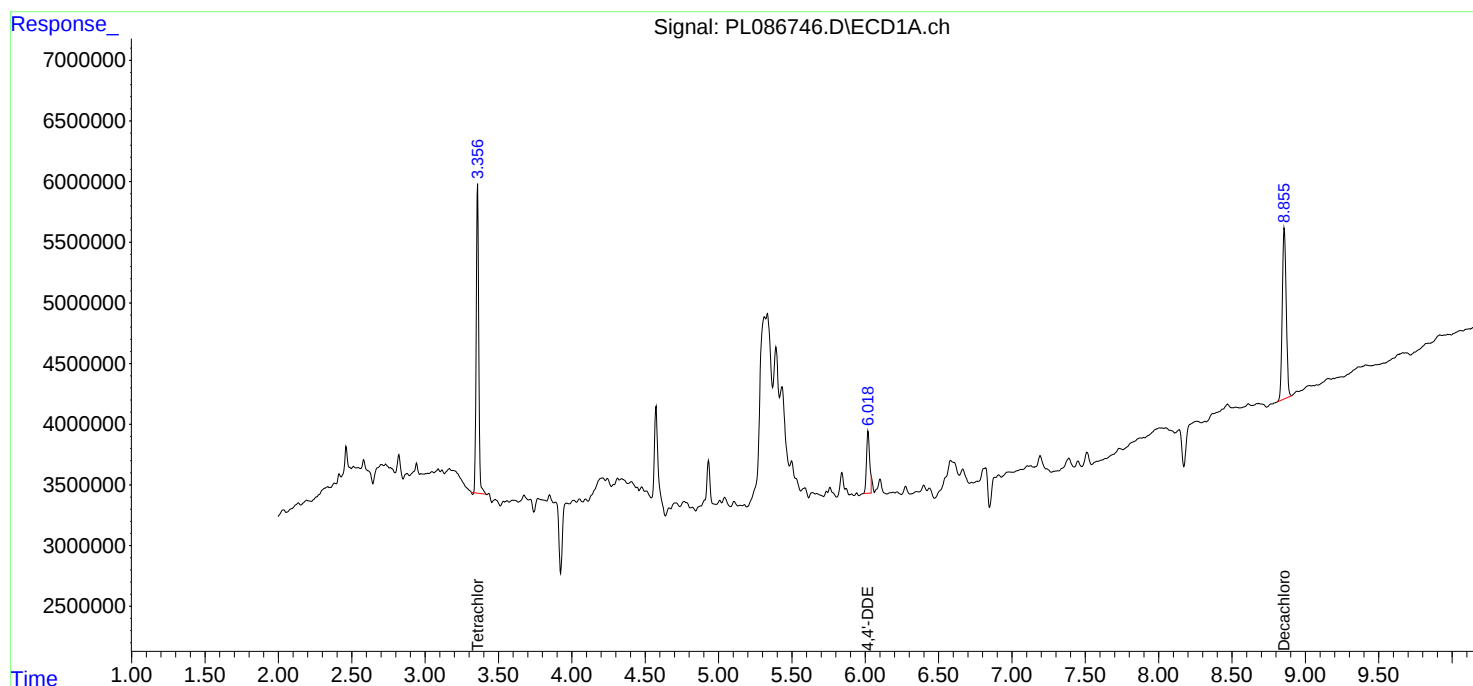

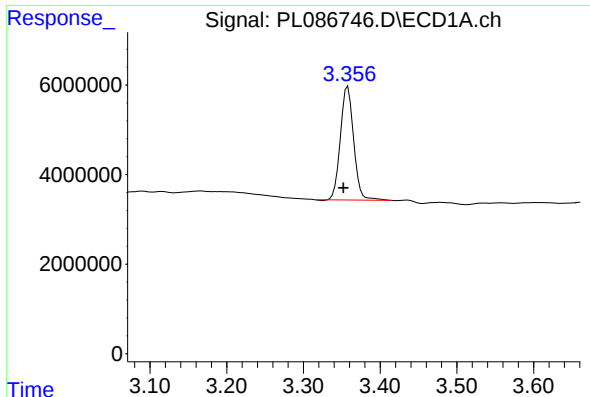


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: 0.006 min
Response: 30509120
Conc: 9.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023

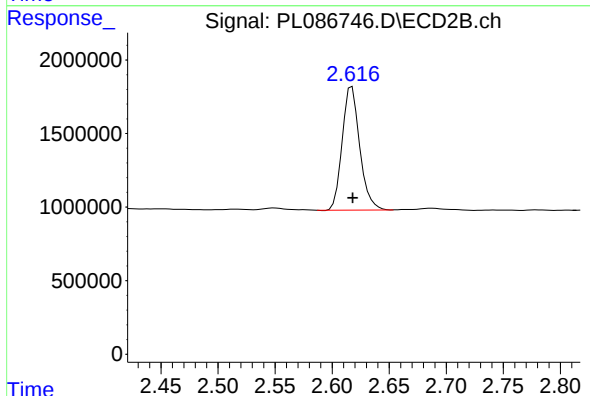


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 8951145
Conc: 9.09 ng/ml

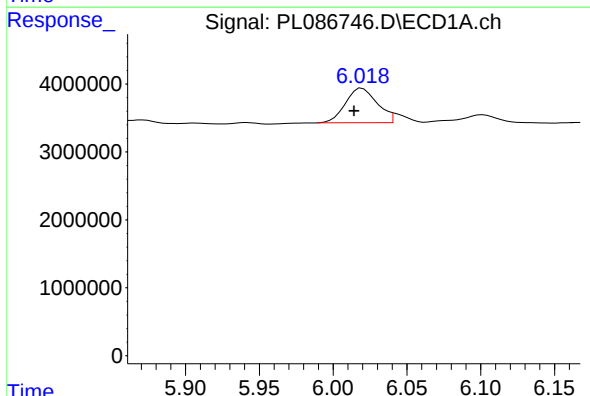


#12 4,4'-DDE

R.T.: 6.018 min
Delta R.T.: 0.004 min
Response: 7428462
Conc: 2.14 ng/ml m

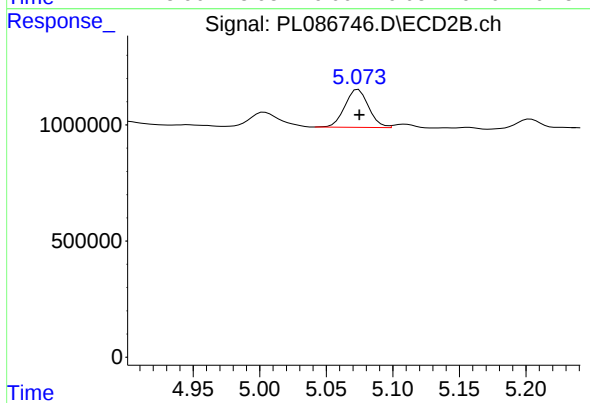

#12 4,4'-DDE

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 2023786
Conc: 1.97 ng/ml

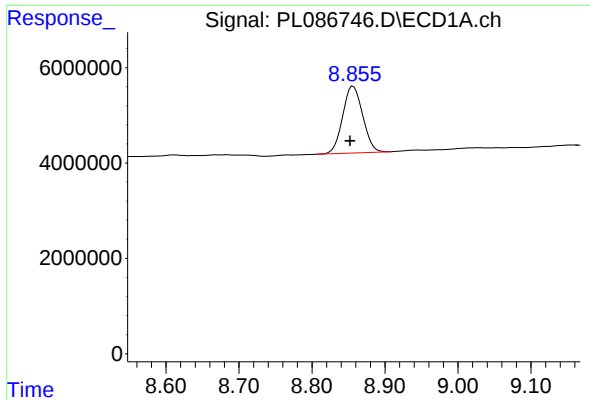


#28 Decachlorobiphenyl

R.T.: 8.856 min
Delta R.T.: 0.004 min
Response: 26775079
Conc: 9.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023

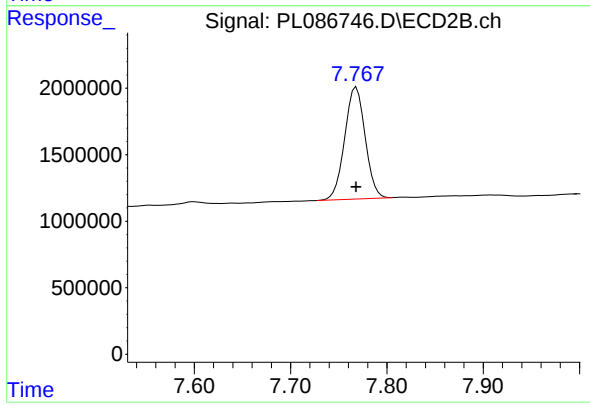

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 12383467
Conc: 10.25 ng/ml