

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
 Data File : PL042366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2018 18:53
 Operator : AJ\SJ
 Sample : J5999-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:05:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	119.1E6	65026234	20.244	22.609
28)	SA Decachlor...	8.206	9.232	119.8E6	48130792	19.005	19.956
Target Compounds							
2)	A alpha-BHC	0.000	4.452f	0	595859	N.D.	0.139 #
4)	MA Heptachlor	4.523f	0.000	646647	0	0.074	N.D. #
6)	B beta-BHC	4.403f	4.906f	20512940	1068459	5.790	0.677 #
8)	B Heptachlo...	0.000	5.997	0	865960	N.D.	0.242 #
9)	A Endosulfan I	5.460f	0.000	7651678	0	1.106	N.D. #
10)	B gamma-Chl...	5.460f	0.000	7651678	0	1.004	N.D. #
11)	B alpha-Chl...	5.460	0.000	7651678	0	1.019	N.D. #
23)	Chlordane-1	4.403	0.000	20512940	0	74.195	N.D. #
25)	Chlordane-3	5.460	0.000	7651678	0	8.729	N.D. #
26)	Chlordane-4	5.460	0.000	7651678	0	10.082	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
Data File : PL042366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2018 18:53
Operator : AJ\SJ
Sample : J5999-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:05:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

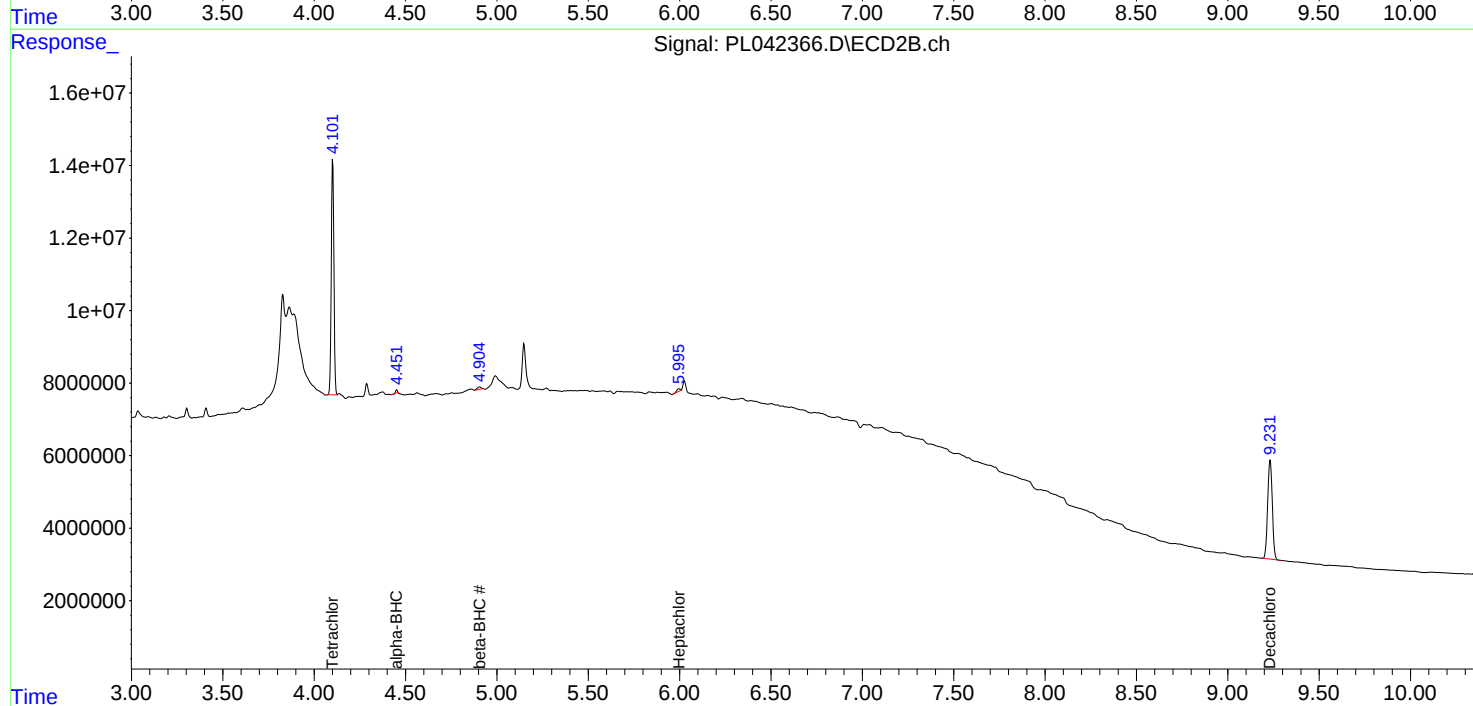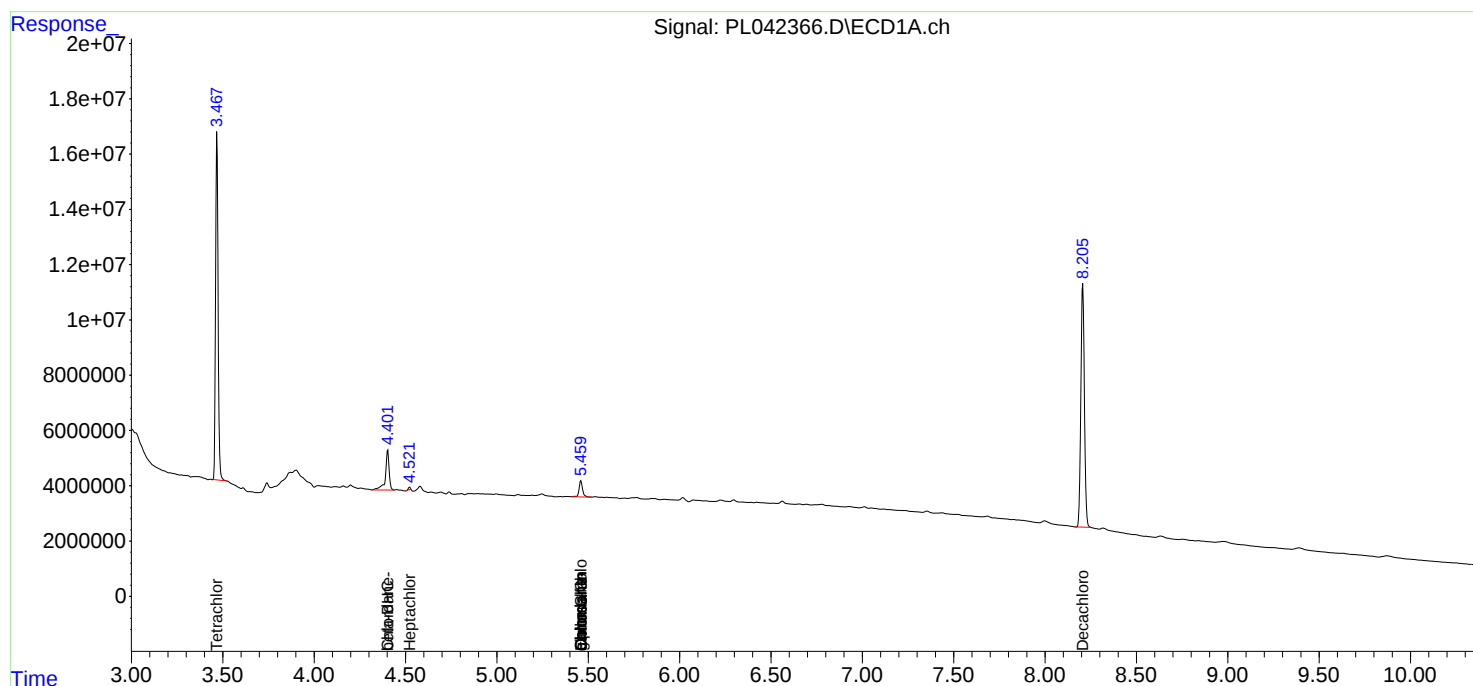


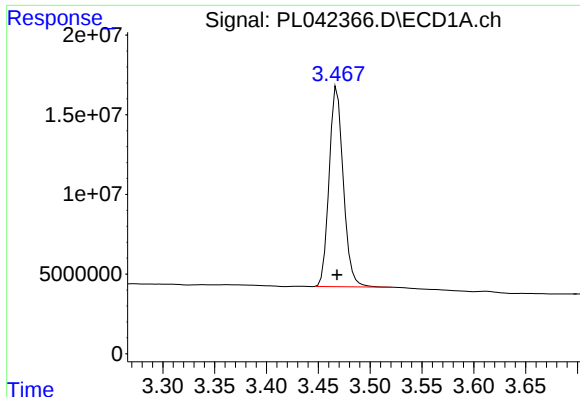

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 119104547
Conc: 20.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

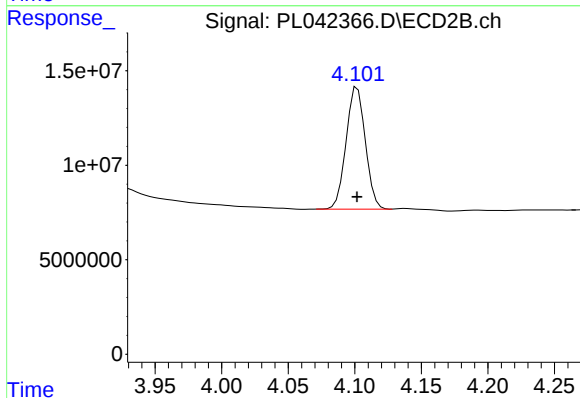


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 65026234
Conc: 22.61 ng/ml

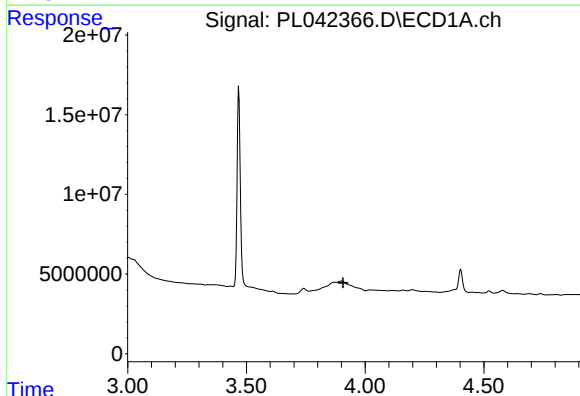


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

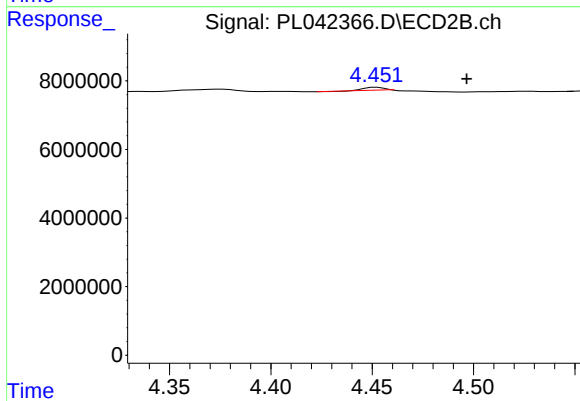

#2 alpha-BHC


R.T.: 4.452 min
Delta R.T.: -0.044 min
Response: 595859
Conc: 0.14 ng/ml

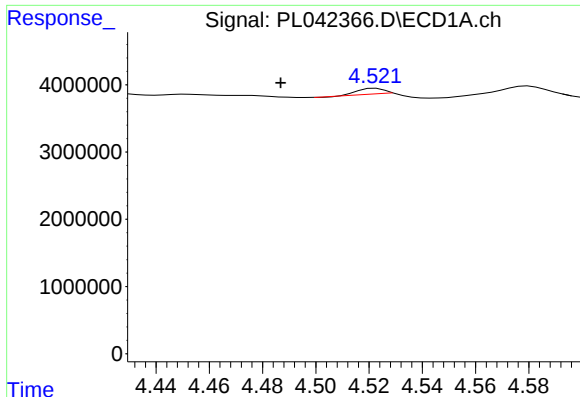

#4 Heptachlor


R.T.: 4.523 min
Delta R.T.: 0.036 min
Response: 646647
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

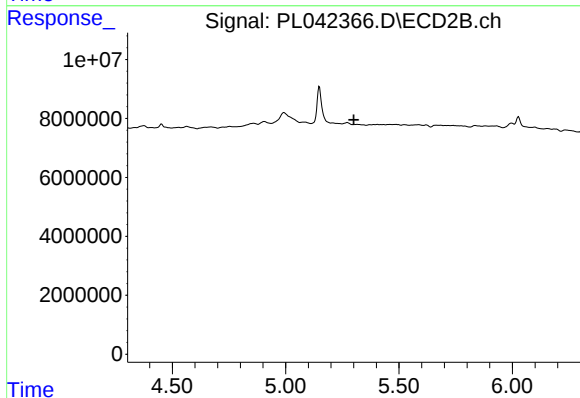


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.301 min
Response: 0
Conc: N.D.

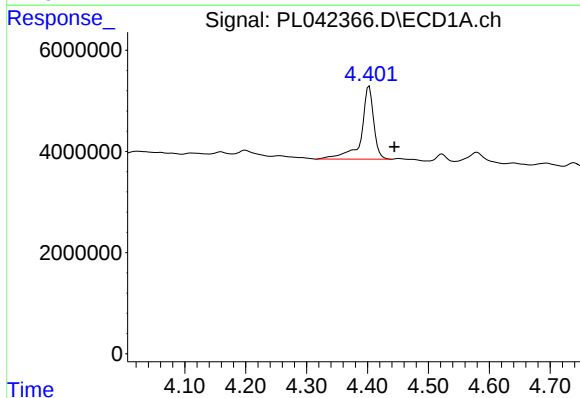


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: -0.041 min
Response: 20512940
Conc: 5.79 ng/ml

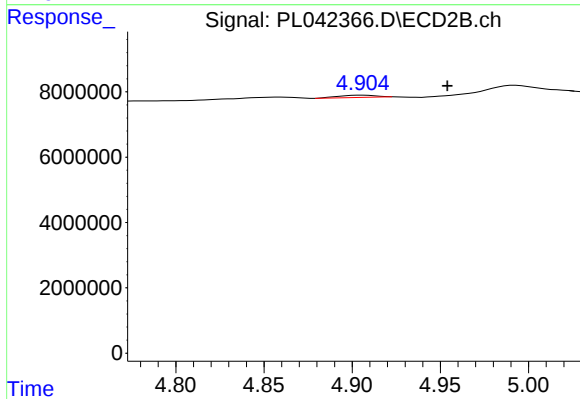

#6 beta-BHC


R.T.: 4.906 min
Delta R.T.: -0.048 min
Response: 1068459
Conc: 0.68 ng/ml

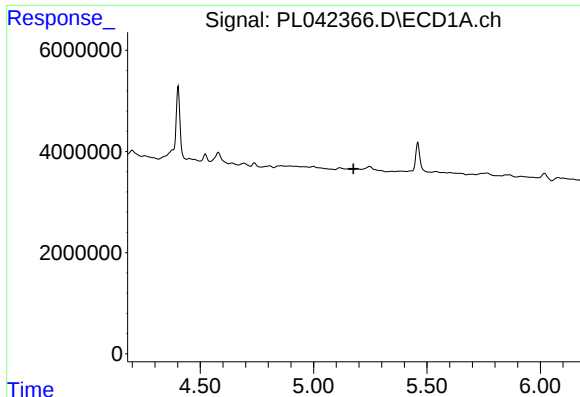

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

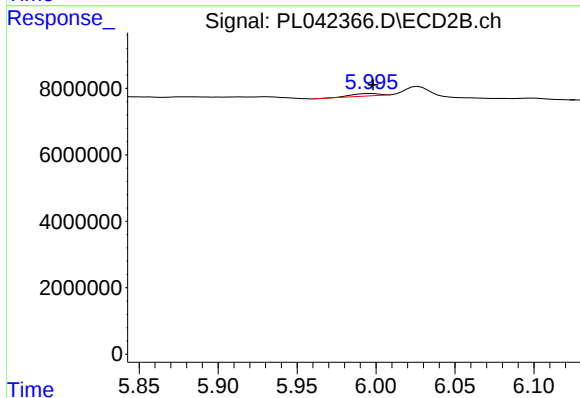


#8 Heptachlor epoxide

R.T.: 5.997 min
Delta R.T.: -0.001 min
Response: 865960
Conc: 0.24 ng/ml

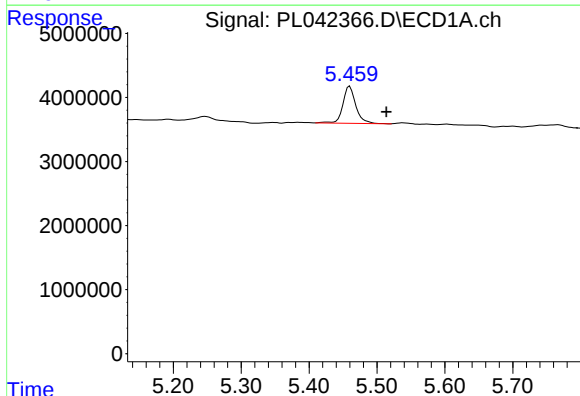


#9 Endosulfan I

R.T.: 5.460 min
Delta R.T.: -0.054 min
Response: 7651678
Conc: 1.11 ng/ml

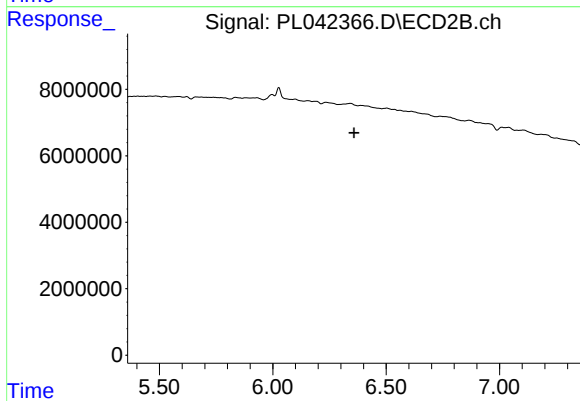

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

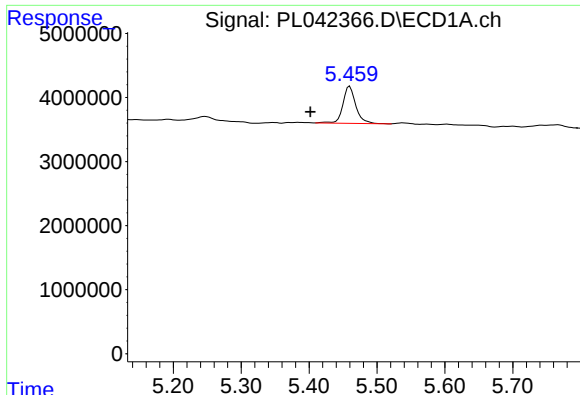

#10 gamma-Chlordane


R.T.: 5.460 min
Delta R.T.: 0.058 min
Response: 7651678
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

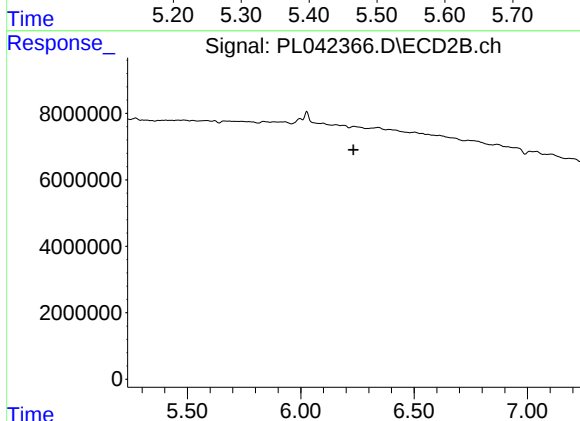


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

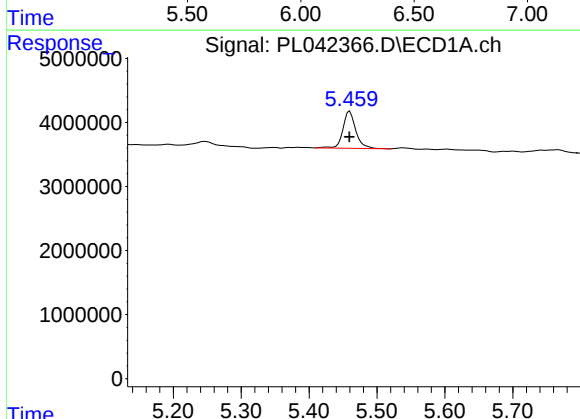


#11 alpha-Chlordane

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 7651678
Conc: 1.02 ng/ml

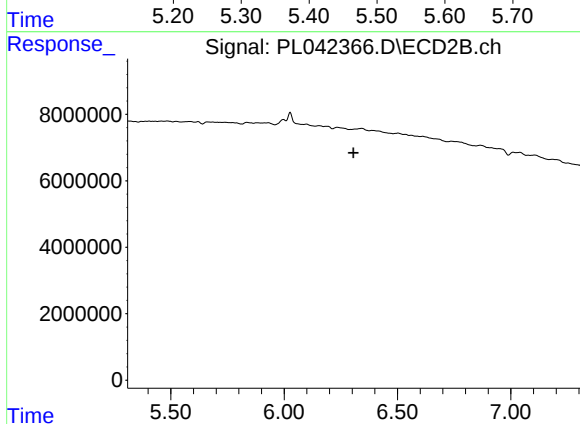

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

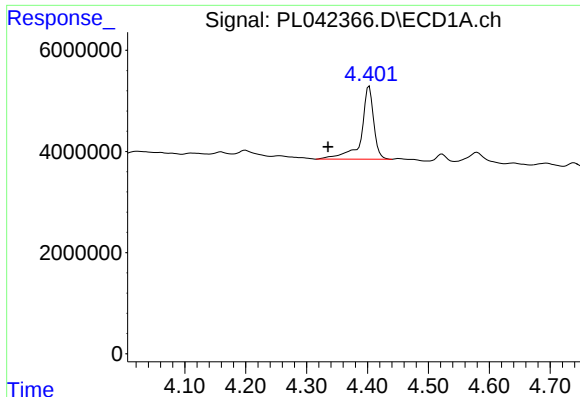

#23 Chlordane-1


R.T.: 4.403 min
Delta R.T.: 0.067 min
Response: 20512940
Conc: 74.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

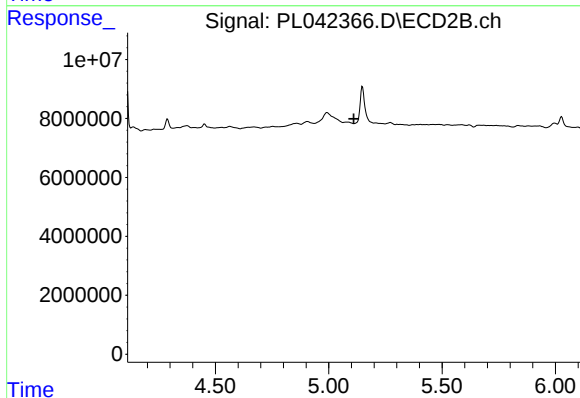


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

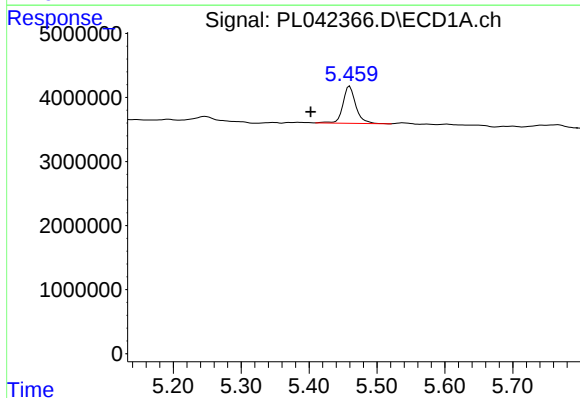


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.058 min
Response: 7651678
Conc: 8.73 ng/ml

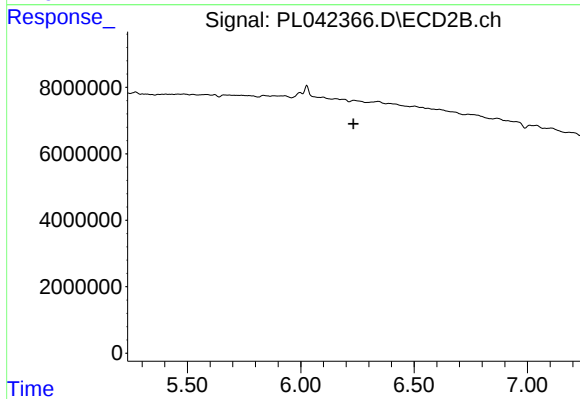

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

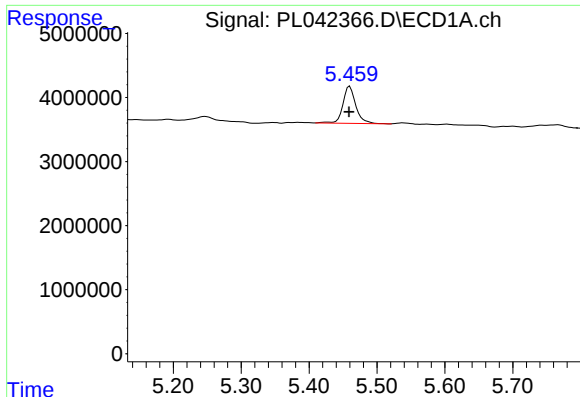

#26 Chlordane-4


R.T.: 5.460 min
Delta R.T.: 0.001 min
Response: 7651678
Conc: 10.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

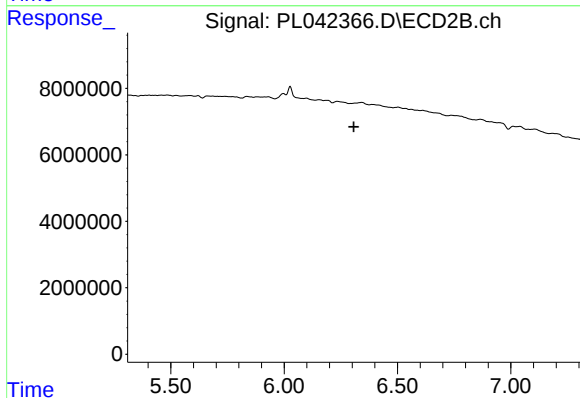


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

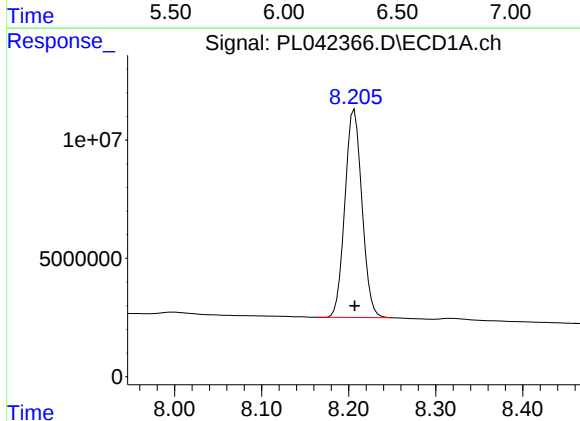

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 119771087
Conc: 19.00 ng/ml

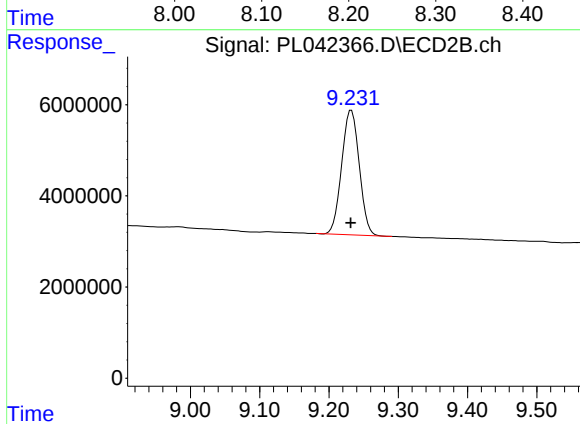

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 48130792
Conc: 19.96 ng/ml