

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
 Data File : PL042381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2018 22:24
 Operator : AJ\SJ
 Sample : PB114969BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:07:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	116.2E6	62824202	19.749	21.843
28)	SA Decachlor...	8.207	9.232	118.7E6	49704155	18.838	20.608
Target Compounds							
6)	B beta-BHC	4.402f	0.000	3600947	0	1.016	N.D. #
8)	B Heptachlo...	0.000	5.994	0	2433002	N.D.	0.679 #
10)	B gamma-Chl...	5.370	0.000	1556302	0	0.204	N.D. #
14)	MA Endrin	5.966f	0.000	1956122	0	0.299	N.D. #
17)	MA 4,4'-DDT	6.369	0.000	1507890	0	0.271	N.D. #
20)	A Methoxychlor	0.000	7.647f	0	2327893	N.D.	1.707 #
23)	Chlordane-1	4.366	0.000	1728253	0	6.251	N.D. #
25)	Chlordane-3	5.370	0.000	1556302	0	1.775	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
Data File : PL042381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2018 22:24
Operator : AJ\SJ
Sample : PB114969BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:07:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

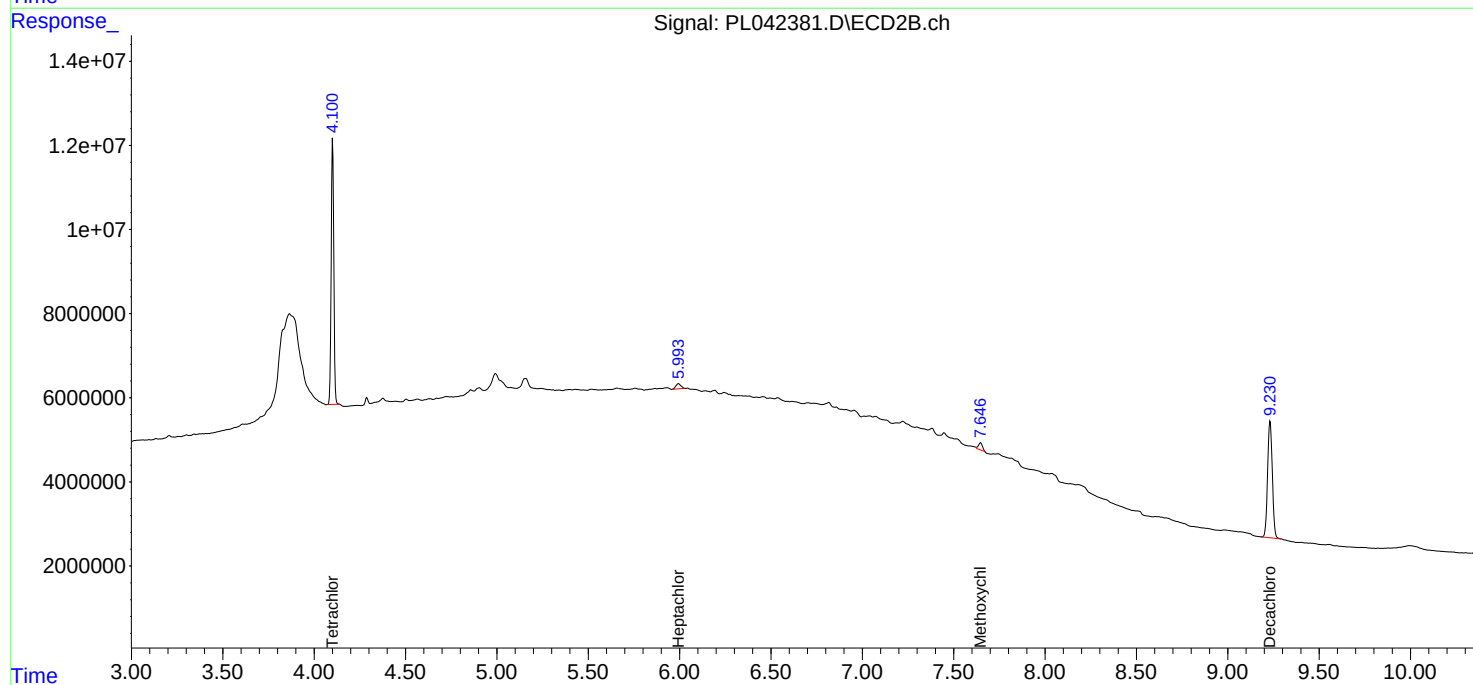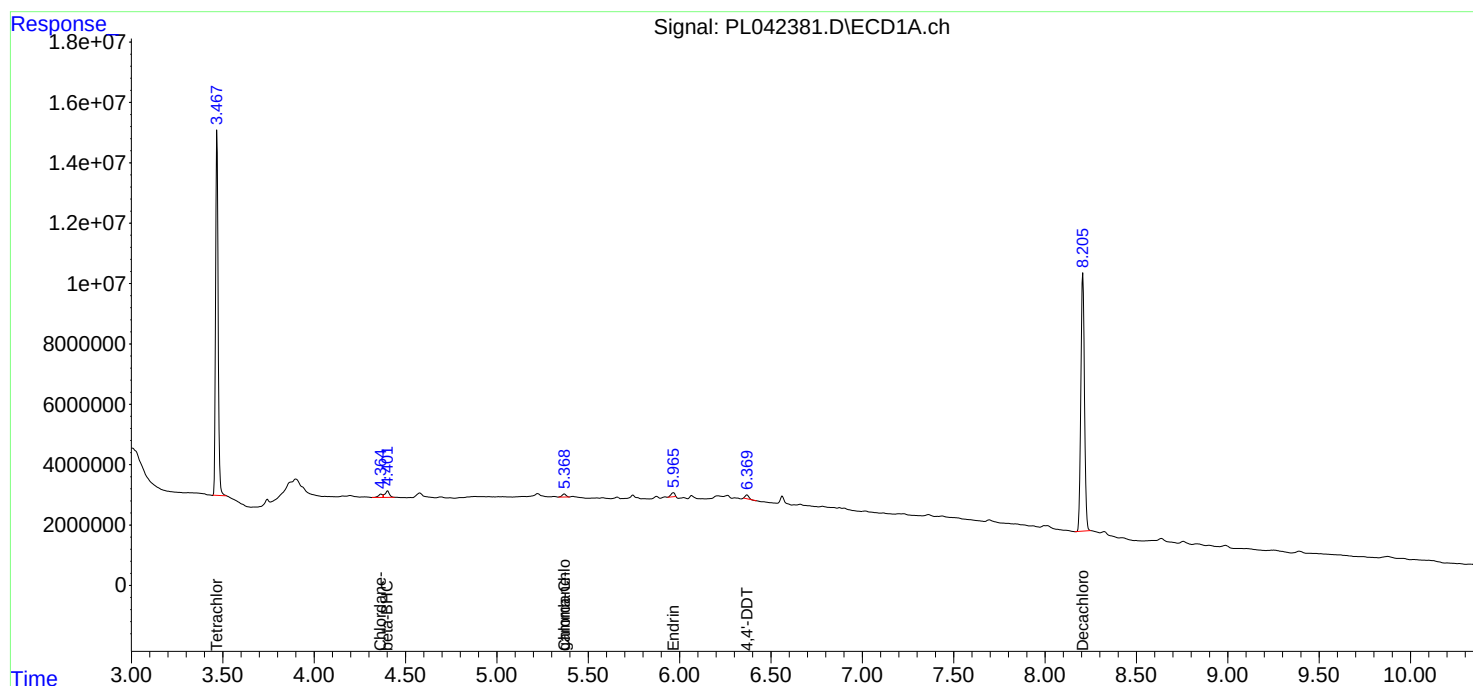


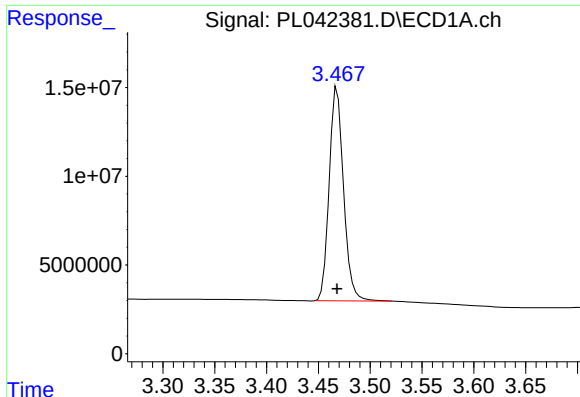

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 116195718
Conc: 19.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

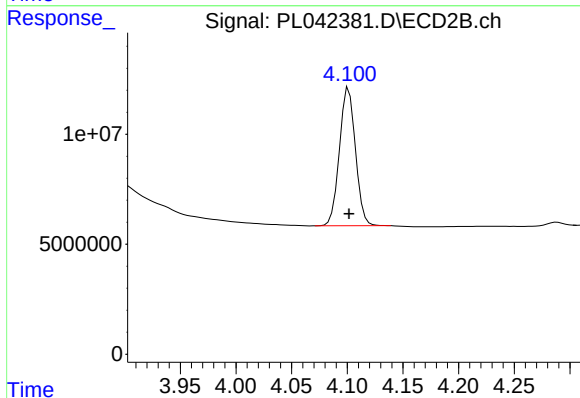


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 62824202
Conc: 21.84 ng/ml

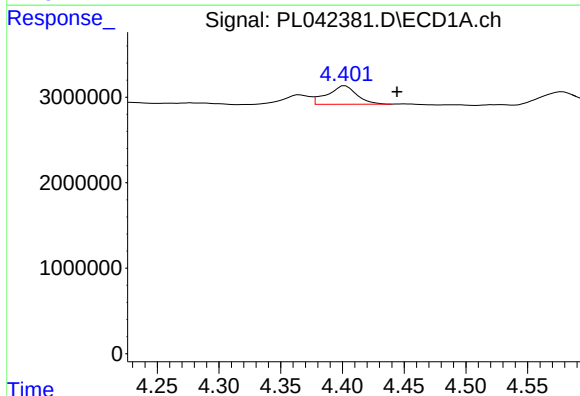


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 3600947
Conc: 1.02 ng/ml

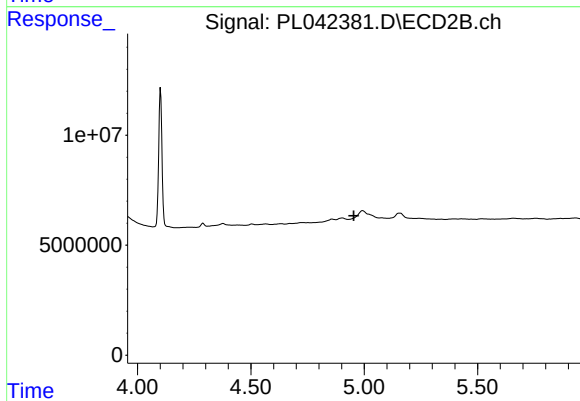

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.954 min
Response: 0
Conc: N.D.

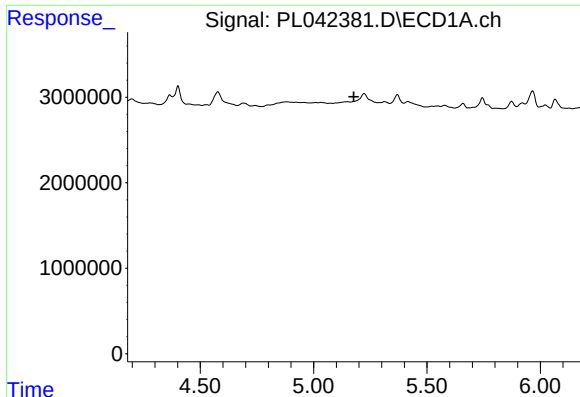

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

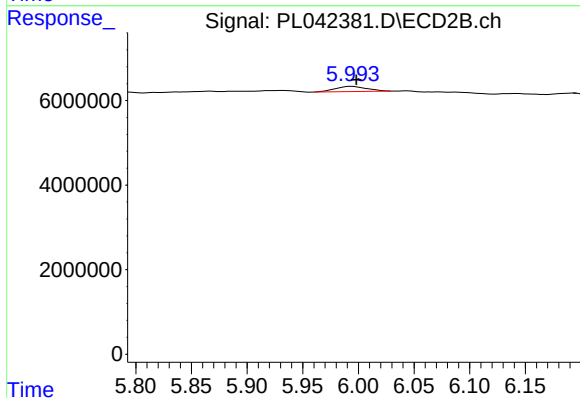


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.004 min
Response: 2433002
Conc: 0.68 ng/ml

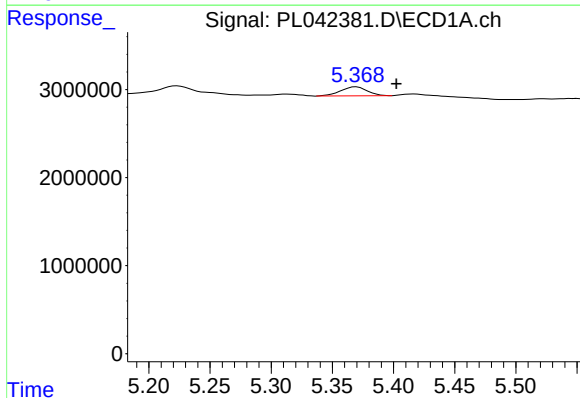


#10 gamma-Chlordane

R.T.: 5.370 min
Delta R.T.: -0.032 min
Response: 1556302
Conc: 0.20 ng/ml

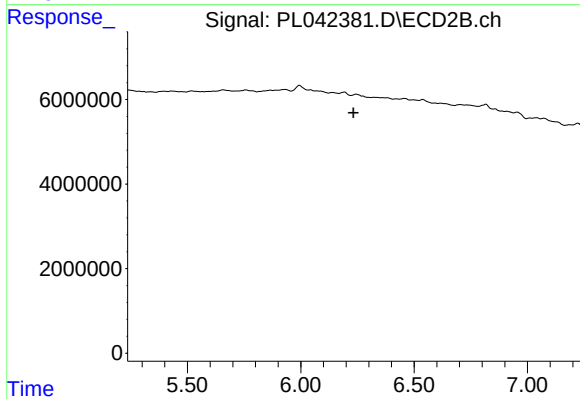

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.233 min
Response: 0
Conc: N.D.

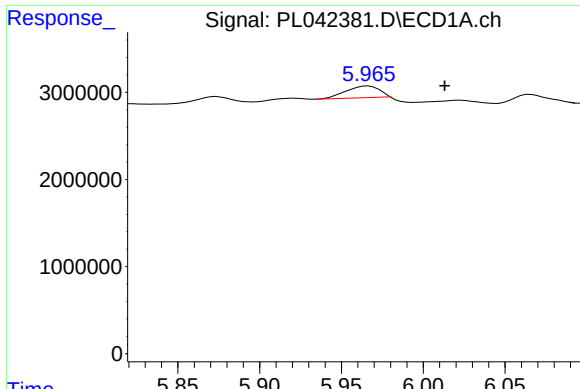

#14 Endrin


R.T.: 5.966 min
Delta R.T.: -0.047 min
Response: 1956122
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

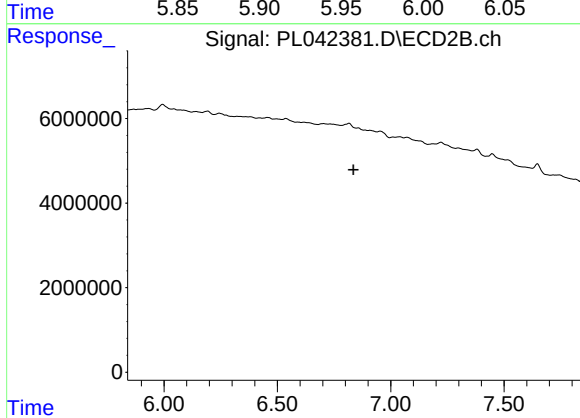


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

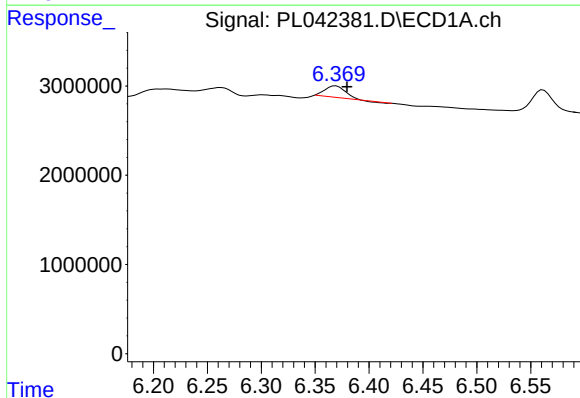


#17 4,4'-DDT

R.T.: 6.369 min
Delta R.T.: -0.011 min
Response: 1507890
Conc: 0.27 ng/ml

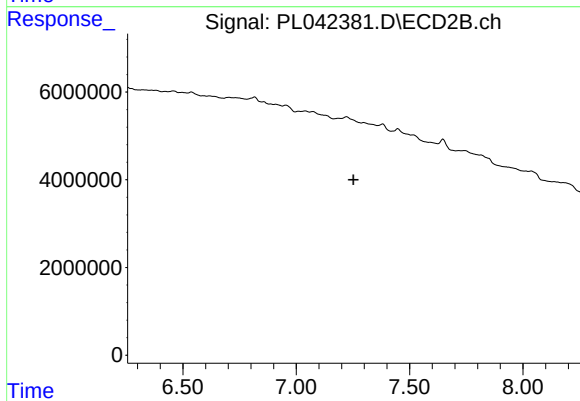

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

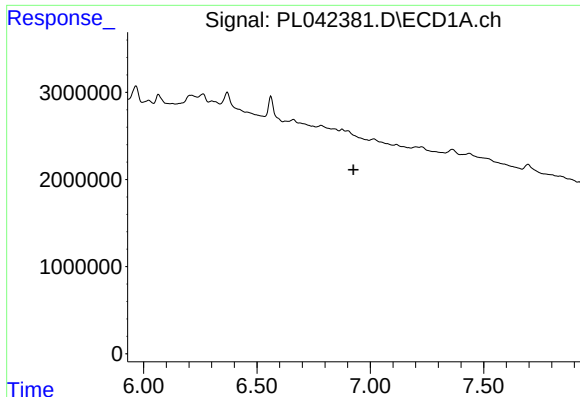

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.926 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

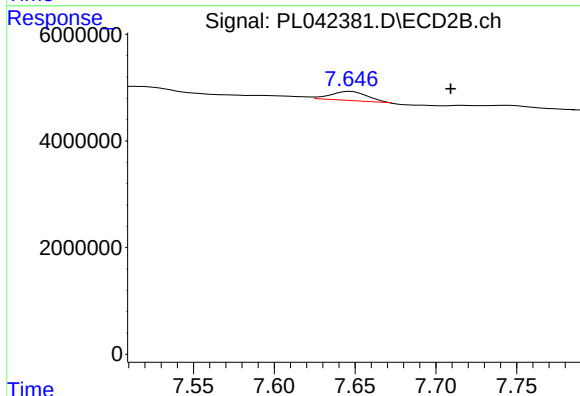


#20 Methoxychlor

R.T.: 7.647 min
Delta R.T.: -0.062 min
Response: 2327893
Conc: 1.71 ng/ml

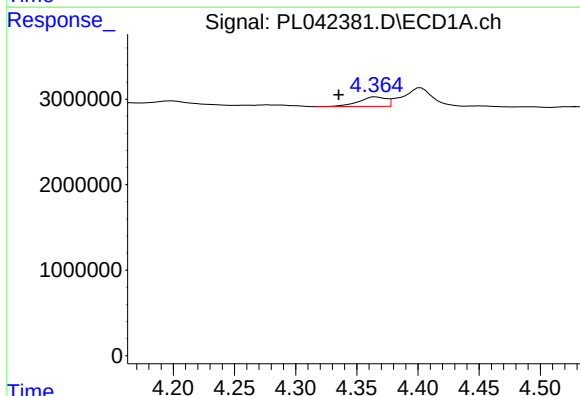


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.030 min
Response: 1728253
Conc: 6.25 ng/ml

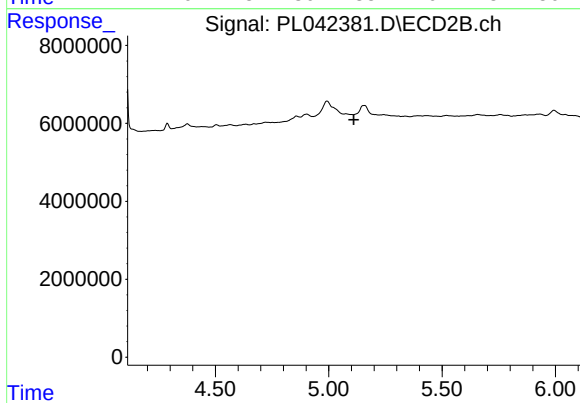

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.111 min
Response: 0
Conc: N.D.

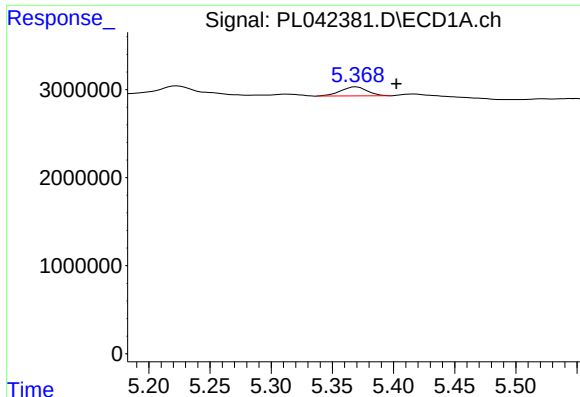

#25 Chlordane-3


R.T.: 5.370 min
Delta R.T.: -0.033 min
Response: 1556302
Conc: 1.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

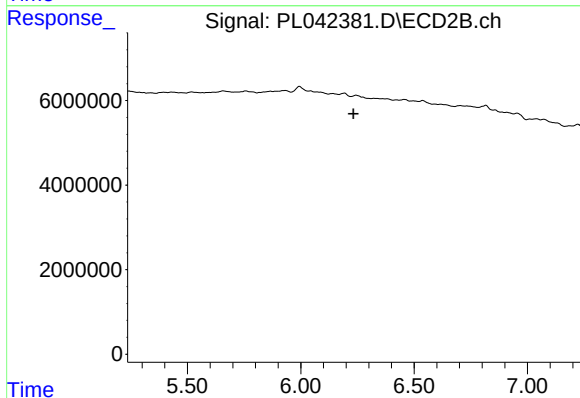


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

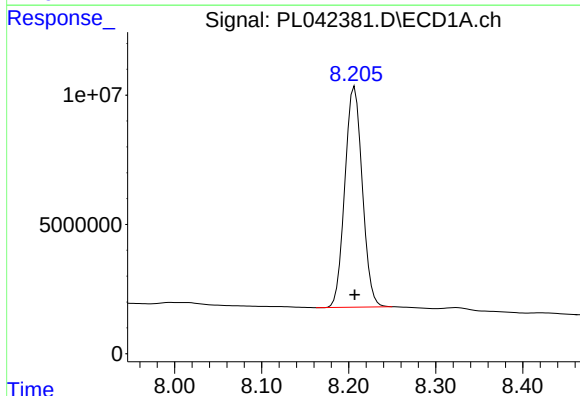

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 118718565
Conc: 18.84 ng/ml

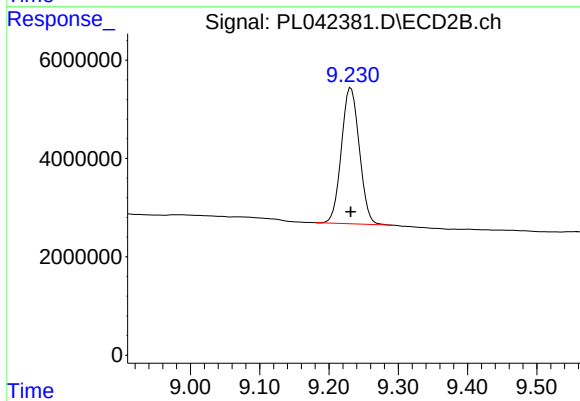

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 49704155
Conc: 20.61 ng/ml