

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
 Data File : PL042393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 01:14
 Operator : AJ\SJ
 Sample : J6006-06
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:36:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	114.7E6	62849987	19.491	21.852
28)	SA Decachlor...	8.206	9.231	125.5E6	51033739	19.921	21.160
Target Compounds							
2)	A alpha-BHC	3.905	0.000	4165826	0	0.462	N.D. #
3)	MA gamma-BHC...	4.155f	0.000	1414118	0	0.172	N.D. #
4)	MA Heptachlor	4.449f	0.000	4305829	0	0.495	N.D. #
6)	B beta-BHC	4.449	4.950	4305829	680631	1.215	0.431 #
8)	B Heptachlo...	5.232f	5.995	3677787	4051663	0.485	1.130 #
9)	A Endosulfan I	0.000	6.377	0	2853539	N.D.	0.904 #
13)	MA Dieldrin	5.751	0.000	1293893	0	0.176	N.D. #
15)	B Endosulfa...	6.300	0.000	1944760	0	0.311	N.D. #
23)	Chlordane-1	4.341	0.000	1757887	0	6.358	N.D. #
24)	Chlordane-2	0.000	5.523	0	1506458	N.D.	10.803 #
26)	Chlordane-4	0.000	6.377	0	2853539	N.D.	5.215 #
27)	Chlordane-5	6.300	0.000	1944760	0	6.527	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
Data File : PL042393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 01:14
Operator : AJ\SJ
Sample : J6006-06
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:36:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

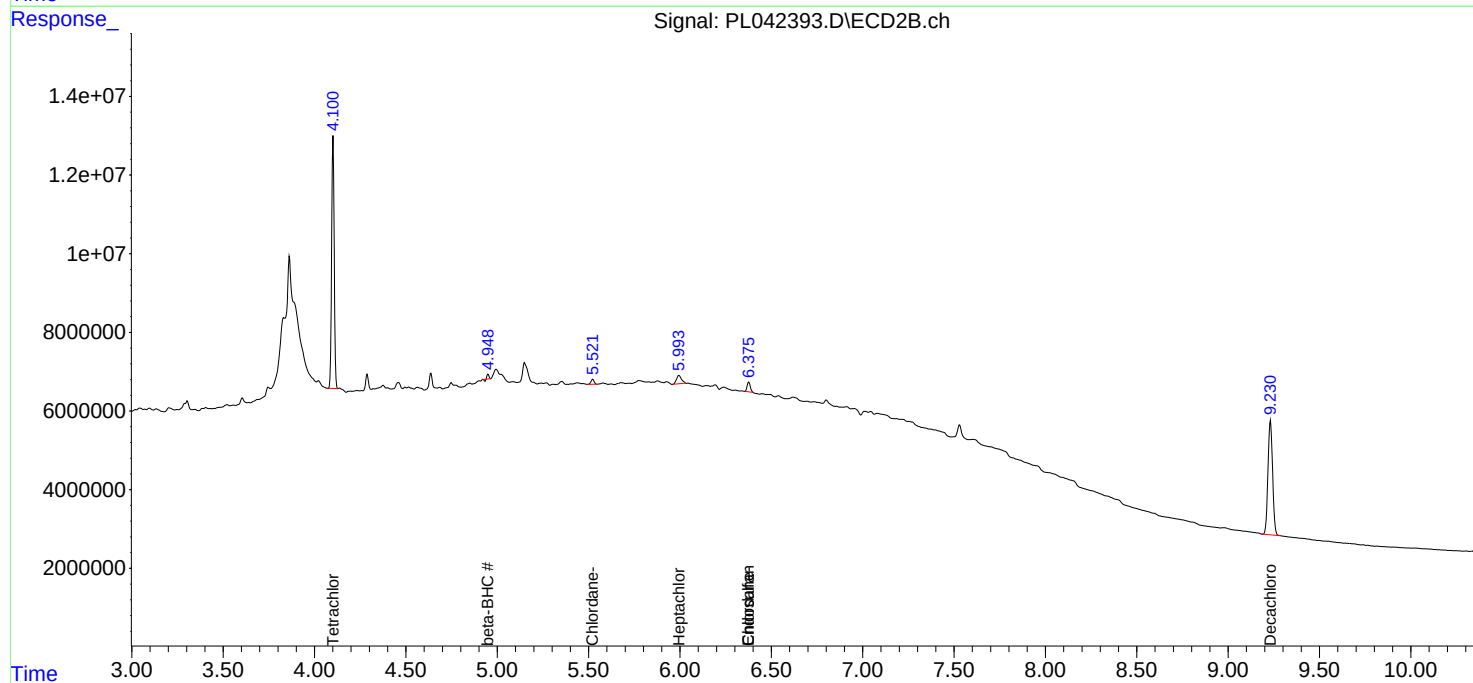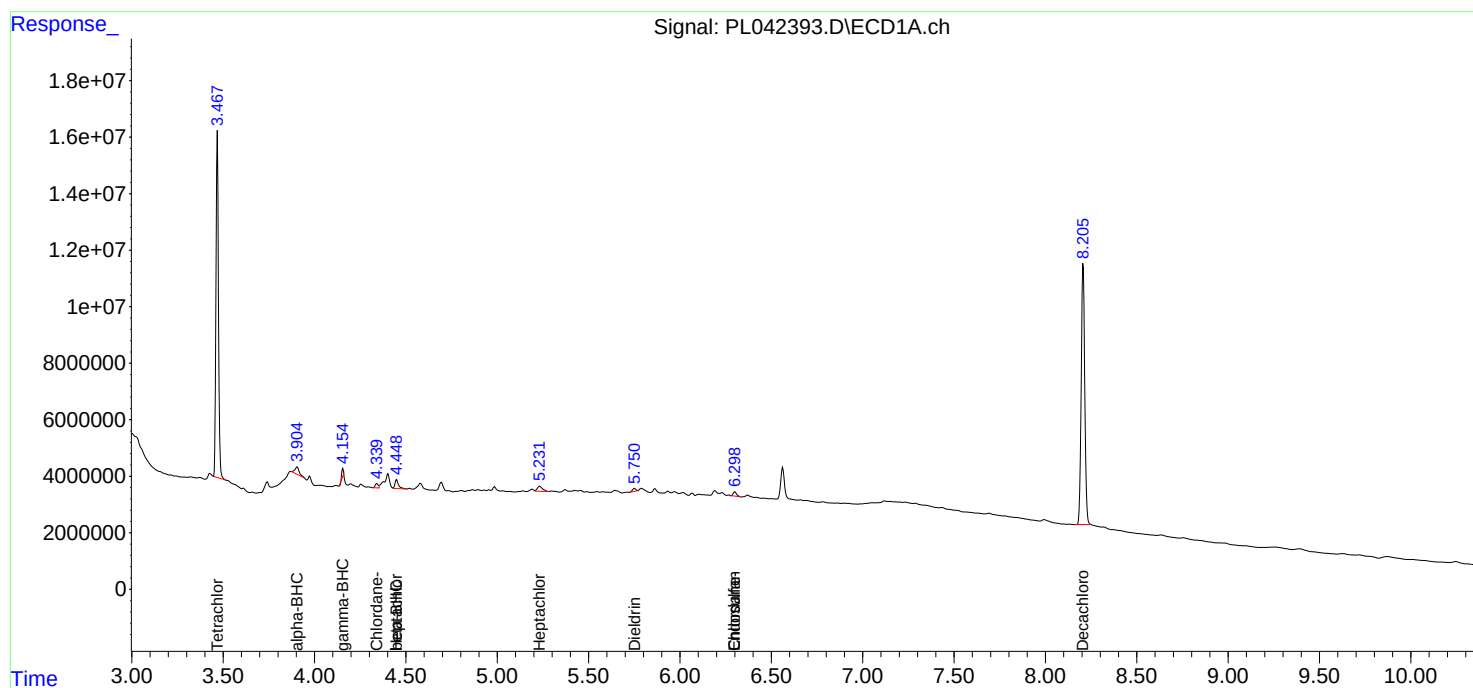


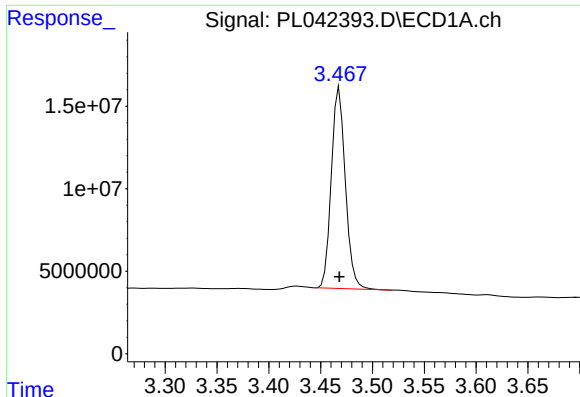

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 114677738
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

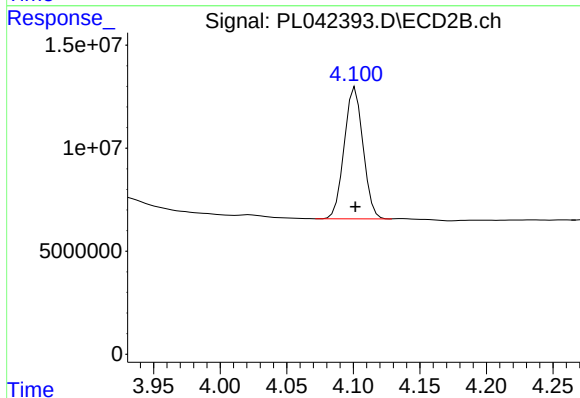


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 62849987
Conc: 21.85 ng/ml

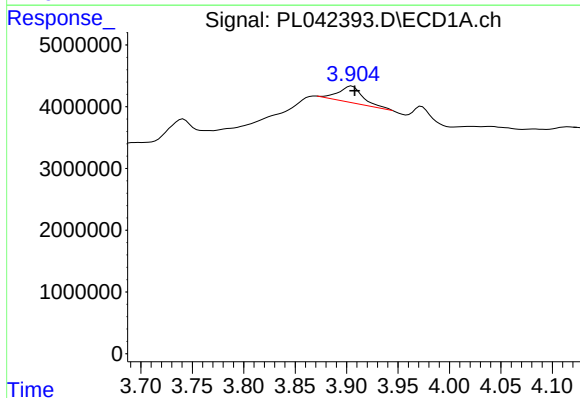


#2 alpha-BHC

R.T.: 3.905 min
Delta R.T.: -0.003 min
Response: 4165826
Conc: 0.46 ng/ml

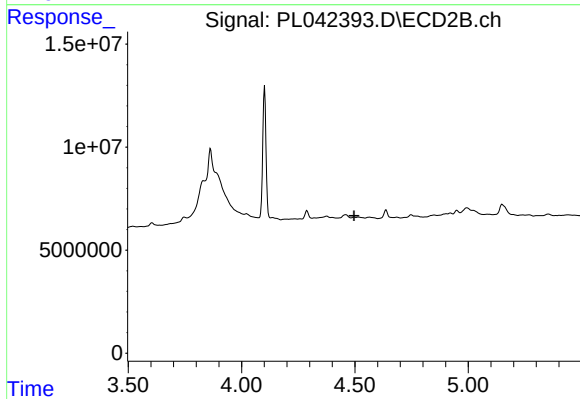

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

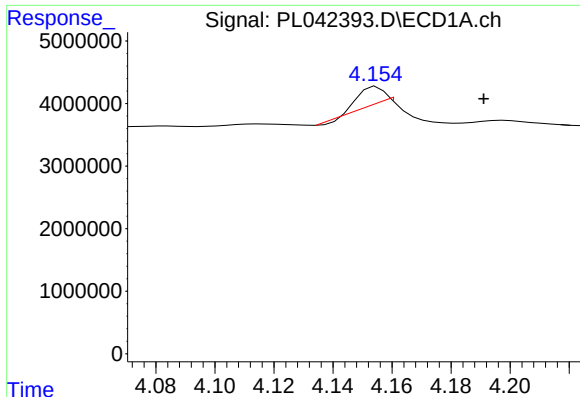

#3 gamma-BHC (Lindane)


R.T.: 4.155 min
Delta R.T.: -0.036 min
Response: 1414118
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

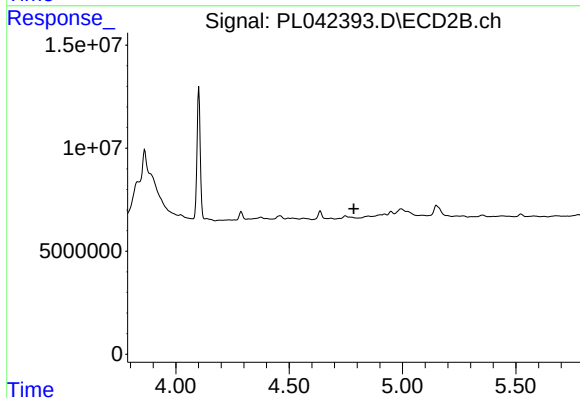


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

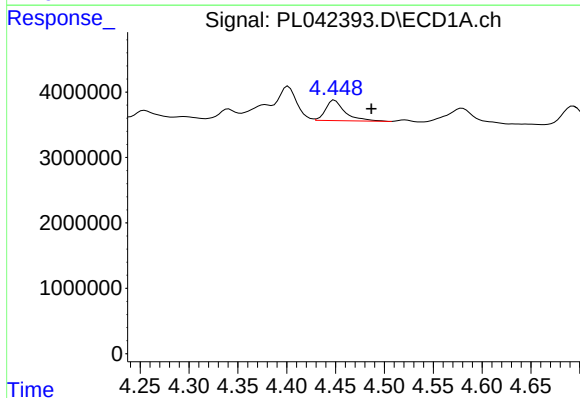


#4 Heptachlor

R.T.: 4.449 min
Delta R.T.: -0.038 min
Response: 4305829
Conc: 0.49 ng/ml

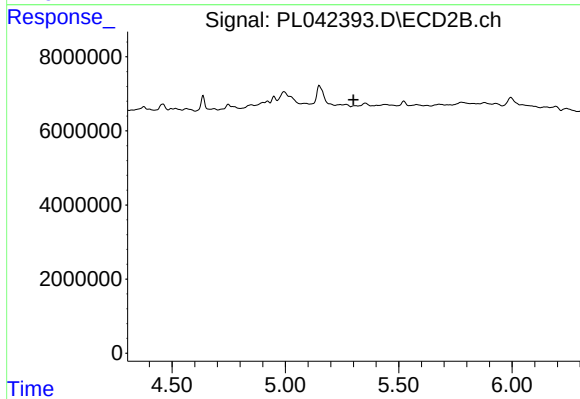

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.301 min
Response: 0
Conc: N.D.

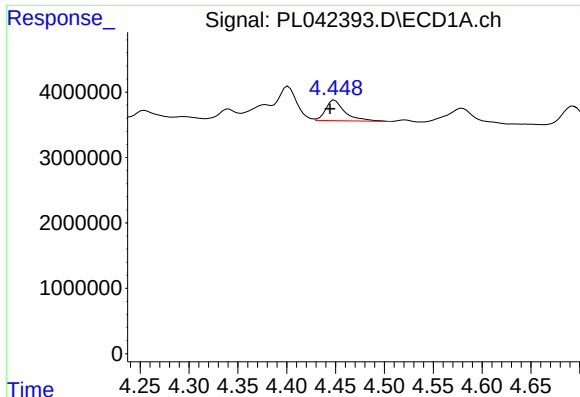

#6 beta-BHC


R.T.: 4.449 min
Delta R.T.: 0.005 min
Response: 4305829
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

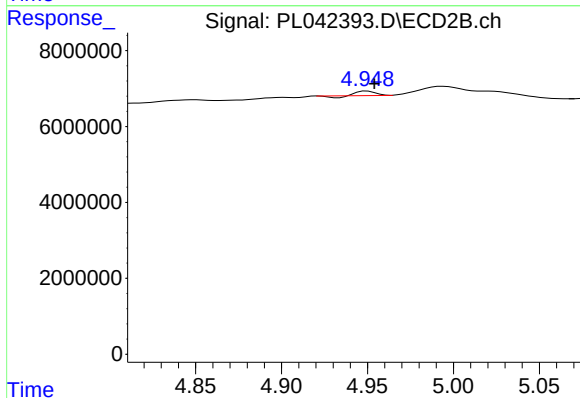


#6 beta-BHC

R.T.: 4.950 min
Delta R.T.: -0.004 min
Response: 680631
Conc: 0.43 ng/ml

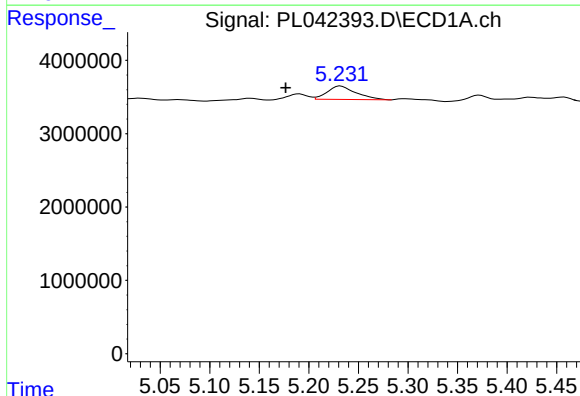


#8 Heptachlor epoxide

R.T.: 5.232 min
Delta R.T.: 0.055 min
Response: 3677787
Conc: 0.49 ng/ml

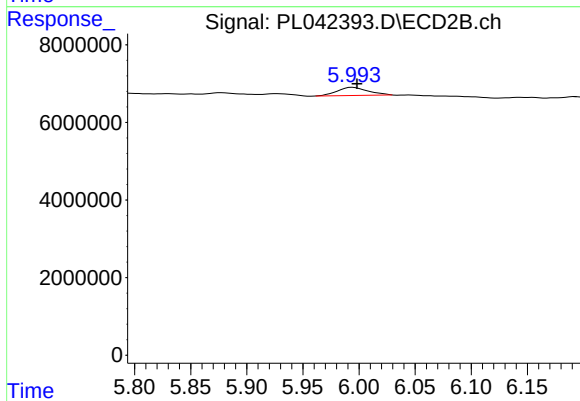

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.004 min
Response: 4051663
Conc: 1.13 ng/ml

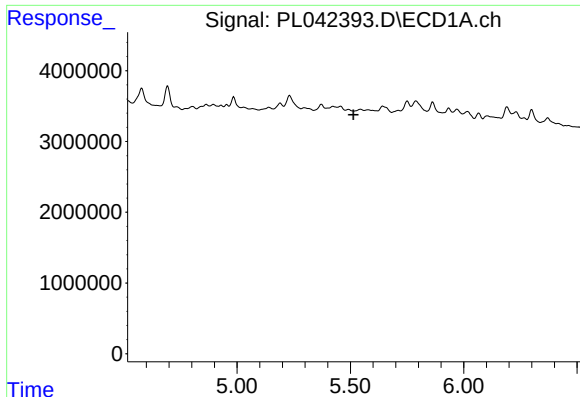

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.514 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

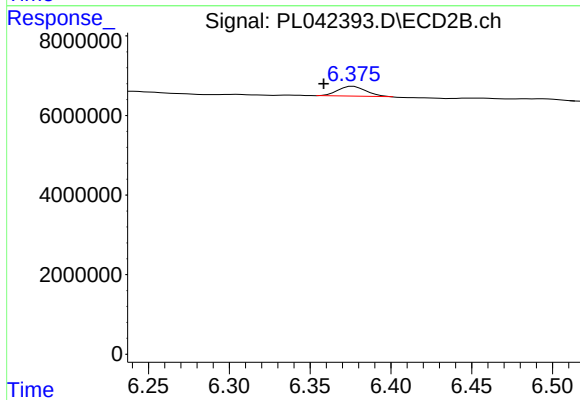


#9 Endosulfan I

R.T.: 6.377 min
Delta R.T.: 0.018 min
Response: 2853539
Conc: 0.90 ng/ml

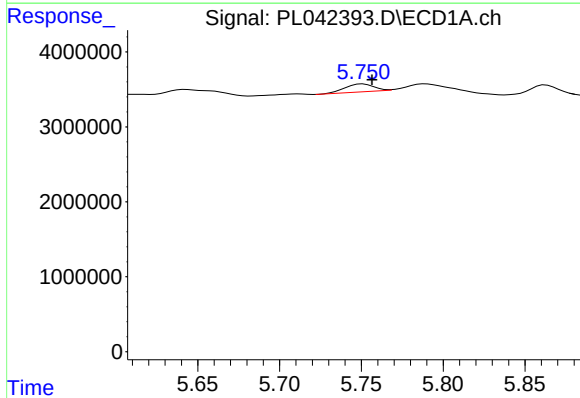


#13 Dieldrin

R.T.: 5.751 min
Delta R.T.: -0.005 min
Response: 1293893
Conc: 0.18 ng/ml

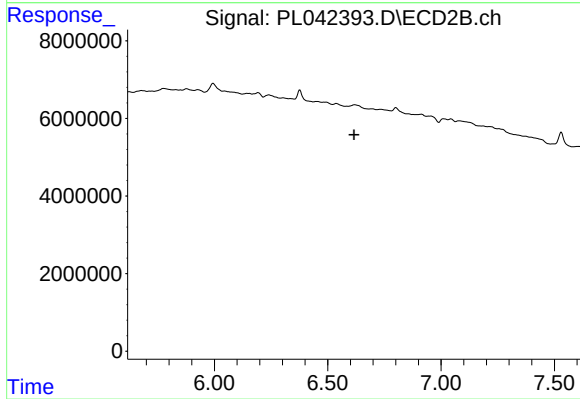

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

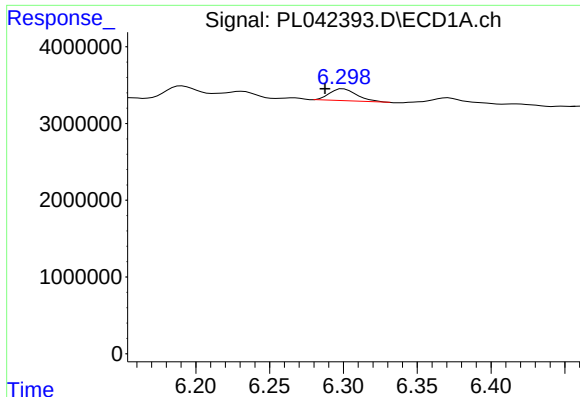

#15 Endosulfan II


R.T.: 6.300 min
Delta R.T.: 0.012 min
Response: 1944760
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

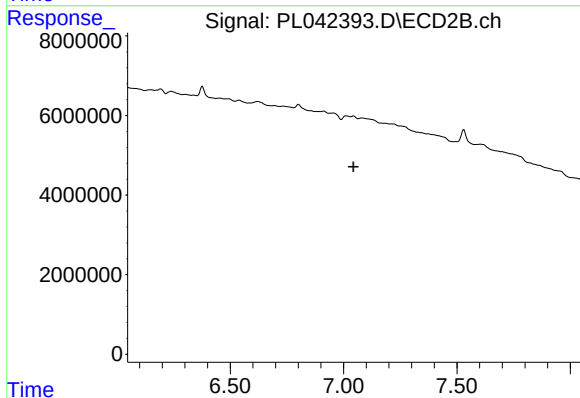


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

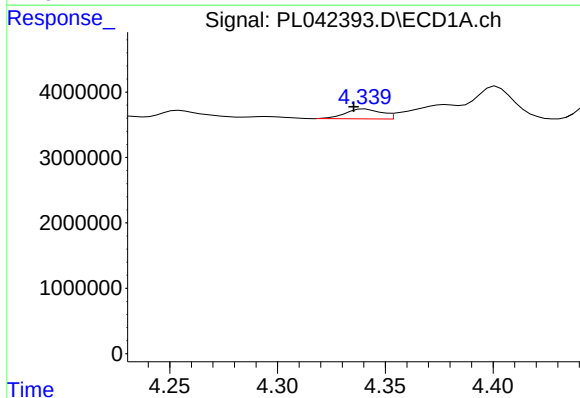


#23 Chlordane-1

R.T.: 4.341 min
Delta R.T.: 0.005 min
Response: 1757887
Conc: 6.36 ng/ml

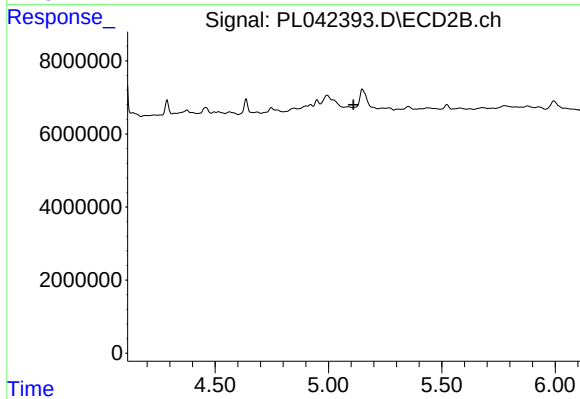

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

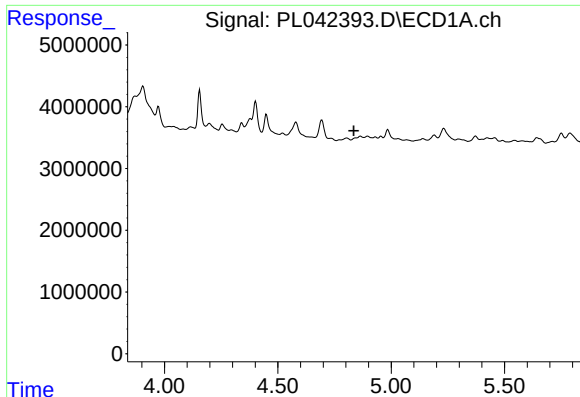

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

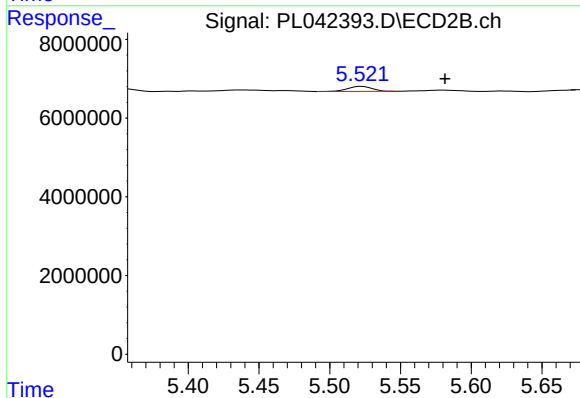


#24 Chlordane-2

R.T.: 5.523 min
Delta R.T.: -0.059 min
Response: 1506458
Conc: 10.80 ng/ml

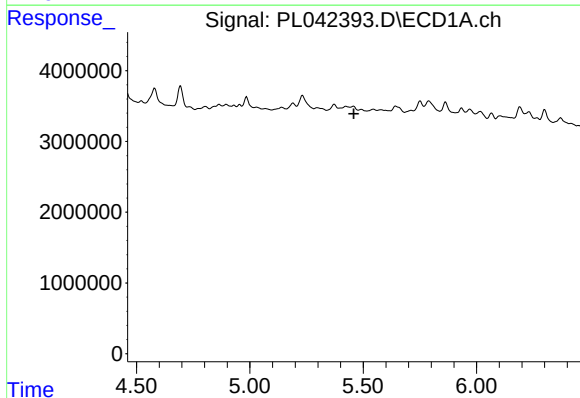


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

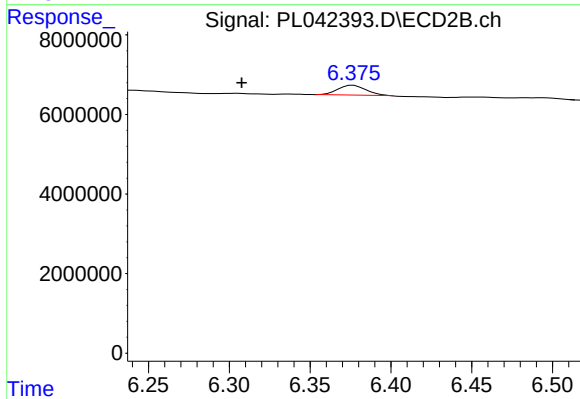

#26 Chlordane-4


R.T.: 6.377 min
Delta R.T.: 0.069 min
Response: 2853539
Conc: 5.22 ng/ml

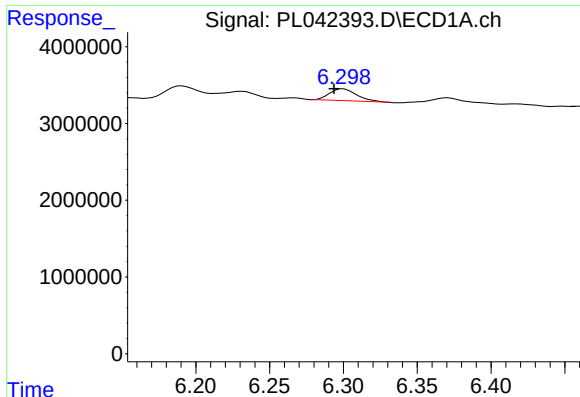

#27 Chlordane-5


R.T.: 6.300 min
Delta R.T.: 0.006 min
Response: 1944760
Conc: 6.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

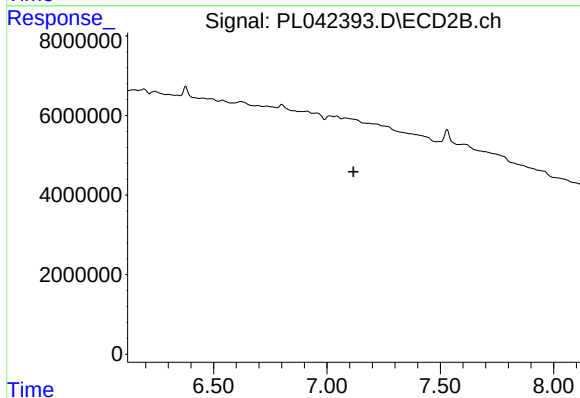


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

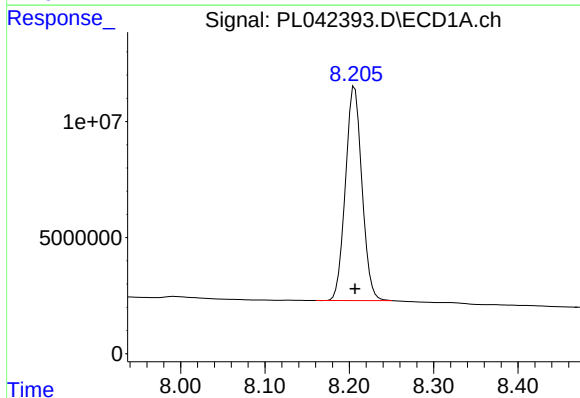

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 125543339
Conc: 19.92 ng/ml

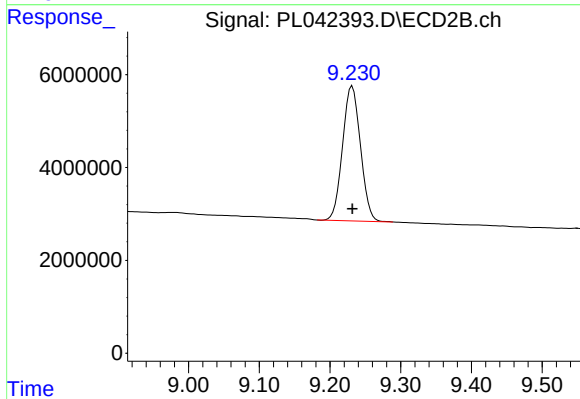

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 51033739
Conc: 21.16 ng/ml