

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
 Data File : PL042394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 01:28
 Operator : AJ\SJ
 Sample : J6010-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 02:38:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	115.3E6	63108928	19.591	21.942
28)	SA Decachlor...	8.206	9.232	116.6E6	46740149	18.504	19.379
Target Compounds							
2)	A alpha-BHC	3.900	4.453f	3738537	606499	0.414	0.142 #
3)	MA gamma-BHC...	0.000	4.745f	0	2658417	N.D.	0.673 #
6)	B beta-BHC	4.402f	0.000	11776553	0	3.324	N.D. #
8)	B Heptachlo...	5.228f	5.996	2306454	4276906	0.304	1.193 #
10)	B gamma-Chl...	5.424	0.000	1649592	0	0.216	N.D. #
11)	B alpha-Chl...	5.424f	0.000	1649592	0	0.220	N.D. #
23)	Chlordane-1	4.402	0.000	11776553	0	42.596	N.D. #
25)	Chlordane-3	5.424	0.000	1649592	0	1.882	N.D. #
26)	Chlordane-4	5.424	0.000	1649592	0	2.174	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
Data File : PL042394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 01:28
Operator : AJ\SJ
Sample : J6010-03
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 02:38:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

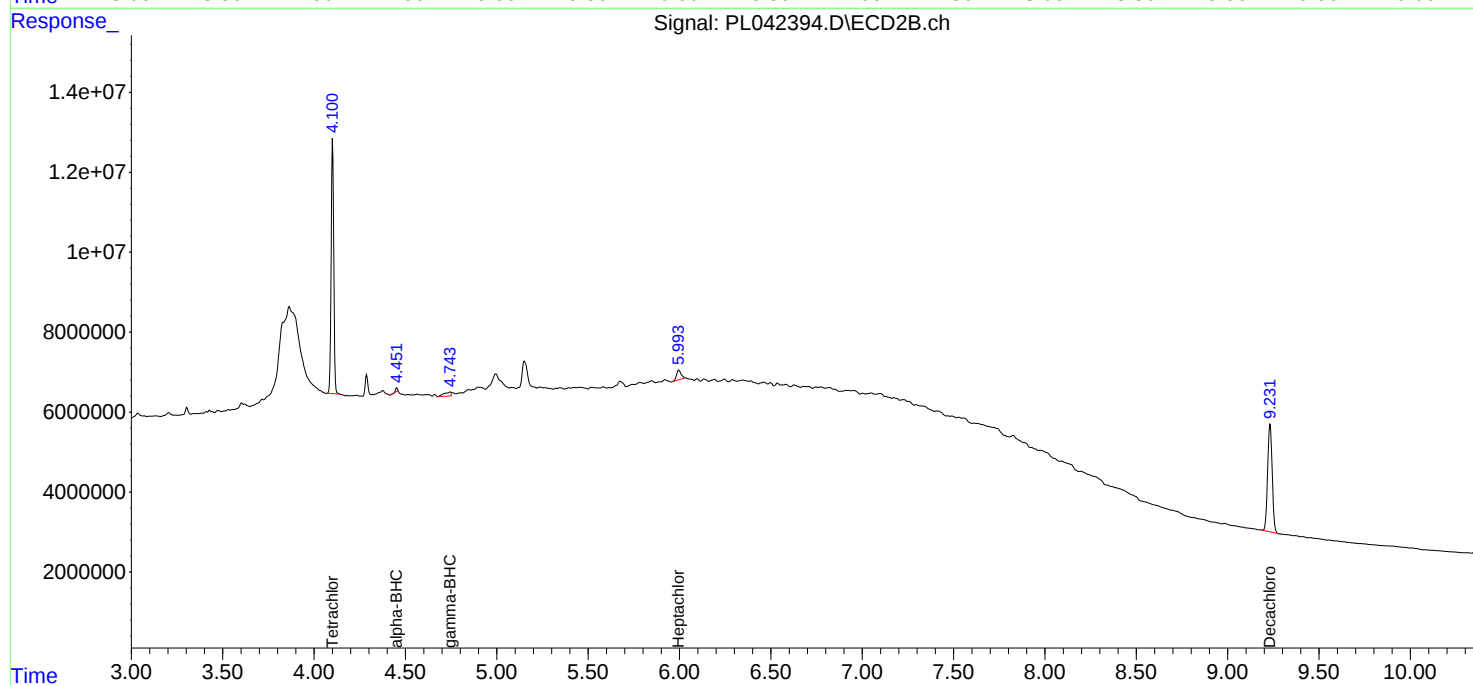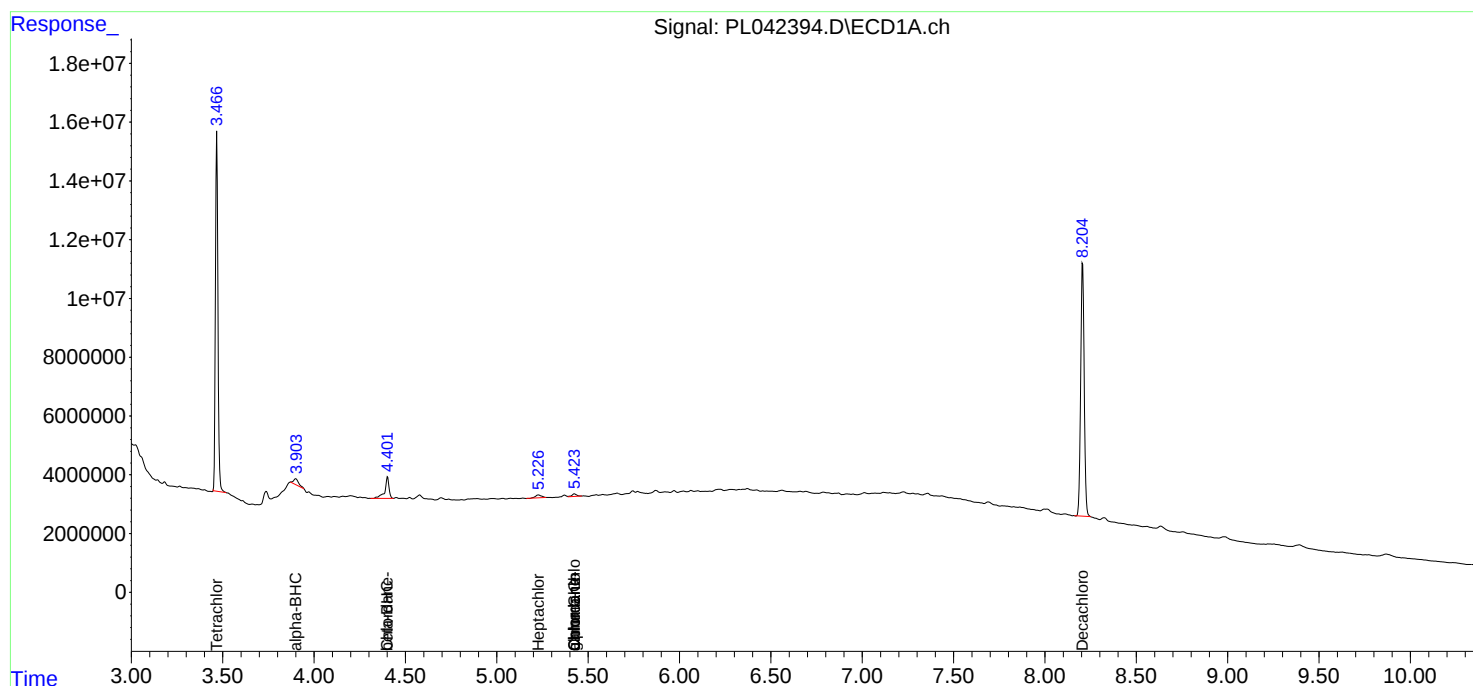


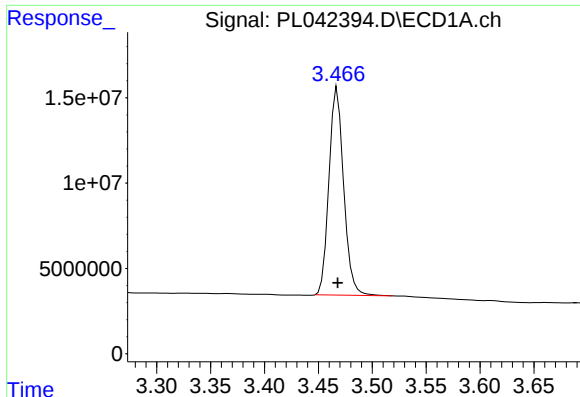

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 115263805
Conc: 19.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

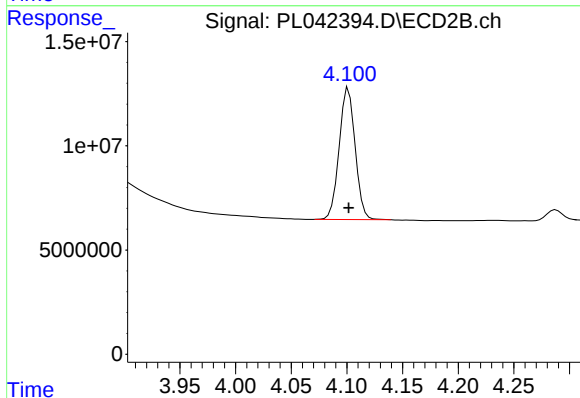


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 63108928
Conc: 21.94 ng/ml

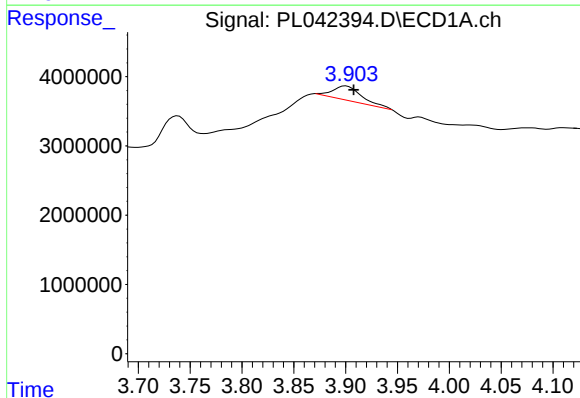


#2 alpha-BHC

R.T.: 3.900 min
Delta R.T.: -0.007 min
Response: 3738537
Conc: 0.41 ng/ml

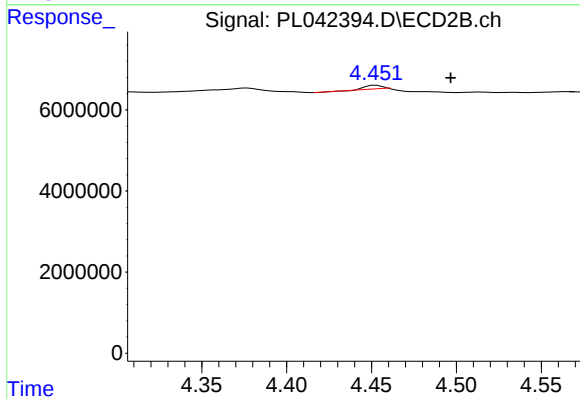

#2 alpha-BHC


R.T.: 4.453 min
Delta R.T.: -0.044 min
Response: 606499
Conc: 0.14 ng/ml

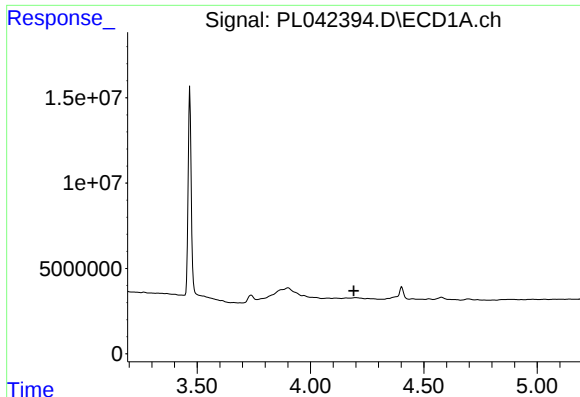

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

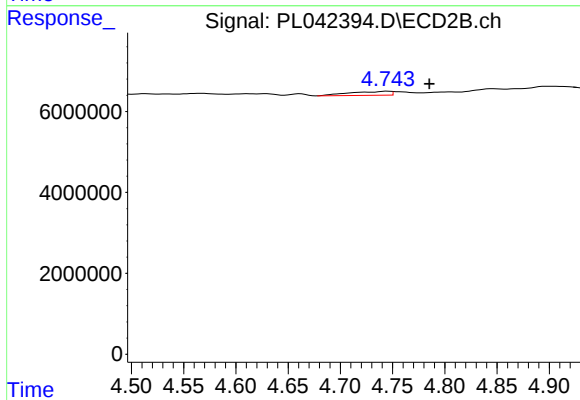


#3 gamma-BHC (Lindane)

R.T.: 4.745 min
Delta R.T.: -0.040 min
Response: 2658417
Conc: 0.67 ng/ml

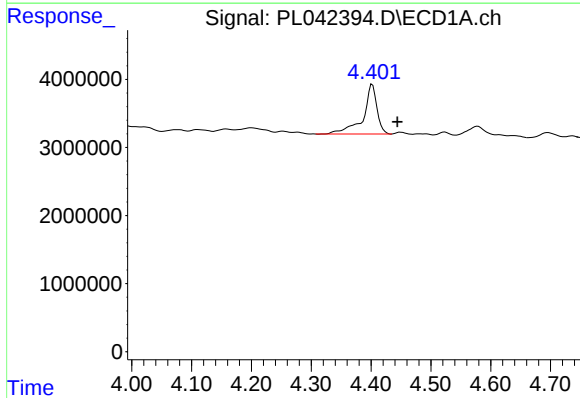


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 11776553
Conc: 3.32 ng/ml

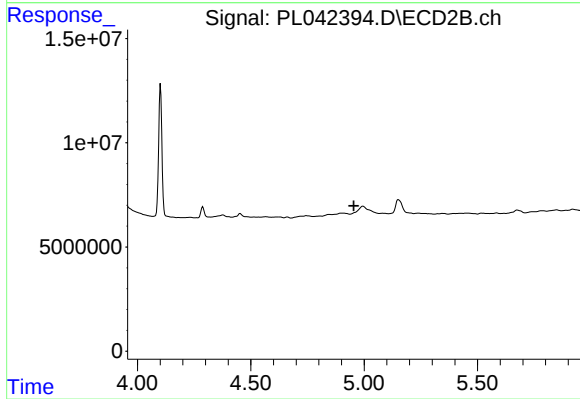

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.954 min
Response: 0
Conc: N.D.

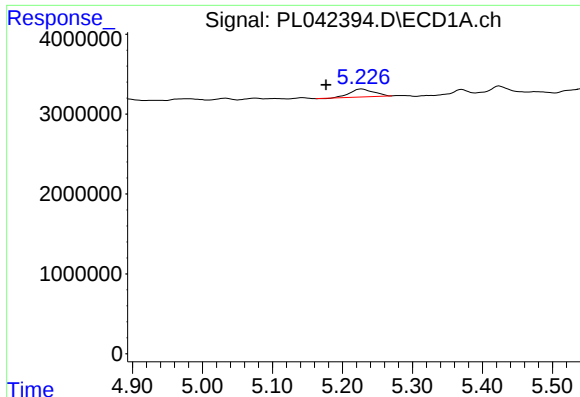

#8 Heptachlor epoxide


R.T.: 5.228 min
Delta R.T.: 0.051 min
Response: 2306454
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

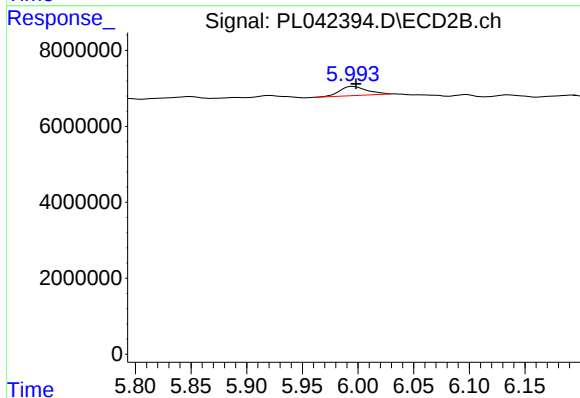


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: -0.003 min
Response: 4276906
Conc: 1.19 ng/ml

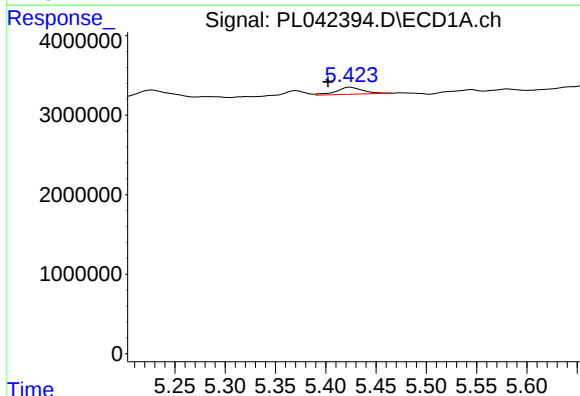


#10 gamma-Chlordane

R.T.: 5.424 min
Delta R.T.: 0.022 min
Response: 1649592
Conc: 0.22 ng/ml

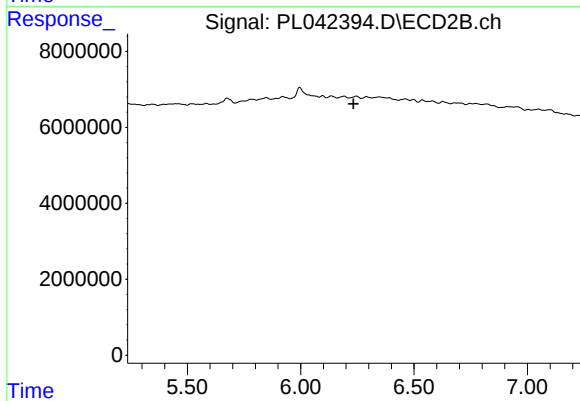

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.233 min
Response: 0
Conc: N.D.

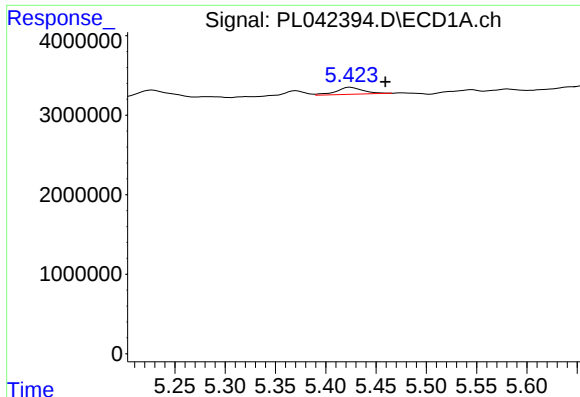

#11 alpha-Chlordane


R.T.: 5.424 min
Delta R.T.: -0.035 min
Response: 1649592
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

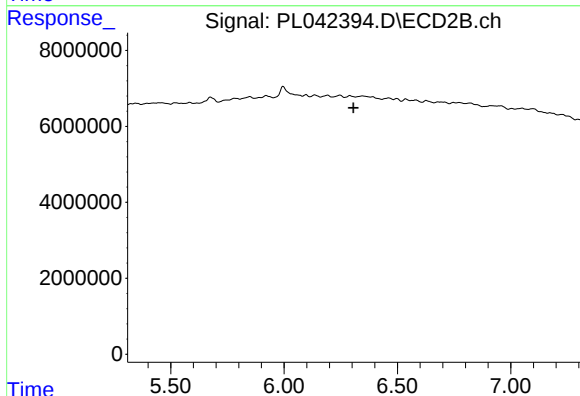


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

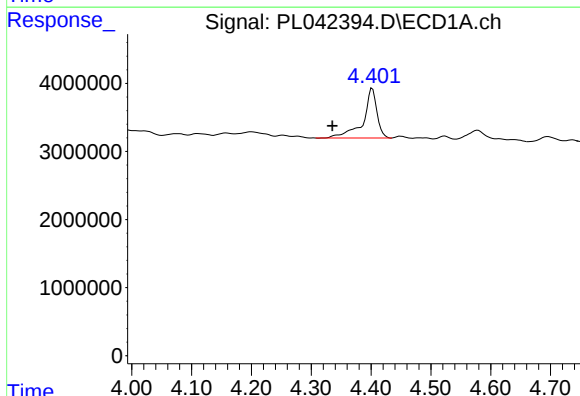


#23 Chlordane-1

R.T.: 4.402 min
Delta R.T.: 0.067 min
Response: 11776553
Conc: 42.60 ng/ml

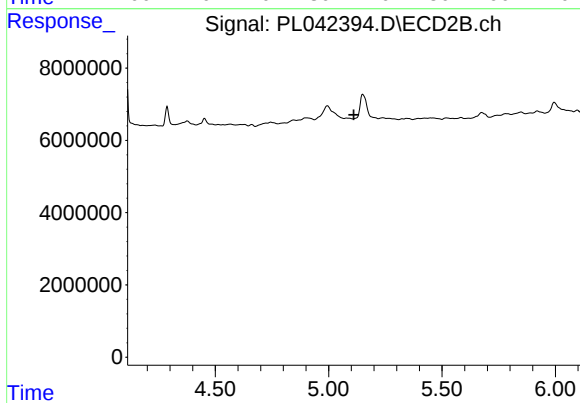

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

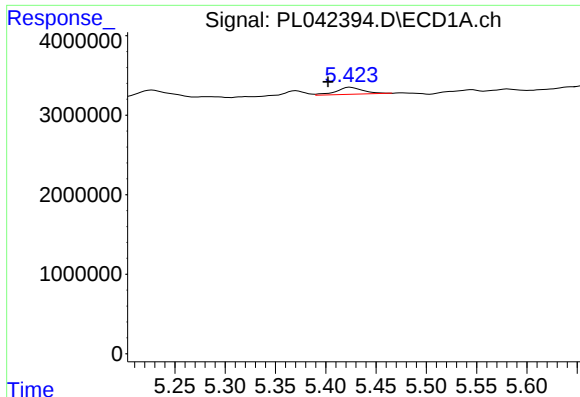

#25 Chlordane-3


R.T.: 5.424 min
Delta R.T.: 0.022 min
Response: 1649592
Conc: 1.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

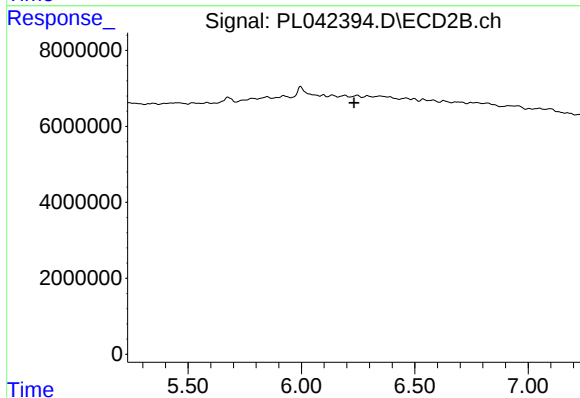


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

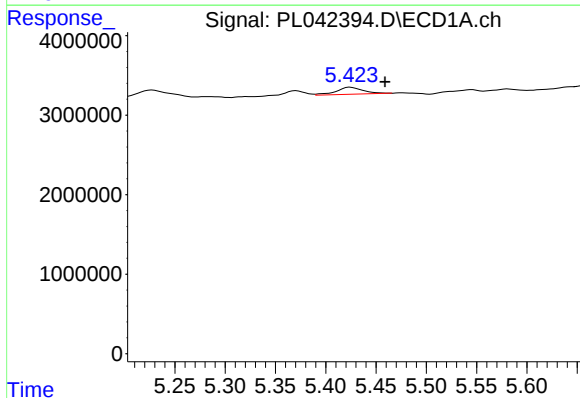


#26 Chlordane-4

R.T.: 5.424 min
Delta R.T.: -0.035 min
Response: 1649592
Conc: 2.17 ng/ml

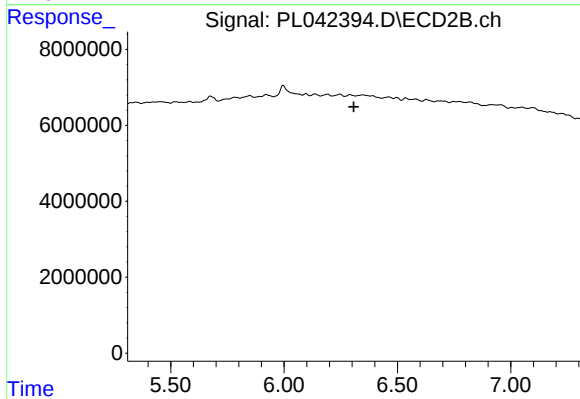

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

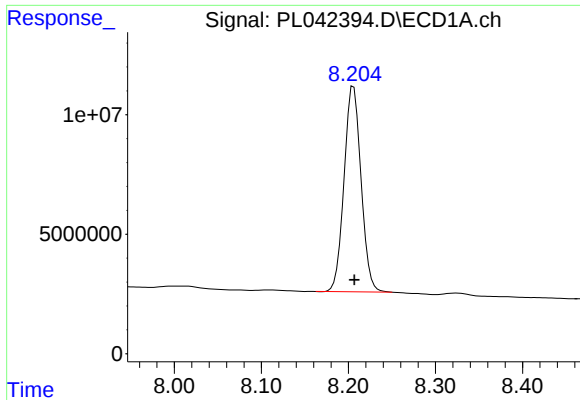

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 116614383
Conc: 18.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

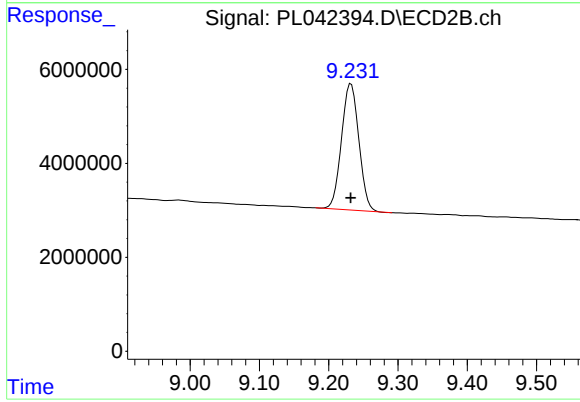

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 46740149
Conc: 19.38 ng/ml