

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
 Data File : PL042395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 01:42
 Operator : AJ\SJ
 Sample : J5775-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 02:38:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	119.7E6	64769113	20.353	22.520
28)	SA Decachlor...	8.206	9.232	113.9E6	45816303	18.075	18.996
Target Compounds							
2)	A alpha-BHC	3.941f	4.489	779941	1718957	0.086	0.401 #
3)	MA gamma-BHC...	0.000	4.833f	0	3190173	N.D.	0.807 #
6)	B beta-BHC	4.403f	0.000	10451163	0	2.950	N.D. #
8)	B Heptachlo...	0.000	5.995	0	4573416	N.D.	1.275 #
9)	A Endosulfan I	5.525	0.000	2947268	0	0.426	N.D. #
11)	B alpha-Chl...	5.525f	0.000	2947268	0	0.393	N.D. #
13)	MA Dieldrin	5.744	0.000	2287462	0	0.311	N.D. #
19)	B Endosulfa...	6.675	0.000	4383373	0	0.703	N.D. #
23)	Chlordane-1	4.403	0.000	10451163	0	37.802	N.D. #
24)	Chlordane-2	4.905	0.000	1654064	0	5.886	N.D. #
26)	Chlordane-4	5.525	0.000	2947268	0	3.884	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
Data File : PL042395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 01:42
Operator : AJ\SJ
Sample : J5775-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 02:38:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

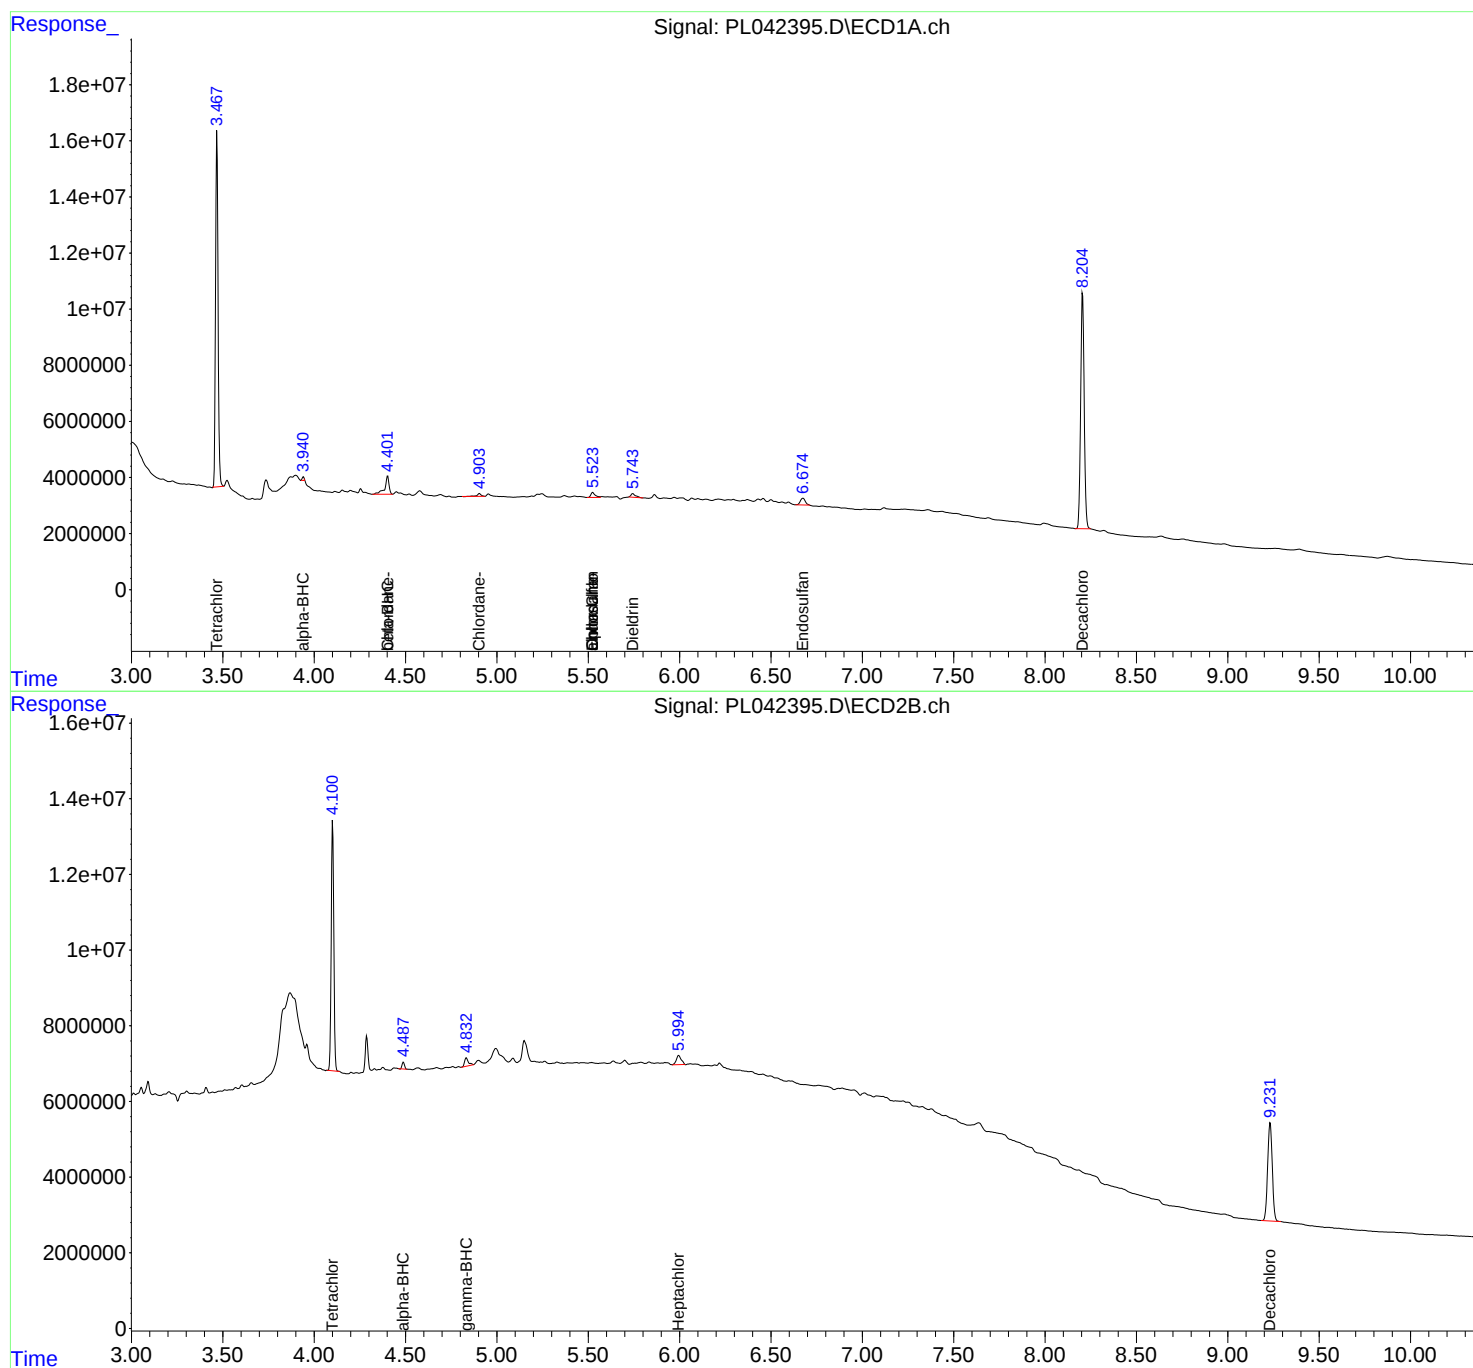


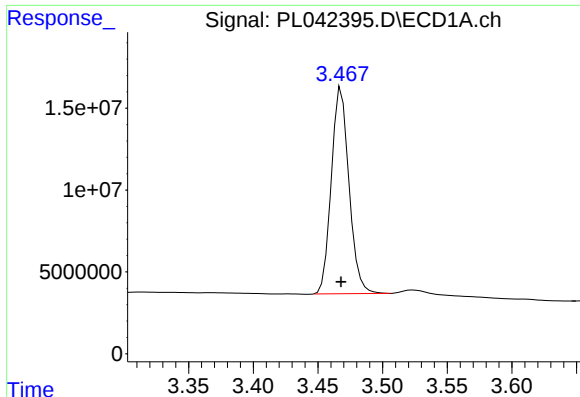

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 119749246
Conc: 20.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

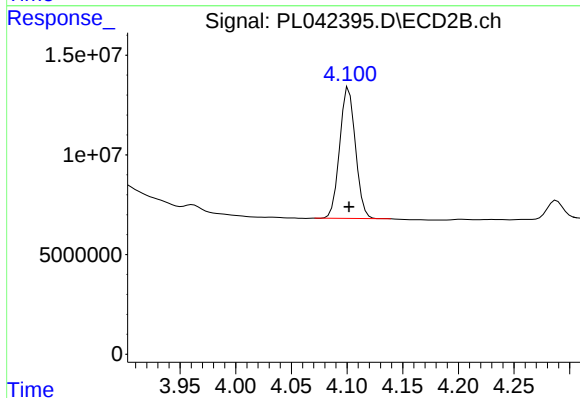


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 64769113
Conc: 22.52 ng/ml

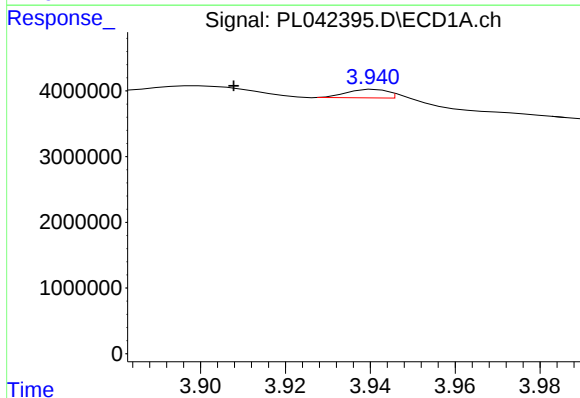


#2 alpha-BHC

R.T.: 3.941 min
Delta R.T.: 0.034 min
Response: 779941
Conc: 0.09 ng/ml

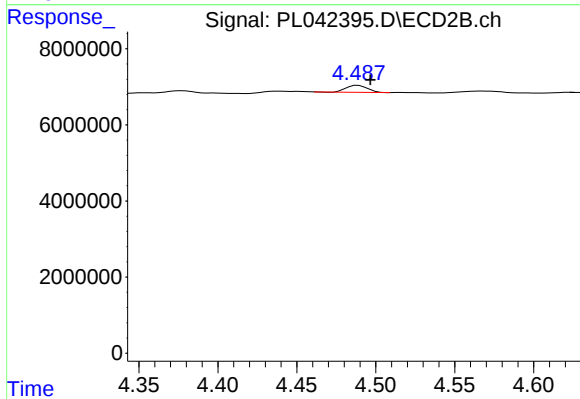

#2 alpha-BHC


R.T.: 4.489 min
Delta R.T.: -0.008 min
Response: 1718957
Conc: 0.40 ng/ml

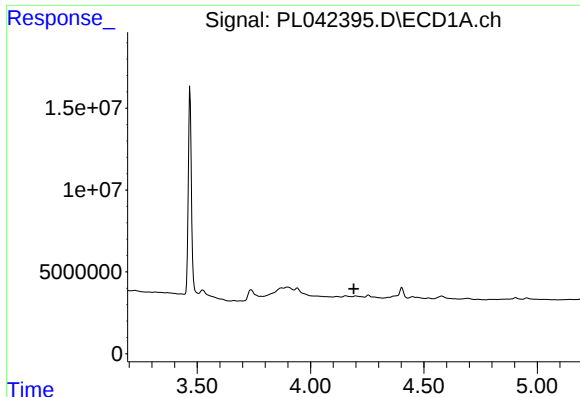

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

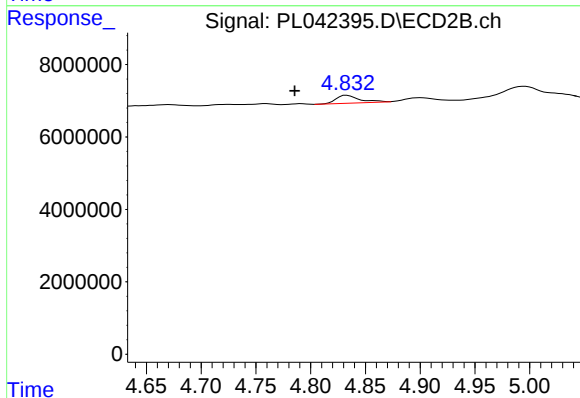


#3 gamma-BHC (Lindane)

R.T.: 4.833 min
Delta R.T.: 0.048 min
Response: 3190173
Conc: 0.81 ng/ml

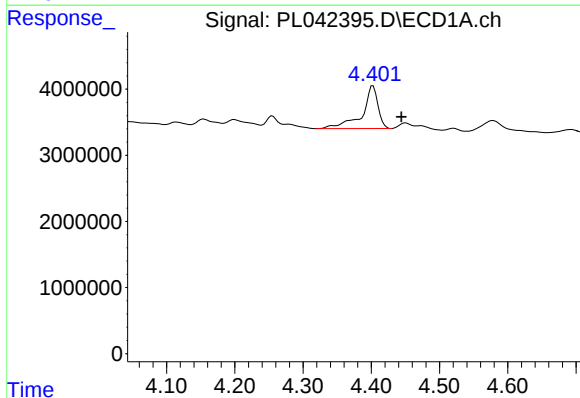


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: -0.042 min
Response: 10451163
Conc: 2.95 ng/ml

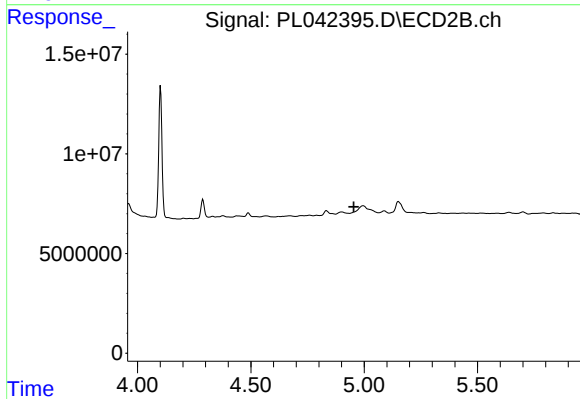

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

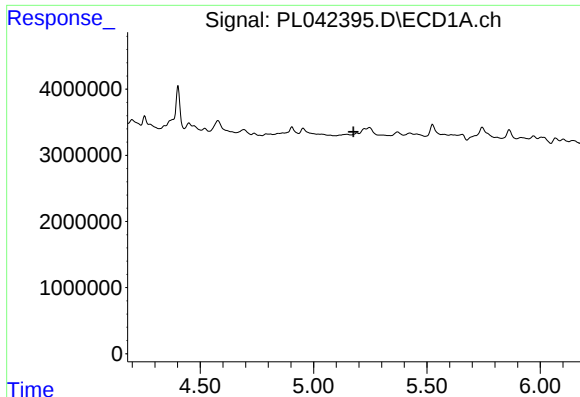

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

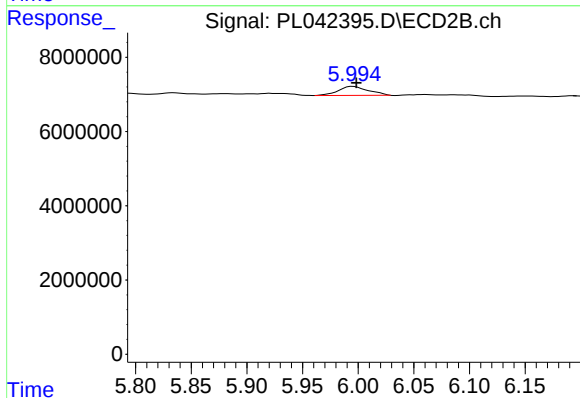


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 4573416
Conc: 1.28 ng/ml

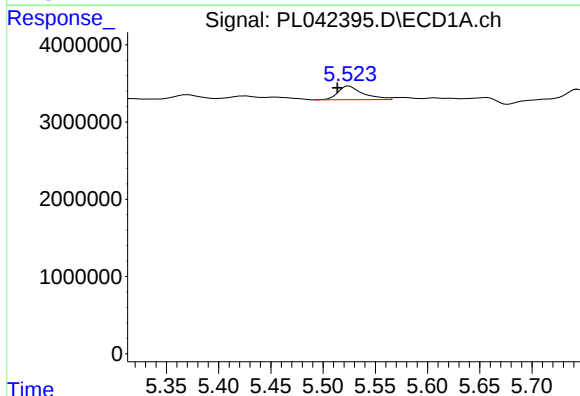


#9 Endosulfan I

R.T.: 5.525 min
Delta R.T.: 0.011 min
Response: 2947268
Conc: 0.43 ng/ml

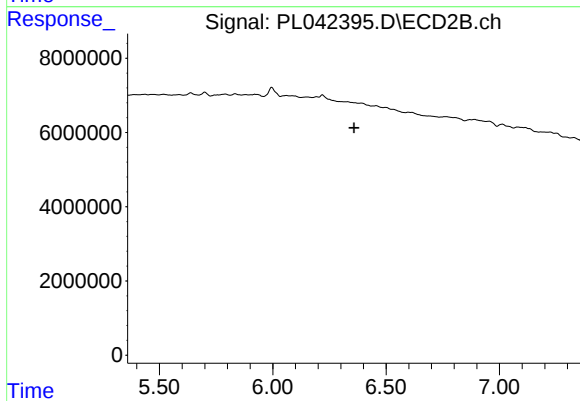

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

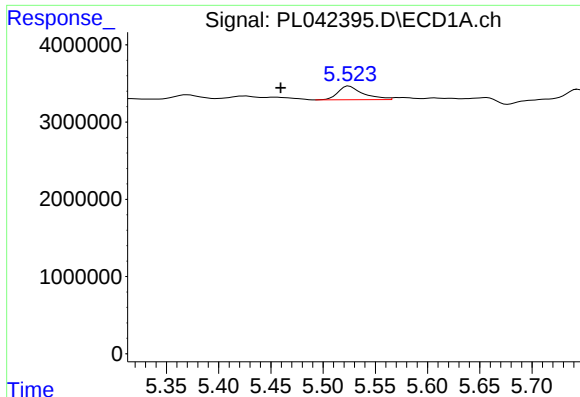

#11 alpha-Chlordane


R.T.: 5.525 min
Delta R.T.: 0.065 min
Response: 2947268
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

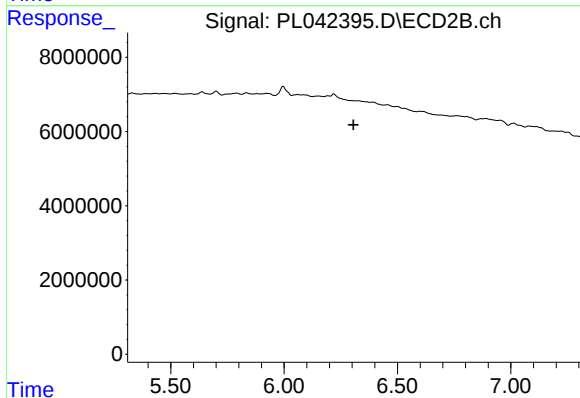


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

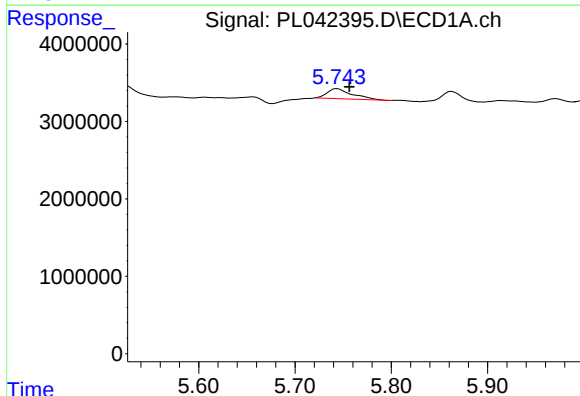


#13 Dieldrin

R.T.: 5.744 min
Delta R.T.: -0.012 min
Response: 2287462
Conc: 0.31 ng/ml

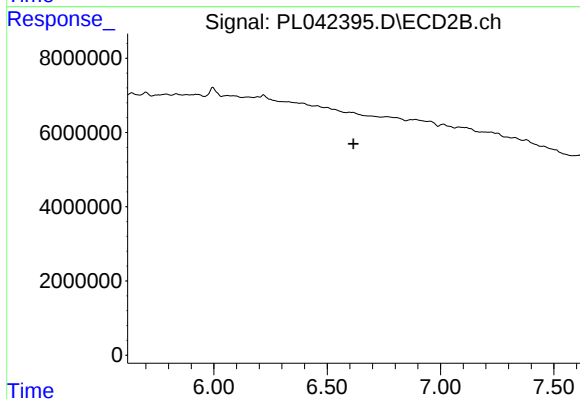

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

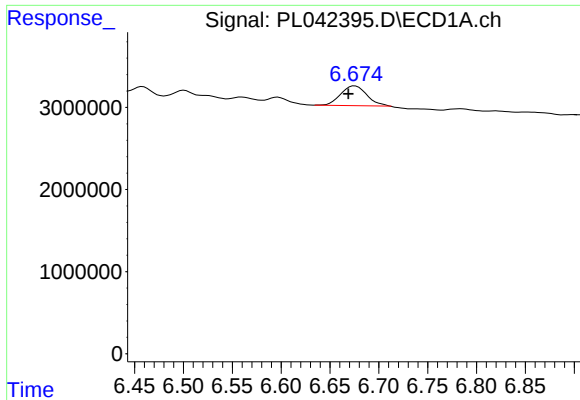

#19 Endosulfan Sulfate


R.T.: 6.675 min
Delta R.T.: 0.007 min
Response: 4383373
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

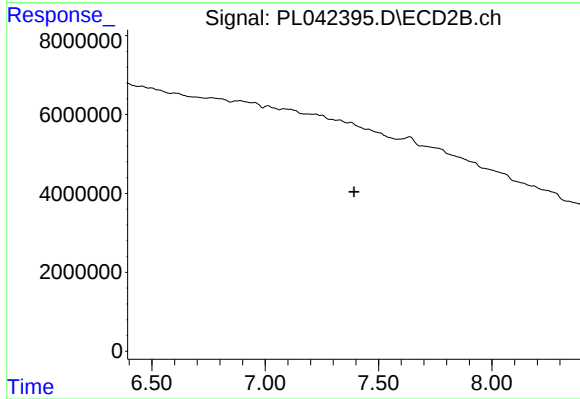


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

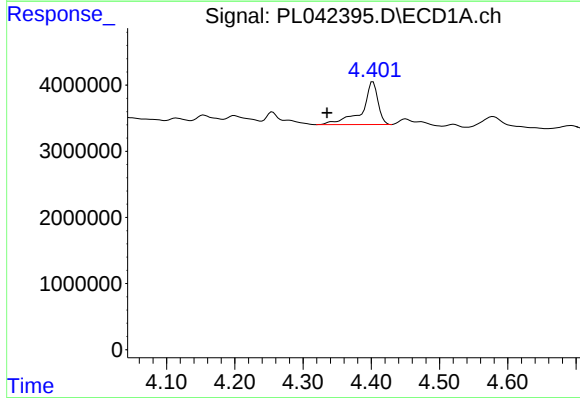


#23 Chlordane-1

R.T.: 4.403 min
Delta R.T.: 0.067 min
Response: 10451163
Conc: 37.80 ng/ml

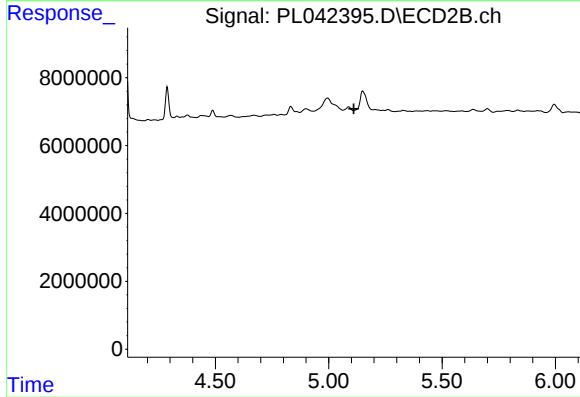

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

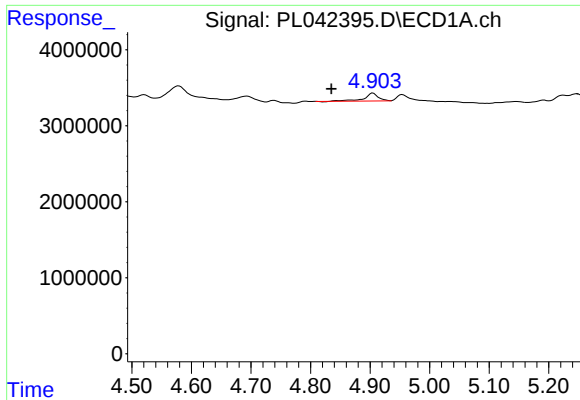

#24 Chlordane-2


R.T.: 4.905 min
Delta R.T.: 0.070 min
Response: 1654064
Conc: 5.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

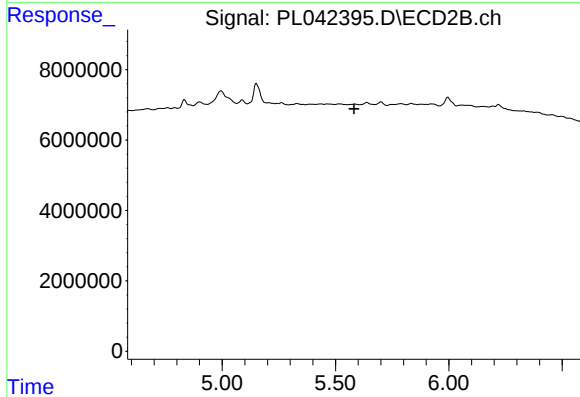


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

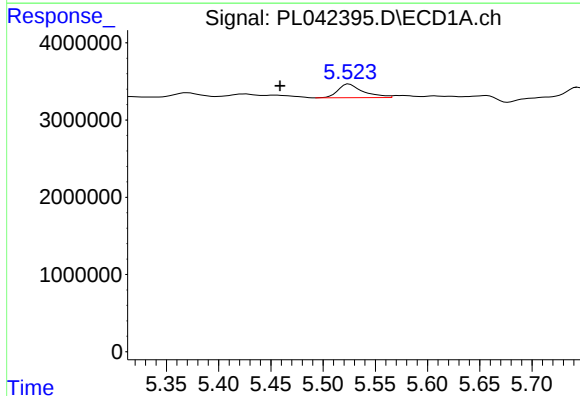


#26 Chlordane-4

R.T.: 5.525 min
Delta R.T.: 0.066 min
Response: 2947268
Conc: 3.88 ng/ml

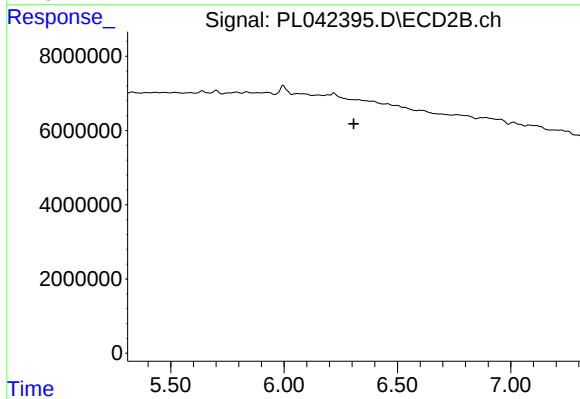

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

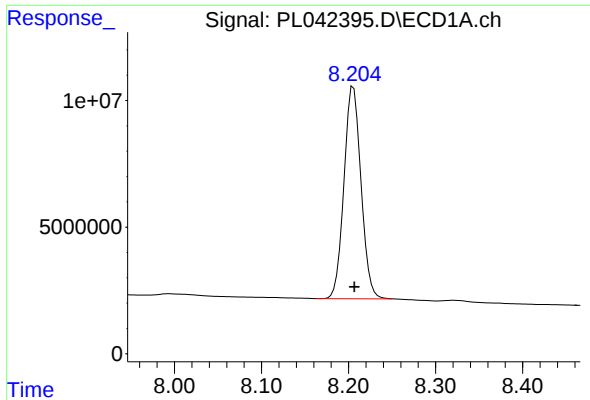

#28 Decachlorobiphenyl


R.T.: 8.206 min

Delta R.T.: -0.001 min

Response: 113908393

Conc: 18.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

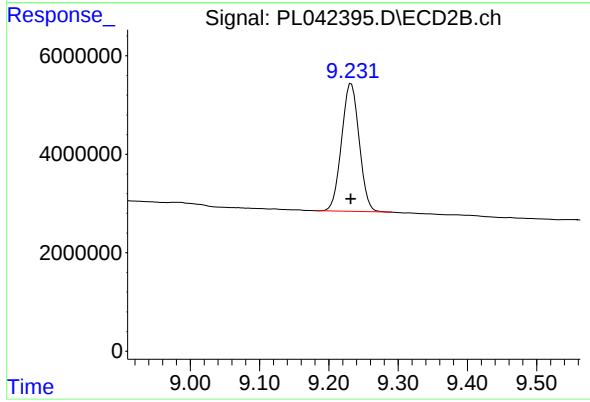

#28 Decachlorobiphenyl

R.T.: 9.232 min

Delta R.T.: 0.000 min

Response: 45816303

Conc: 19.00 ng/ml