

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
 Data File : PL042373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2018 20:32
 Operator : AJ\SJ
 Sample : J5996-25
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AOC1-06-A

Manual Integrations
 APPROVED

Sohil
 11/21/2018 7:54:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:06:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	42525920	22545152	7.228	7.839
28)	SA Decachlor...	8.207	9.232	55211546	22562323	8.761	9.355
Target Compounds							
10)	B gamma-Chl...	5.406	6.232	6598299	5454586	0.865m	1.602m#
11)	B alpha-Chl...	5.458	6.308	13364837	19801947	1.780	5.922 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112118\
Data File : PL042373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2018 20:32
Operator : AJ\SJ
Sample : J5996-25
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AOC1-06-A


Manual Integrations
APPROVED

Sohil
11/21/2018 7:54:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:06:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

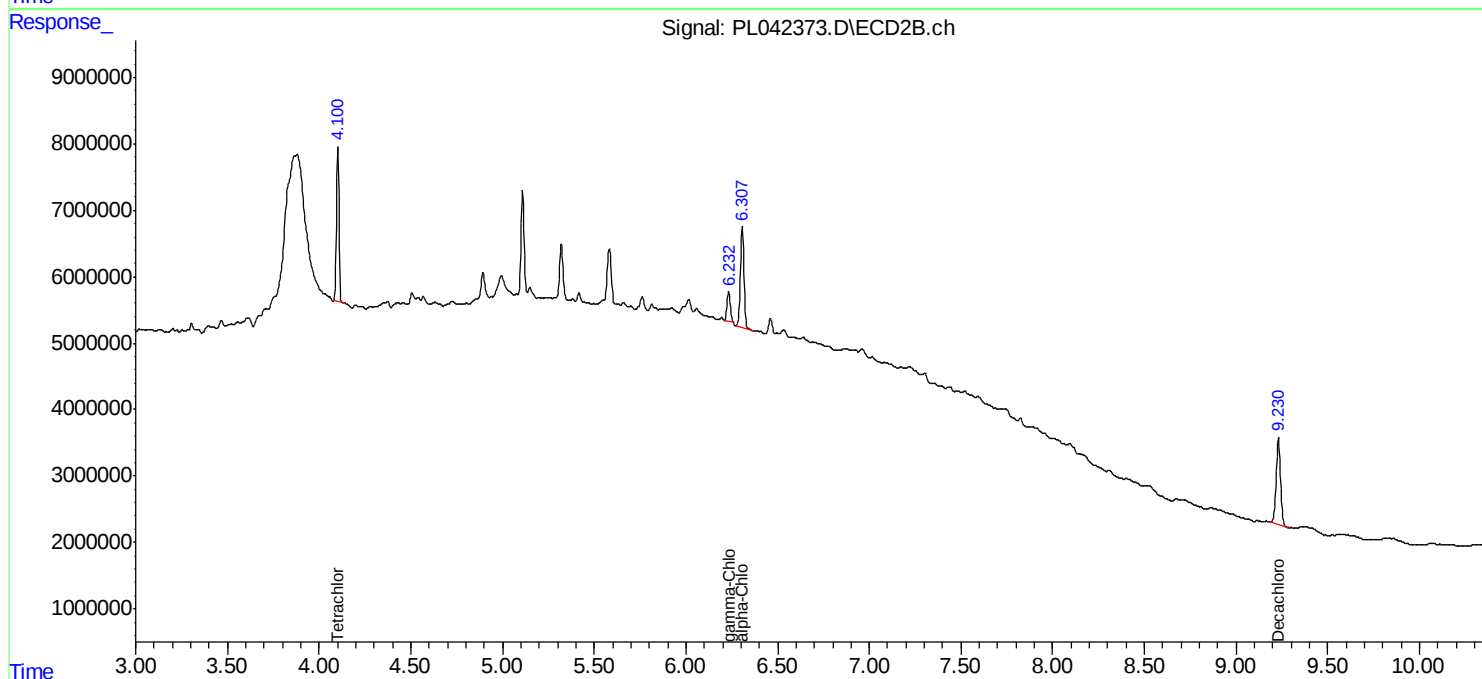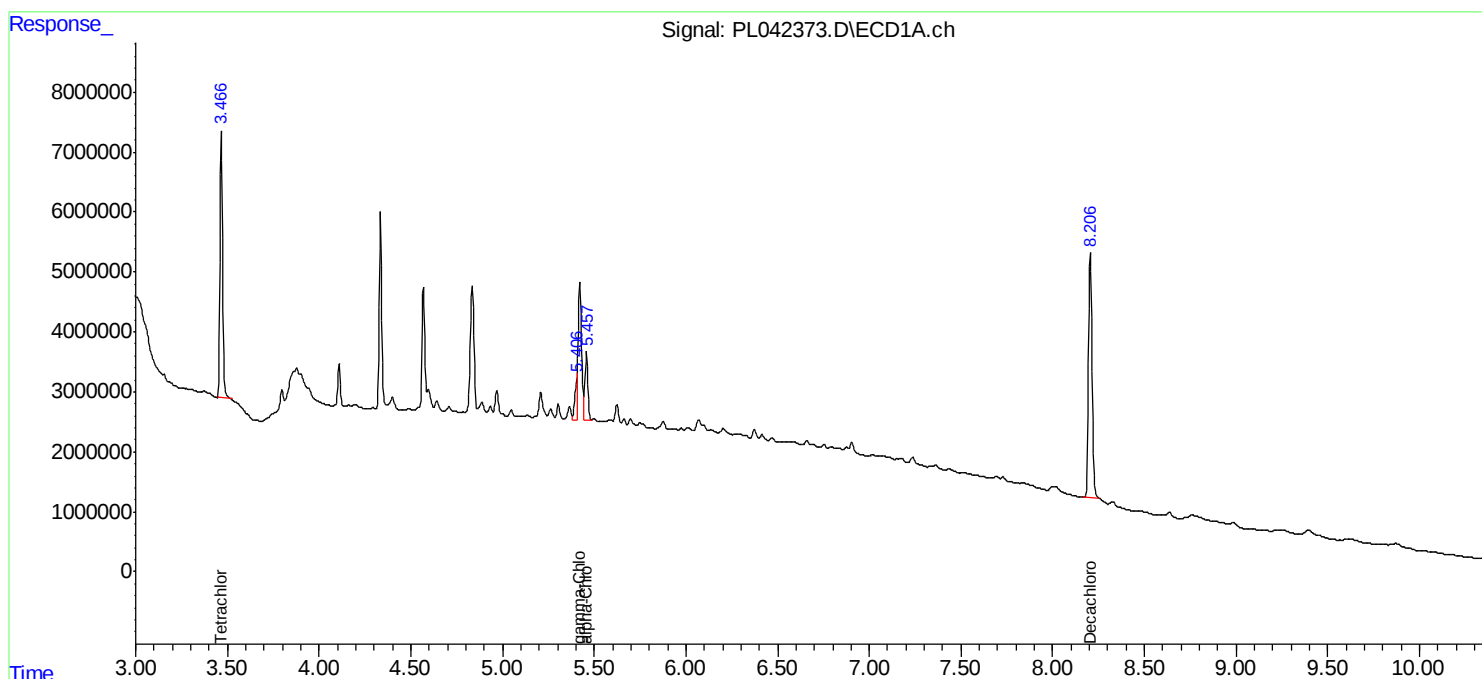

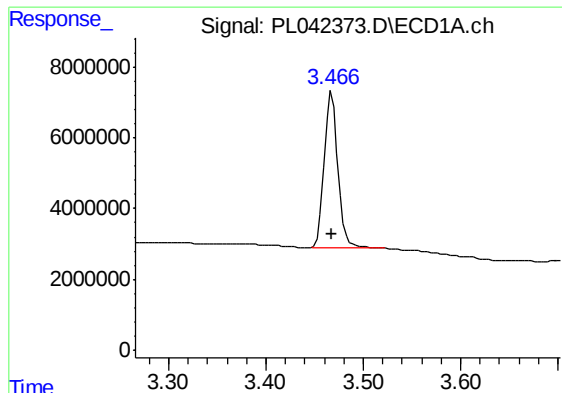


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 42525920
Conc: 7.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
AOC1-06-A


Manual Integrations
APPROVED

Sohil
11/21/2018 7:54:42 AM

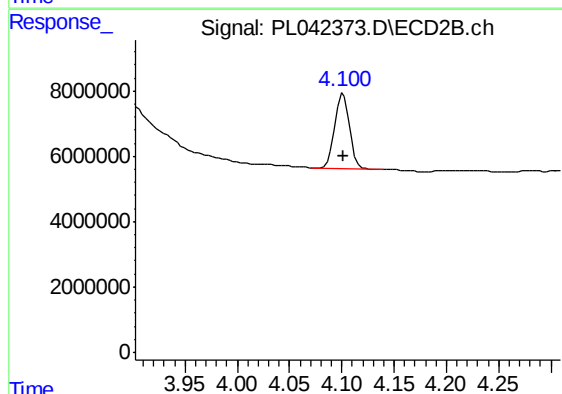


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 22545152
Conc: 7.84 ng/ml

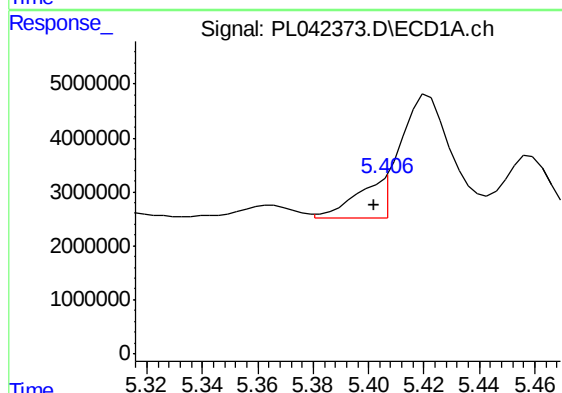


#10 gamma-Chlordane

R.T.: 5.406 min
Delta R.T.: 0.004 min
Response: 6598299
Conc: 0.87 ng/ml m

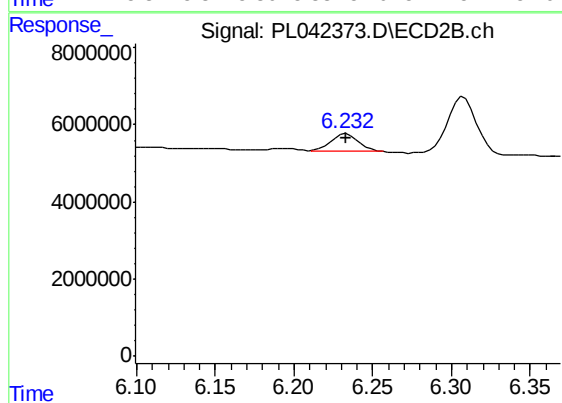

#10 gamma-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 5454586
Conc: 1.60 ng/ml m

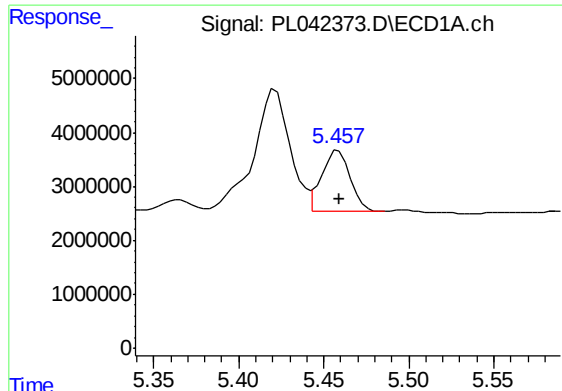


#11 alpha-Chlordane

R.T.: 5.458 min
Delta R.T.: 0.000 min
Response: 13364837
Conc: 1.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
AOC1-06-A


Manual Integrations
APPROVED

Sohil
11/21/2018 7:54:42 AM

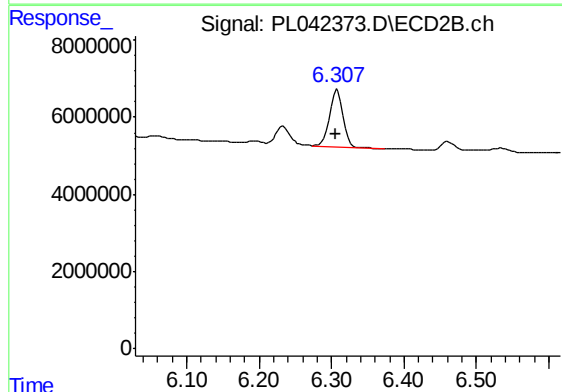


#11 alpha-Chlordane

R.T.: 6.308 min
Delta R.T.: 0.001 min
Response: 19801947
Conc: 5.92 ng/ml

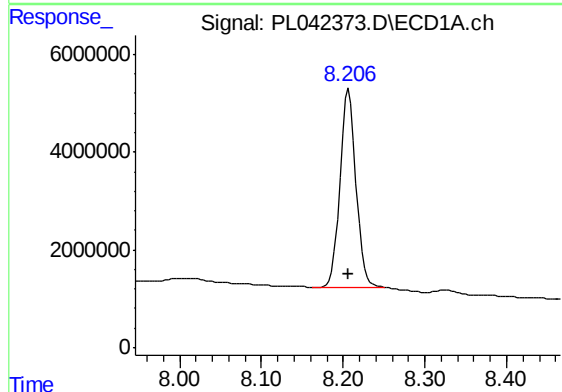

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 55211546
Conc: 8.76 ng/ml

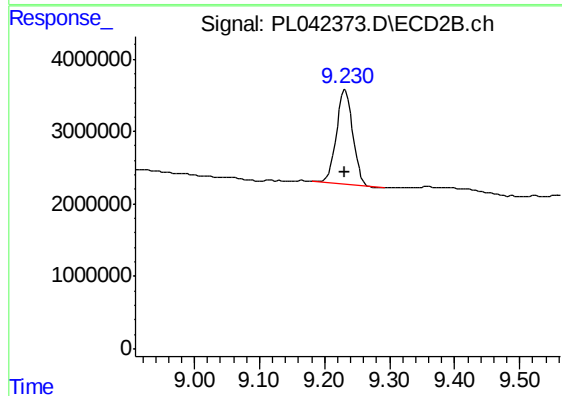

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 22562323
Conc: 9.35 ng/ml