

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112119\
 Data File : PL054532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2019 18:09
 Operator : SG\AJ
 Sample : K5948-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-1-6-12

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:39:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.044	130.0E6	32310668	12.505	13.263
28)	SA Decachlor...	8.320	9.123	98225499	27782803	11.098	11.491
Target Compounds							
4)	MA Heptachlor	4.550f	0.000	31035612	0	2.027	N.D. #
6)	B beta-BHC	4.550f	0.000	31035612	0	4.827	N.D. #
12)	B 4,4'-DDE	5.720	6.384	9502372	2720349	0.822	1.139 #
16)	A 4,4'-DDD	6.238	6.877	7908712	3709939	0.959	2.096 #
17)	MA 4,4'-DDT	6.475	7.146f	9015575	979129	0.994	0.499 #
19)	B Endosulfa...	6.765	0.000	4569901	0	0.488	N.D. #
20)	A Methoxychlor	7.011f	0.000	10949242	0	2.392	N.D. #
23)	Chlordane-1	4.423	0.000	19947837	0	51.358	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112119\
Data File : PL054532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2019 18:09
Operator : SG\AJ
Sample : K5948-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
B-1-6-12

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:39:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

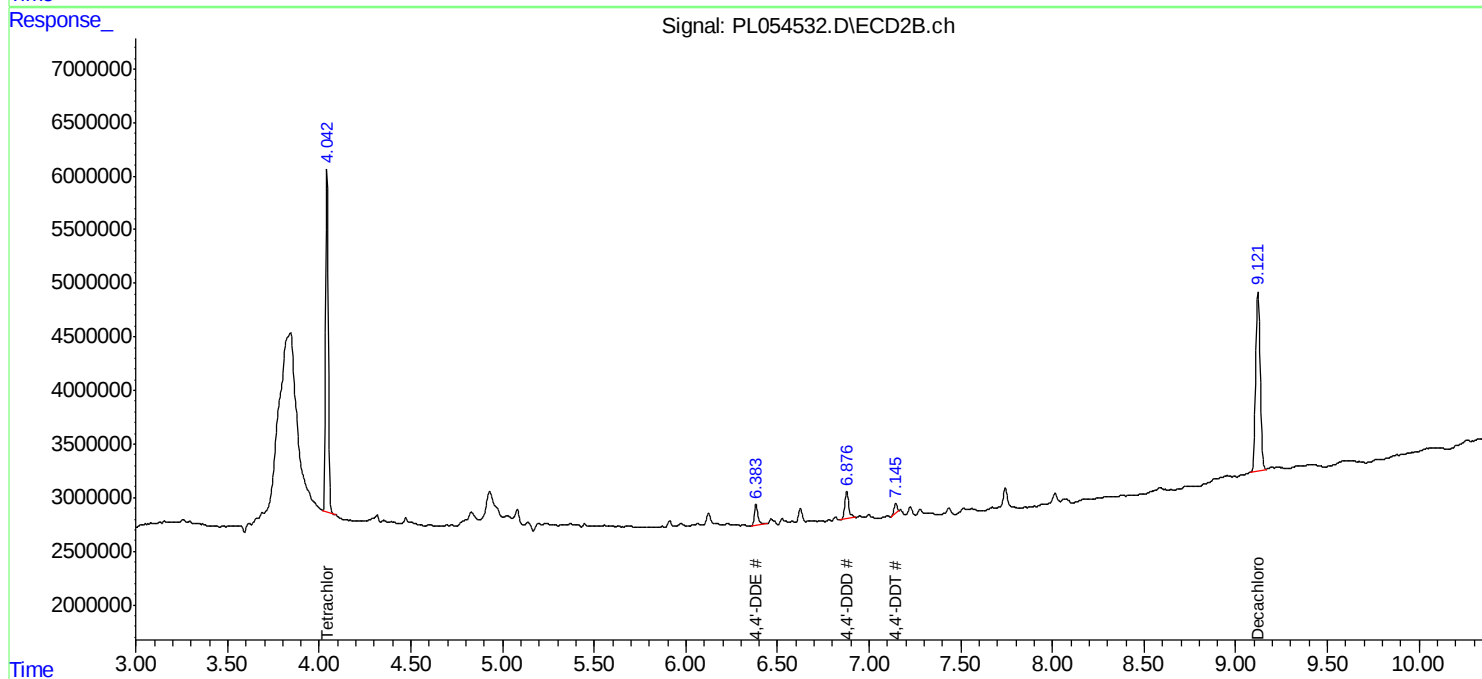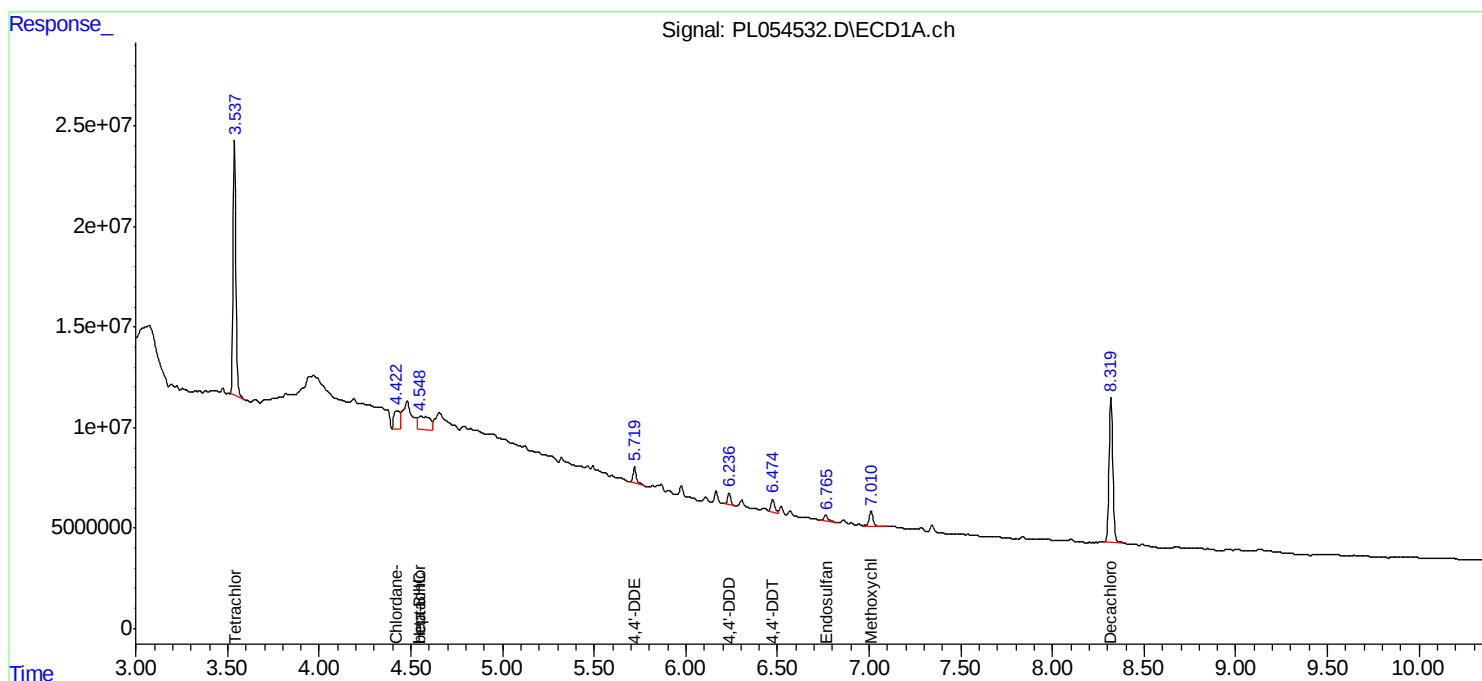


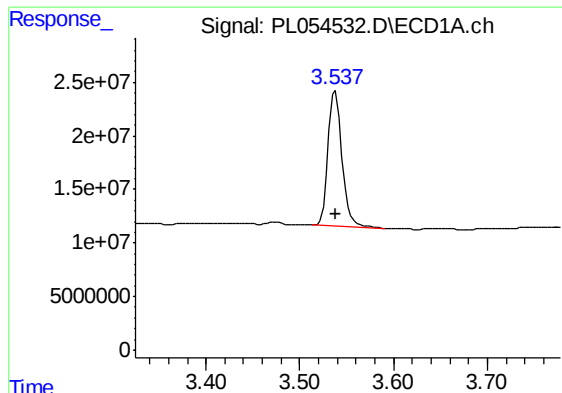

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 130018176
Conc: 12.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-1-6-12

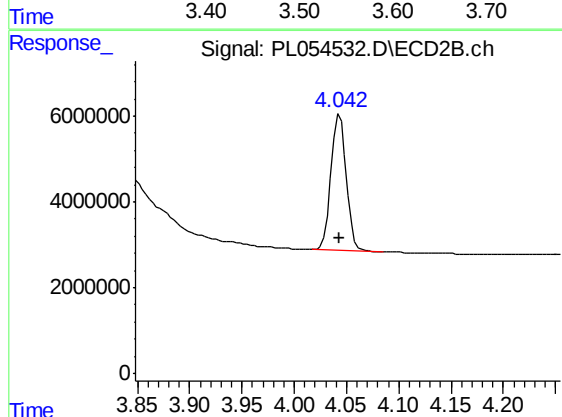


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 32310668
Conc: 13.26 ng/ml

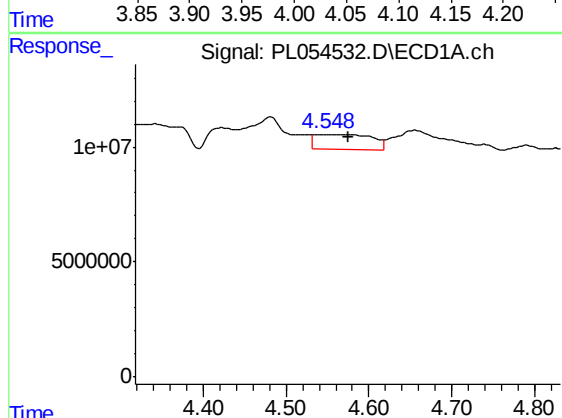


#4 Heptachlor

R.T.: 4.550 min
Delta R.T.: -0.026 min
Response: 31035612
Conc: 2.03 ng/ml

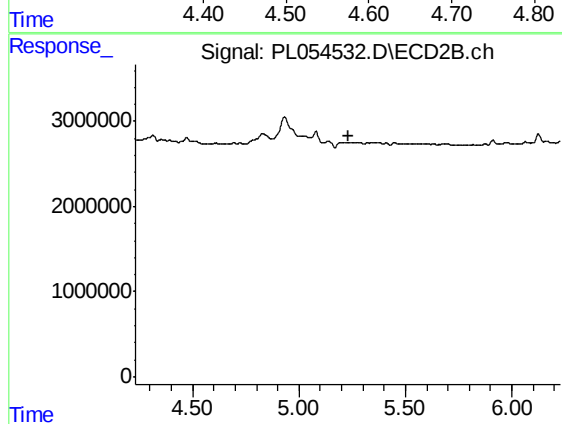

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.230 min
Response: 0
Conc: N.D.

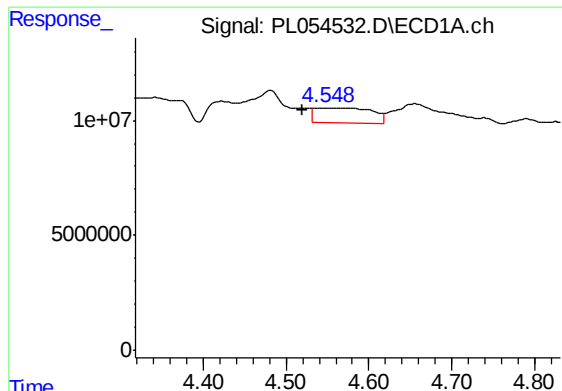

#6 beta-BHC


R.T.: 4.550 min
Delta R.T.: 0.030 min
Response: 31035612
Conc: 4.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-1-6-12

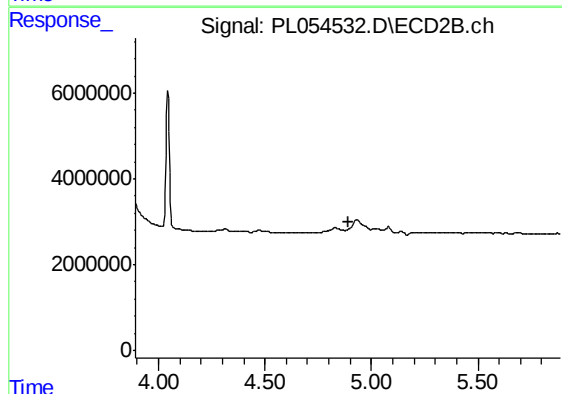


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.891 min
Response: 0
Conc: N.D.

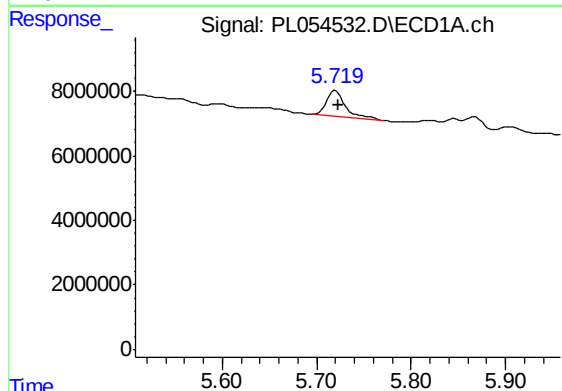


#12 4,4'-DDE

R.T.: 5.720 min
Delta R.T.: -0.002 min
Response: 9502372
Conc: 0.82 ng/ml

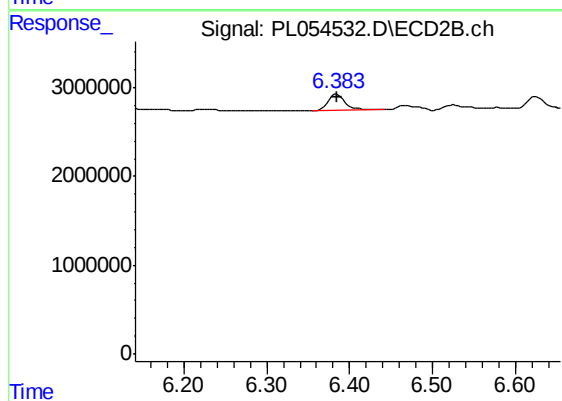

#12 4,4'-DDE


R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 2720349
Conc: 1.14 ng/ml

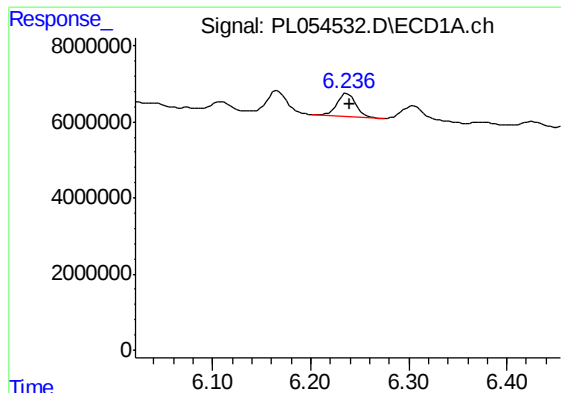

#16 4,4'-DDD


R.T.: 6.238 min
Delta R.T.: -0.003 min
Response: 7908712
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-1-6-12

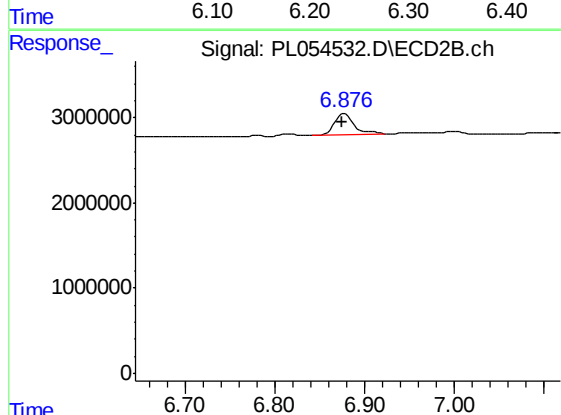


#16 4,4'-DDD

R.T.: 6.877 min
Delta R.T.: 0.002 min
Response: 3709939
Conc: 2.10 ng/ml

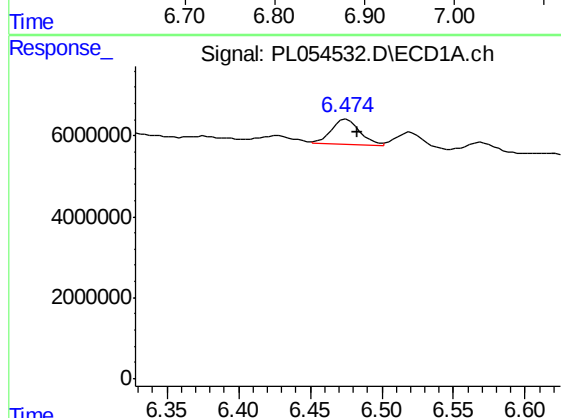


#17 4,4'-DDT

R.T.: 6.475 min
Delta R.T.: -0.007 min
Response: 9015575
Conc: 0.99 ng/ml

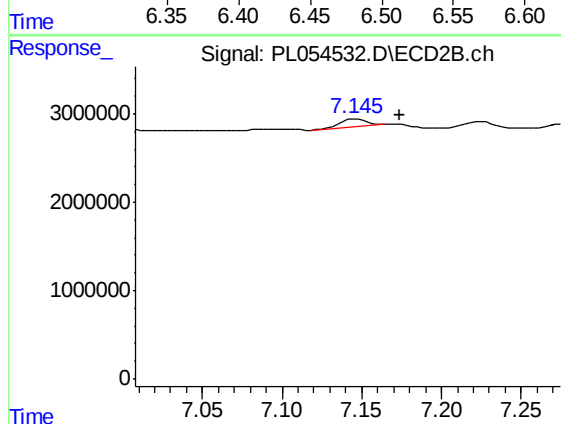

#17 4,4'-DDT


R.T.: 7.146 min
Delta R.T.: -0.028 min
Response: 979129
Conc: 0.50 ng/ml

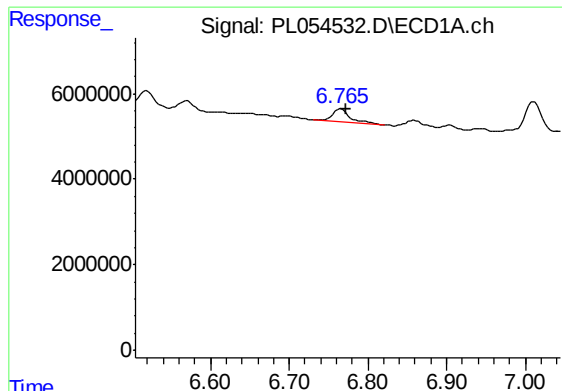

#19 Endosulfan Sulfate


R.T.: 6.765 min
Delta R.T.: -0.007 min
Response: 4569901
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-1-6-12

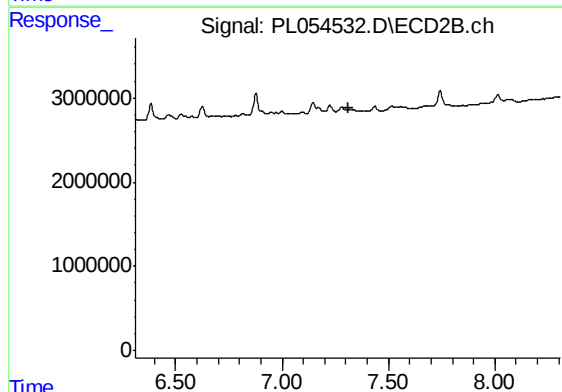


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.310 min
Response: 0
Conc: N.D.

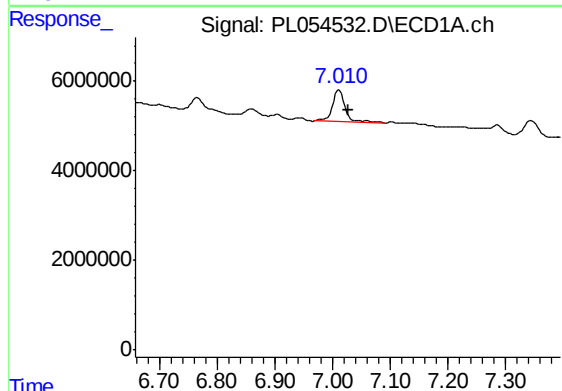


#20 Methoxychlor

R.T.: 7.011 min
Delta R.T.: -0.017 min
Response: 10949242
Conc: 2.39 ng/ml

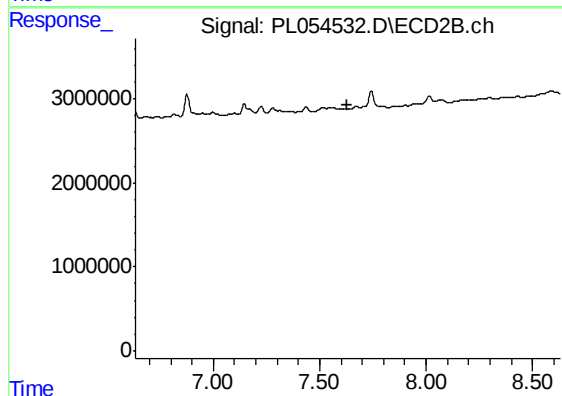

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.633 min
Response: 0
Conc: N.D.

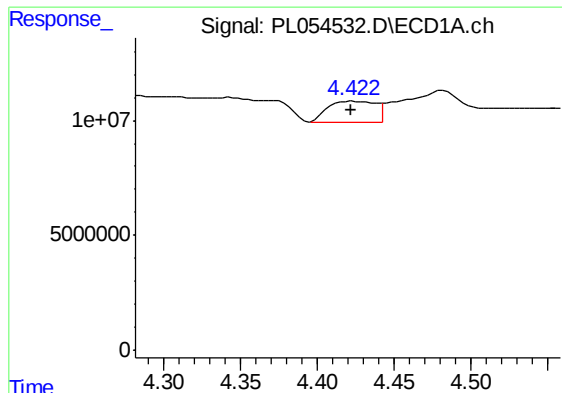

#23 Chlordane-1


R.T.: 4.423 min
Delta R.T.: 0.002 min
Response: 19947837
Conc: 51.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-1-6-12

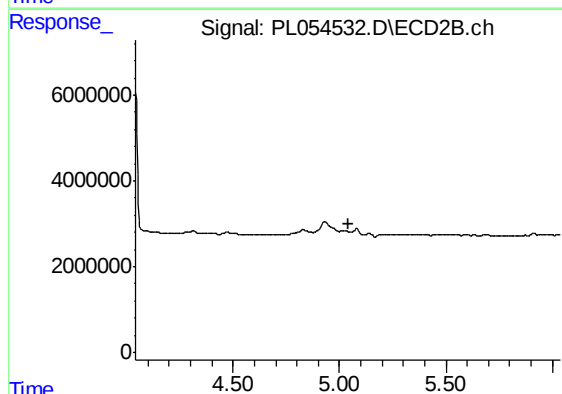


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.041 min
Response: 0
Conc: N.D.

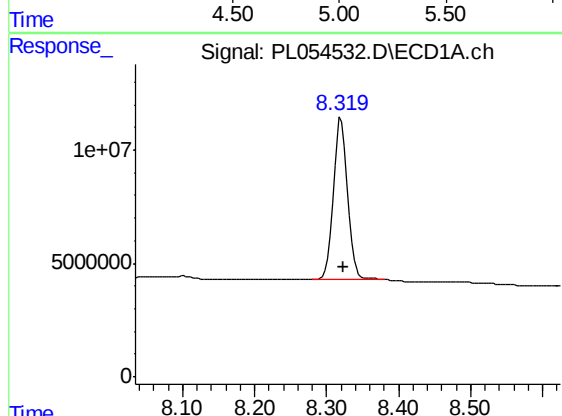

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.003 min
Response: 98225499
Conc: 11.10 ng/ml

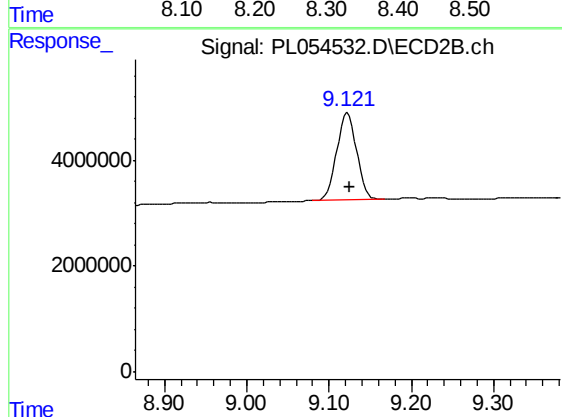

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.002 min
Response: 27782803
Conc: 11.49 ng/ml