

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112119\
 Data File : PL054533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2019 18:23
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:39:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.538	4.044	184.4E6	44172861	17.731	18.132
28) SA	Decachlor...	8.320	9.123	140.2E6	42444860	15.836	17.555
Target Compounds							
8) B	Heptachlo...	5.272	5.915	65700028	25557520	5.087	10.754 #
9) A	Endosulfan I	5.618	0.000	6509903	0	0.550	N.D. #
12) B	4,4'-DDE	5.742f	0.000	15541837	0	1.344	N.D. #
14) MA	Endrin	6.116	6.745	10384201	7191376	0.940	3.393 #
15) B	Endosulfa...	6.395	0.000	1107308	0	0.106	N.D. #
27)	Chlordane-5	6.395	0.000	1107308	0	3.002	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112119\
Data File : PL054533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2019 18:23
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:39:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

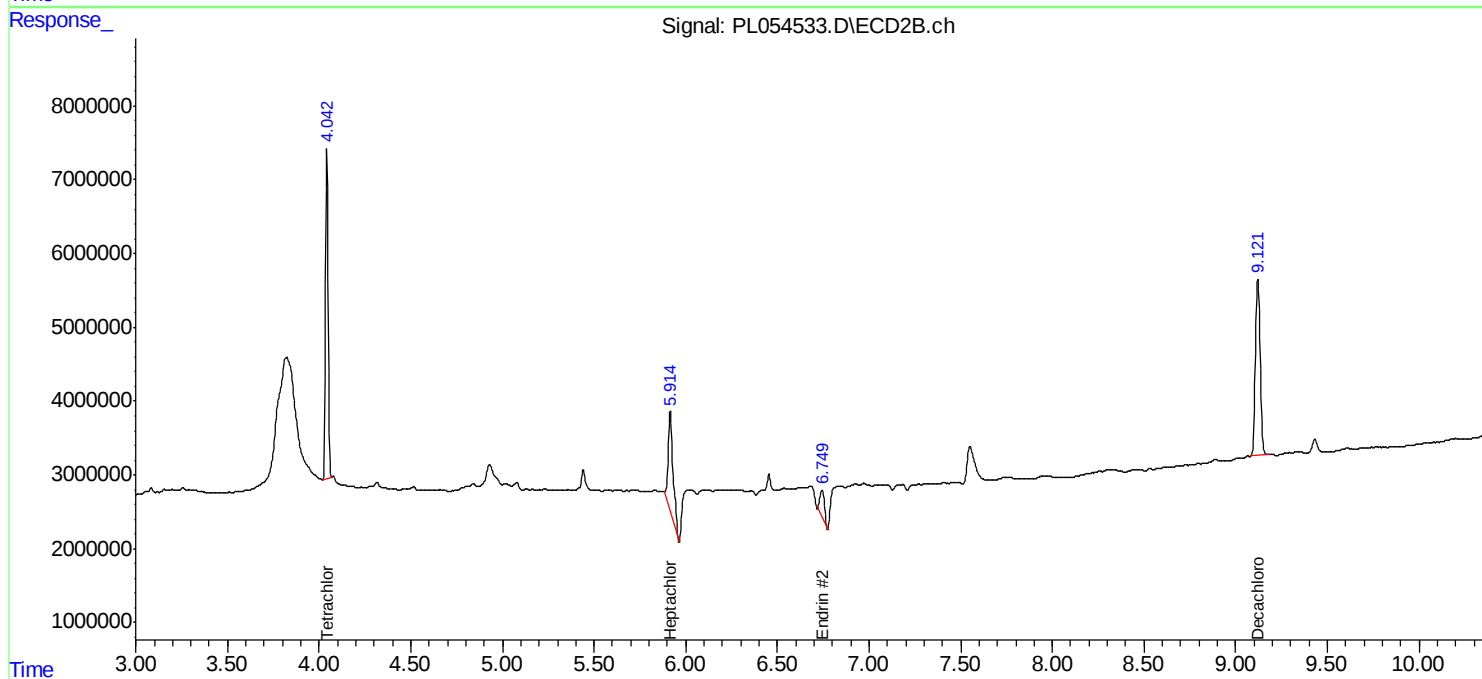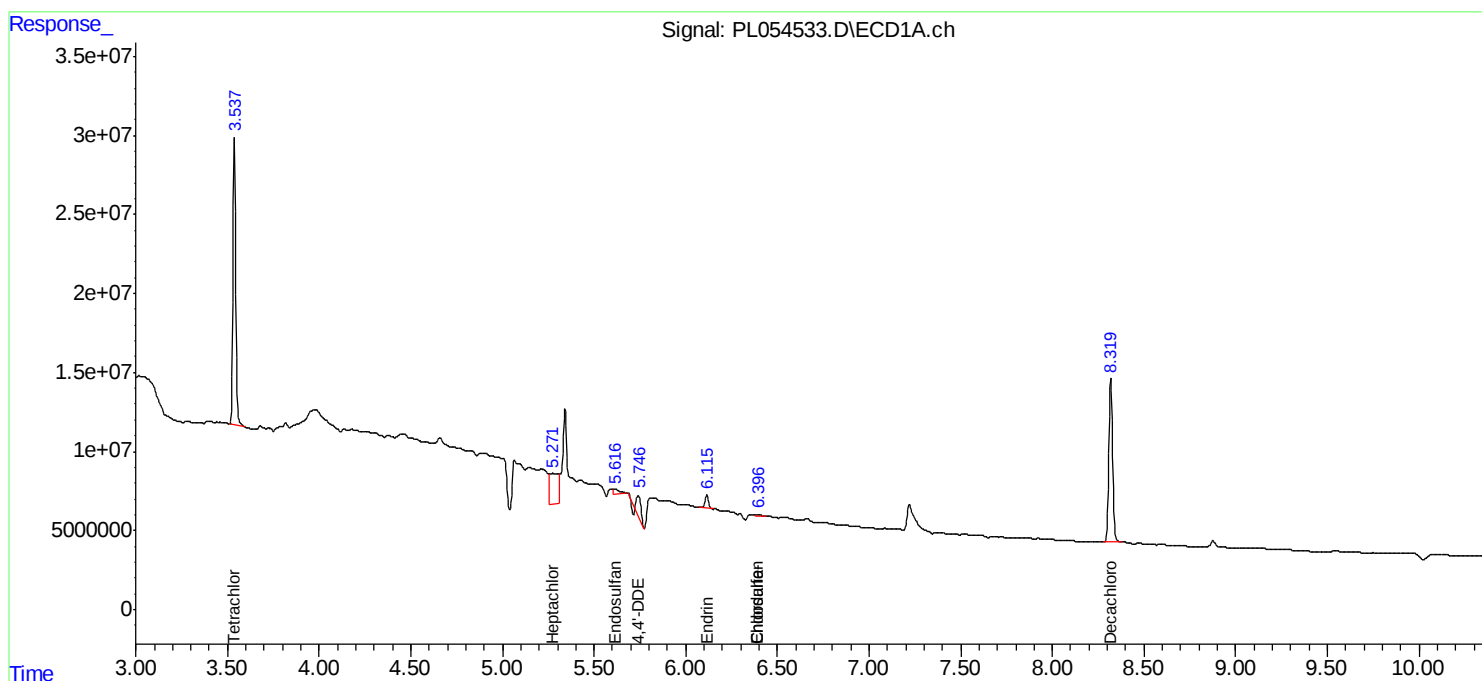


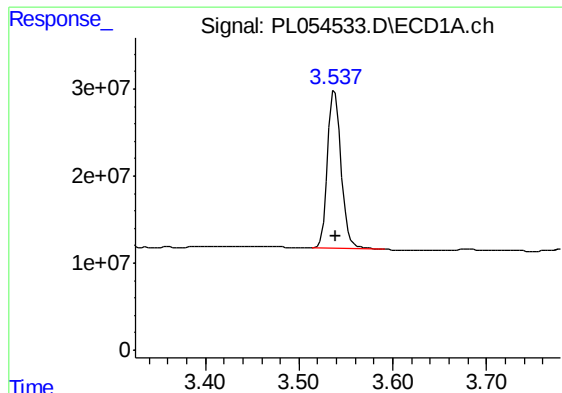

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 184352900
Conc: 17.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

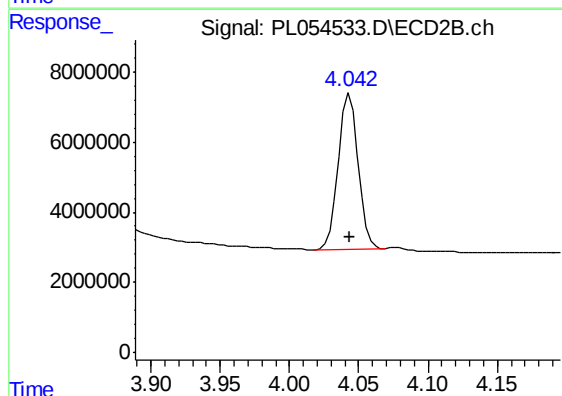


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 44172861
Conc: 18.13 ng/ml

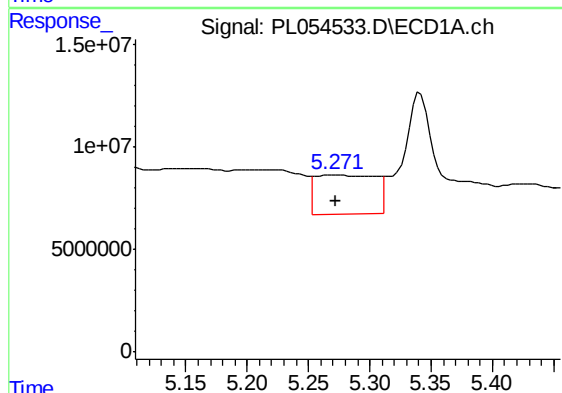


#8 Heptachlor epoxide

R.T.: 5.272 min
Delta R.T.: 0.000 min
Response: 65700028
Conc: 5.09 ng/ml

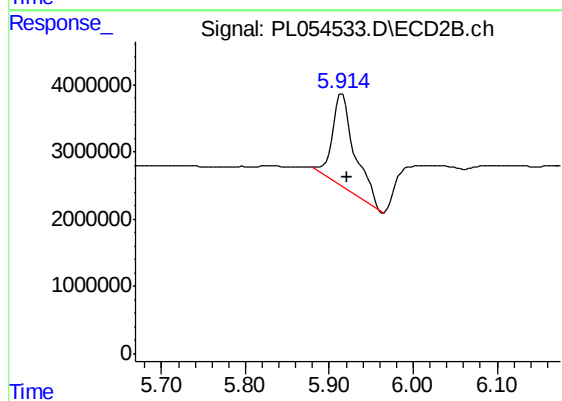

#8 Heptachlor epoxide


R.T.: 5.915 min
Delta R.T.: -0.007 min
Response: 25557520
Conc: 10.75 ng/ml

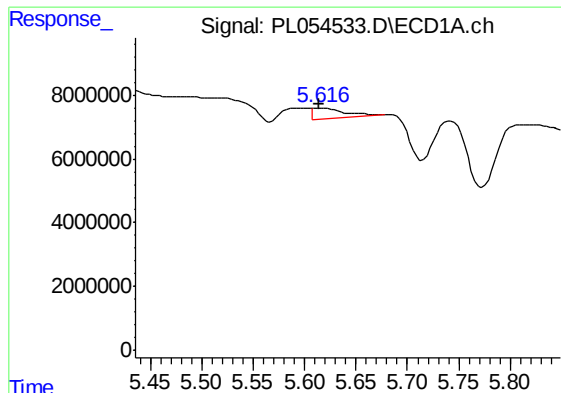

#9 Endosulfan I


R.T.: 5.618 min
Delta R.T.: 0.003 min
Response: 6509903
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

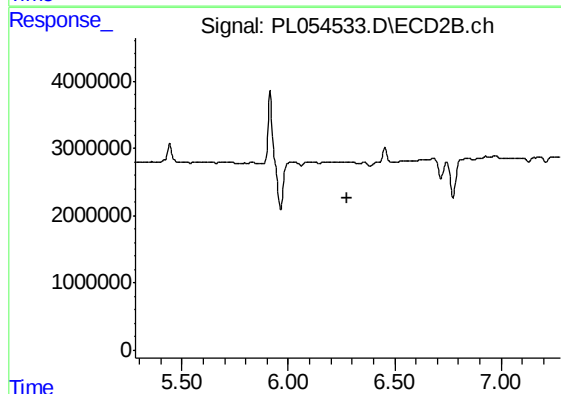


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

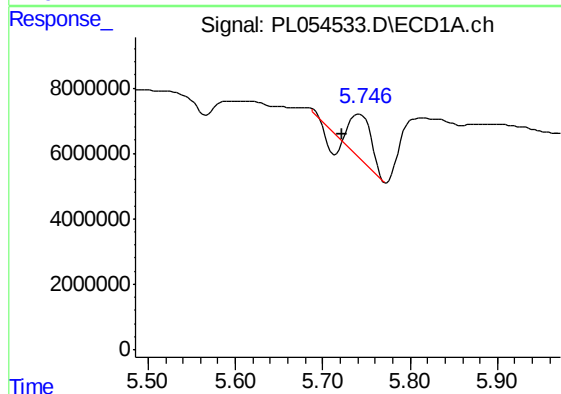


#12 4,4'-DDE

R.T.: 5.742 min
Delta R.T.: 0.019 min
Response: 15541837
Conc: 1.34 ng/ml

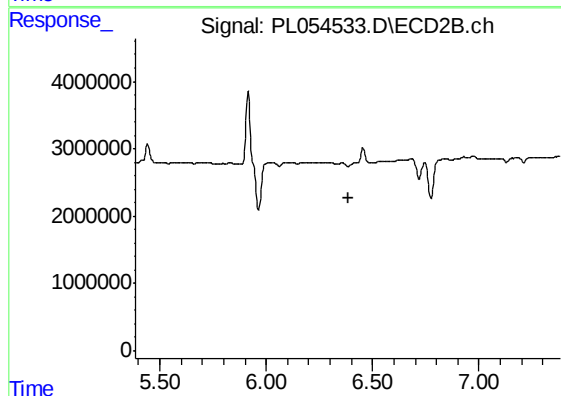

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

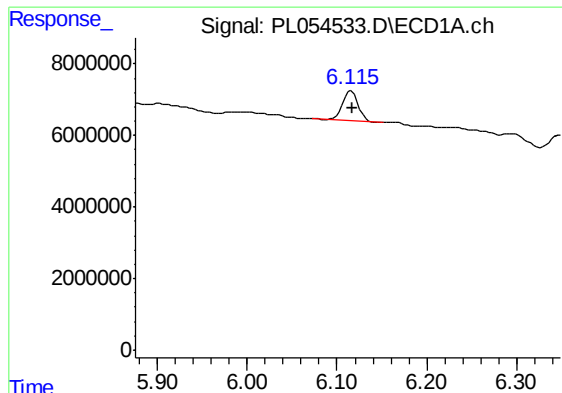

#14 Endrin


R.T.: 6.116 min
Delta R.T.: -0.002 min
Response: 10384201
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

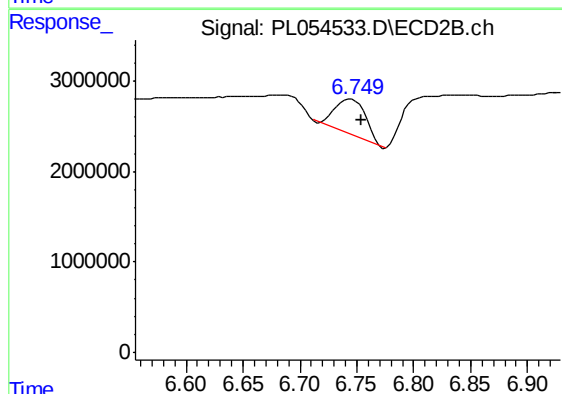


#14 Endrin

R.T.: 6.745 min
Delta R.T.: -0.009 min
Response: 7191376
Conc: 3.39 ng/ml

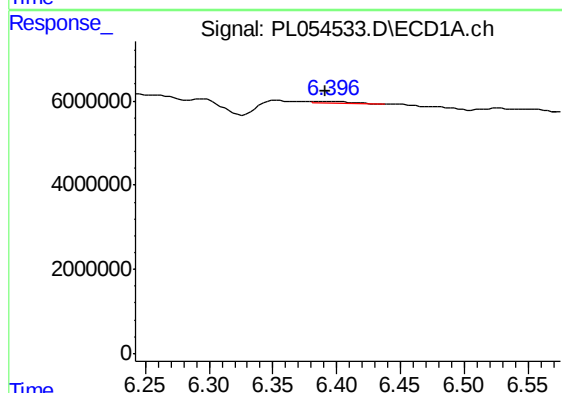


#15 Endosulfan II

R.T.: 6.395 min
Delta R.T.: 0.003 min
Response: 1107308
Conc: 0.11 ng/ml

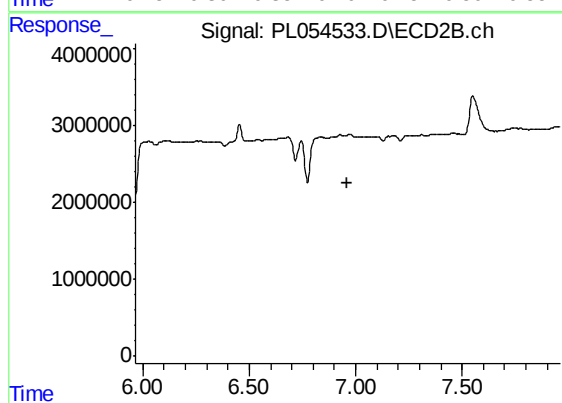

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.964 min
Response: 0
Conc: N.D.

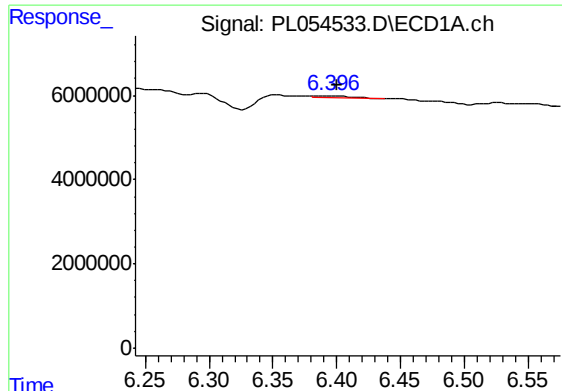

#27 Chlordane-5


R.T.: 6.395 min
Delta R.T.: -0.006 min
Response: 1107308
Conc: 3.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

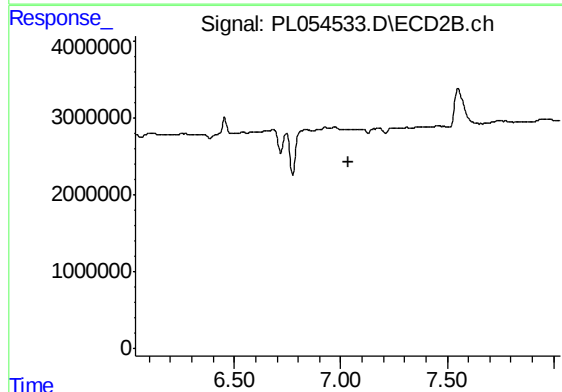


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.035 min
Response: 0
Conc: N.D.

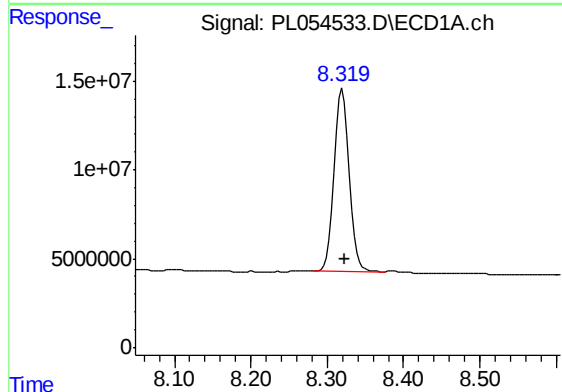

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.003 min
Response: 140166160
Conc: 15.84 ng/ml

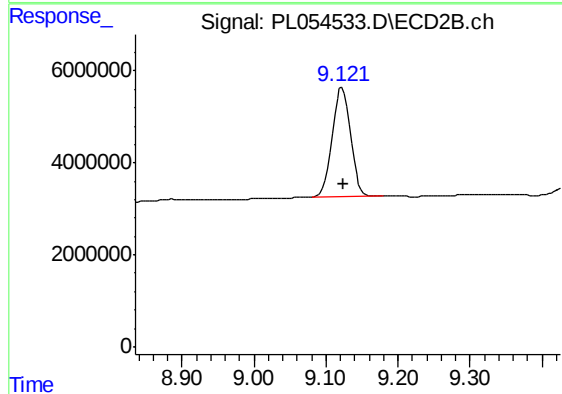

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.002 min
Response: 42444860
Conc: 17.56 ng/ml