

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112122\
 Data File : PL079321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2022 10:31
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:23:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.326	2.563	108.5E6	146.0E6	52.114	57.330
28)	SA Decachlor...	8.776	7.634	88767578	99016075	53.067	47.731
Target Compounds							
23)	Chlordane-1	4.474	3.529	47008665	47489076	536.493	459.640
24)	Chlordane-2	5.008	4.095	50774705	47644691	498.839	448.658
25)	Chlordane-3	5.718	4.715	201.5E6	148.5E6	523.087	466.235
26)	Chlordane-4	5.795	4.776	245.3E6	159.5E6	518.342	464.806
27)	Chlordane-5	6.650	5.438	39353868	40695723	530.409	477.263



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112122\
Data File : PL079321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2022 10:31
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:23:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

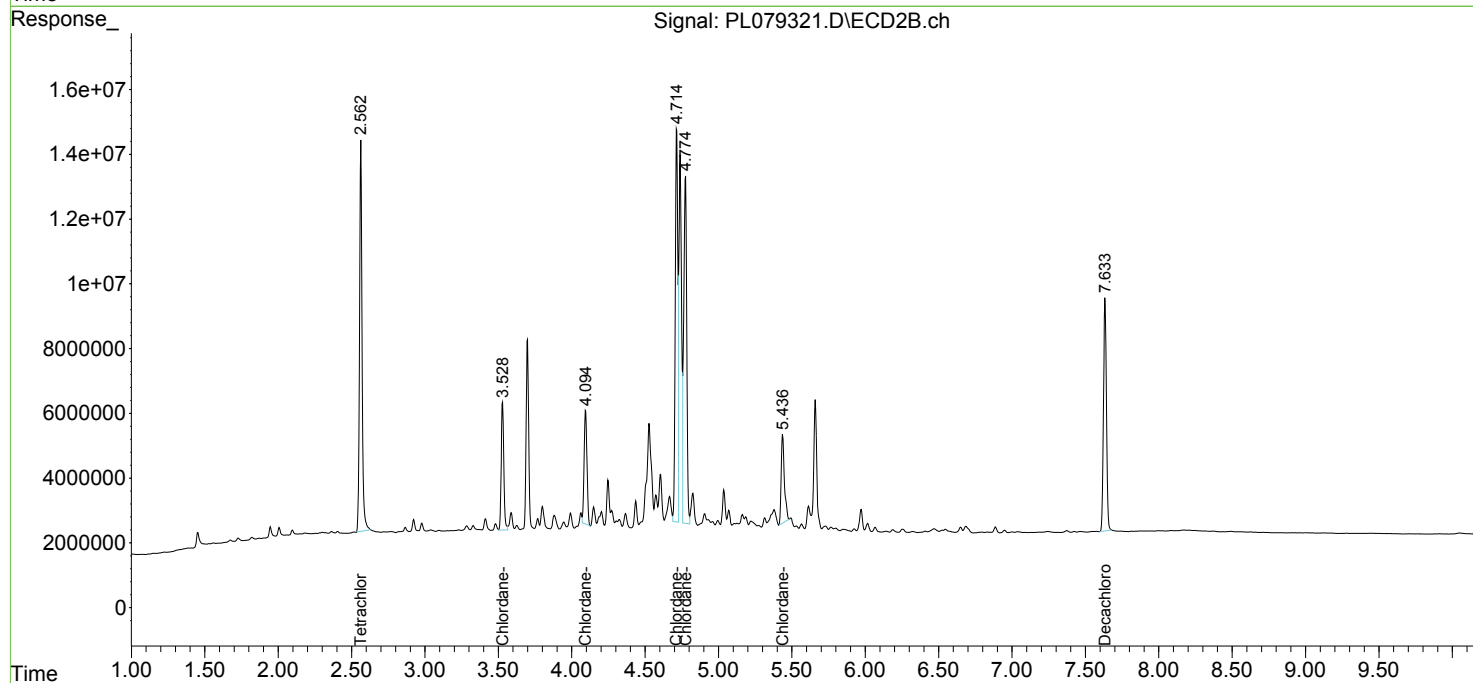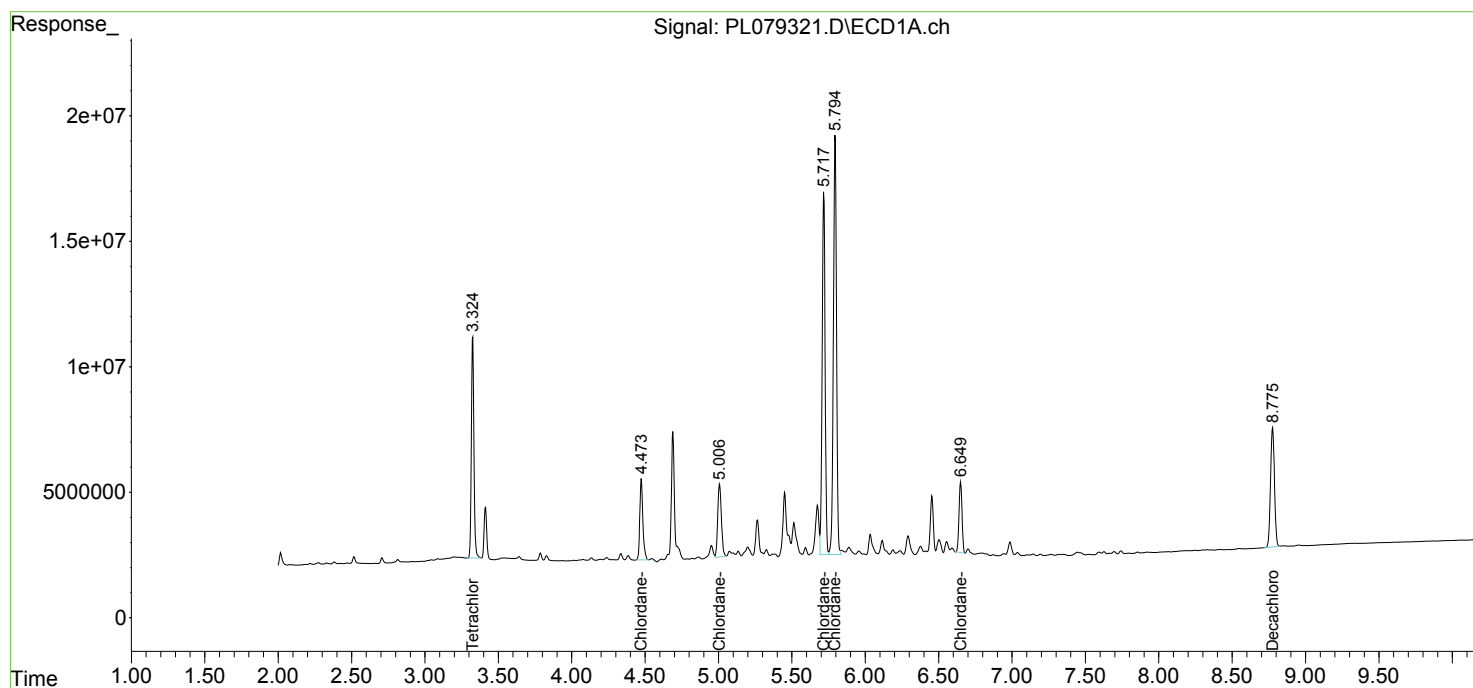


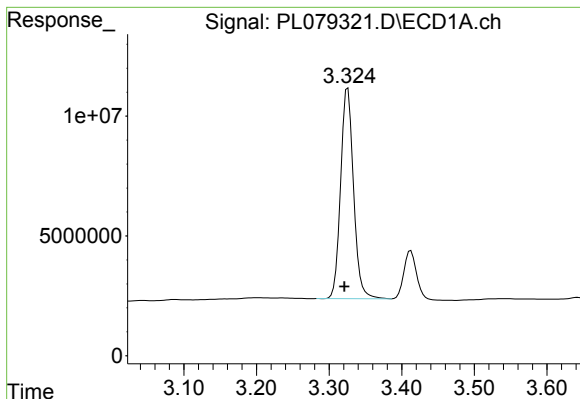

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: 0.005 min
Response: 108522686
Conc: 52.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

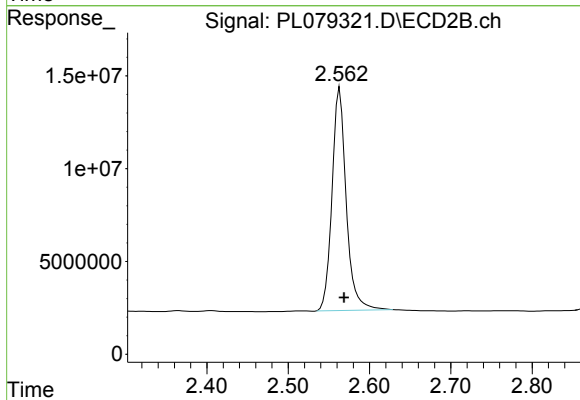


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: -0.005 min
Response: 146010735
Conc: 57.33 ng/ml

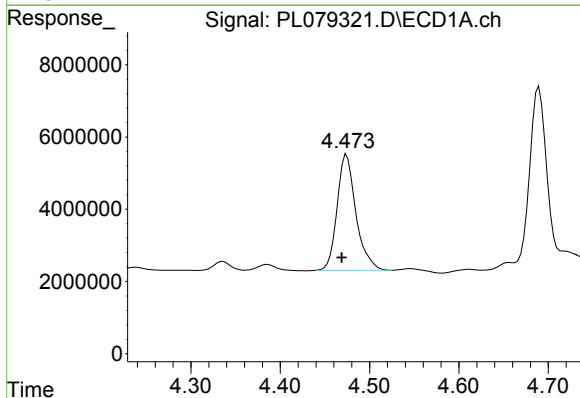


#23 Chlordane-1

R.T.: 4.474 min
Delta R.T.: 0.005 min
Response: 47008665
Conc: 536.49 ng/ml

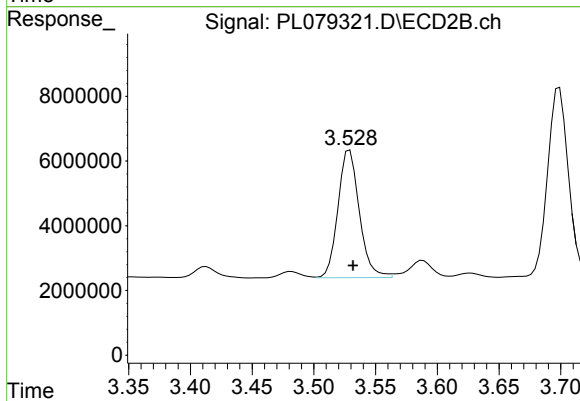

#23 Chlordane-1


R.T.: 3.529 min
Delta R.T.: -0.003 min
Response: 47489076
Conc: 459.64 ng/ml

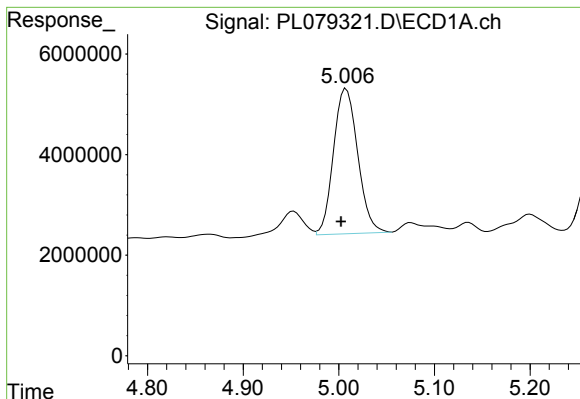

#24 Chlordane-2


R.T.: 5.008 min
Delta R.T.: 0.006 min
Response: 50774705
Conc: 498.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

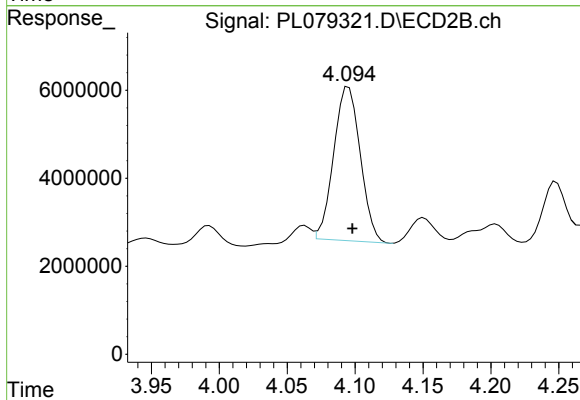


#24 Chlordane-2

R.T.: 4.095 min
Delta R.T.: -0.003 min
Response: 47644691
Conc: 448.66 ng/ml

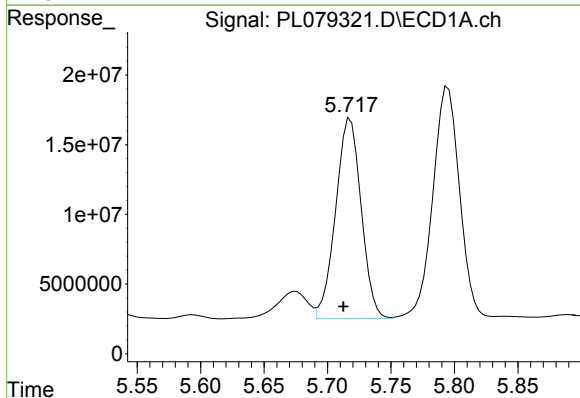


#25 Chlordane-3

R.T.: 5.718 min
Delta R.T.: 0.006 min
Response: 201494103
Conc: 523.09 ng/ml

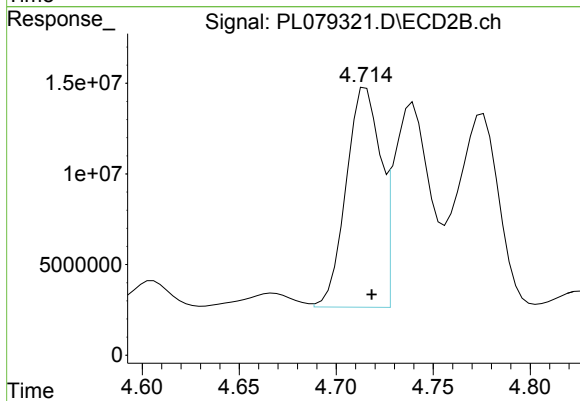

#25 Chlordane-3


R.T.: 4.715 min
Delta R.T.: -0.003 min
Response: 148549430
Conc: 466.23 ng/ml

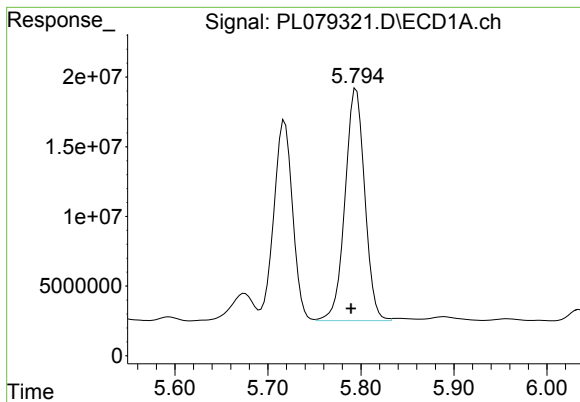

#26 Chlordane-4


R.T.: 5.795 min
Delta R.T.: 0.005 min
Response: 245260299
Conc: 518.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

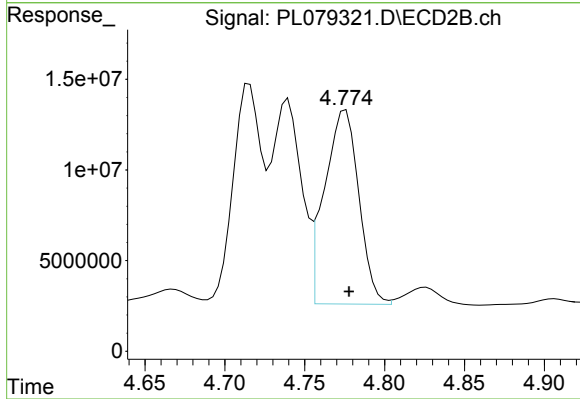


#26 Chlordane-4

R.T.: 4.776 min
Delta R.T.: -0.002 min
Response: 159504215
Conc: 464.81 ng/ml

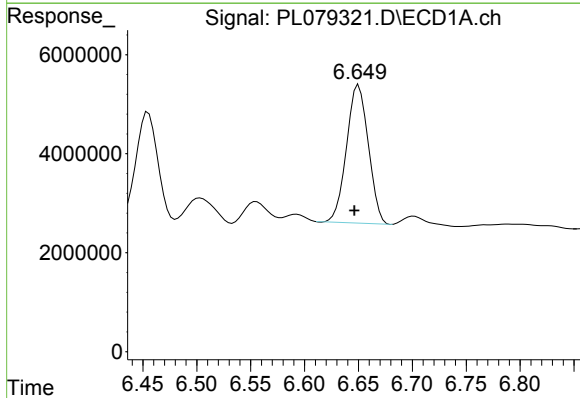


#27 Chlordane-5

R.T.: 6.650 min
Delta R.T.: 0.004 min
Response: 39353868
Conc: 530.41 ng/ml

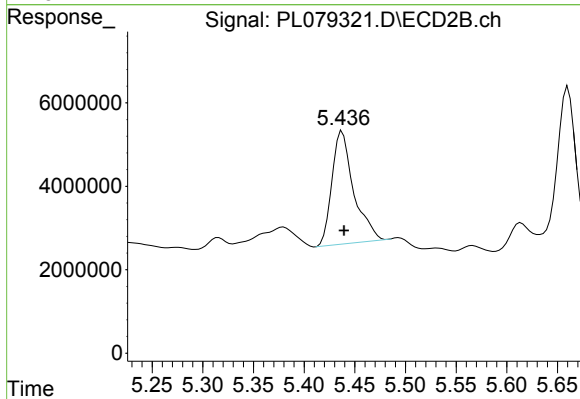

#27 Chlordane-5


R.T.: 5.438 min
Delta R.T.: -0.002 min
Response: 40695723
Conc: 477.26 ng/ml

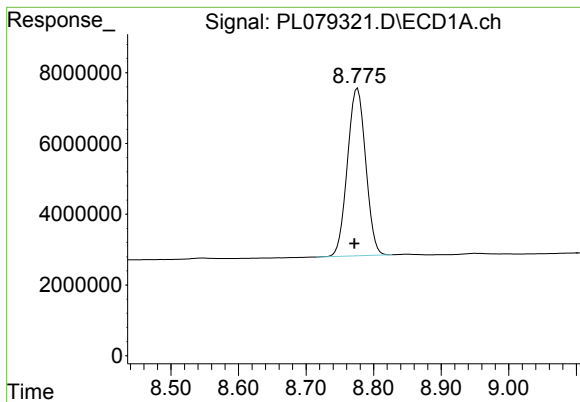

#28 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.004 min
Response: 88767578
Conc: 53.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

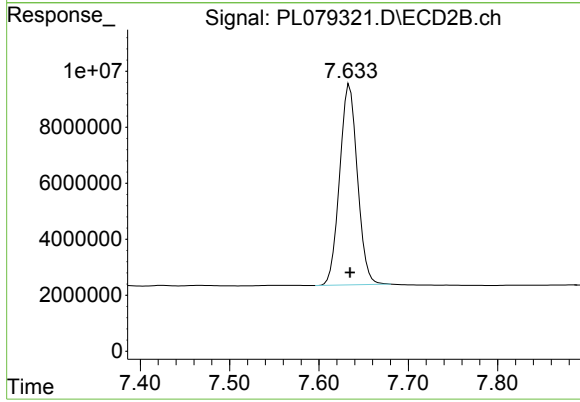

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: 0.000 min
Response: 99016075
Conc: 47.73 ng/ml