

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112122\
 Data File : PL079333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2022 15:38
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:25:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.566	102.2E6	141.1E6	49.091	55.409
28)	SA Decachlor...	8.773	7.635	84748494	100.5E6	50.664	48.462
Target Compounds							
23)	Chlordane-1	4.470	3.531	43910186	46506532	501.131	450.130
24)	Chlordane-2	5.004	4.097	48703843	48265710	478.494	454.505
25)	Chlordane-3	5.713	4.718	191.5E6	148.1E6	497.093	464.757
26)	Chlordane-4	5.791	4.778	232.7E6	157.5E6	491.900	459.007
27)	Chlordane-5	6.647	5.439	37705265	39897974	508.189	467.907



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112122\
Data File : PL079333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2022 15:38
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:25:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

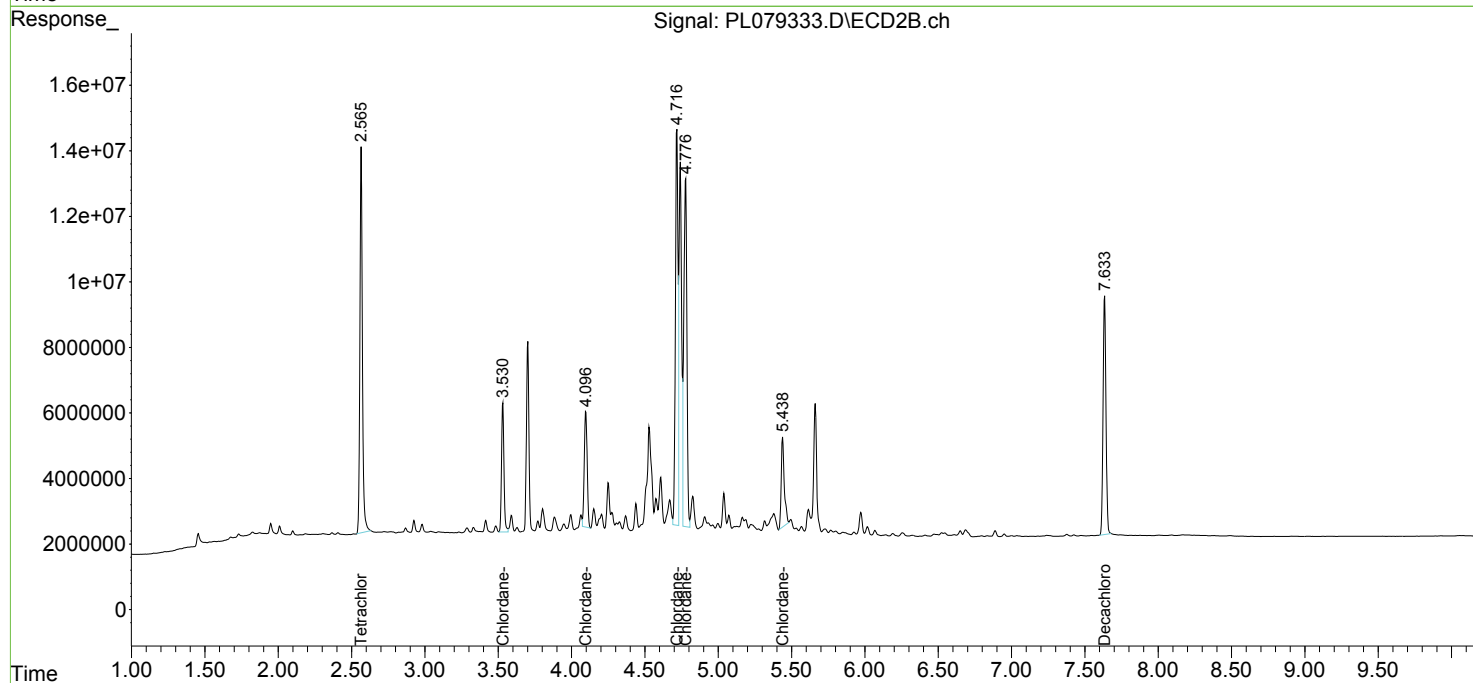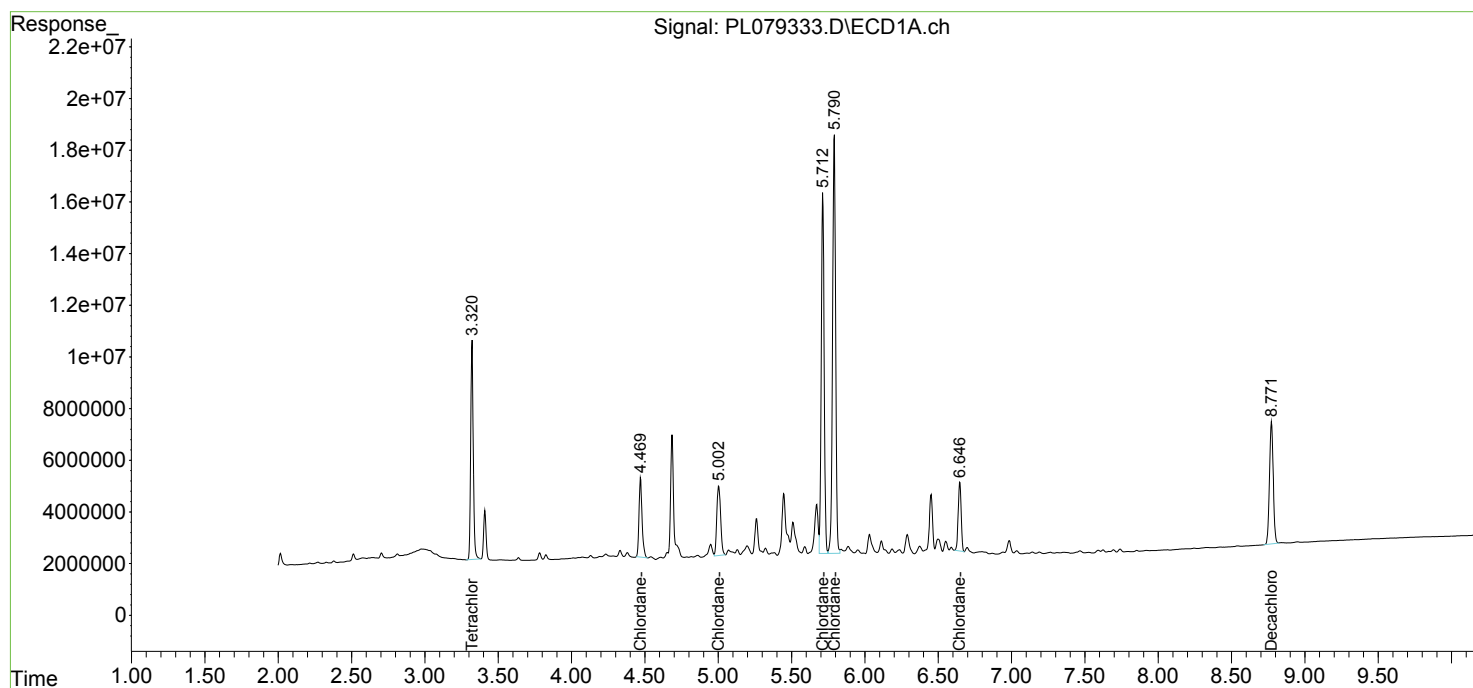


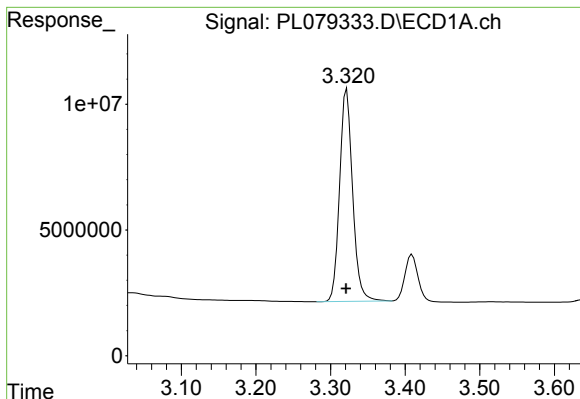

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 102227306
Conc: 49.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

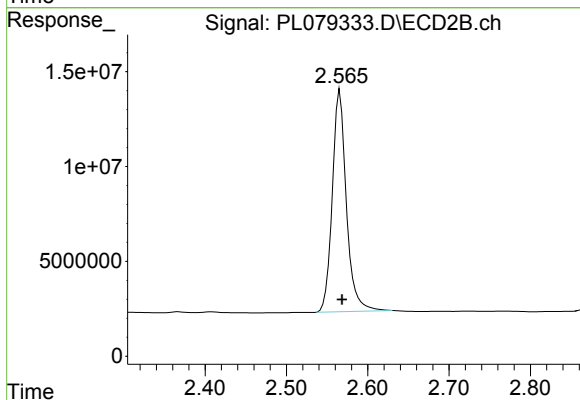


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: -0.003 min
Response: 141119128
Conc: 55.41 ng/ml

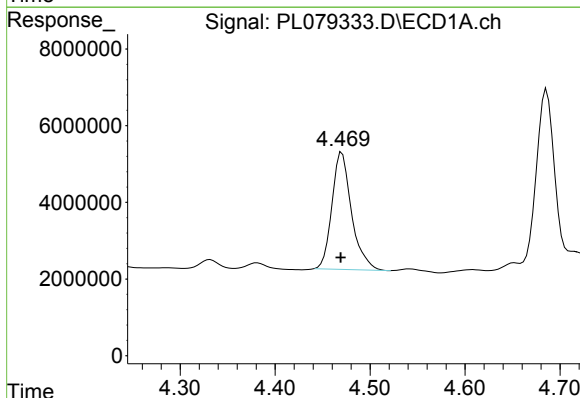


#23 Chlordane-1

R.T.: 4.470 min
Delta R.T.: 0.001 min
Response: 43910186
Conc: 501.13 ng/ml

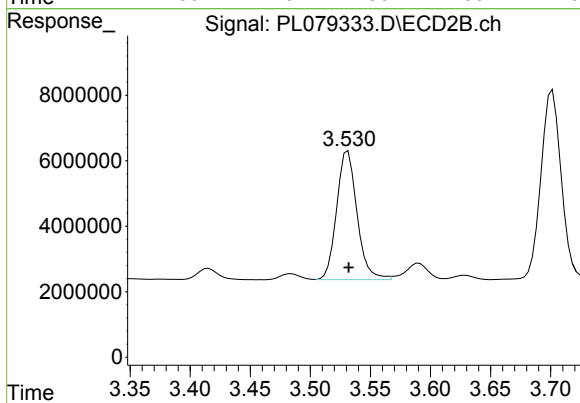

#23 Chlordane-1


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 46506532
Conc: 450.13 ng/ml

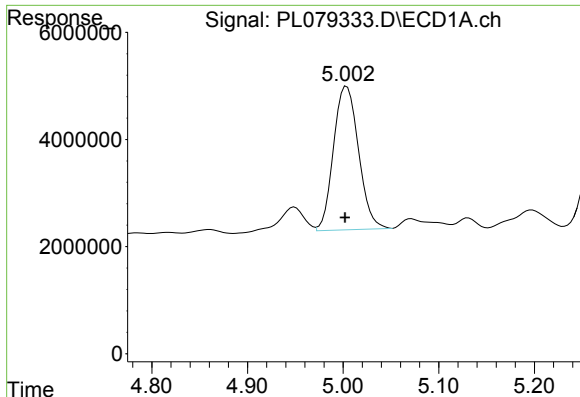

#24 Chlordane-2


R.T.: 5.004 min
Delta R.T.: 0.002 min
Response: 48703843
Conc: 478.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

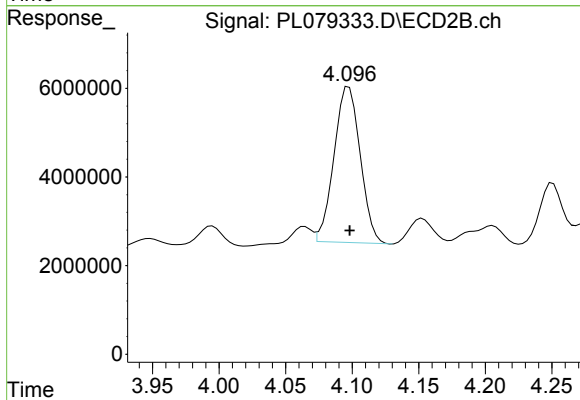


#24 Chlordane-2

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 48265710
Conc: 454.51 ng/ml

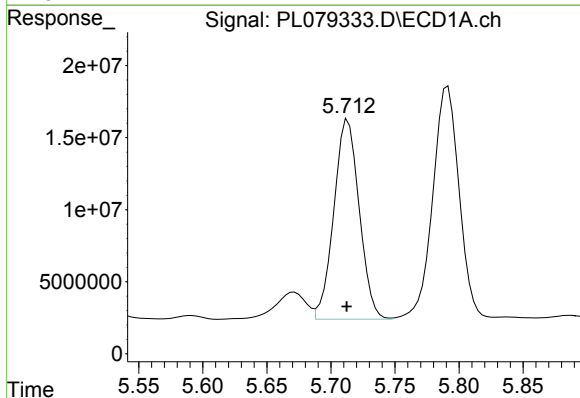


#25 Chlordane-3

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 191481206
Conc: 497.09 ng/ml

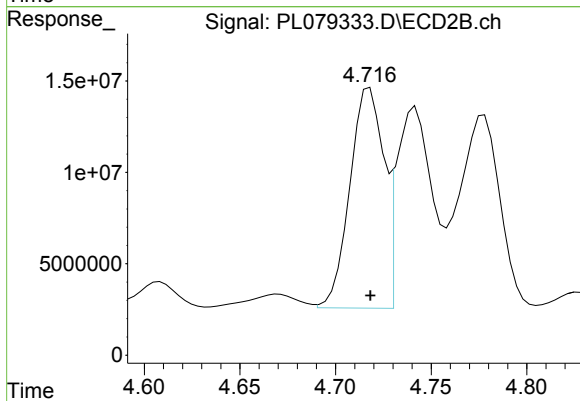

#25 Chlordane-3


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 148078713
Conc: 464.76 ng/ml

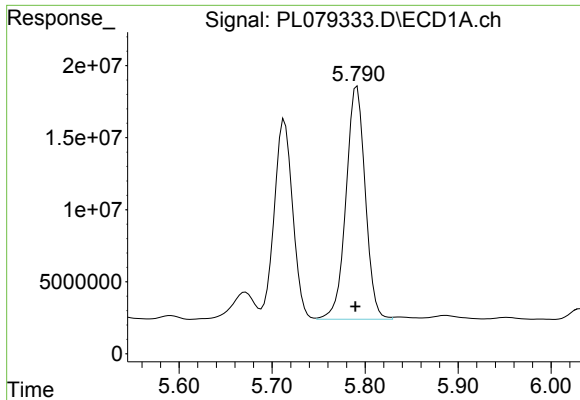

#26 Chlordane-4


R.T.: 5.791 min
Delta R.T.: 0.002 min
Response: 232748957
Conc: 491.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

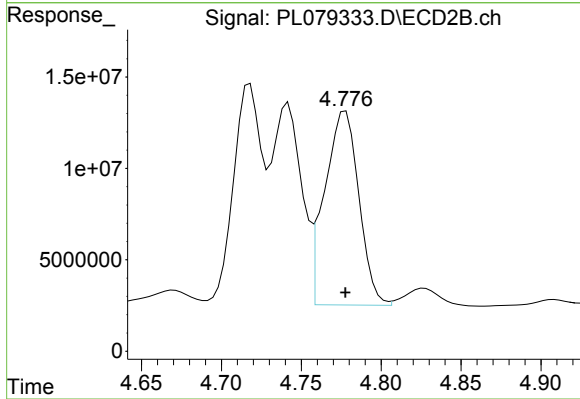


#26 Chlordane-4

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 157514269
Conc: 459.01 ng/ml

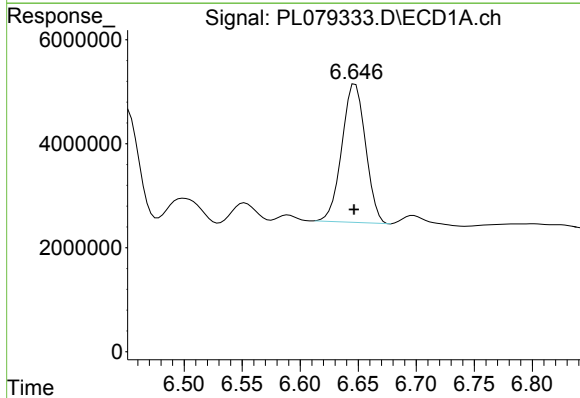


#27 Chlordane-5

R.T.: 6.647 min
Delta R.T.: 0.001 min
Response: 37705265
Conc: 508.19 ng/ml

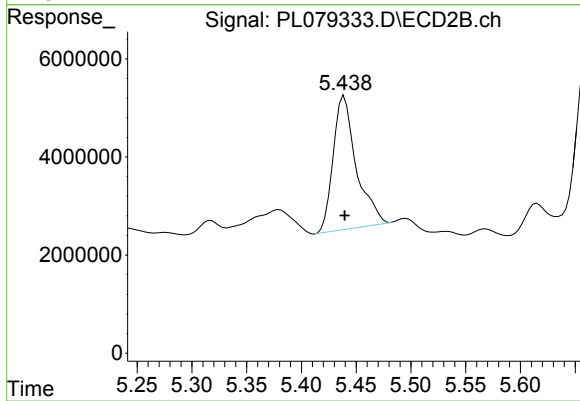

#27 Chlordane-5


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 39897974
Conc: 467.91 ng/ml

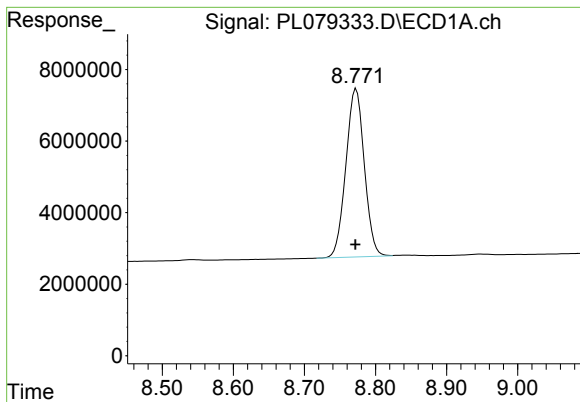

#28 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.001 min
Response: 84748494
Conc: 50.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

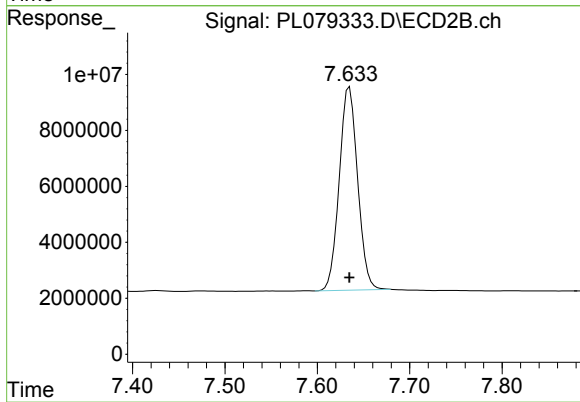

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: 0.000 min
Response: 100532794
Conc: 48.46 ng/ml