

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112123\
 Data File : PL086786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 14:40
 Operator : AR\AJ
 Sample : 05503-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 358

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2023
 Supervised By :Ankita Jodhani 11/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 20:21:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.349	2.616	19996940	9449026	6.159m	9.596 #
28) SA Decachlor...	8.849	7.764	29183849	15254361	9.970	12.632 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112123\
Data File : PL086786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 14:40
Operator : AR\AJ
Sample : 05503-02
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
358


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2023
Supervised By :Ankita Jodhani 11/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 20:21:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

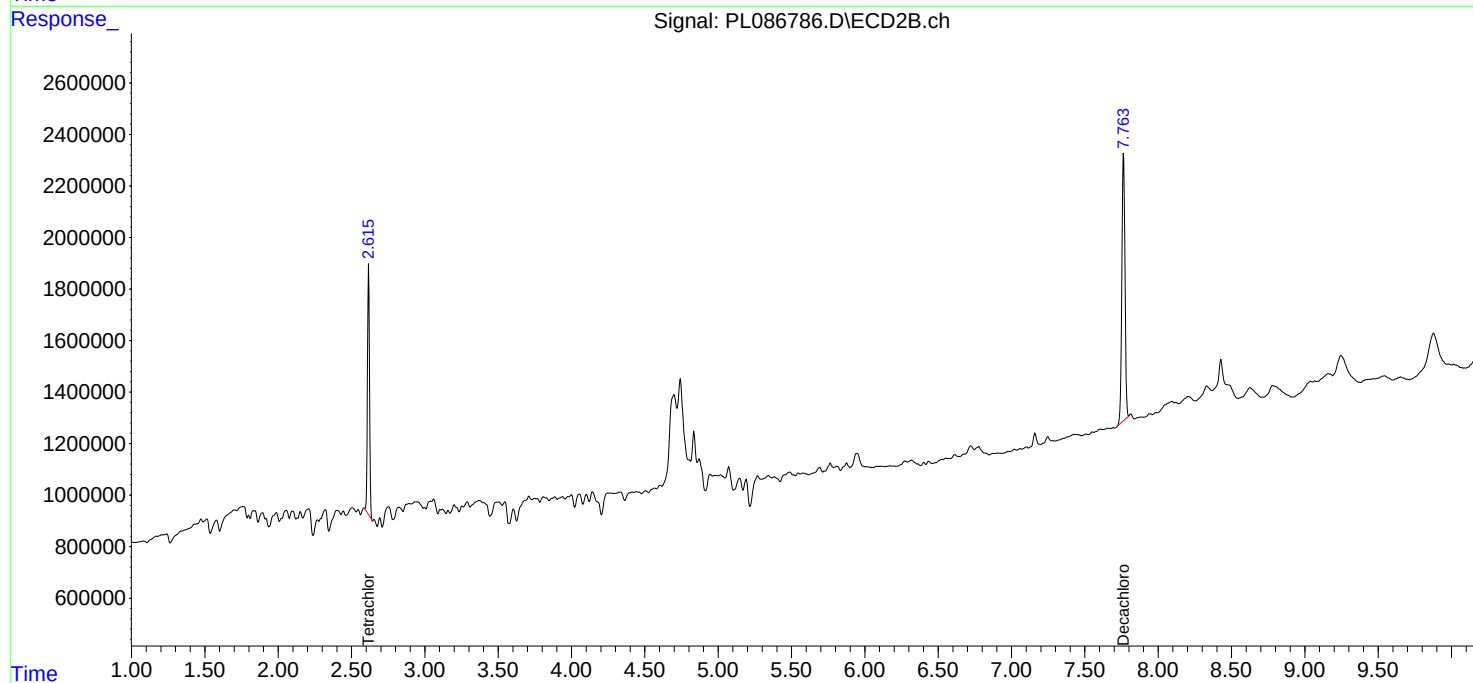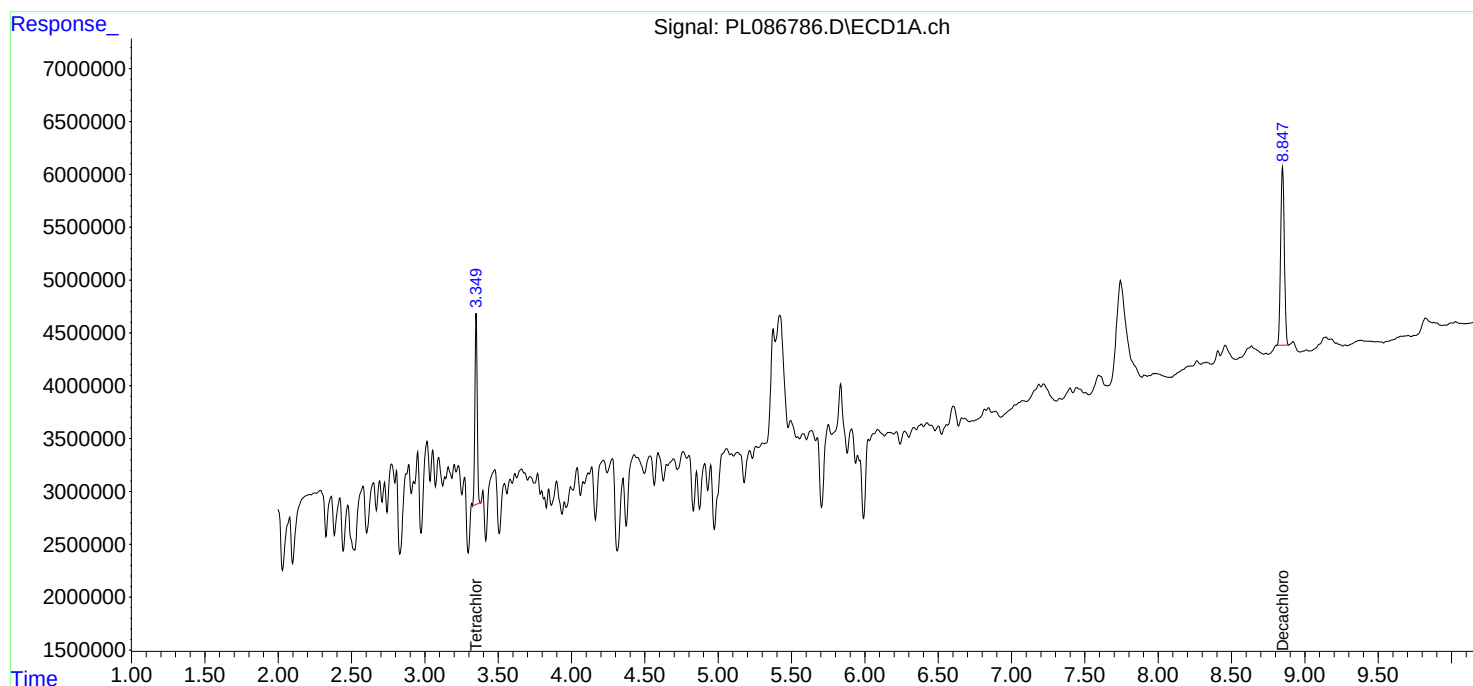

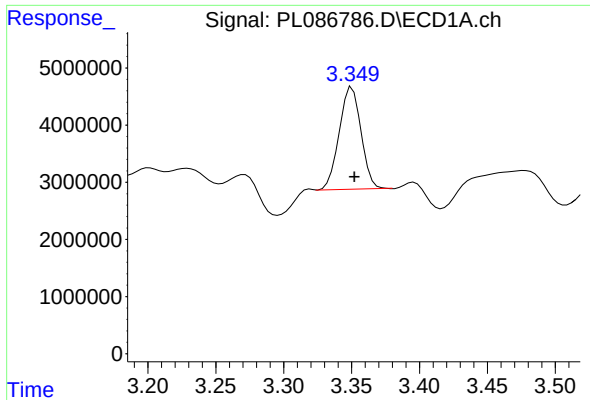


#1 Tetrachloro-m-xylene

R.T.: 3.349 min
Delta R.T.: -0.003 min
Response: 19996940
Conc: 6.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
358


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2023
Supervised By :Ankita Jodhani 11/22/2023

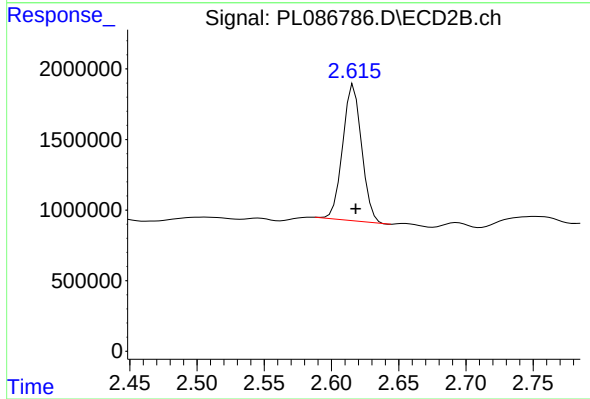


#1 Tetrachloro-m-xylene

R.T.: 2.616 min
Delta R.T.: -0.001 min
Response: 9449026
Conc: 9.60 ng/ml

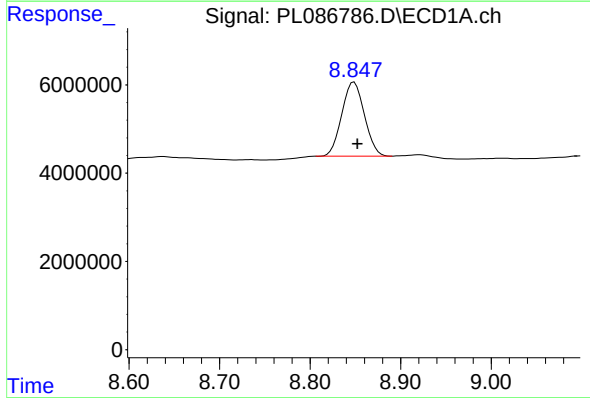

#28 Decachlorobiphenyl

R.T.: 8.849 min
Delta R.T.: -0.004 min
Response: 29183849
Conc: 9.97 ng/ml

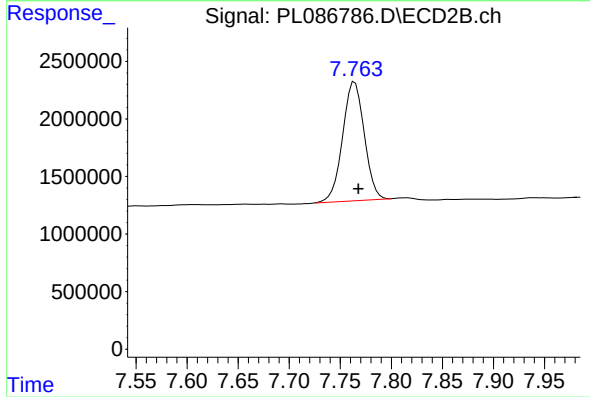

#28 Decachlorobiphenyl

R.T.: 7.764 min
Delta R.T.: -0.004 min
Response: 15254361
Conc: 12.63 ng/ml