

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
 Data File : PL042405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 12:16
 Operator : AJ\SJ
 Sample : PB115002BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:40:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.100	110.2E6	57841795	18.737	20.111
28)	SA Decachlor...	8.203	9.231	124.4E6	50103952	19.741	20.774
Target Compounds							
2)	A alpha-BHC	3.896	0.000	4608848	0	0.511	N.D. #
6)	B beta-BHC	4.399f	0.000	4580082	0	1.293	N.D. #
8)	B Heptachlo...	0.000	5.991	0	10583546	N.D.	2.952 #
10)	B gamma-Chl...	5.368	0.000	1487755	0	0.195	N.D. #
14)	MA Endrin	5.969f	0.000	1048627	0	0.160	N.D. #
17)	MA 4,4'-DDT	6.369	0.000	1632024	0	0.293	N.D. #
23)	Chlordane-1	4.362	0.000	1768212	0	6.396	N.D. #
25)	Chlordane-3	5.368	0.000	1487755	0	1.697	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
Data File : PL042405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 12:16
Operator : AJ\SJ
Sample : PB115002BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:40:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

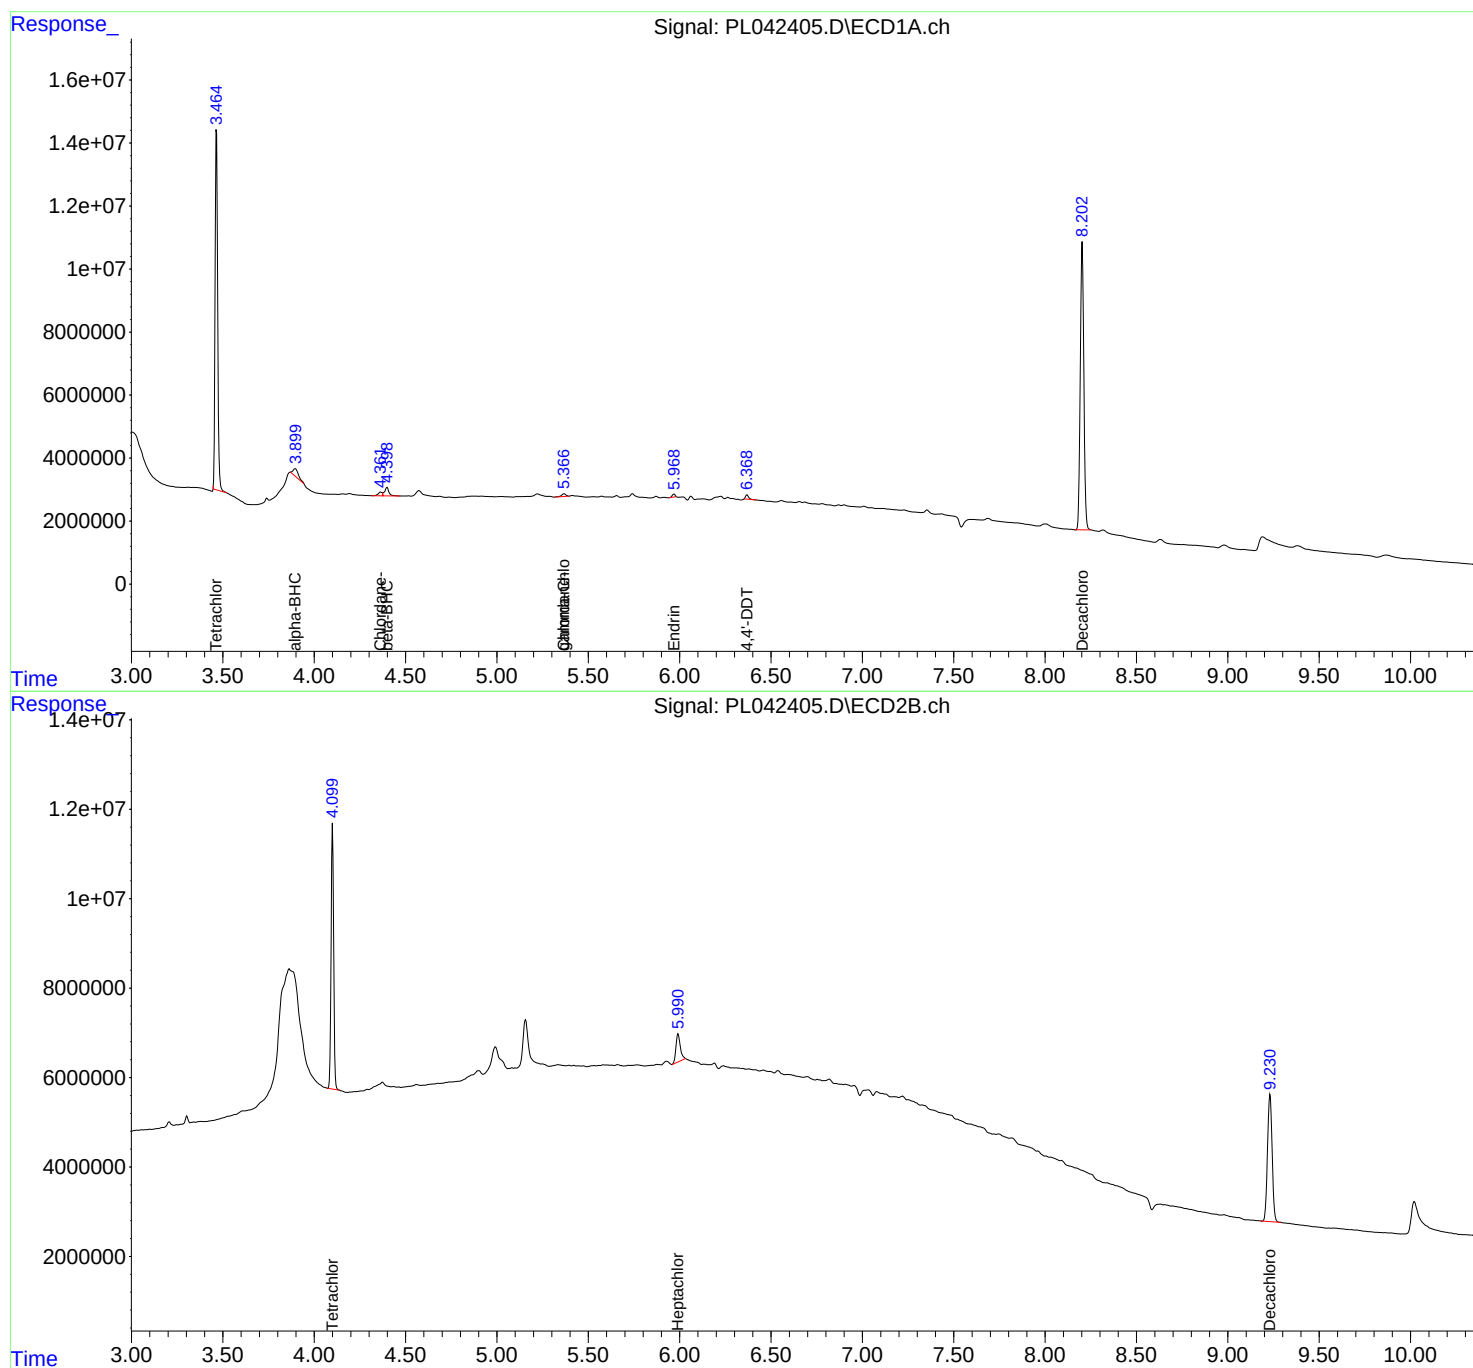


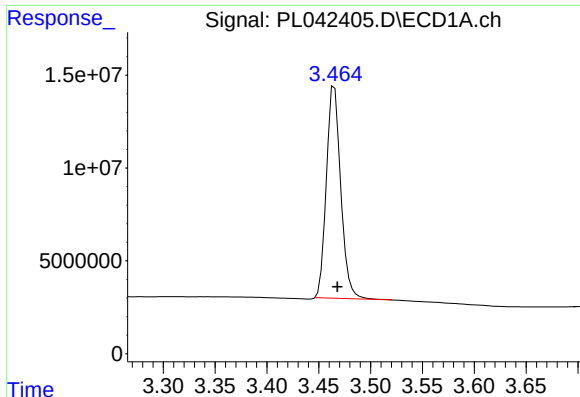

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.003 min
Response: 110236387
Conc: 18.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

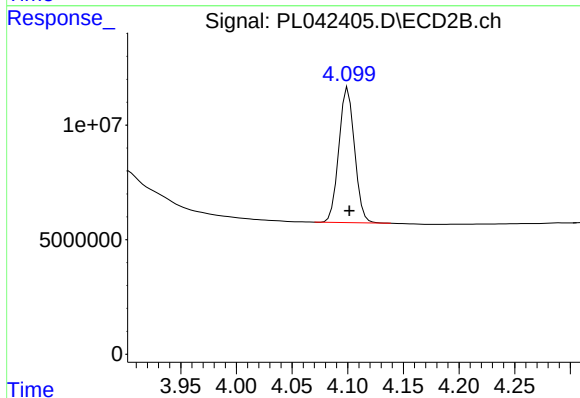


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.001 min
Response: 57841795
Conc: 20.11 ng/ml

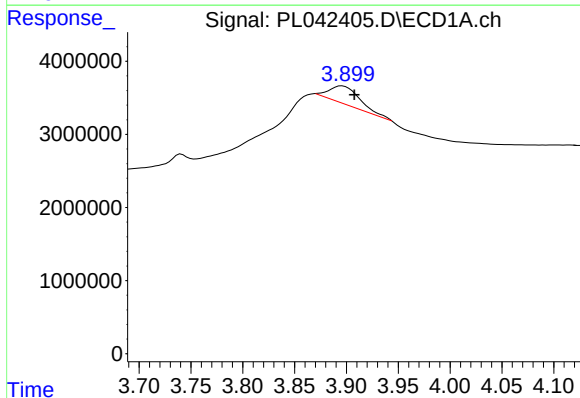


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: -0.012 min
Response: 4608848
Conc: 0.51 ng/ml

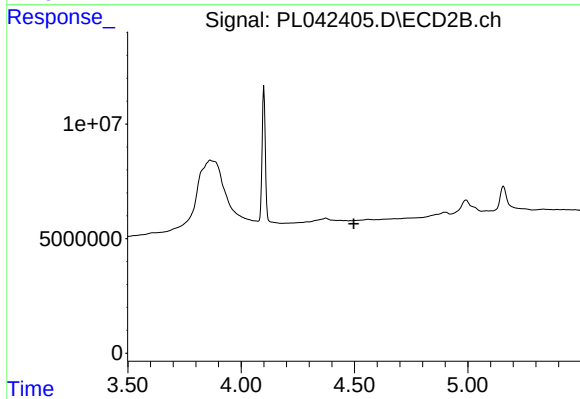

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

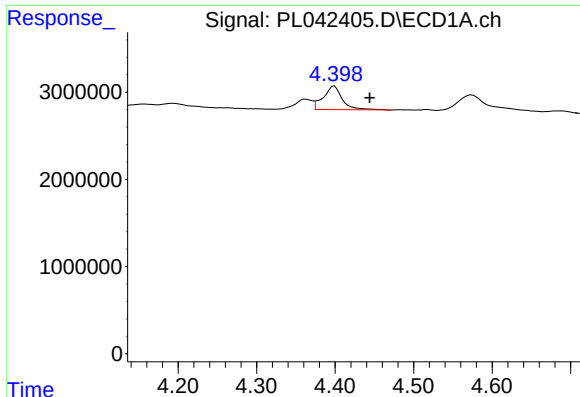

#6 beta-BHC


R.T.: 4.399 min
Delta R.T.: -0.045 min
Response: 4580082
Conc: 1.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

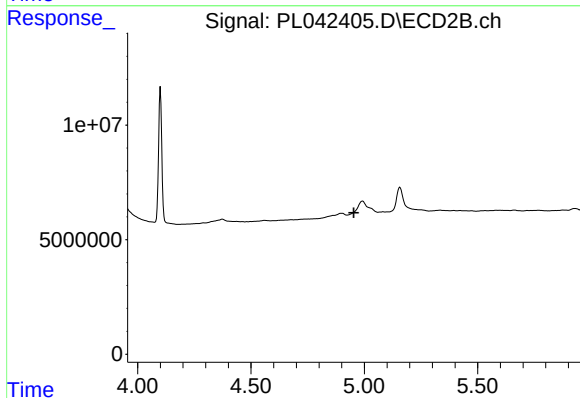


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

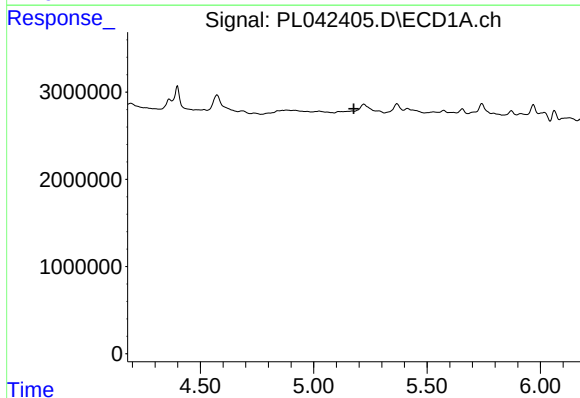


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

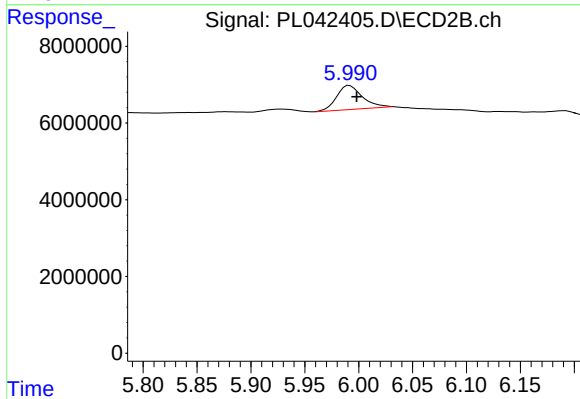

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: -0.007 min
Response: 10583546
Conc: 2.95 ng/ml

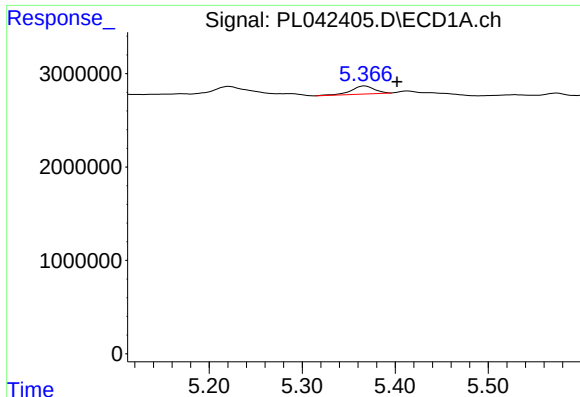

#10 gamma-Chlordane


R.T.: 5.368 min
Delta R.T.: -0.035 min
Response: 1487755
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

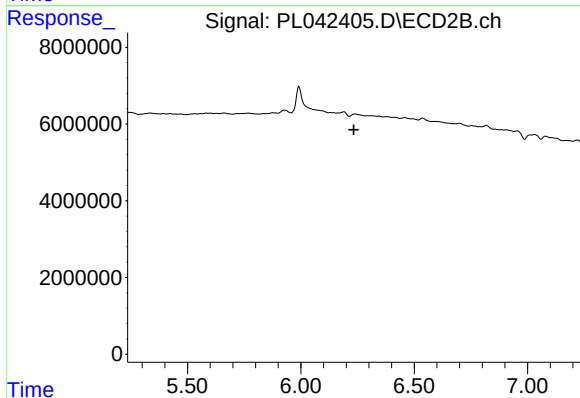


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

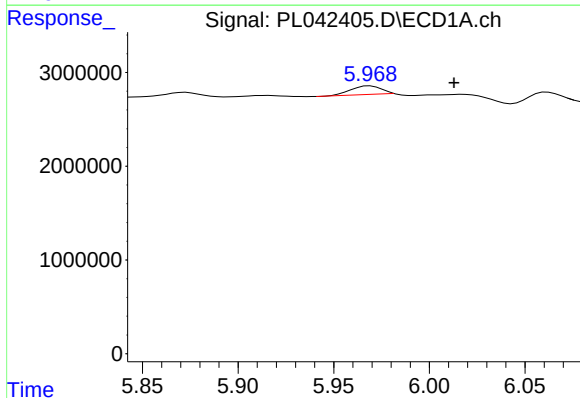


#14 Endrin

R.T.: 5.969 min
Delta R.T.: -0.044 min
Response: 1048627
Conc: 0.16 ng/ml

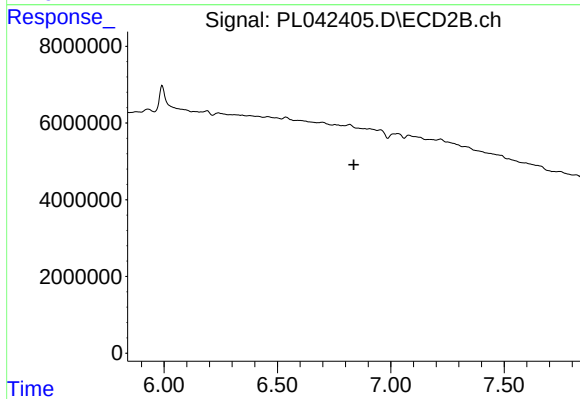

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

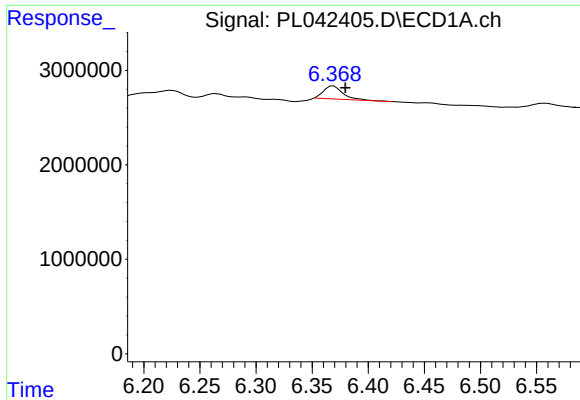

#17 4,4'-DDT


R.T.: 6.369 min
Delta R.T.: -0.011 min
Response: 1632024
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

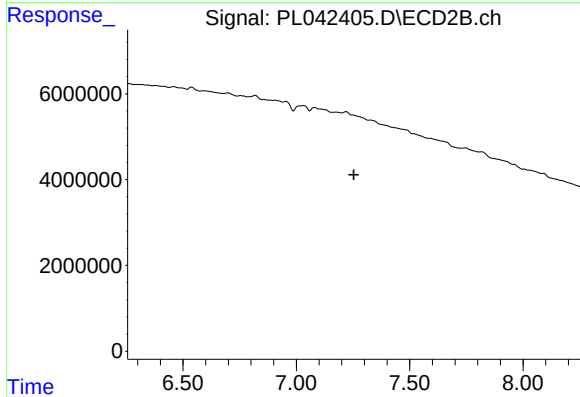


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

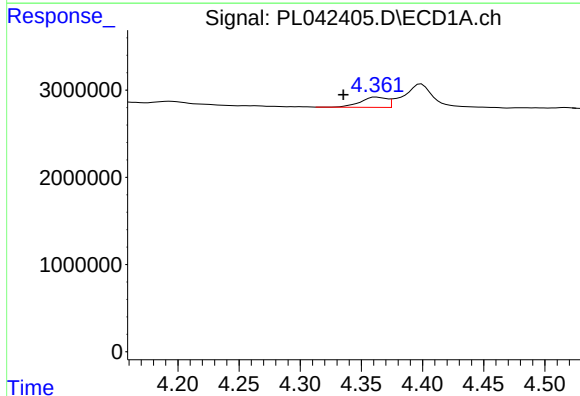


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.027 min
Response: 1768212
Conc: 6.40 ng/ml

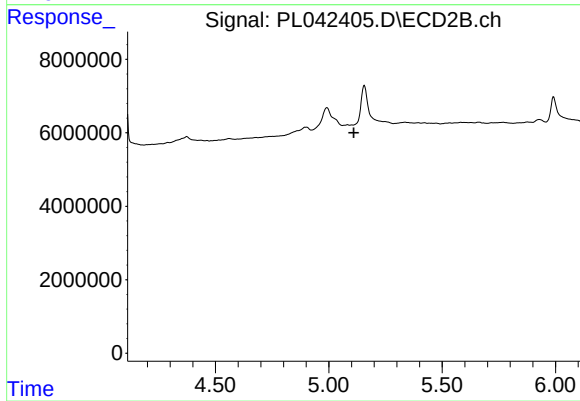

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

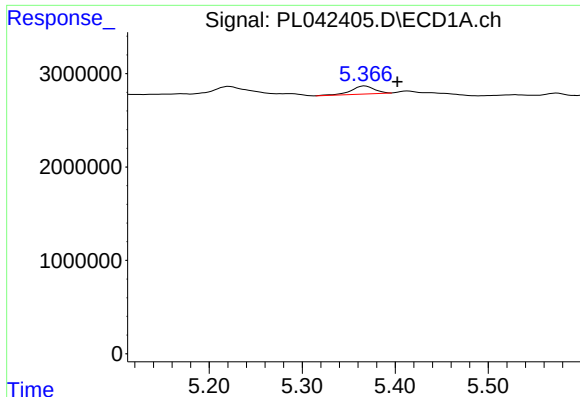

#25 Chlordane-3


R.T.: 5.368 min
Delta R.T.: -0.035 min
Response: 1487755
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

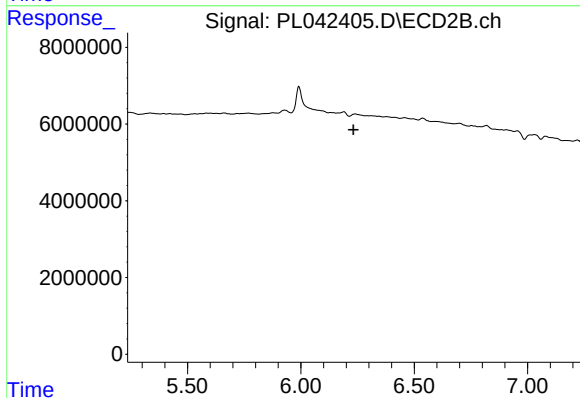


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

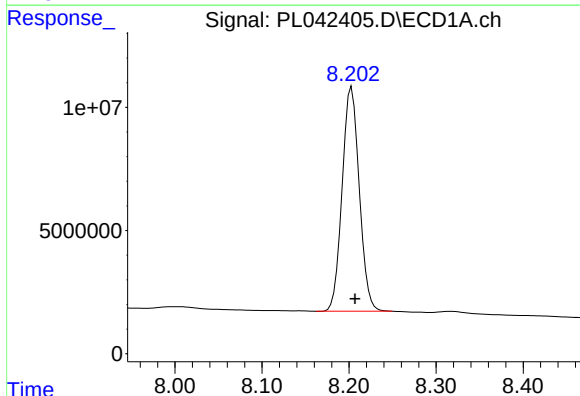

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 124407575
Conc: 19.74 ng/ml

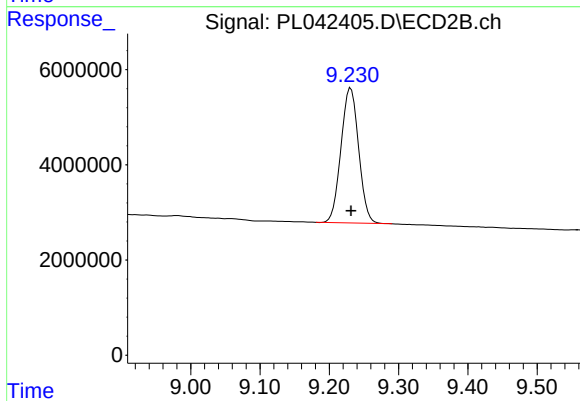

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 50103952
Conc: 20.77 ng/ml