

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
 Data File : PL042421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 16:19
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:42:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	120.6E6	61502723	20.504	21.384
28)	SA Decachlor...	8.205	9.231	121.9E6	51008112	19.345	21.149
Target Compounds							
6)	B beta-BHC	4.400f	0.000	3106337	0	0.877	N.D. #
8)	B Heptachlo...	5.218f	5.994	2023999	3797949	0.267	1.059 #
23)	Chlordane-1	4.364	0.000	1414833	0	5.117	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
Data File : PL042421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 16:19
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:42:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

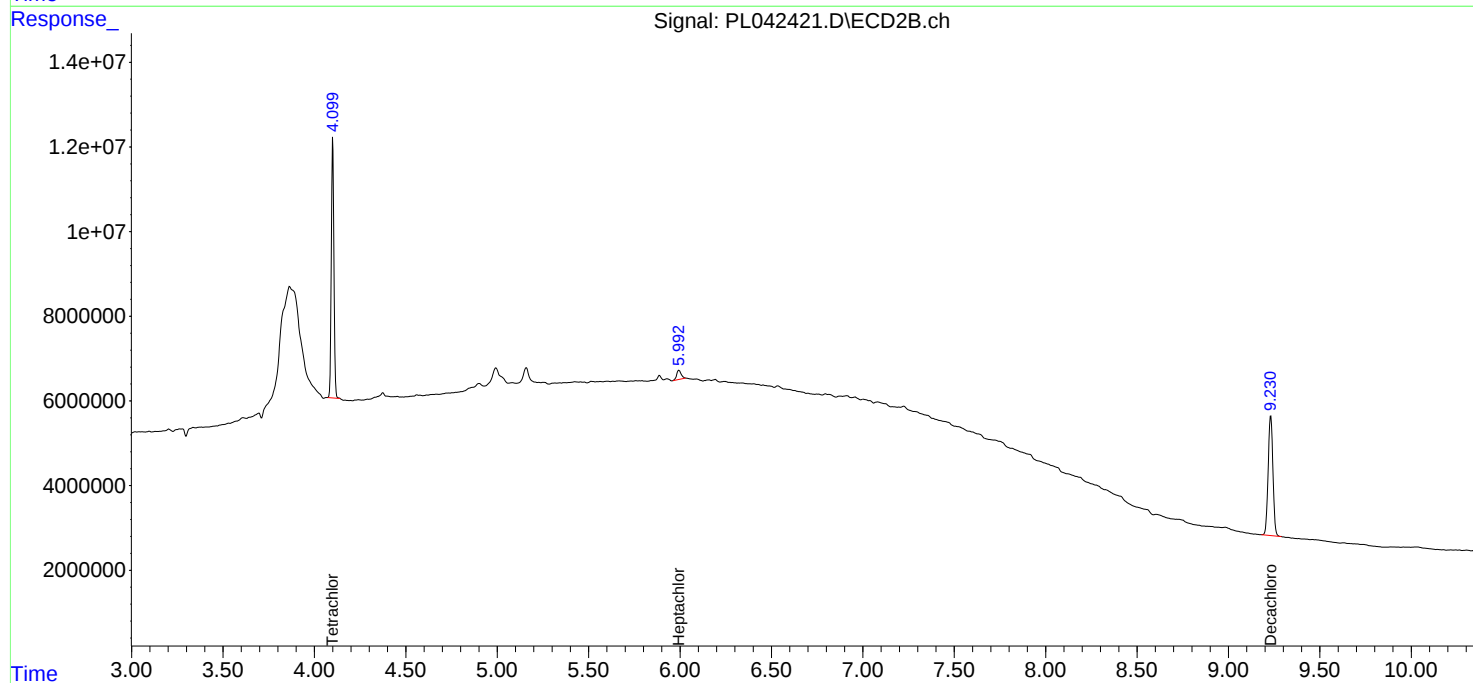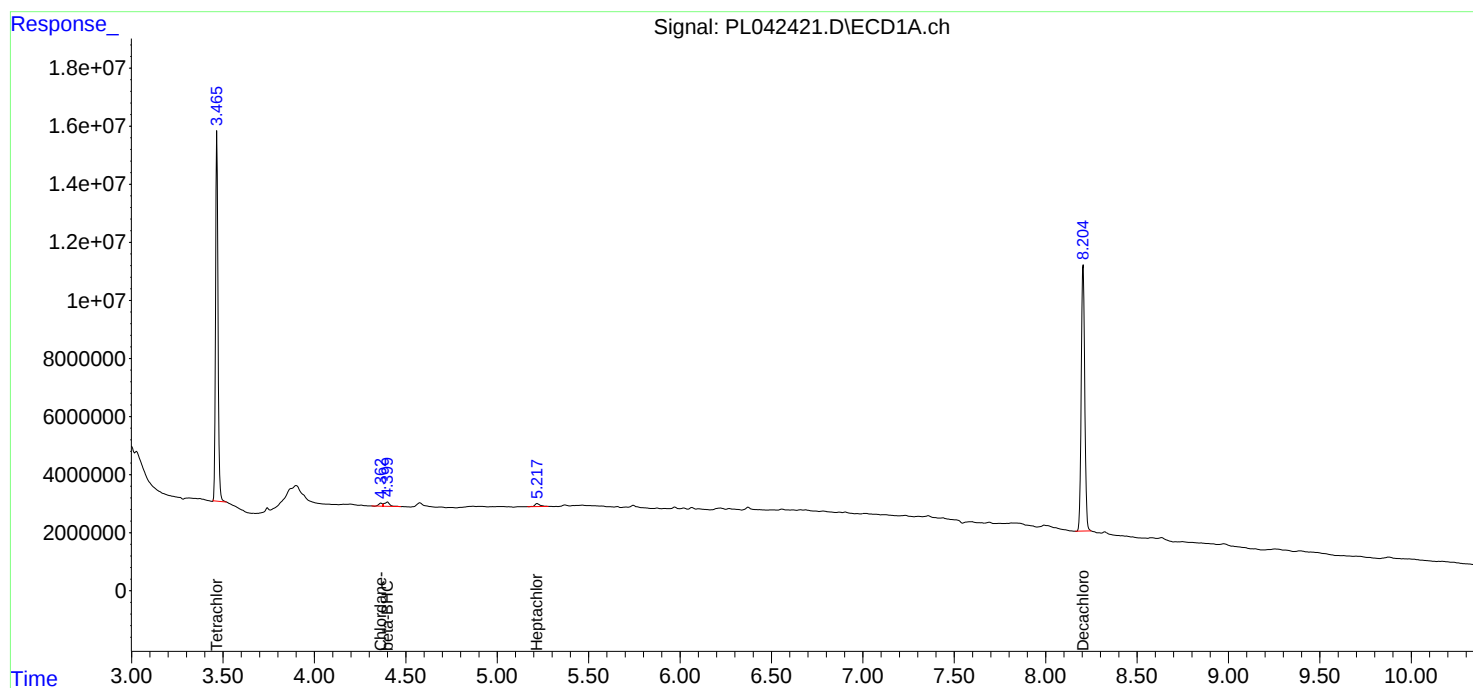


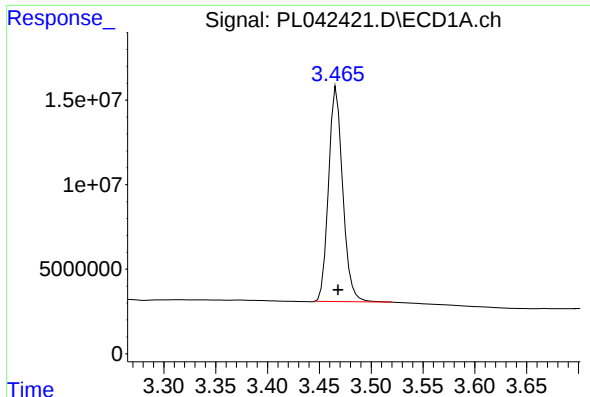

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 120633346
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

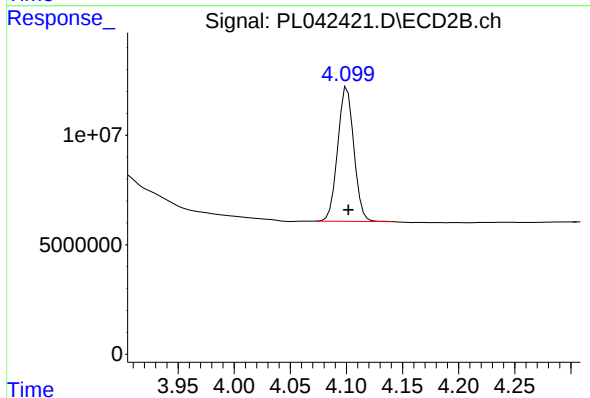


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 61502723
Conc: 21.38 ng/ml

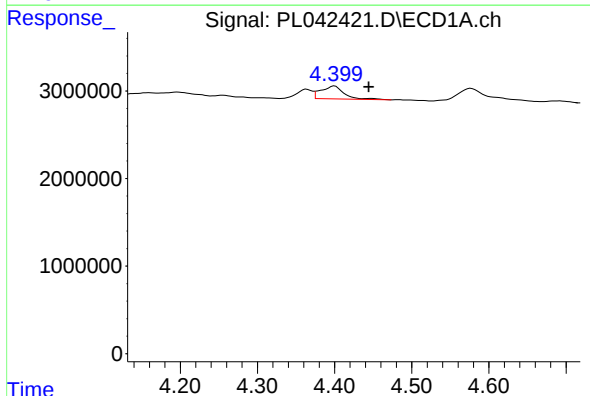


#6 beta-BHC

R.T.: 4.400 min
Delta R.T.: -0.044 min
Response: 3106337
Conc: 0.88 ng/ml

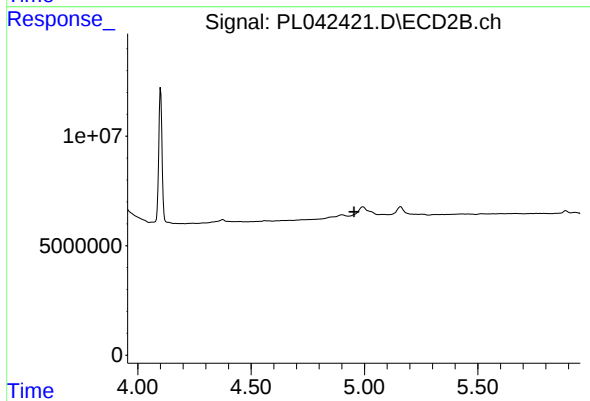

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

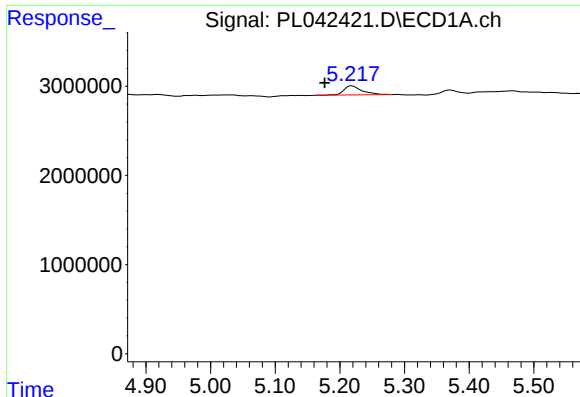

#8 Heptachlor epoxide


R.T.: 5.218 min
Delta R.T.: 0.041 min
Response: 2023999
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

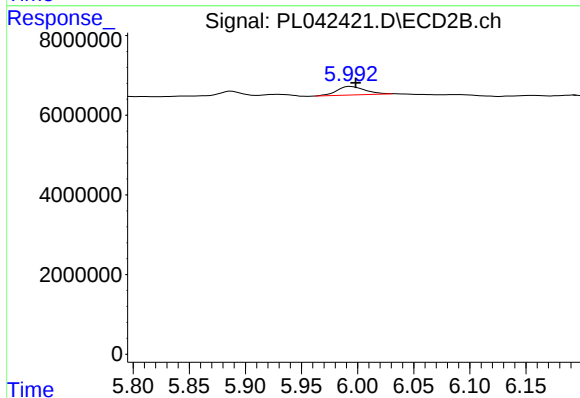


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.005 min
Response: 3797949
Conc: 1.06 ng/ml

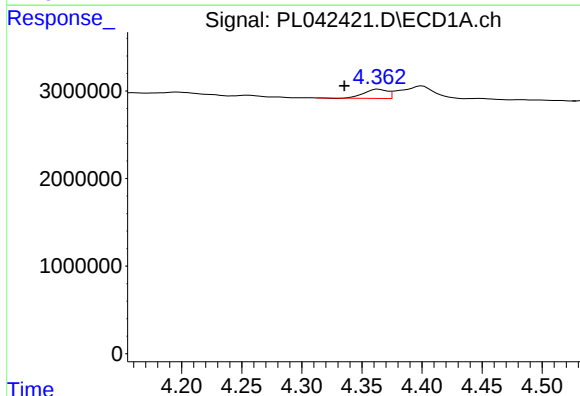


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.028 min
Response: 1414833
Conc: 5.12 ng/ml

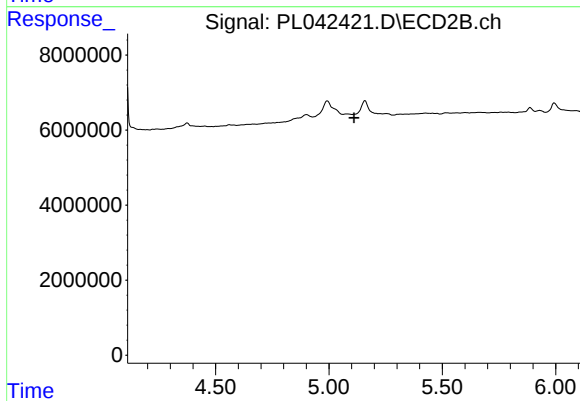

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.111 min
Response: 0
Conc: N.D.

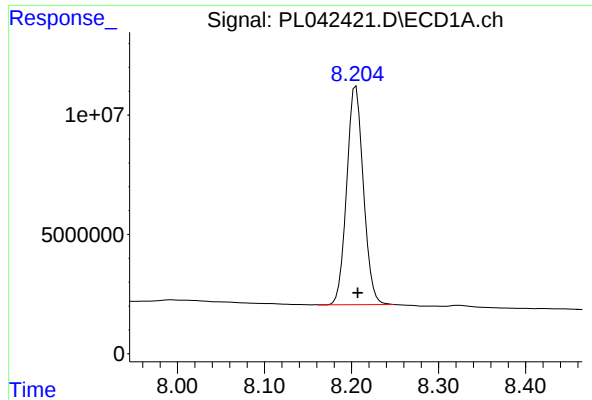

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 121914929
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

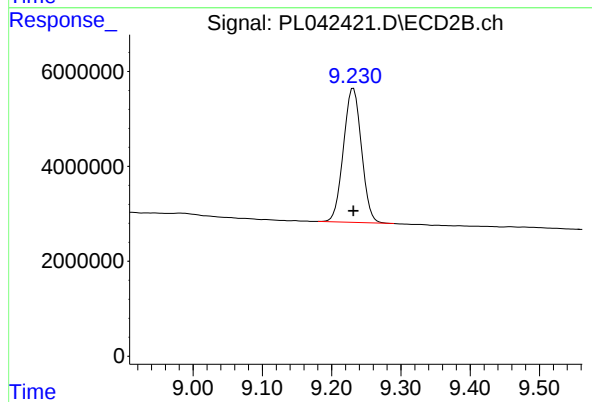

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 51008112
Conc: 21.15 ng/ml