

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
 Data File : PL042431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 19:04
 Operator : AJ\SJ
 Sample : J5768-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:43:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	118.5E6	61785972	20.144	21.482
28)	SA Decachlor...	8.205	9.231	125.0E6	52886921	19.841	21.928
Target Compounds							
2)	A alpha-BHC	0.000	4.452f	0	2215975	N.D.	0.517 #
6)	B beta-BHC	4.402f	0.000	15265934	0	4.309	N.D. #
8)	B Heptachlo...	0.000	5.995	0	5064000	N.D.	1.412 #
13)	MA Dieldrin	5.743	0.000	2744473	0	0.373	N.D. #
17)	MA 4,4'-DDT	6.373	0.000	1838493	0	0.330	N.D. #
23)	Chlordane-1	4.402	0.000	15265934	0	55.217	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
Data File : PL042431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 19:04
Operator : AJ\SJ
Sample : J5768-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:43:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

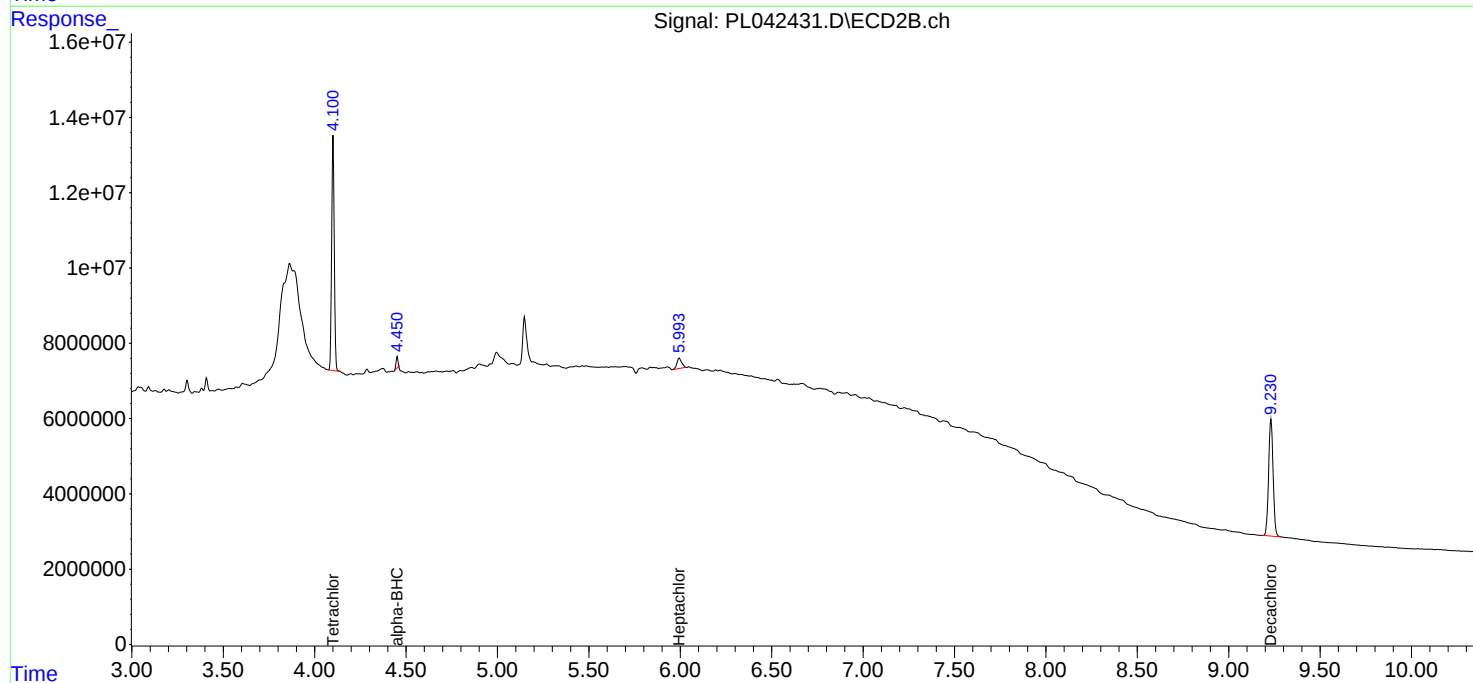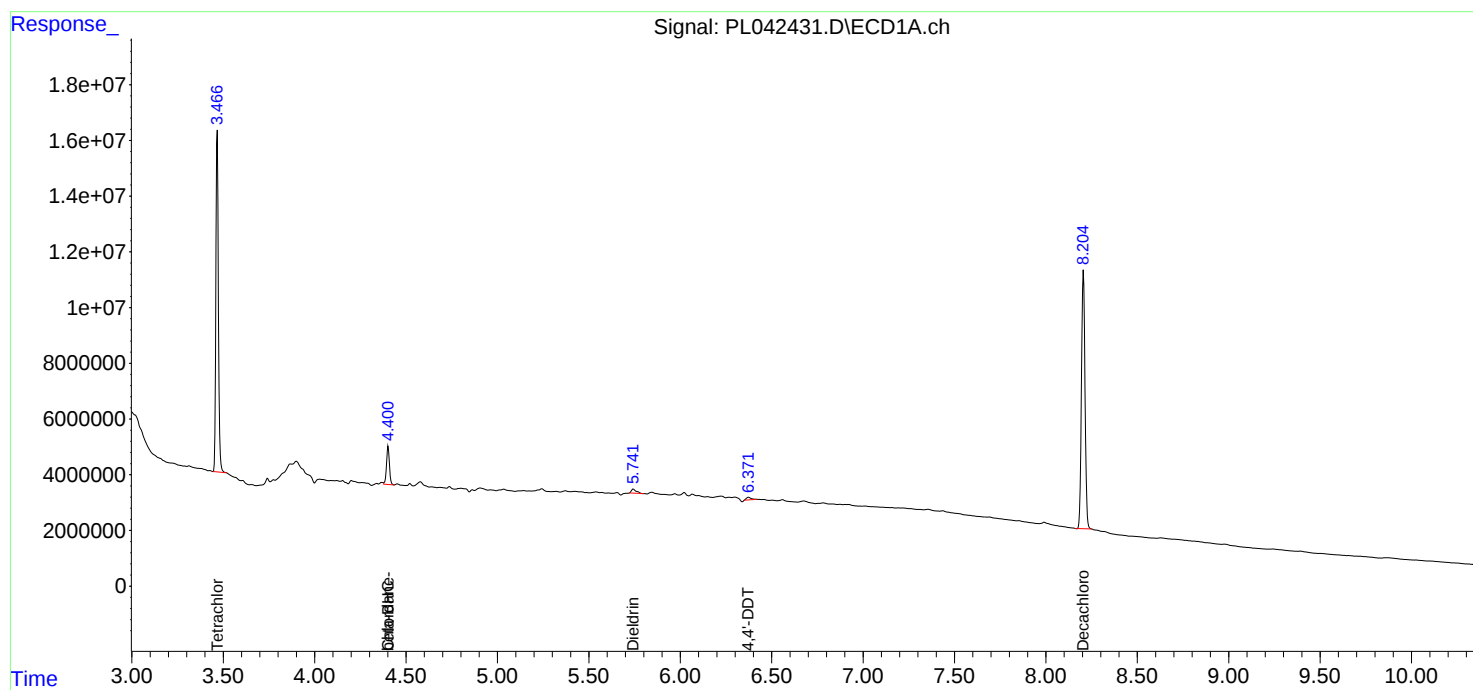


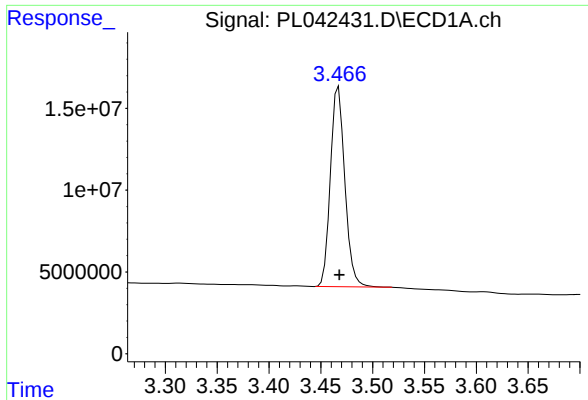

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 118515743
Conc: 20.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

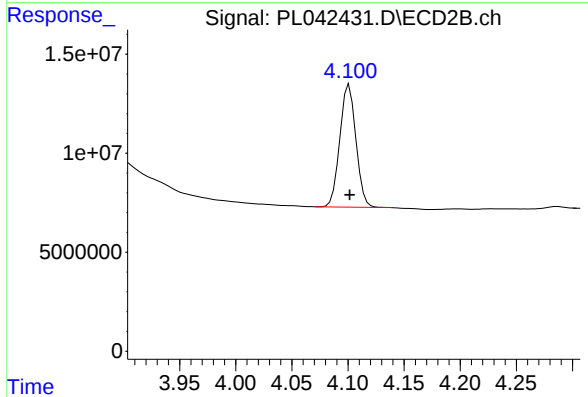


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 61785972
Conc: 21.48 ng/ml

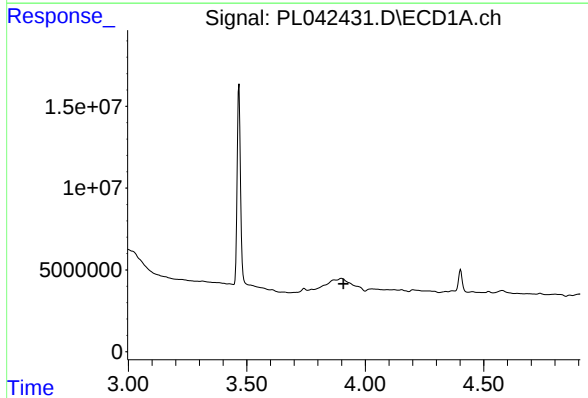


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

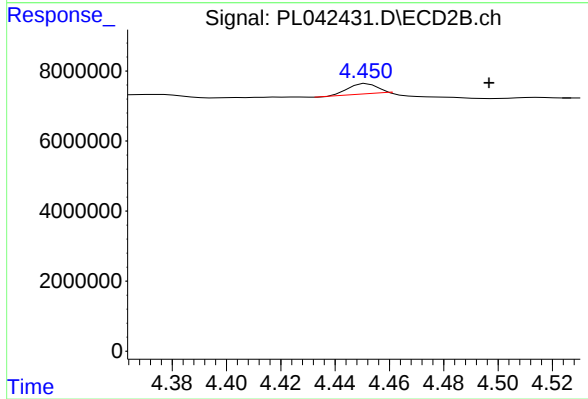

#2 alpha-BHC


R.T.: 4.452 min
Delta R.T.: -0.045 min
Response: 2215975
Conc: 0.52 ng/ml

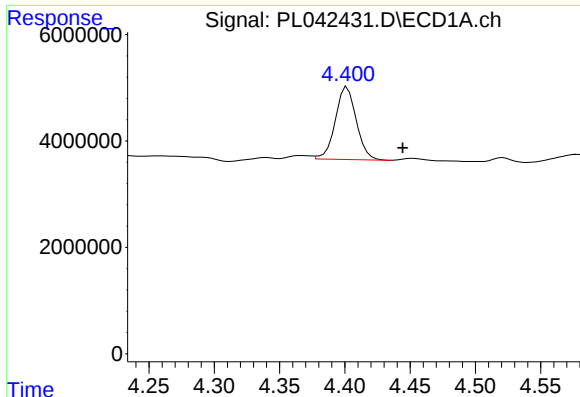

#6 beta-BHC


R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 15265934
Conc: 4.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

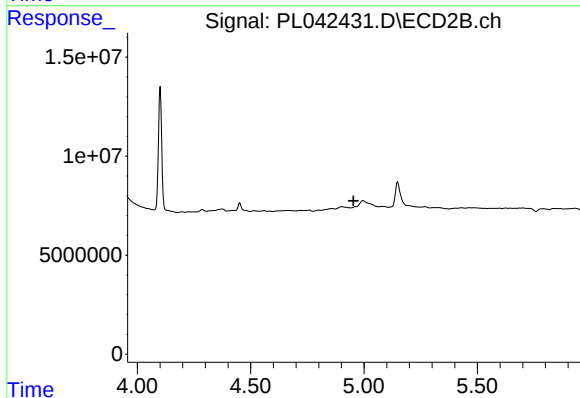


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

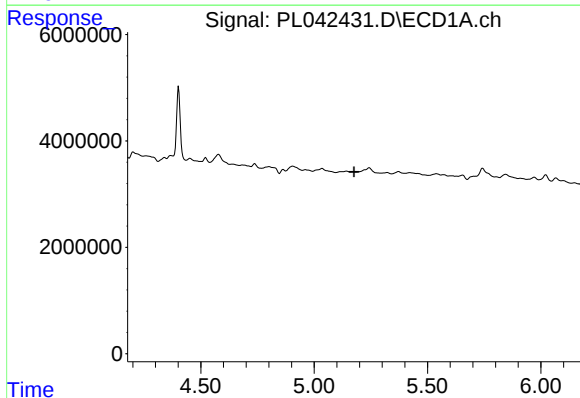


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

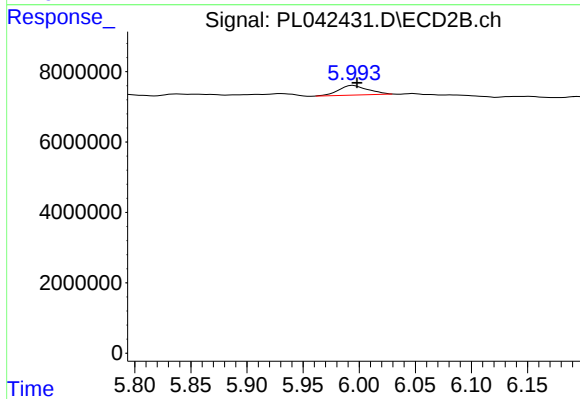

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.004 min
Response: 5064000
Conc: 1.41 ng/ml

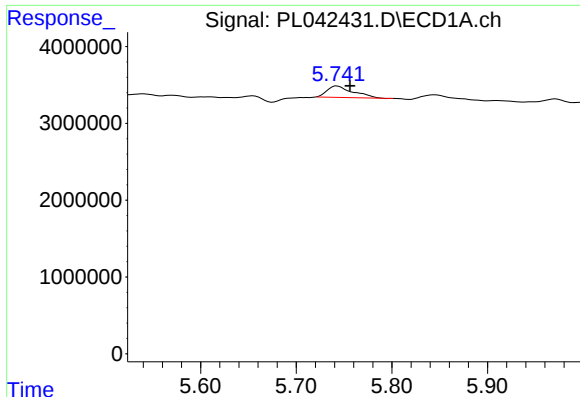

#13 Dieldrin


R.T.: 5.743 min
Delta R.T.: -0.014 min
Response: 2744473
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

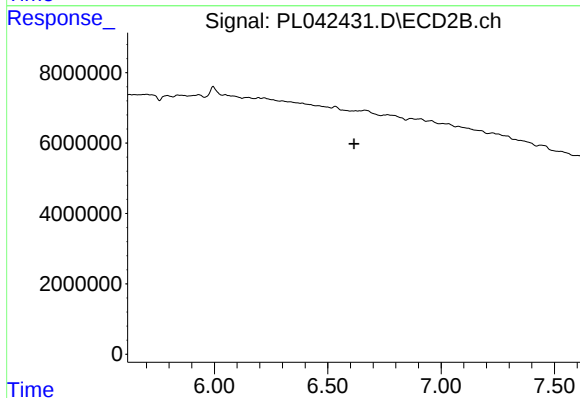


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

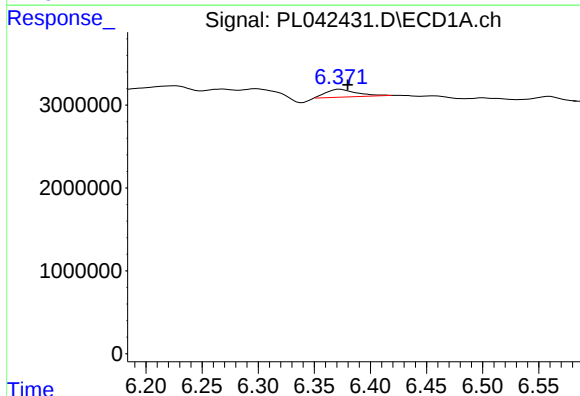


#17 4,4'-DDT

R.T.: 6.373 min
Delta R.T.: -0.007 min
Response: 1838493
Conc: 0.33 ng/ml

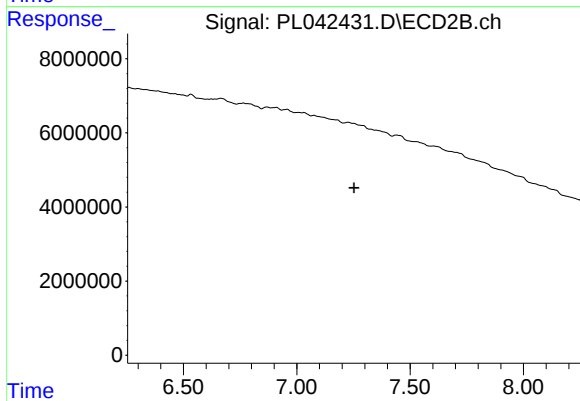

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

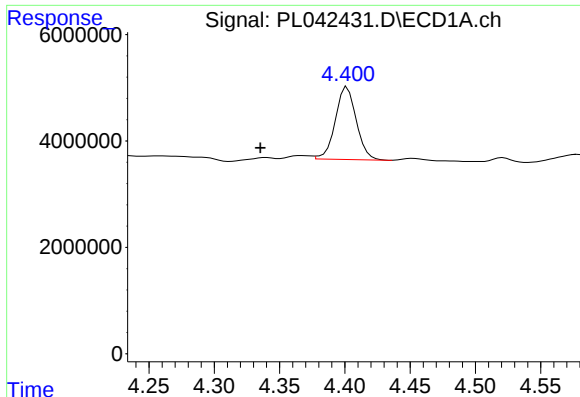

#23 Chlordane-1


R.T.: 4.402 min
Delta R.T.: 0.067 min
Response: 15265934
Conc: 55.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

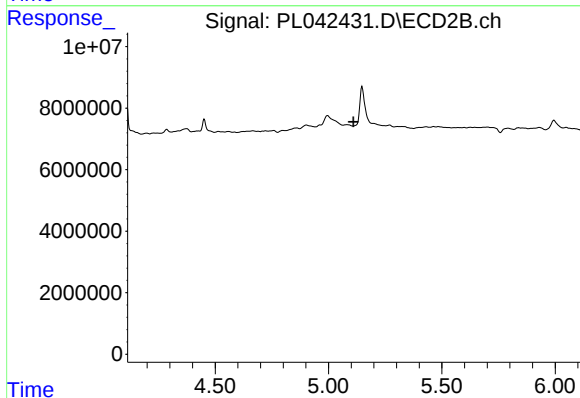


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

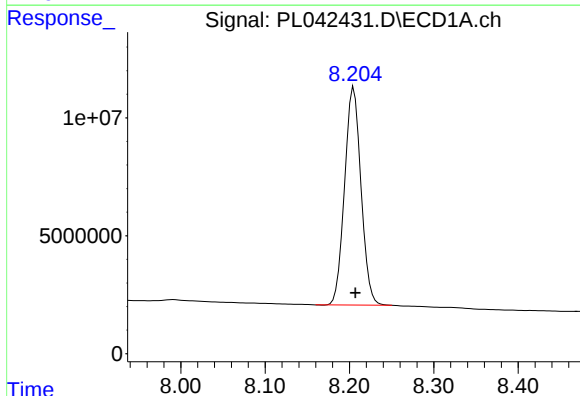

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 125041491
Conc: 19.84 ng/ml

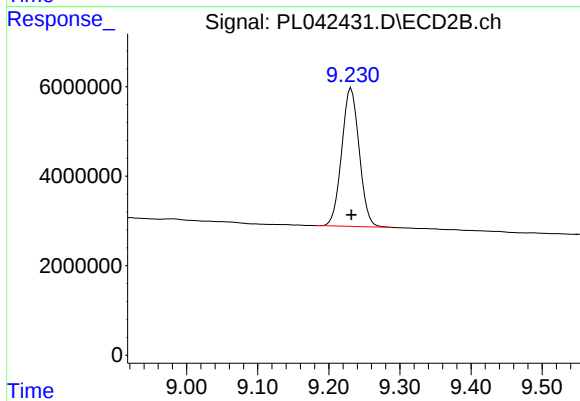

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 52886921
Conc: 21.93 ng/ml