

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
 Data File : PL042434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 19:46
 Operator : AJ\SJ
 Sample : J5765-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:43:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	113.2E6	58948206	19.234	20.496
28)	SA Decachlor...	8.205	9.231	107.4E6	42361899	17.044	17.564
Target Compounds							
3)	MA gamma-BHC...	4.200	0.000	1861793	0	0.226	N.D. #
6)	B beta-BHC	4.401f	0.000	14395811	0	4.063	N.D. #
7)	B delta-BHC	4.657	0.000	1699873	0	0.222	N.D. #
8)	B Heptachlo...	5.243f	5.994	10669947	4196375	1.408	1.170
9)	A Endosulfan I	5.542	0.000	2196166	0	0.317	N.D. #
10)	B gamma-Chl...	0.000	6.220	0	1716843	N.D.	0.504 #
13)	MA Dieldrin	5.742	0.000	7816341	0	1.062	N.D. #
23)	Chlordane-1	4.342	0.000	2260535	0	8.176	N.D. #
24)	Chlordane-2	4.897	0.000	2439740	0	8.682	N.D. #
25)	Chlordane-3	0.000	6.220	0	1716843	N.D.	3.653 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
Data File : PL042434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 19:46
Operator : AJ\SJ
Sample : J5765-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:43:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

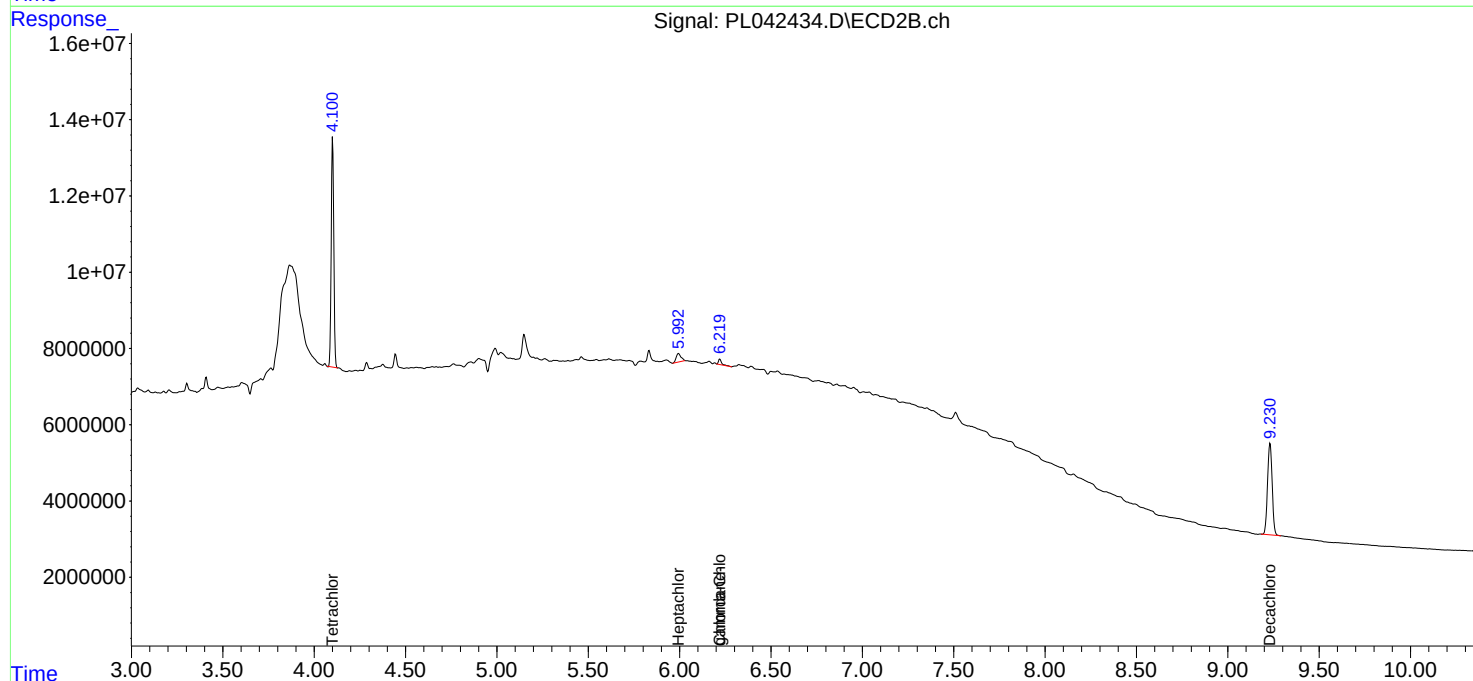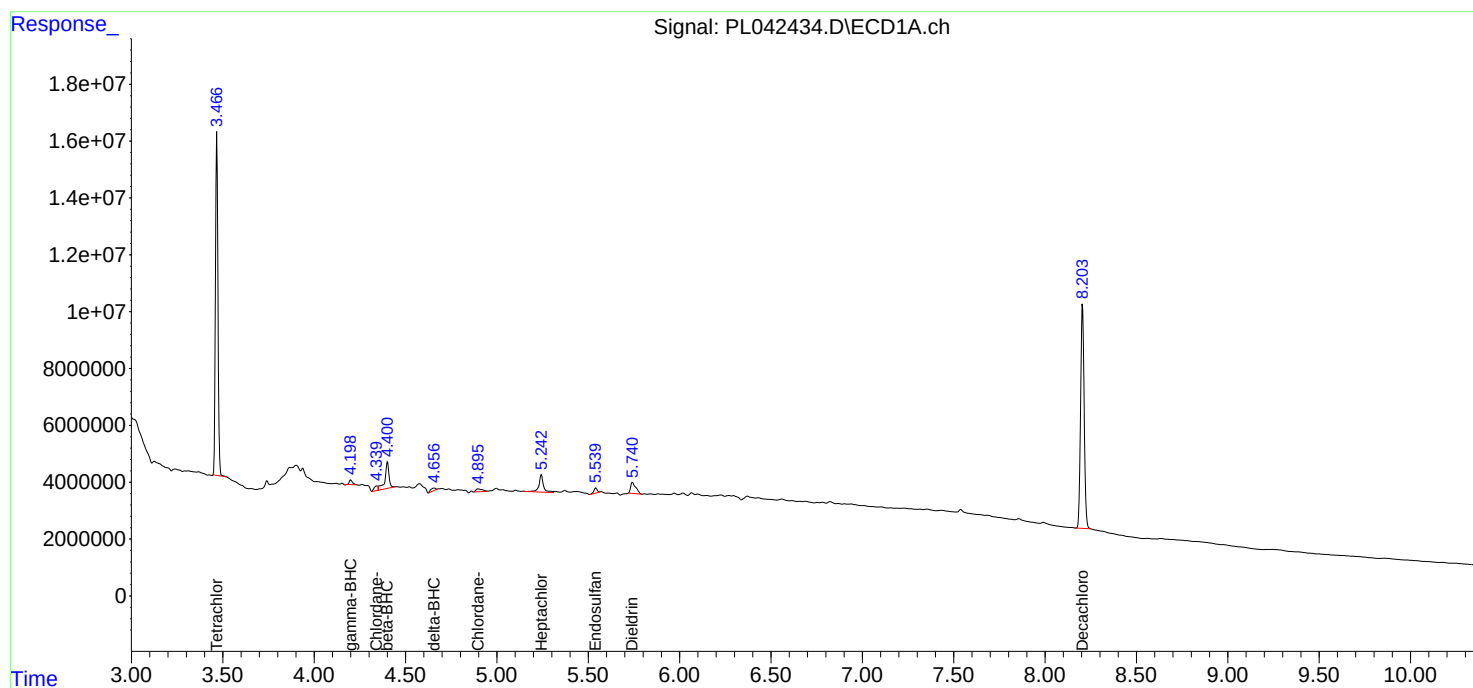


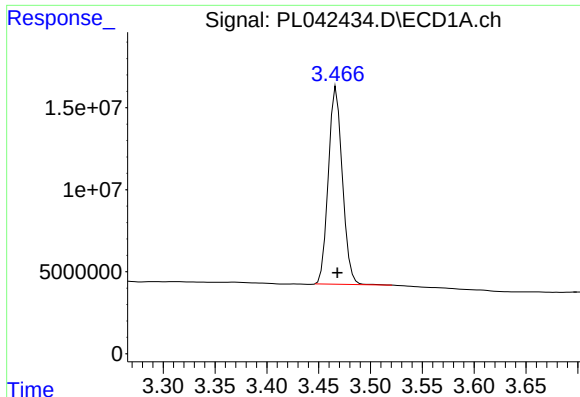

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 113164831
Conc: 19.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

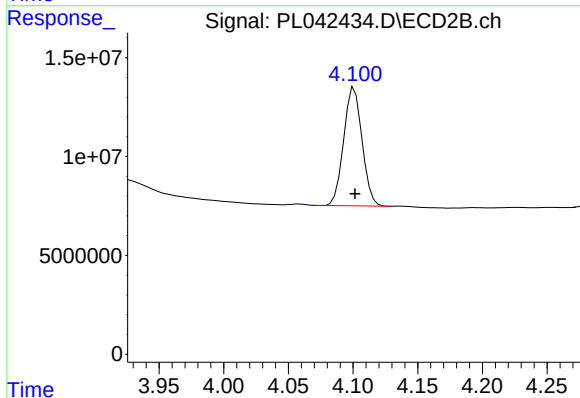


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 58948206
Conc: 20.50 ng/ml

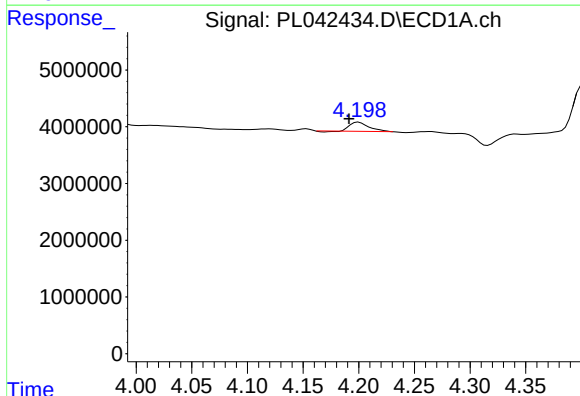


#3 gamma-BHC (Lindane)

R.T.: 4.200 min
Delta R.T.: 0.009 min
Response: 1861793
Conc: 0.23 ng/ml

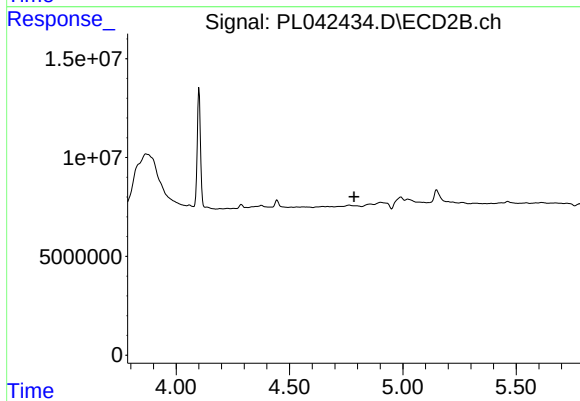

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

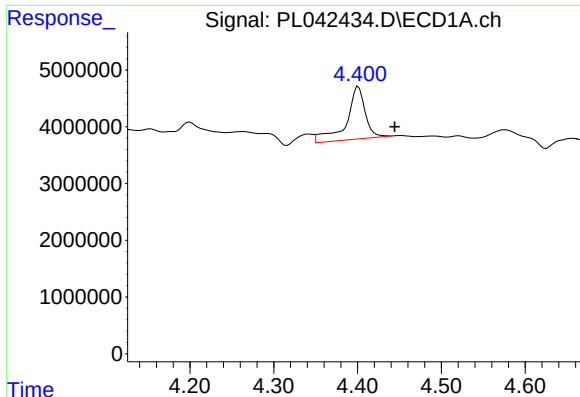

#6 beta-BHC


R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 14395811
Conc: 4.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

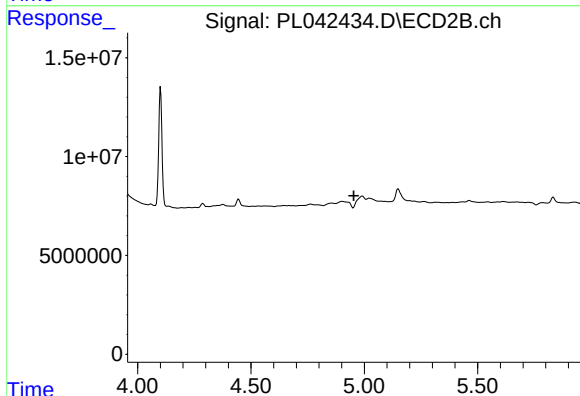


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

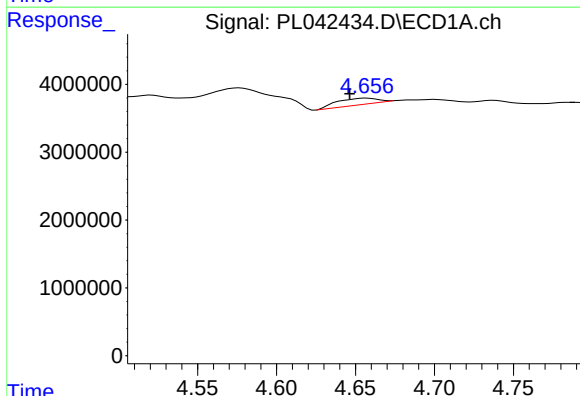


#7 delta-BHC

R.T.: 4.657 min
Delta R.T.: 0.011 min
Response: 1699873
Conc: 0.22 ng/ml

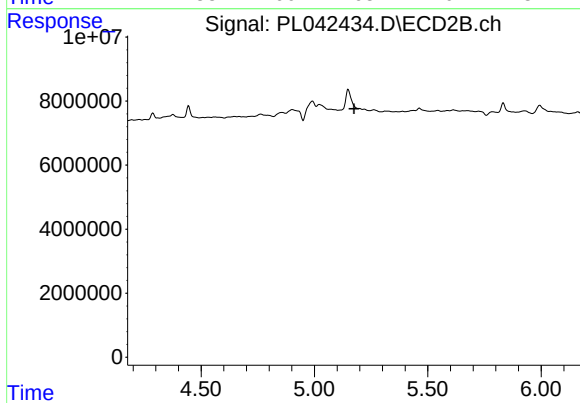

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

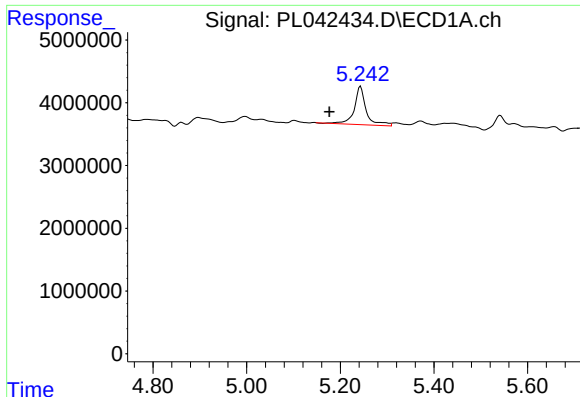

#8 Heptachlor epoxide


R.T.: 5.243 min
Delta R.T.: 0.067 min
Response: 10669947
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

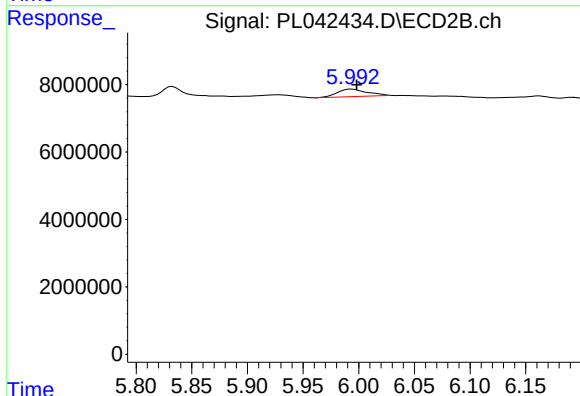


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.004 min
Response: 4196375
Conc: 1.17 ng/ml

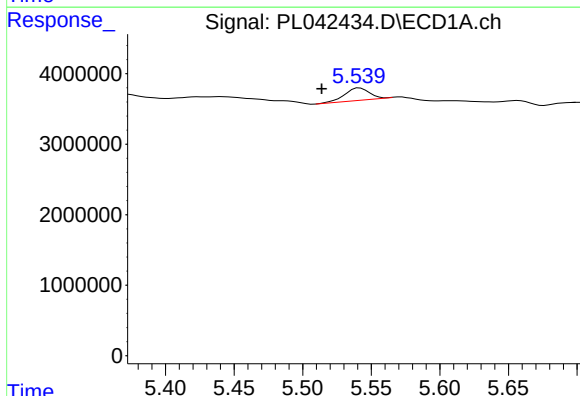


#9 Endosulfan I

R.T.: 5.542 min
Delta R.T.: 0.028 min
Response: 2196166
Conc: 0.32 ng/ml

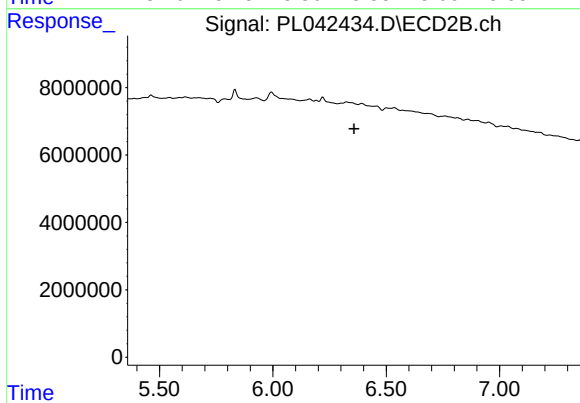

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

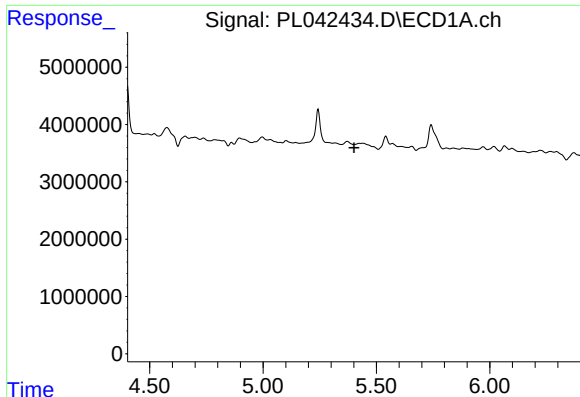

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

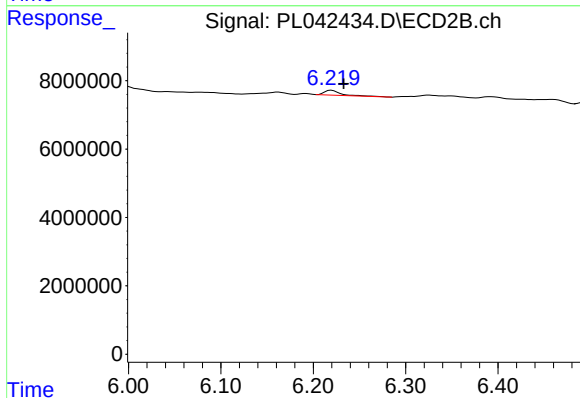


#10 gamma-Chlordane

R.T.: 6.220 min
Delta R.T.: -0.013 min
Response: 1716843
Conc: 0.50 ng/ml

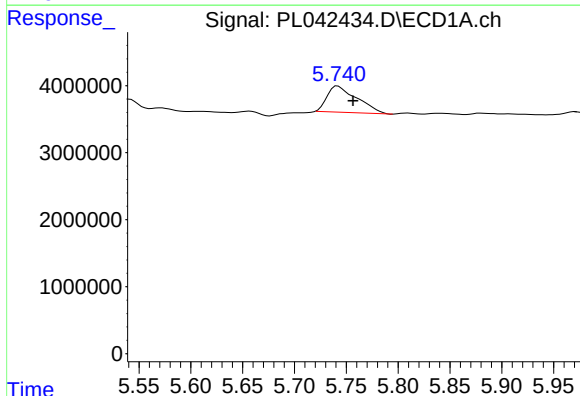


#13 Dieldrin

R.T.: 5.742 min
Delta R.T.: -0.015 min
Response: 7816341
Conc: 1.06 ng/ml

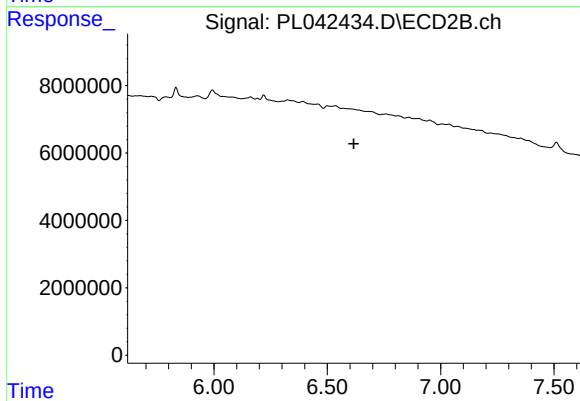

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

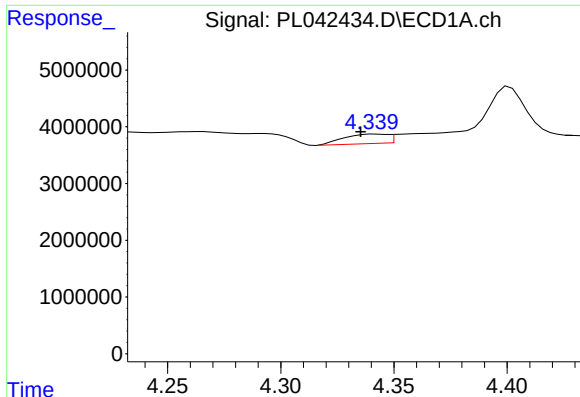

#23 Chlordane-1


R.T.: 4.342 min
Delta R.T.: 0.006 min
Response: 2260535
Conc: 8.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

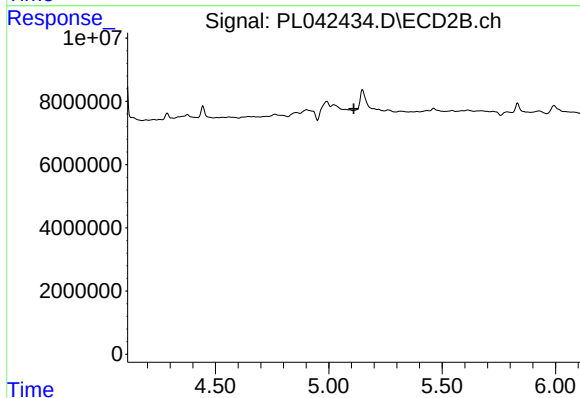


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

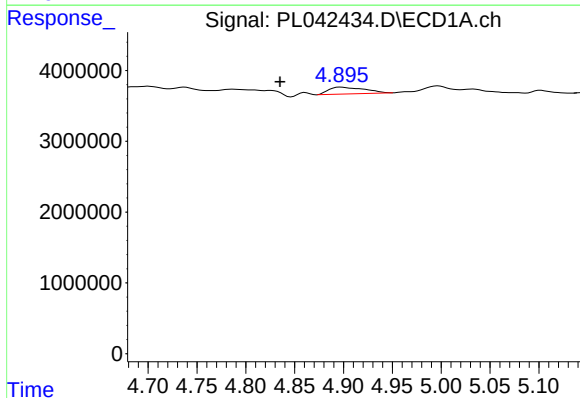


#24 Chlordane-2

R.T.: 4.897 min
Delta R.T.: 0.062 min
Response: 2439740
Conc: 8.68 ng/ml

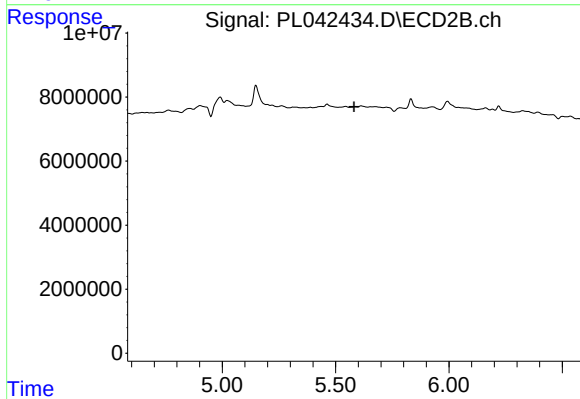

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

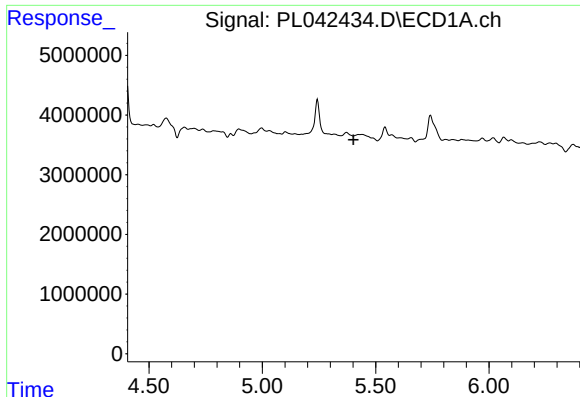

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

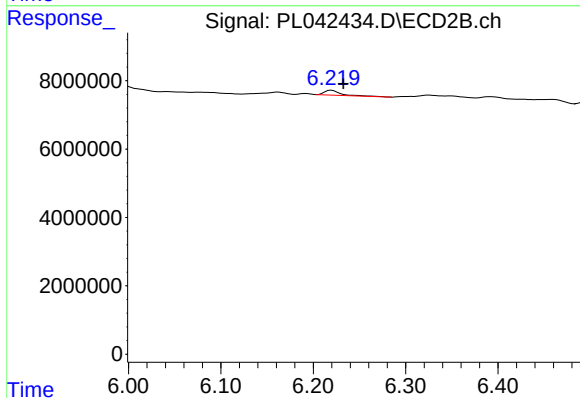


#25 Chlordane-3

R.T.: 6.220 min
Delta R.T.: -0.013 min
Response: 1716843
Conc: 3.65 ng/ml

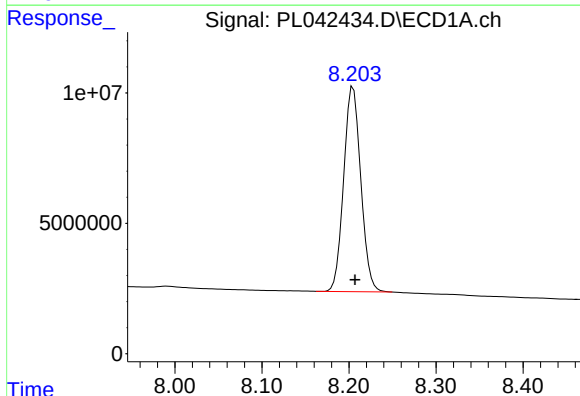

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 107414402
Conc: 17.04 ng/ml

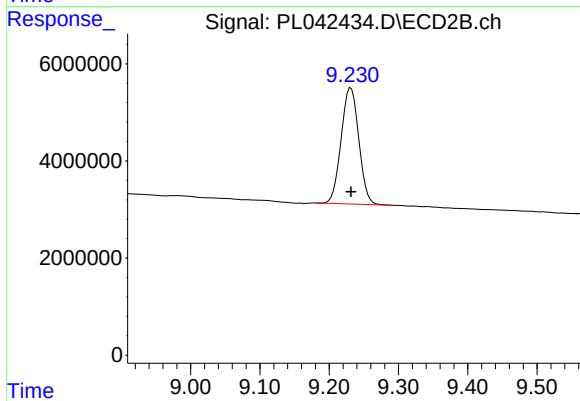

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 42361899
Conc: 17.56 ng/ml