

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
 Data File : PL042419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 15:50
 Operator : AJ\SJ
 Sample : J5999-05 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1115-S-AB-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:42:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.467	4.101	8786775	4254291	1.493	1.479
28) SA Decachlor...	8.205	9.233	6132712	1948083	0.973	0.808
Target Compounds						
12) B 4,4'-DDE	5.624	6.461	5747741	4694877	0.878	1.411 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112218\
Data File : PL042419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 15:50
Operator : AJ\SJ
Sample : J5999-05 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-1115-S-AB-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:42:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

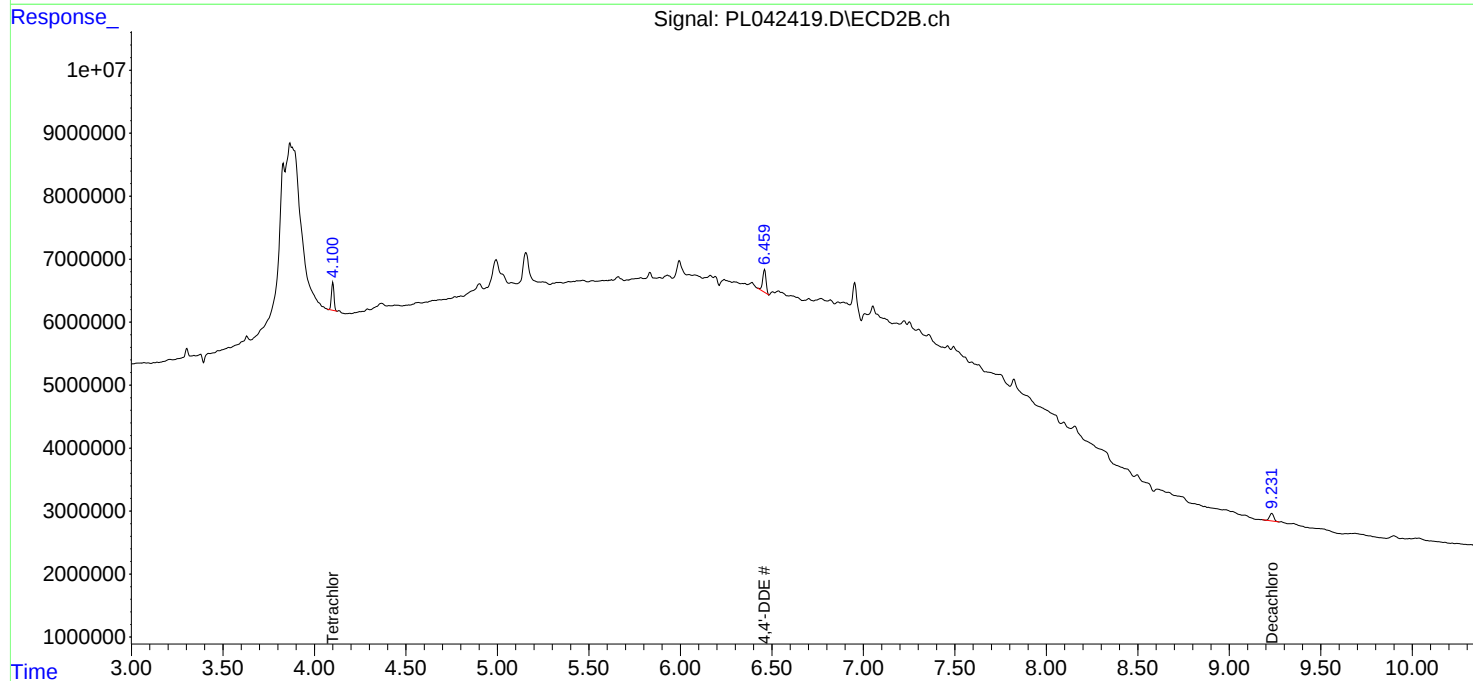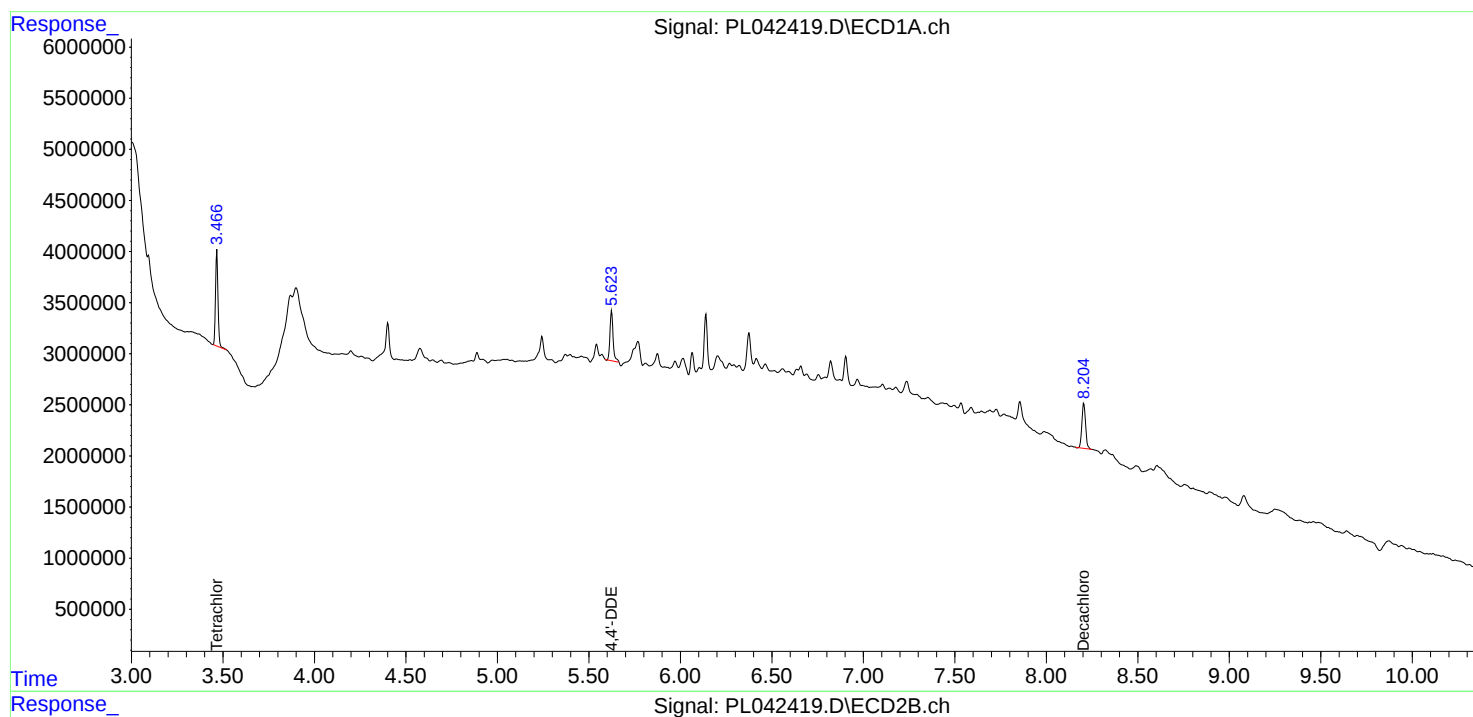


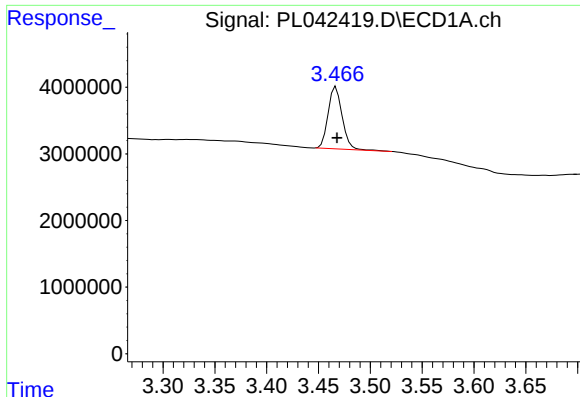

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 8786775
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1115-S-AB-1

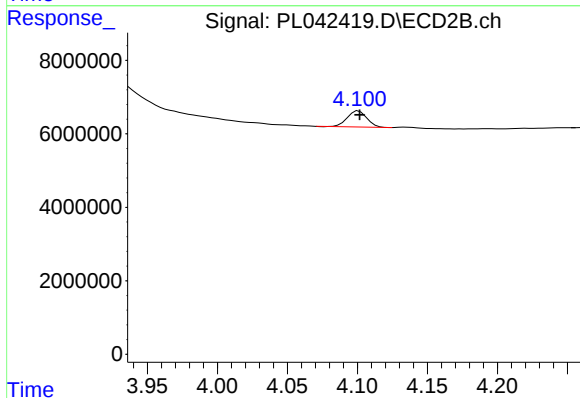


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 4254291
Conc: 1.48 ng/ml

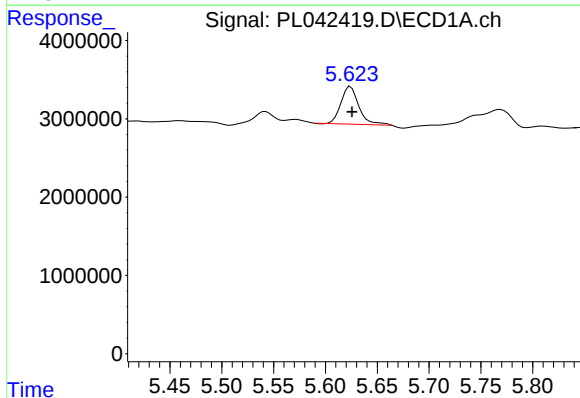


#12 4,4'-DDE

R.T.: 5.624 min
Delta R.T.: -0.002 min
Response: 5747741
Conc: 0.88 ng/ml

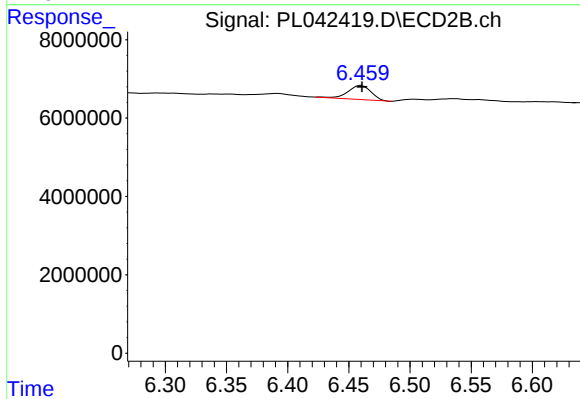

#12 4,4'-DDE


R.T.: 6.461 min
Delta R.T.: 0.000 min
Response: 4694877
Conc: 1.41 ng/ml

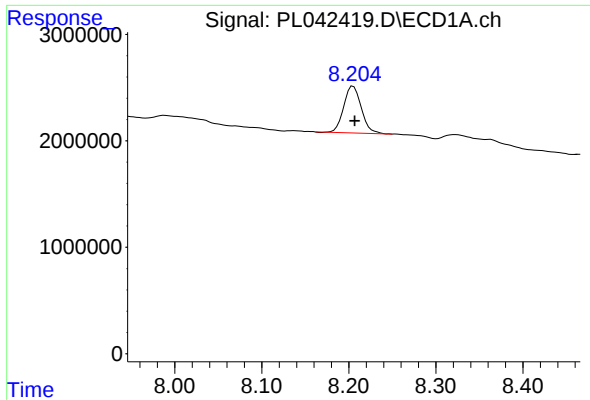

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 6132712
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1115-S-AB-1

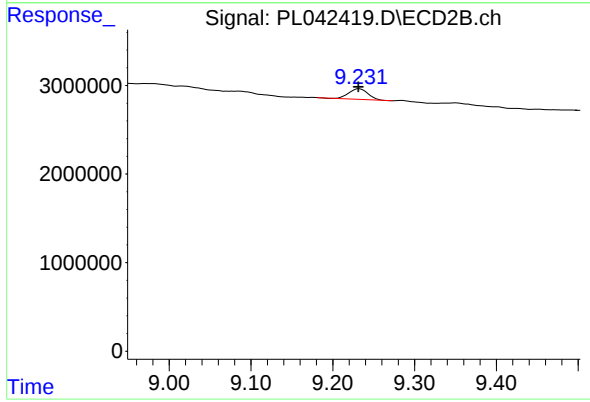

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.001 min
Response: 1948083
Conc: 0.81 ng/ml