

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112219\
 Data File : PL054535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 09:46
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 22:21:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	5.277	5.917	56896428	52642008	4.405 22.150 #
9) A	Endosulfan I	5.616	0.000	22307338	0	1.883 N.D. #
10) B	gamma-Chl...	0.000	6.177f	0	2645523	N.D. 1.063 #
12) B	4,4'-DDE	5.746f	0.000	39390739	0	3.406 N.D. #
14) MA	Endrin	6.119	6.748	11709390	8521263	1.060 4.020 #
15) B	Endosulfa...	6.400	0.000	5065821	0	0.484 N.D. #
17) MA	4,4'-DDT	0.000	7.186	0	3576920	N.D. 1.823 #
18) B	Endrin al...	0.000	7.091	0	7528949	N.D. 3.980 #
24)	Chlordane-2	4.920	0.000	31067622	0	74.483 N.D. #
25)	Chlordane-3	0.000	6.177f	0	2645523	N.D. 7.941 #
27)	Chlordane-5	6.400	0.000	5065821	0	13.735 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112219\
Data File : PL054535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 09:46
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 22:21:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

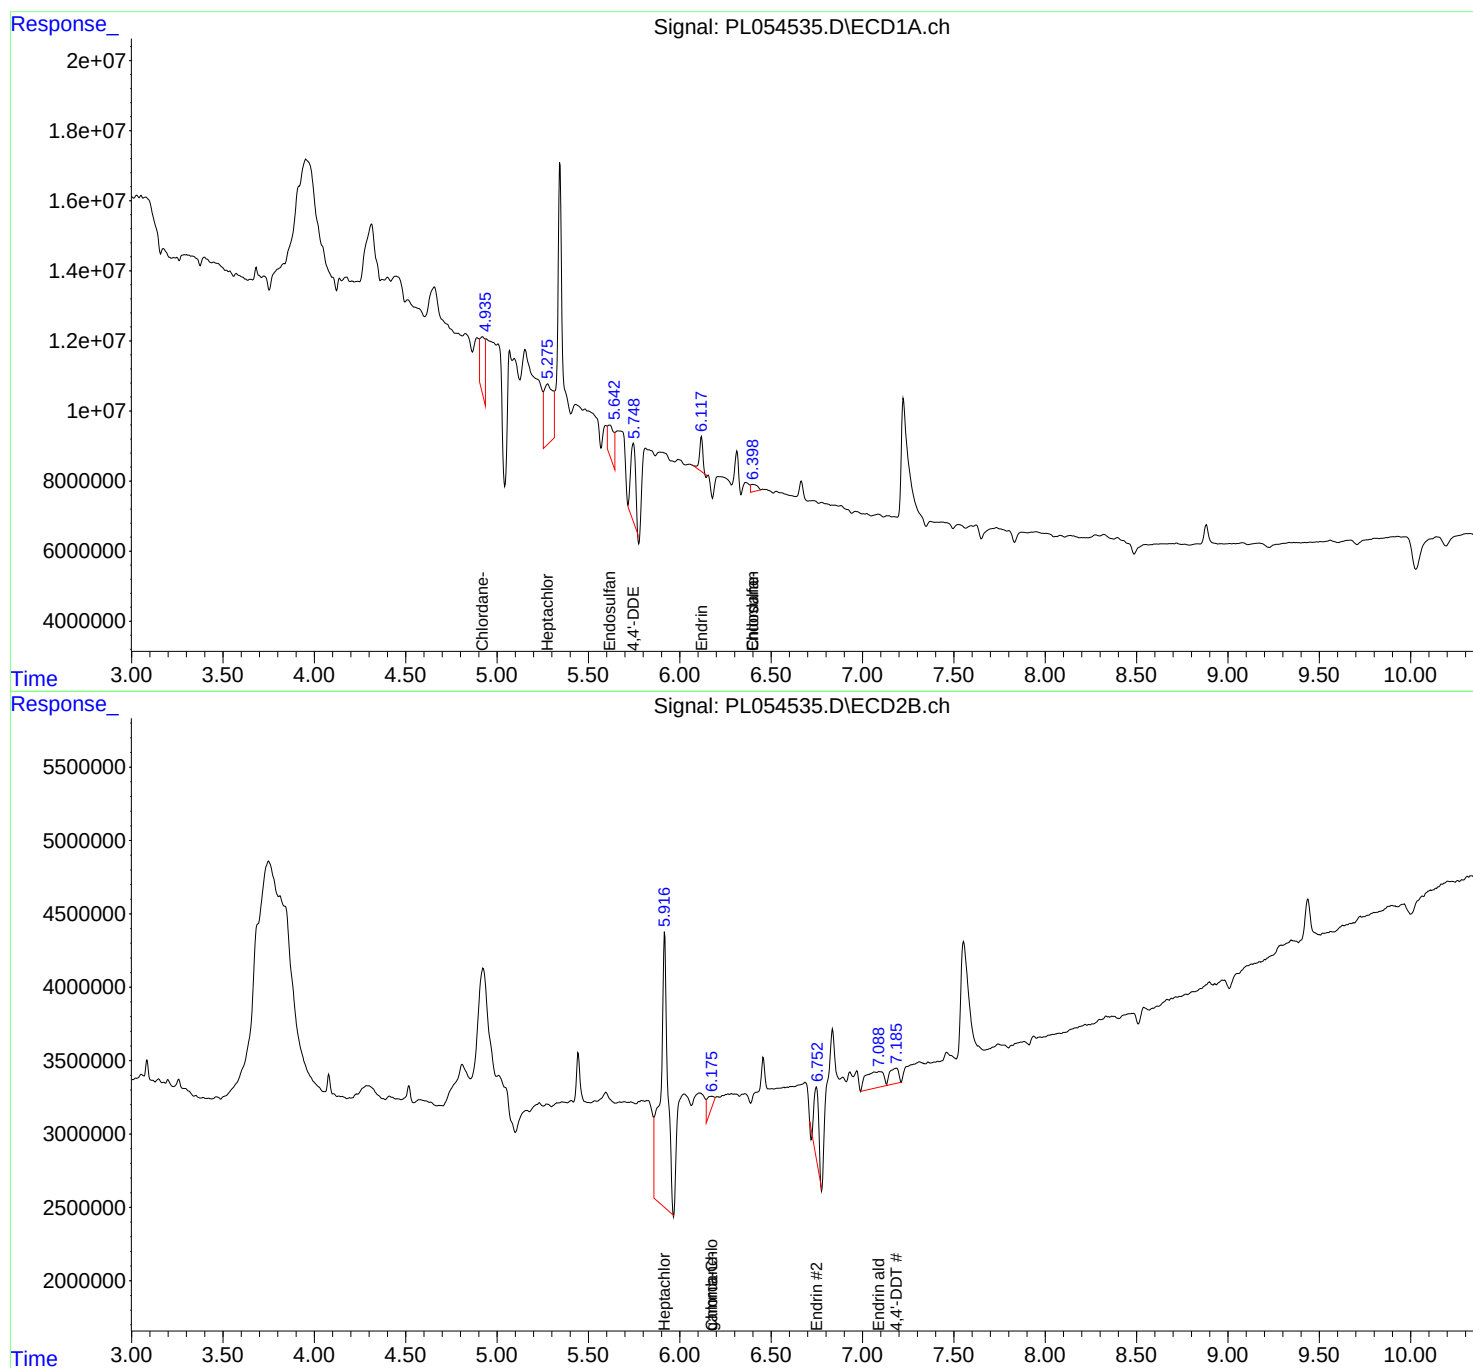


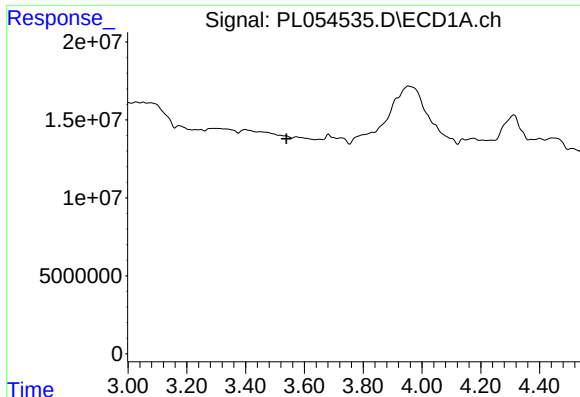

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.539 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

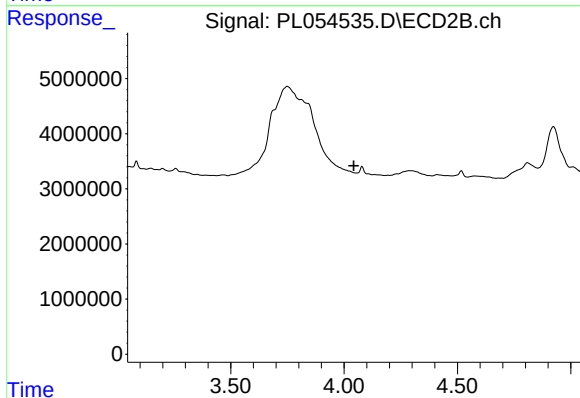


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.043 min
Response: 0
Conc: N.D.

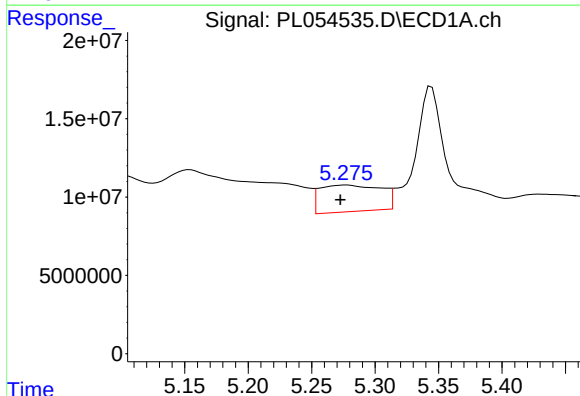


#8 Heptachlor epoxide

R.T.: 5.277 min
Delta R.T.: 0.005 min
Response: 56896428
Conc: 4.41 ng/ml

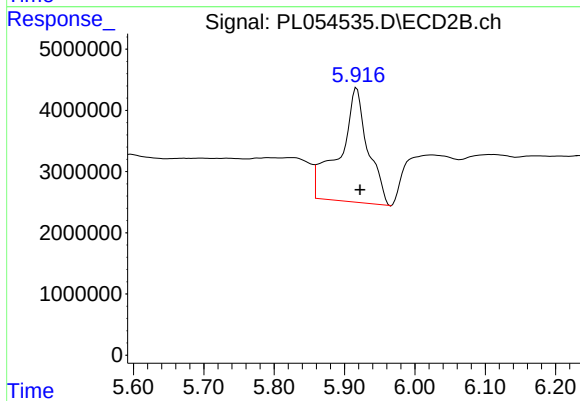

#8 Heptachlor epoxide


R.T.: 5.917 min
Delta R.T.: -0.005 min
Response: 52642008
Conc: 22.15 ng/ml

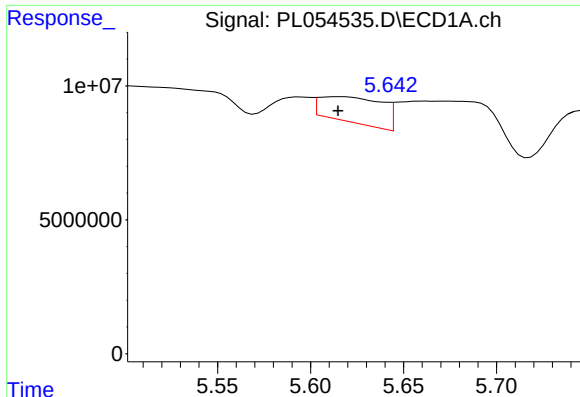

#9 Endosulfan I


R.T.: 5.616 min
Delta R.T.: 0.001 min
Response: 22307338
Conc: 1.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

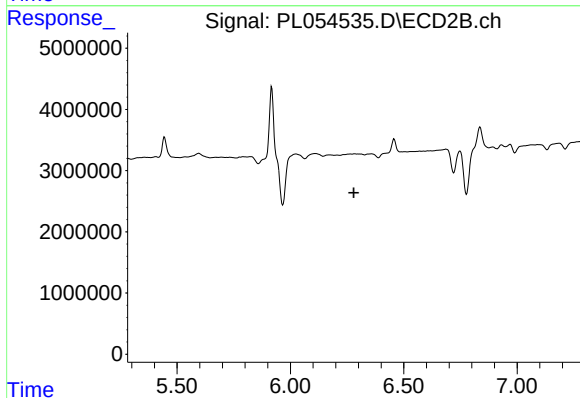


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

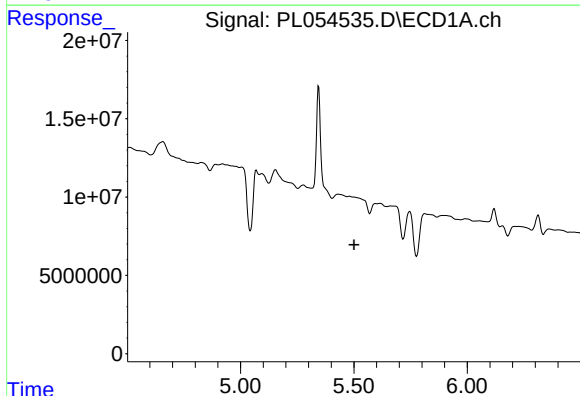


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

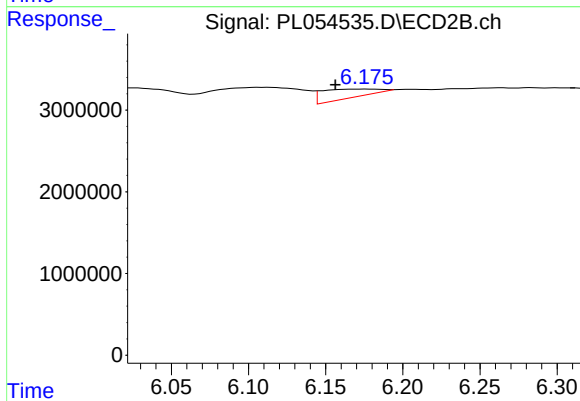

#10 gamma-Chlordane


R.T.: 6.177 min
Delta R.T.: 0.020 min
Response: 2645523
Conc: 1.06 ng/ml

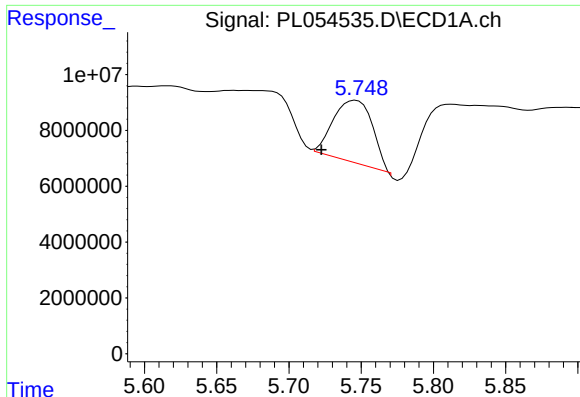

#12 4,4'-DDE


R.T.: 5.746 min
Delta R.T.: 0.024 min
Response: 39390739
Conc: 3.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

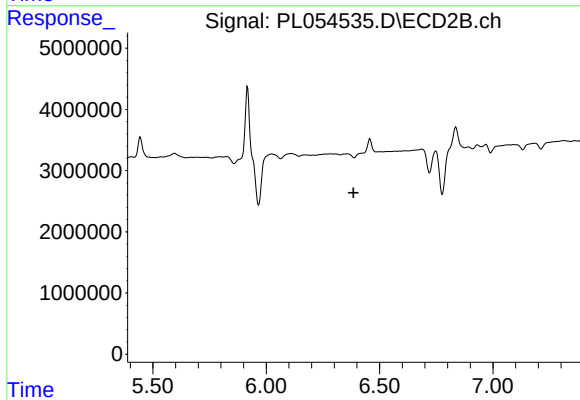


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

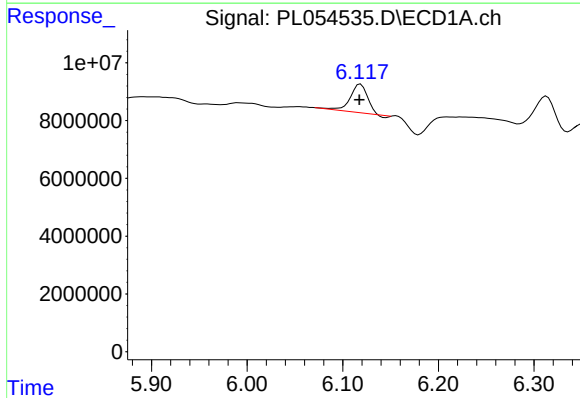


#14 Endrin

R.T.: 6.119 min
Delta R.T.: 0.001 min
Response: 11709390
Conc: 1.06 ng/ml

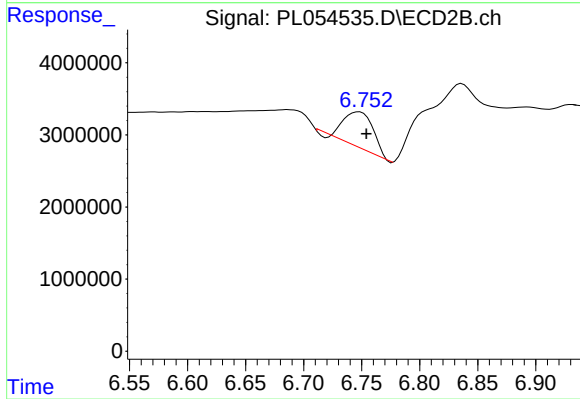

#14 Endrin


R.T.: 6.748 min
Delta R.T.: -0.006 min
Response: 8521263
Conc: 4.02 ng/ml

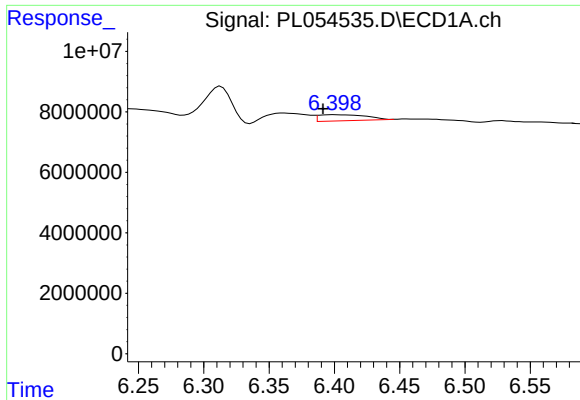

#15 Endosulfan II


R.T.: 6.400 min
Delta R.T.: 0.009 min
Response: 5065821
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

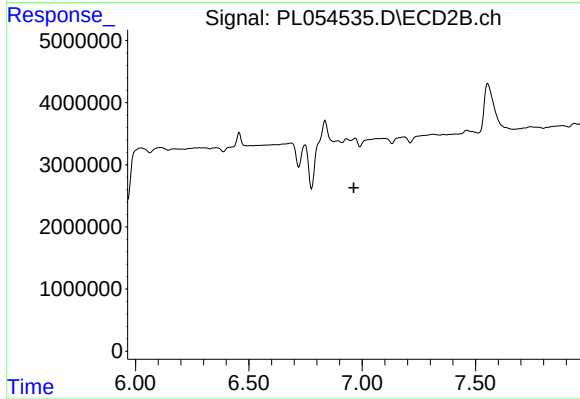


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.964 min
Response: 0
Conc: N.D.

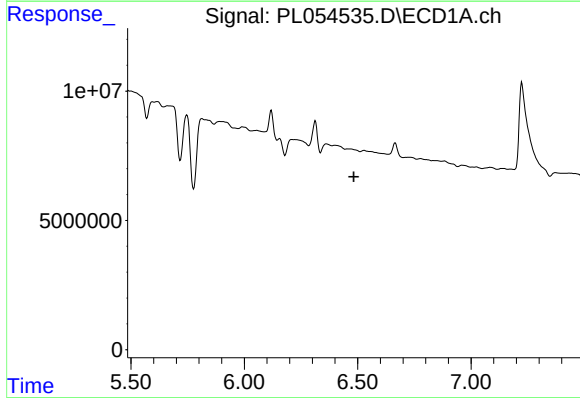


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.483 min
Response: 0
Conc: N.D.

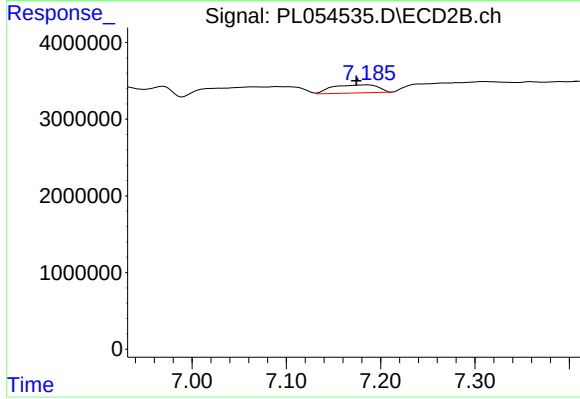

#17 4,4'-DDT


R.T.: 7.186 min
Delta R.T.: 0.012 min
Response: 3576920
Conc: 1.82 ng/ml

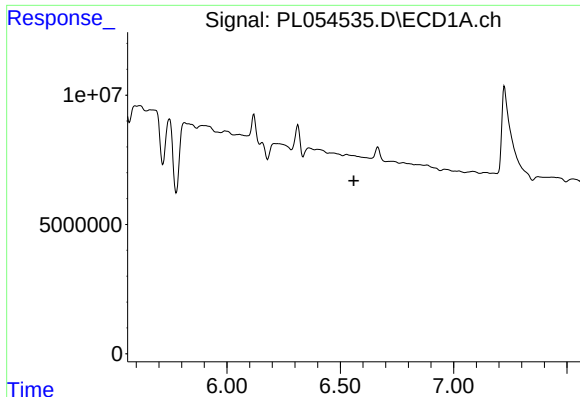

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.559 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

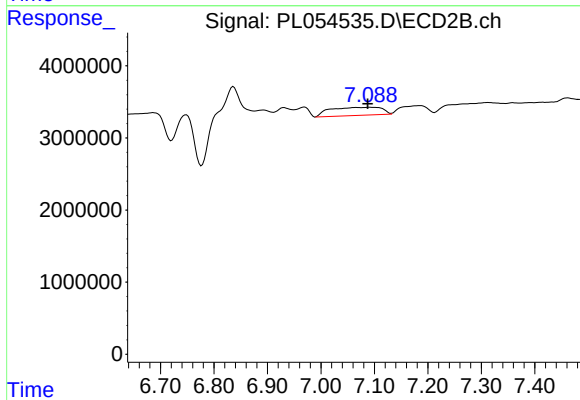


#18 Endrin aldehyde

R.T.: 7.091 min
Delta R.T.: 0.004 min
Response: 7528949
Conc: 3.98 ng/ml

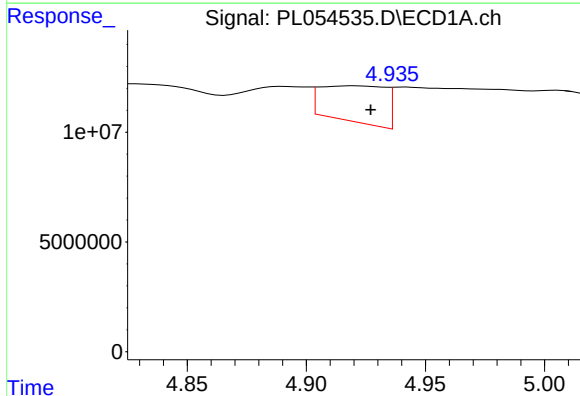


#24 Chlordane-2

R.T.: 4.920 min
Delta R.T.: -0.007 min
Response: 31067622
Conc: 74.48 ng/ml

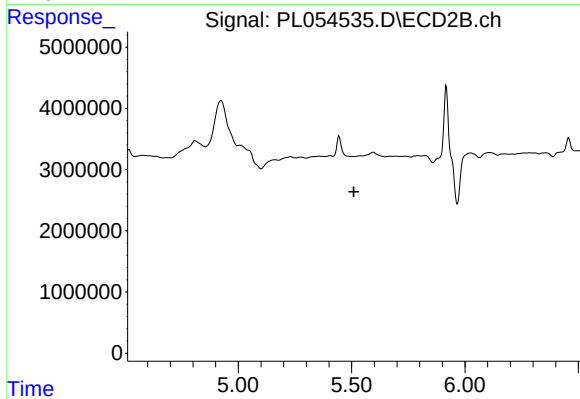

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.510 min
Response: 0
Conc: N.D.

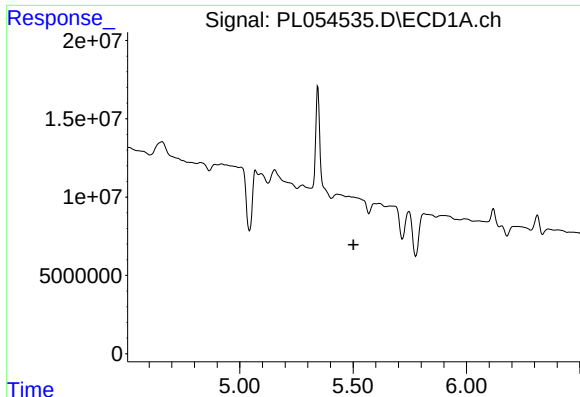

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

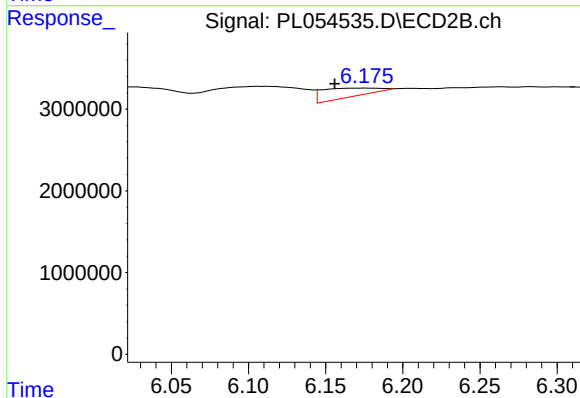


#25 Chlordane-3

R.T.: 6.177 min
Delta R.T.: 0.021 min
Response: 2645523
Conc: 7.94 ng/ml

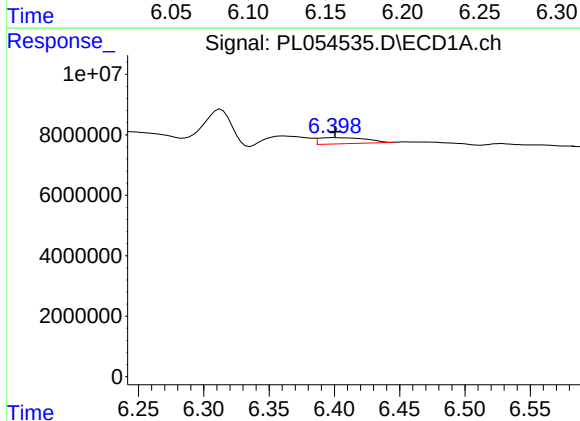


#27 Chlordane-5

R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 5065821
Conc: 13.73 ng/ml

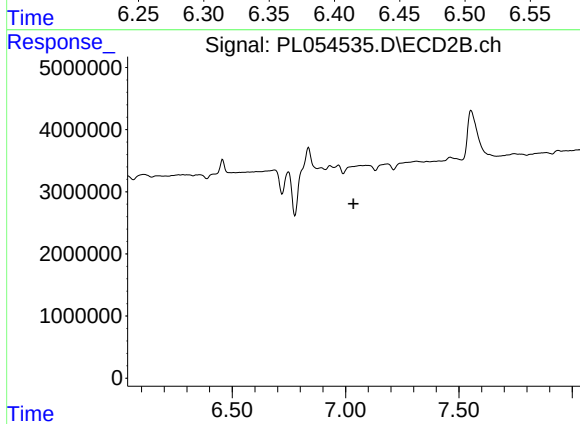

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.035 min
Response: 0
Conc: N.D.

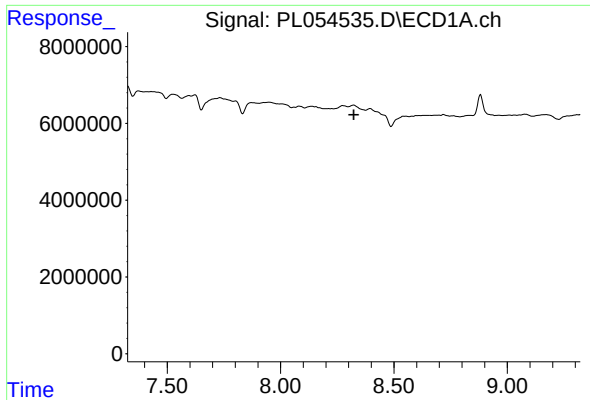

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

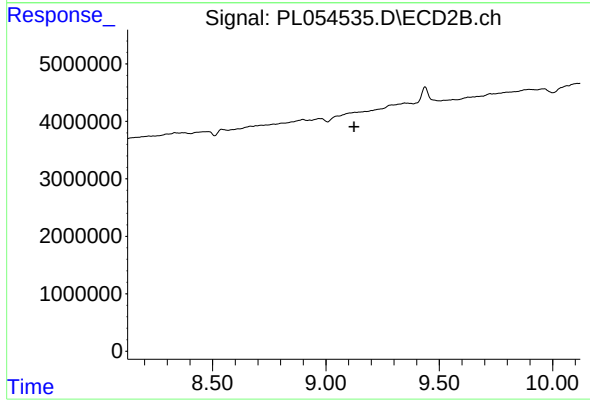

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.125 min
Response: 0
Conc: N.D.