

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112219\
 Data File : PL054575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 23:35
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 00:41:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.053	246.5E6	56137358	23.710	23.043
28)	SA Decachlor...	8.321	9.150f	209.9E6	50458440	23.716	20.870
Target Compounds							
2)	A alpha-BHC	3.977	0.000	13868029	0	0.814	N.D. #
8)	B Heptachlo...	5.284	0.000	2275089	0	0.176	N.D. #
10)	B gamma-Chl...	0.000	6.133f	0	4326760	N.D.	1.739 #
12)	B 4,4'-DDE	5.740f	0.000	17382776	0	1.503	N.D. #
23)	Chlordane-1	4.447f	0.000	5748844	0	14.801	N.D. #
25)	Chlordane-3	0.000	6.133f	0	4326760	N.D.	12.987 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112219\
Data File : PL054575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 23:35
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 00:41:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

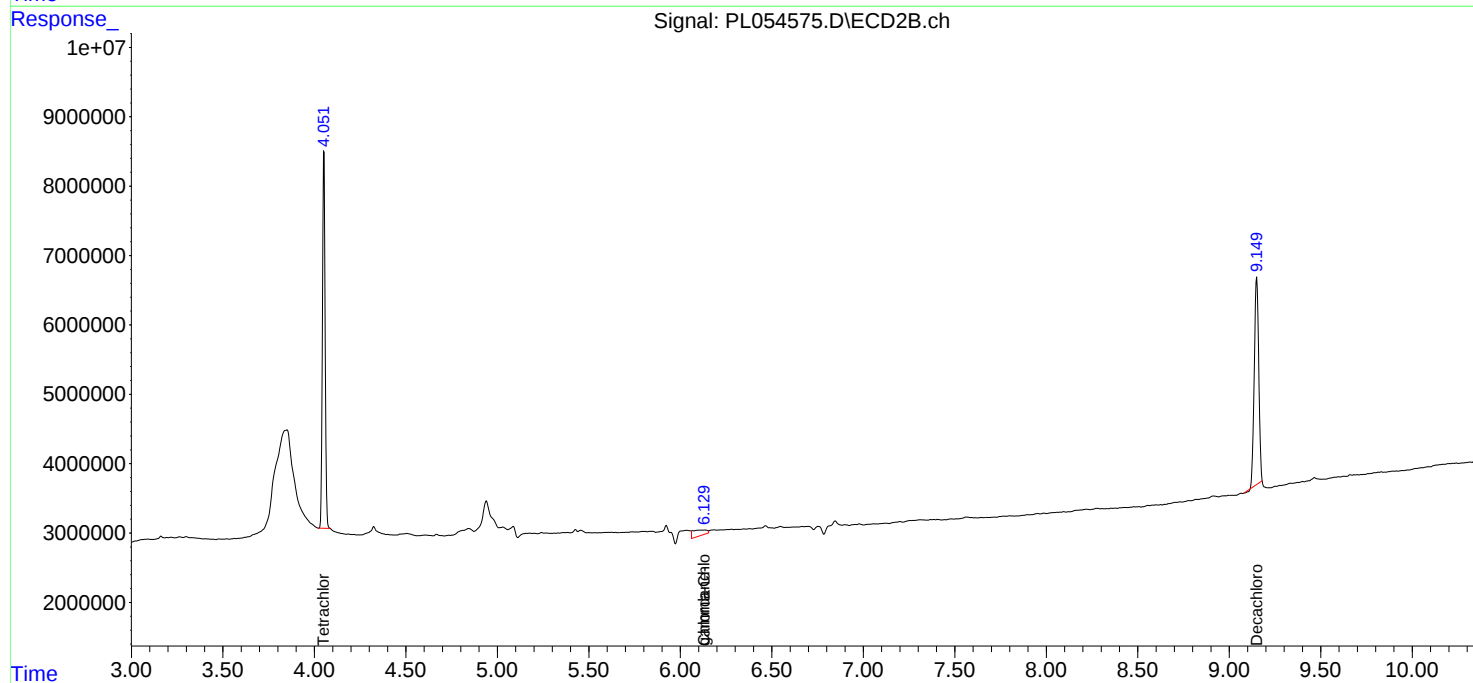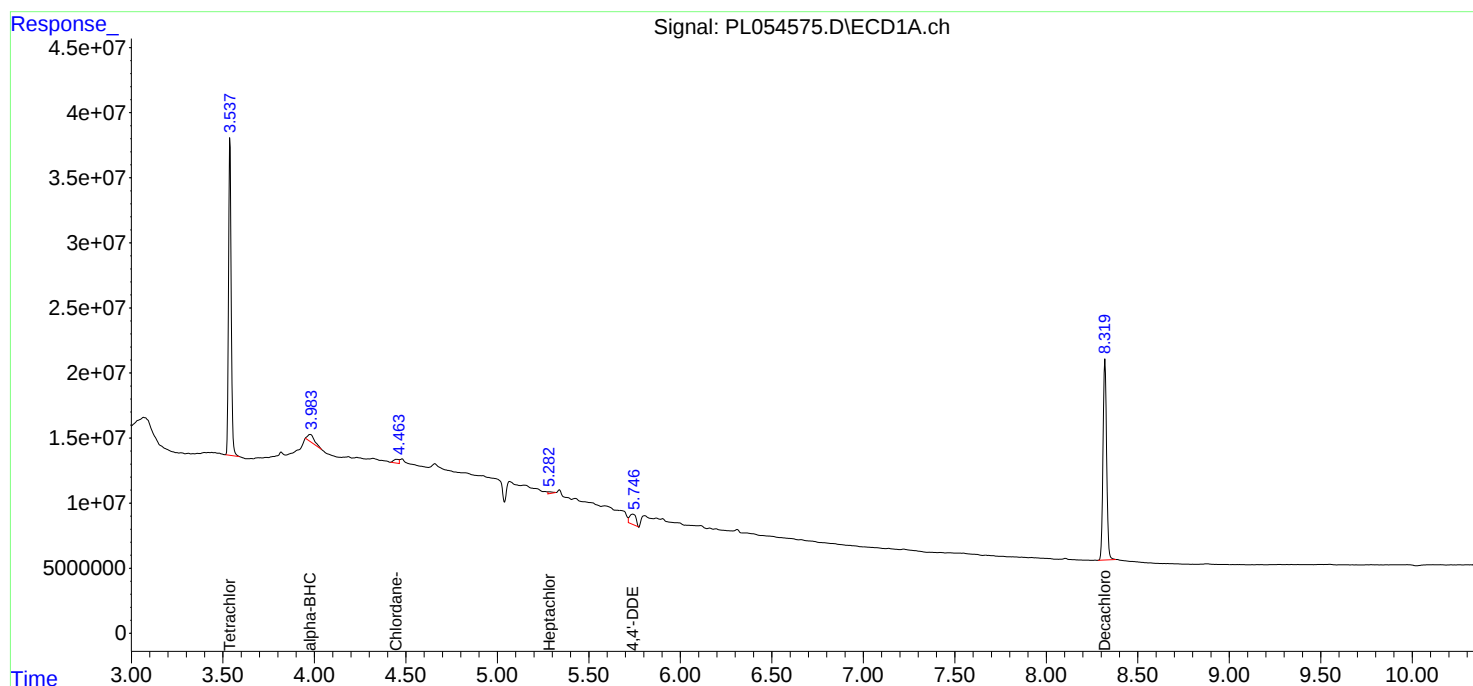


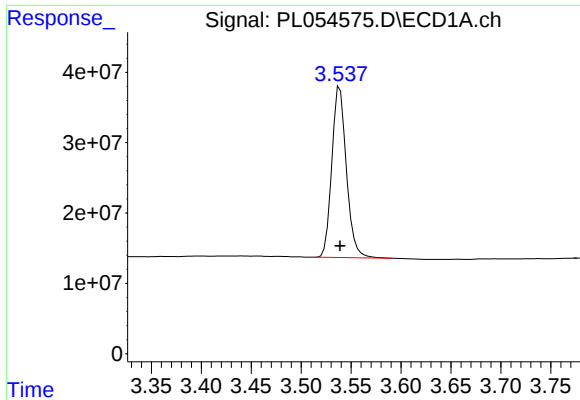

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 246517964
Conc: 23.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

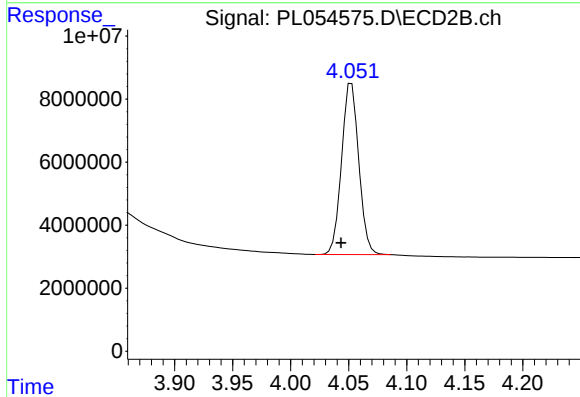


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: 0.009 min
Response: 56137358
Conc: 23.04 ng/ml

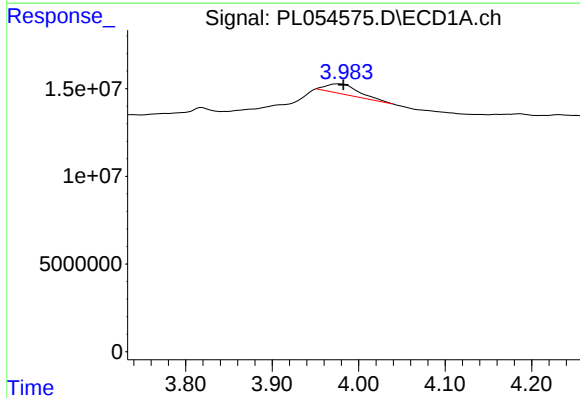


#2 alpha-BHC

R.T.: 3.977 min
Delta R.T.: -0.005 min
Response: 13868029
Conc: 0.81 ng/ml

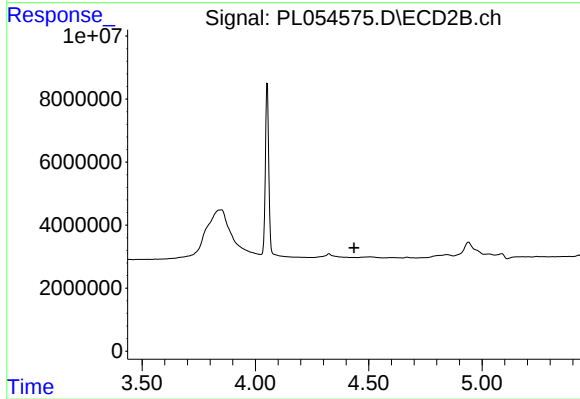

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.435 min
Response: 0
Conc: N.D.

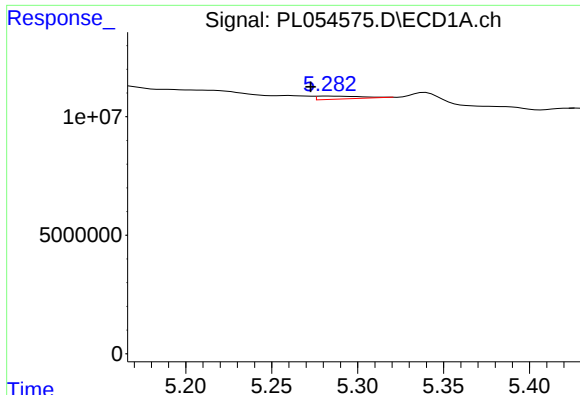

#8 Heptachlor epoxide


R.T.: 5.284 min
Delta R.T.: 0.011 min
Response: 2275089
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

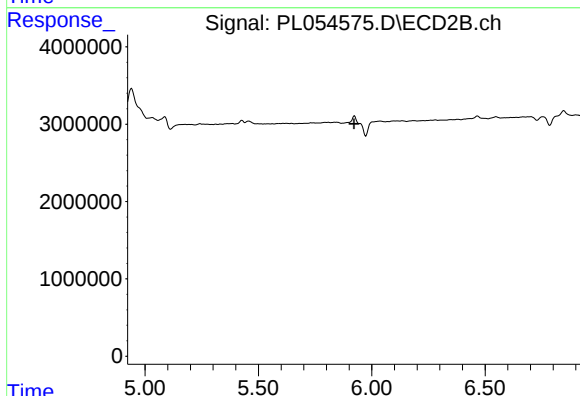


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.922 min
Response: 0
Conc: N.D.

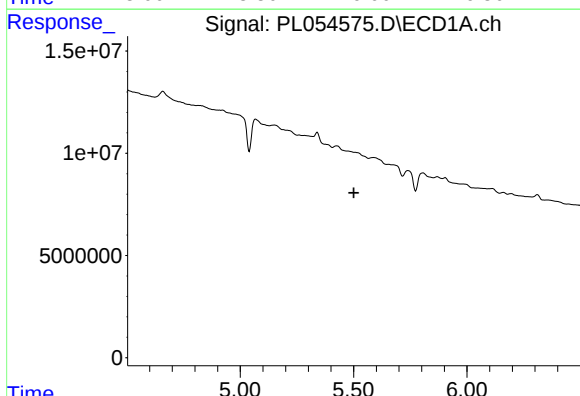


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

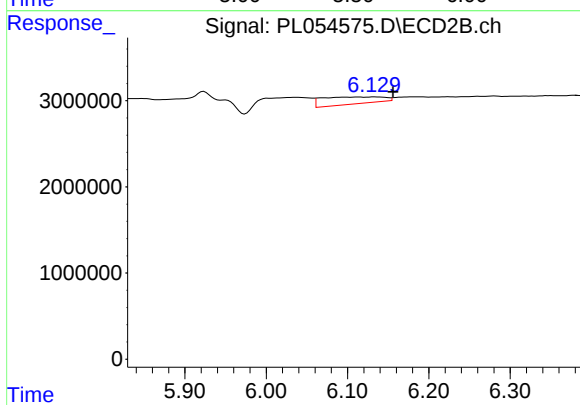

#10 gamma-Chlordane


R.T.: 6.133 min
Delta R.T.: -0.023 min
Response: 4326760
Conc: 1.74 ng/ml

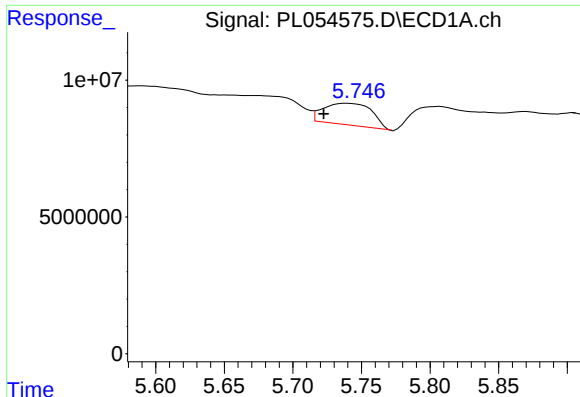

#12 4,4'-DDE


R.T.: 5.740 min
Delta R.T.: 0.017 min
Response: 17382776
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

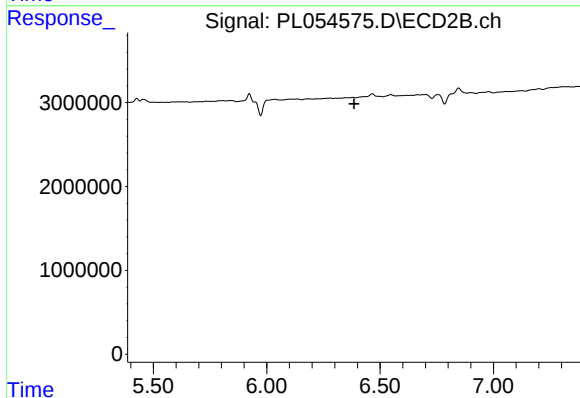


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

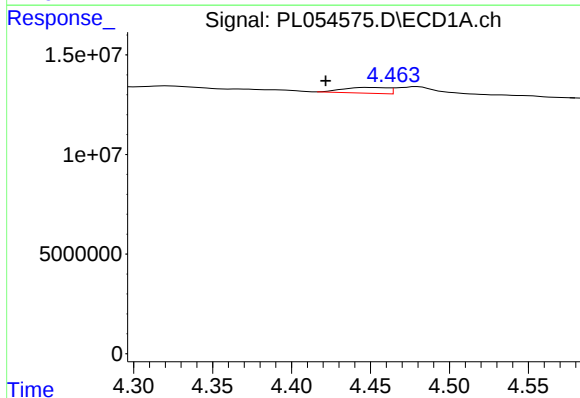


#23 Chlordane-1

R.T.: 4.447 min
Delta R.T.: 0.026 min
Response: 5748844
Conc: 14.80 ng/ml

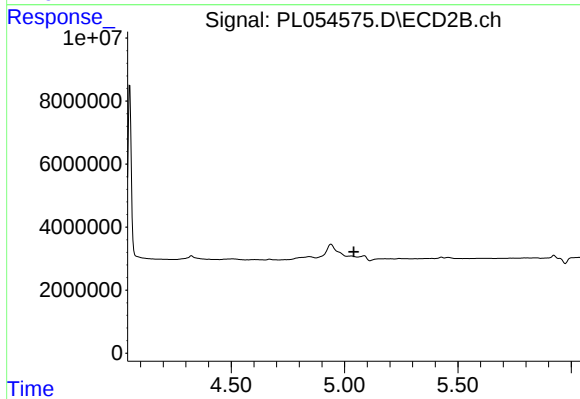

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.041 min
Response: 0
Conc: N.D.

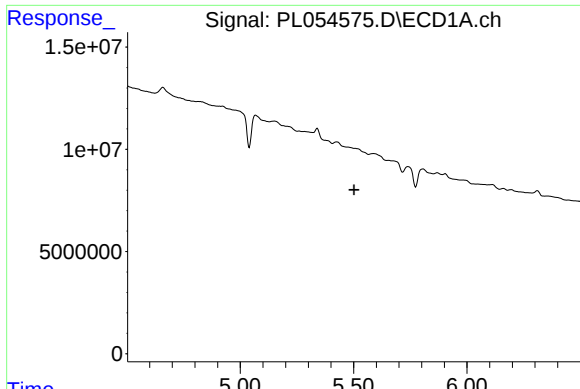

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

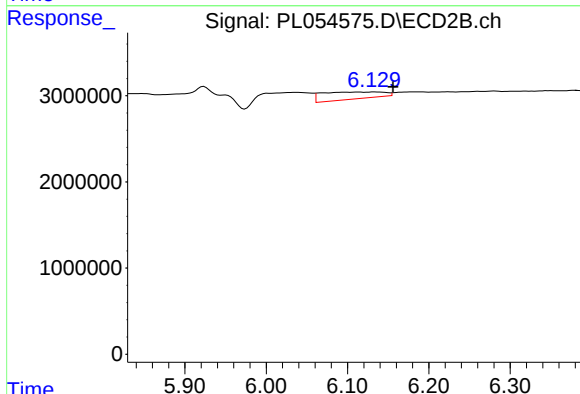


#25 Chlordane-3

R.T.: 6.133 min
Delta R.T.: -0.023 min
Response: 4326760
Conc: 12.99 ng/ml

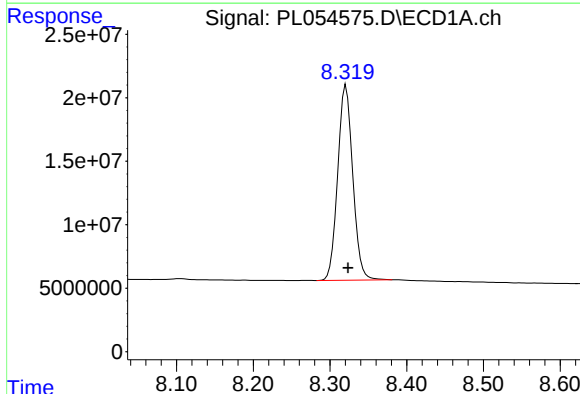

#28 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.003 min
Response: 209910572
Conc: 23.72 ng/ml

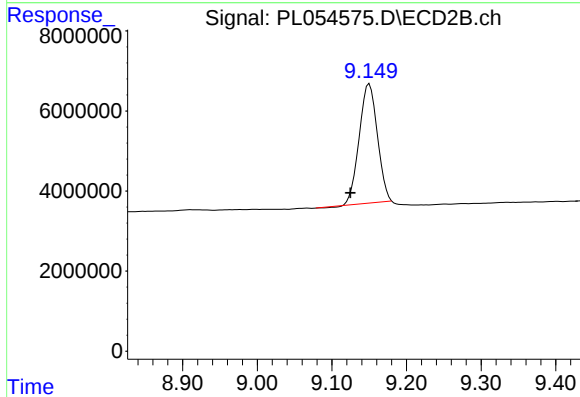

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: 0.025 min
Response: 50458440
Conc: 20.87 ng/ml