

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112221\
 Data File : PL071099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2021 09:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 04:44:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.570	5.504	10364190	25016297	21.160	19.841
28)	SA Decachlor...	10.333	11.396	13700840	24447113	20.051	18.280
Target Compounds							
2)	A alpha-BHC	5.257f	0.000	610789	0	0.912	N.D. #
4)	MA Heptachlor	6.085f	0.000	109083	0	0.152	N.D. #
6)	B beta-BHC	6.085	0.000	109083	0	0.336	N.D. #
15)	B Endosulfa...	8.274f	0.000	295951	0	0.489	N.D. #
17)	MA 4,4'-DDT	0.000	9.350	0	240744	N.D.	0.191 #
20)	A Methoxychlor	9.018	0.000	2399718	0	6.559	N.D. #
23)	Chlordane-1	0.000	6.900f	0	222438	N.D.	4.581 #
27)	Chlordane-5	8.274f	0.000	295951	0	13.237	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112221\
Data File : PL071099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2021 09:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 04:44:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

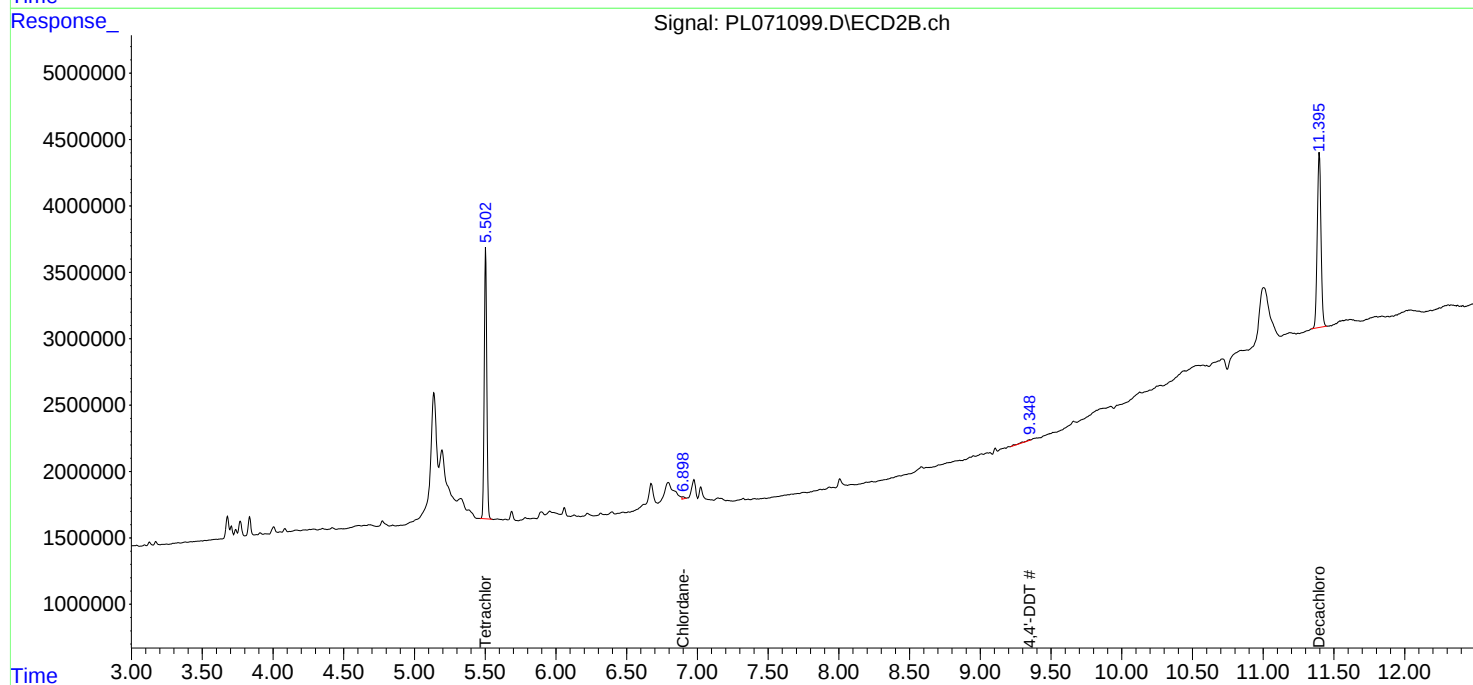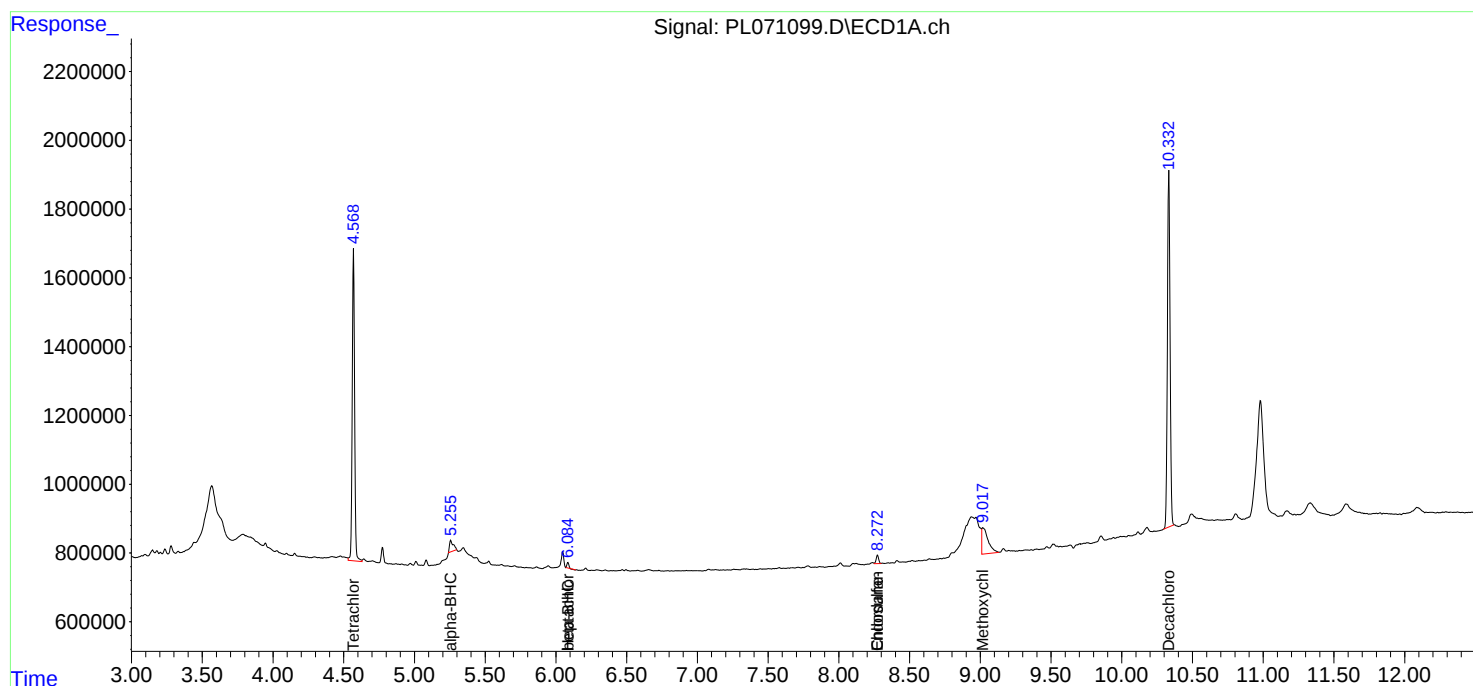


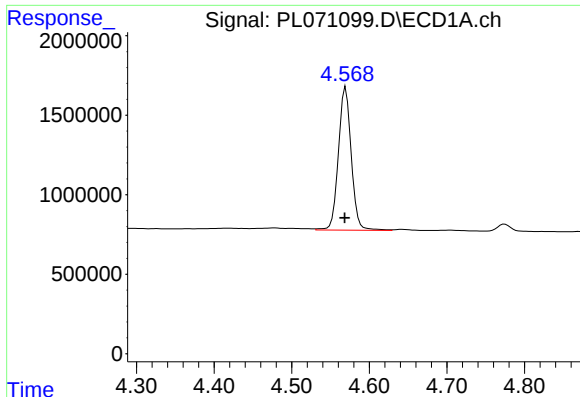

#1 Tetrachloro-m-xylene


R.T.: 4.570 min
Delta R.T.: 0.002 min
Response: 10364190
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

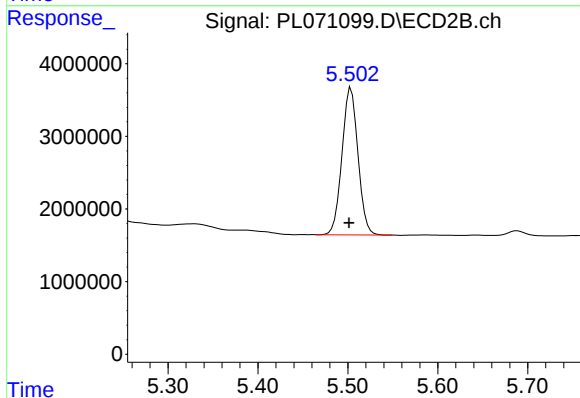


#1 Tetrachloro-m-xylene

R.T.: 5.504 min
Delta R.T.: 0.002 min
Response: 25016297
Conc: 19.84 ng/ml

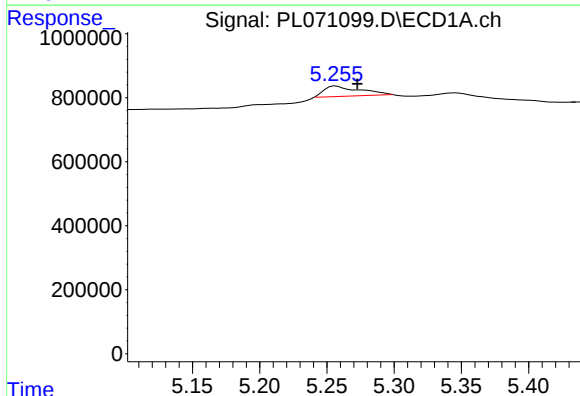


#2 alpha-BHC

R.T.: 5.257 min
Delta R.T.: -0.016 min
Response: 610789
Conc: 0.91 ng/ml

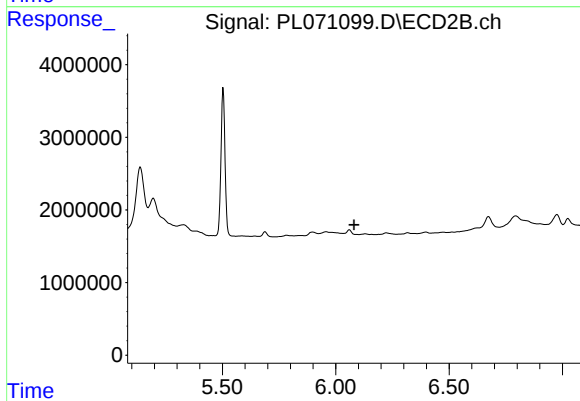

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.081 min
Response: 0
Conc: N.D.

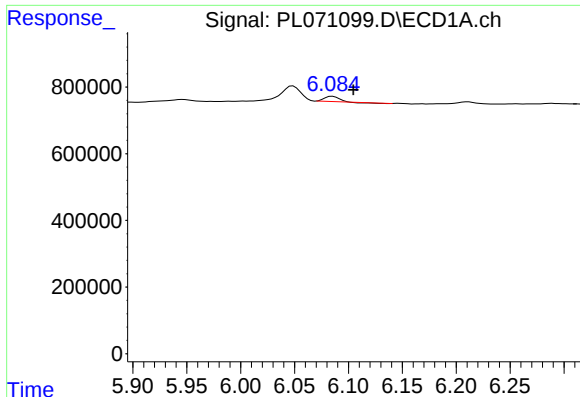

#4 Heptachlor


R.T.: 6.085 min
Delta R.T.: -0.019 min
Response: 109083
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

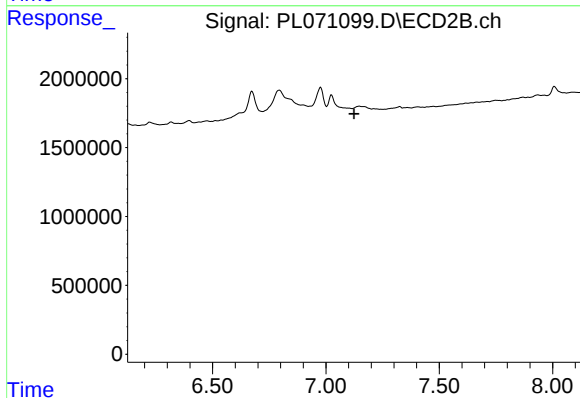


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.124 min
Response: 0
Conc: N.D.

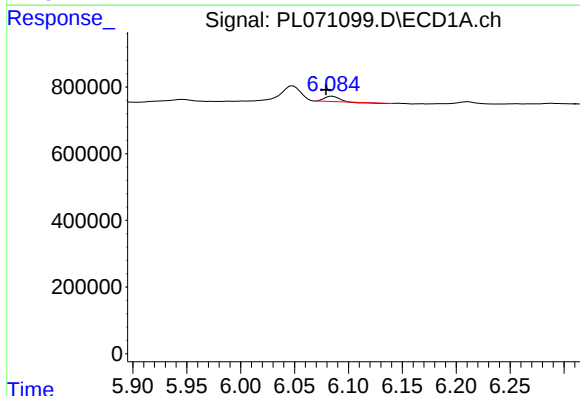


#6 beta-BHC

R.T.: 6.085 min
Delta R.T.: 0.006 min
Response: 109083
Conc: 0.34 ng/ml

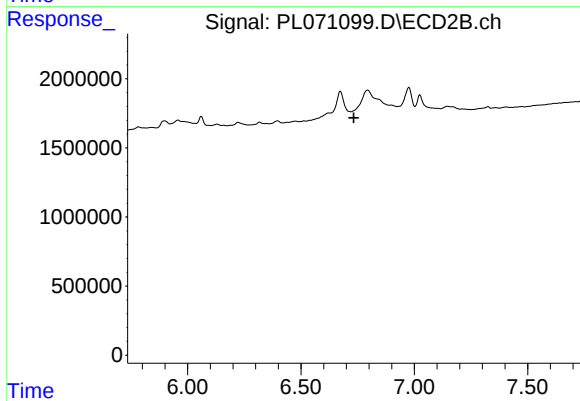

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.733 min
Response: 0
Conc: N.D.

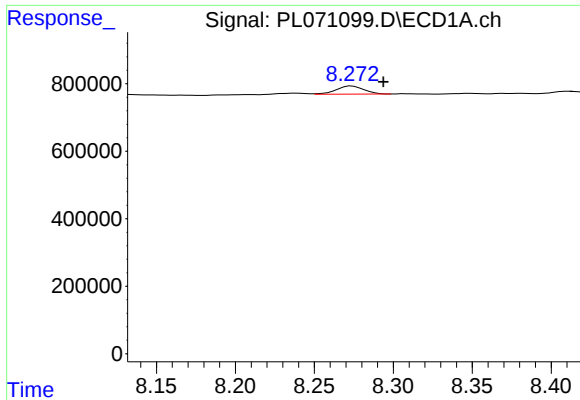

#15 Endosulfan II


R.T.: 8.274 min
Delta R.T.: -0.020 min
Response: 295951
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

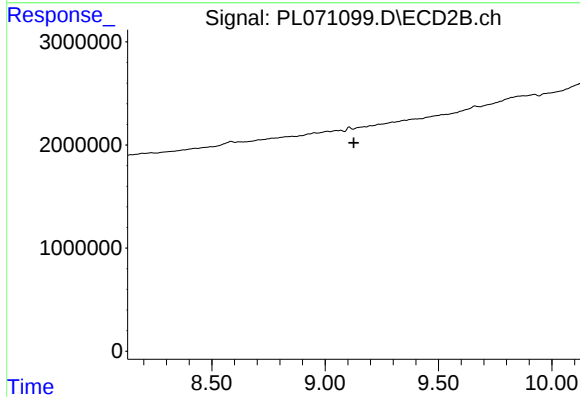


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.

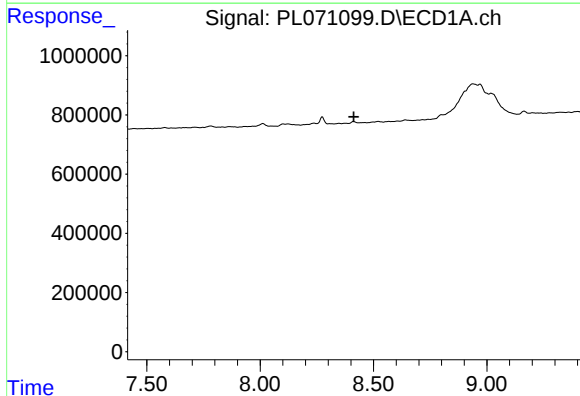


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.413 min
Response: 0
Conc: N.D.

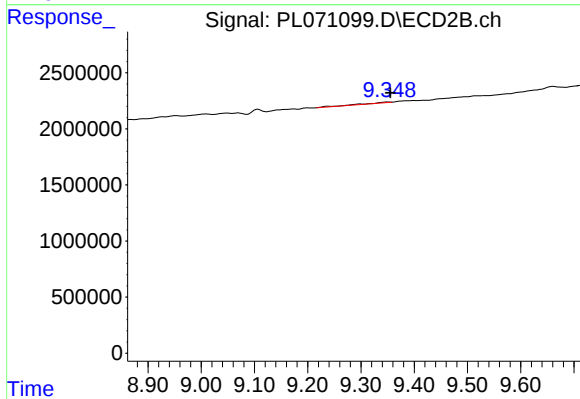

#17 4,4'-DDT


R.T.: 9.350 min
Delta R.T.: -0.005 min
Response: 240744
Conc: 0.19 ng/ml

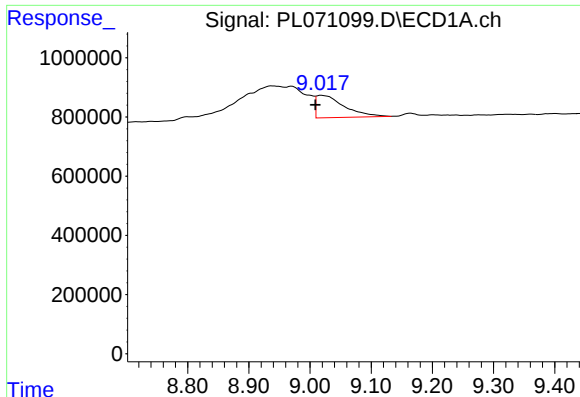

#20 Methoxychlor


R.T.: 9.018 min
Delta R.T.: 0.010 min
Response: 2399718
Conc: 6.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

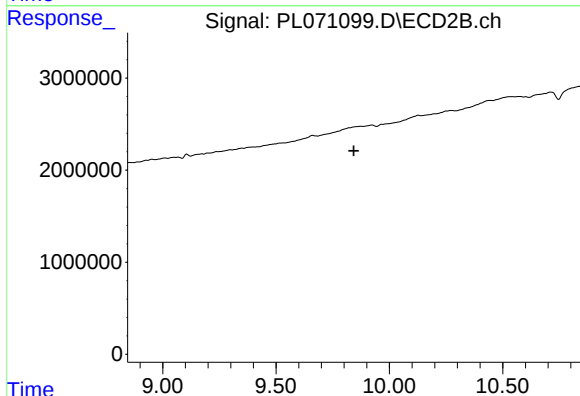


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.842 min
Response: 0
Conc: N.D.

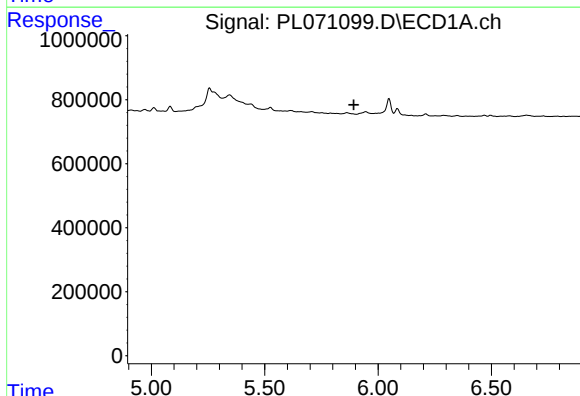


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.893 min
Response: 0
Conc: N.D.

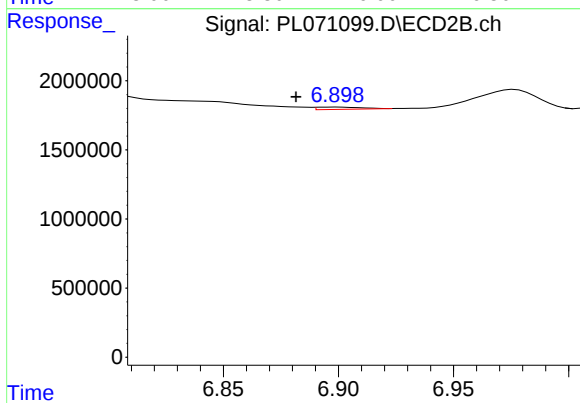

#23 Chlordane-1


R.T.: 6.900 min
Delta R.T.: 0.019 min
Response: 222438
Conc: 4.58 ng/ml

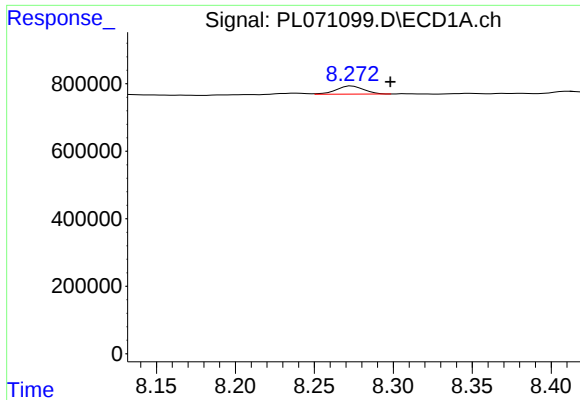

#27 Chlordane-5


R.T.: 8.274 min
Delta R.T.: -0.024 min
Response: 295951
Conc: 13.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

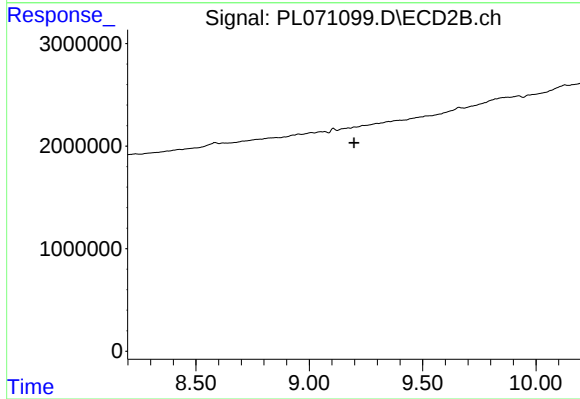


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

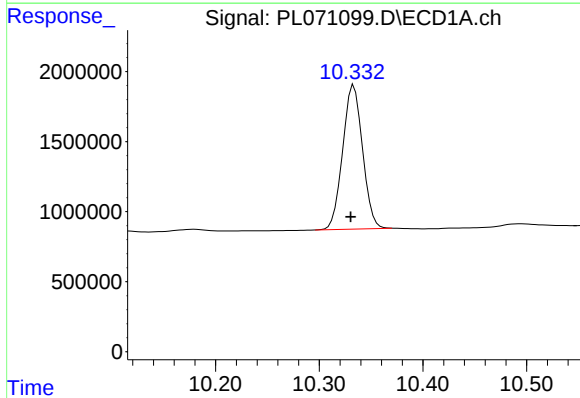

#28 Decachlorobiphenyl

R.T.: 10.333 min
Delta R.T.: 0.003 min
Response: 13700840
Conc: 20.05 ng/ml

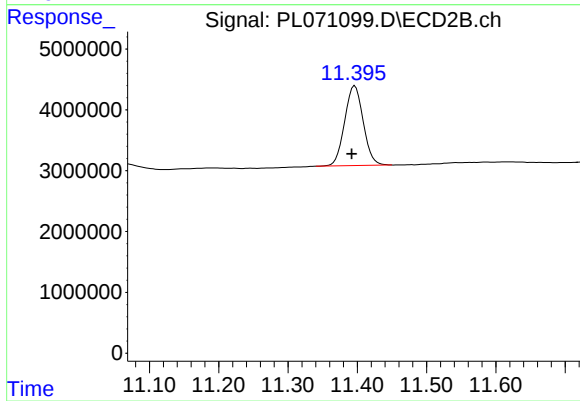

#28 Decachlorobiphenyl

R.T.: 11.396 min
Delta R.T.: 0.005 min
Response: 24447113
Conc: 18.28 ng/ml