

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL112221\  
 Data File : PL071115.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 22 Nov 2021 17:35  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 23 04:48:19 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL110321.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Nov 04 19:28:07 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|---------|
| -----                       |                 |        |        |          |          |        |         |
| System Monitoring Compounds |                 |        |        |          |          |        |         |
| 1)                          | SA Tetrachlo... | 4.566  | 5.501  | 10080660 | 25365406 | 20.581 | 20.118  |
| 28)                         | SA Decachlor... | 10.329 | 11.392 | 14050545 | 25697934 | 20.563 | 19.215  |
| Target Compounds            |                 |        |        |          |          |        |         |
| 7)                          | B delta-BHC     | 0.000  | 7.021f | 0        | 660192   | N.D.   | 0.395 # |
| 14)                         | MA Endrin       | 8.007f | 0.000  | 181650   | 0        | 0.320  | N.D. #  |
| 15)                         | B Endosulfa...  | 8.270f | 0.000  | 374485   | 0        | 0.619  | N.D. #  |
| 27)                         | Chlordane-5     | 8.270f | 0.000  | 374485   | 0        | 16.750 | N.D. #  |
| -----                       |                 |        |        |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL112221\  
Data File : PL071115.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 Nov 2021 17:35  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 23 04:48:19 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL110321.M  
Quant Title : GC Extractables  
QLast Update : Thu Nov 04 19:28:07 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

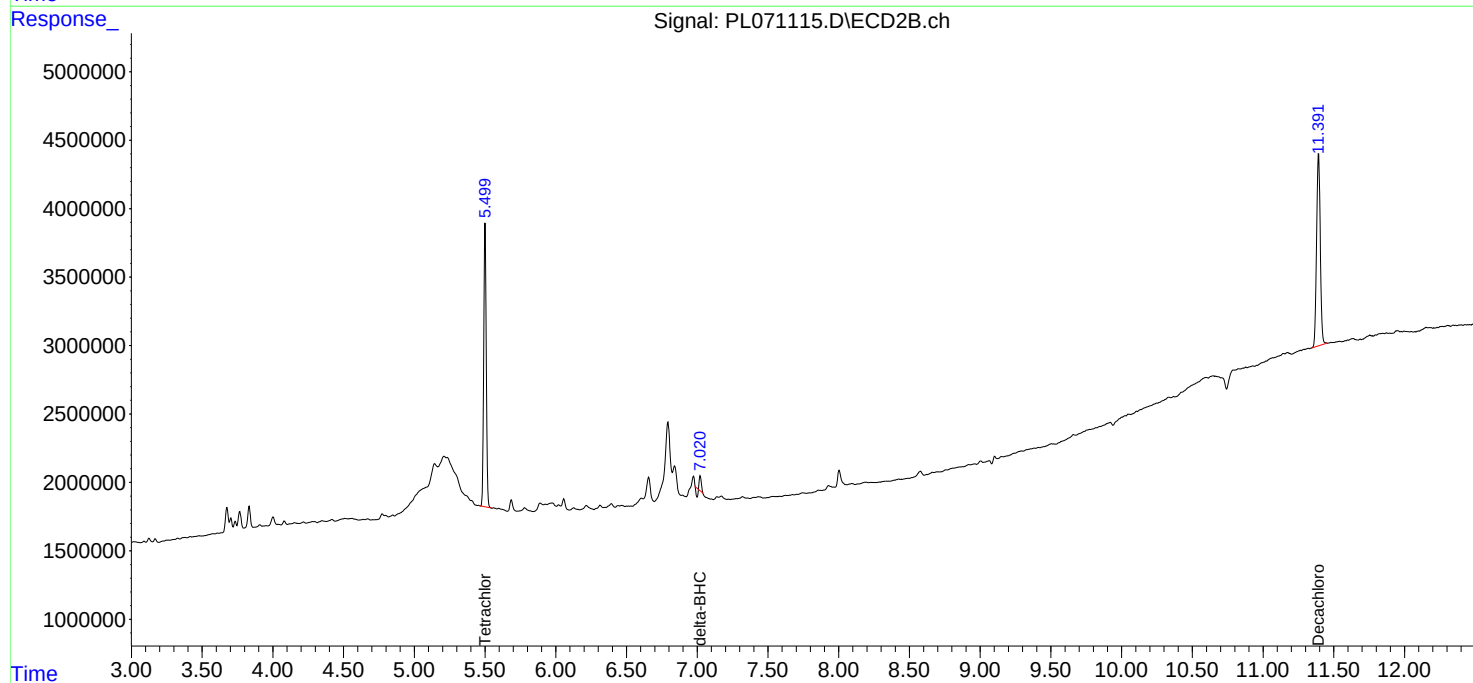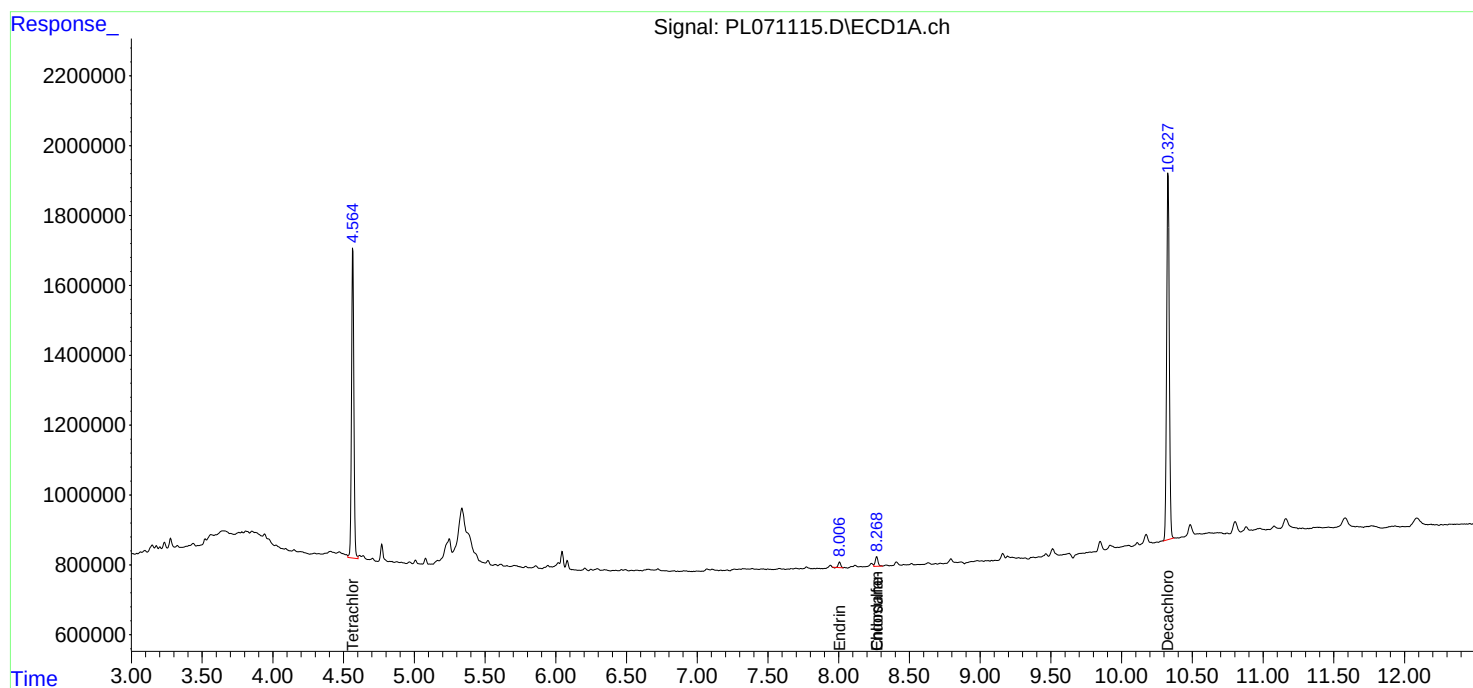


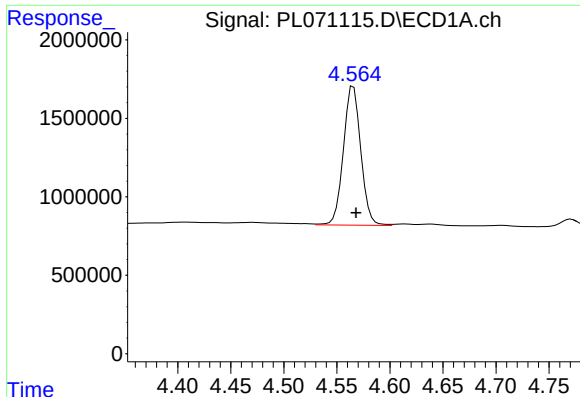

#1 Tetrachloro-m-xylene


R.T.: 4.566 min  
Delta R.T.: -0.002 min  
Response: 10080660  
Conc: 20.58 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
I.BLK

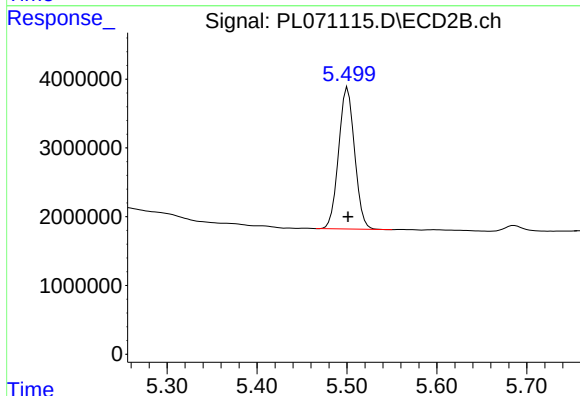


#1 Tetrachloro-m-xylene

R.T.: 5.501 min  
Delta R.T.: 0.000 min  
Response: 25365406  
Conc: 20.12 ng/ml

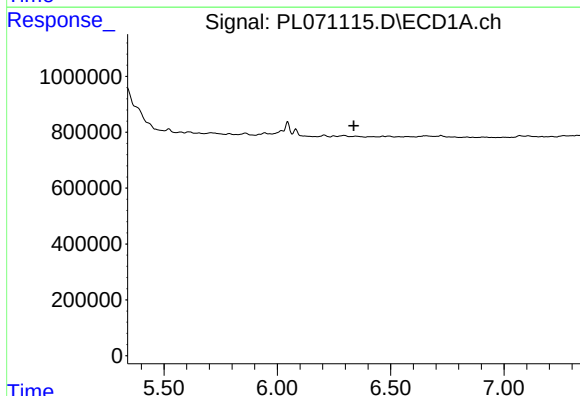


#7 delta-BHC

R.T.: 0.000 min  
Exp R.T. : 6.338 min  
Response: 0  
Conc: N.D.

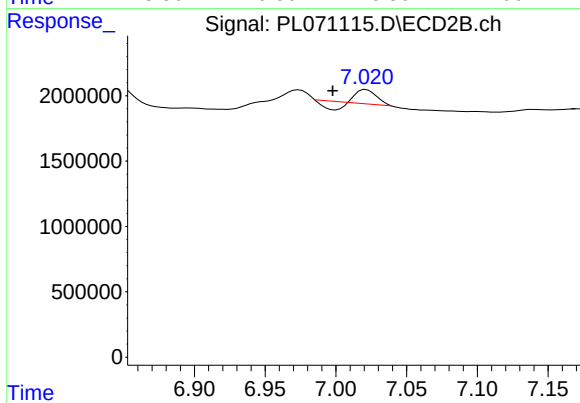

#7 delta-BHC


R.T.: 7.021 min  
Delta R.T.: 0.024 min  
Response: 660192  
Conc: 0.39 ng/ml

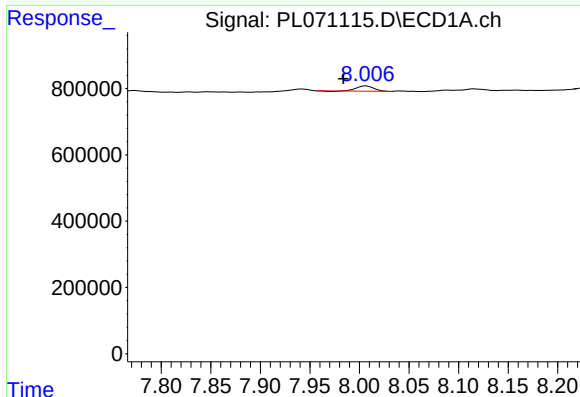

#14 Endrin


R.T.: 8.007 min  
Delta R.T.: 0.023 min  
Response: 181650  
Conc: 0.32 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
I.BLK

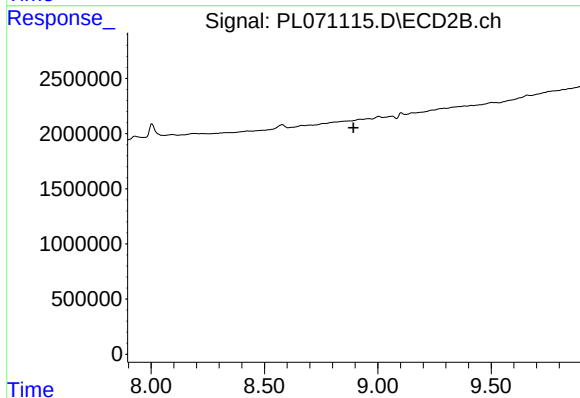


#14 Endrin

R.T.: 0.000 min  
Exp R.T. : 8.893 min  
Response: 0  
Conc: N.D.

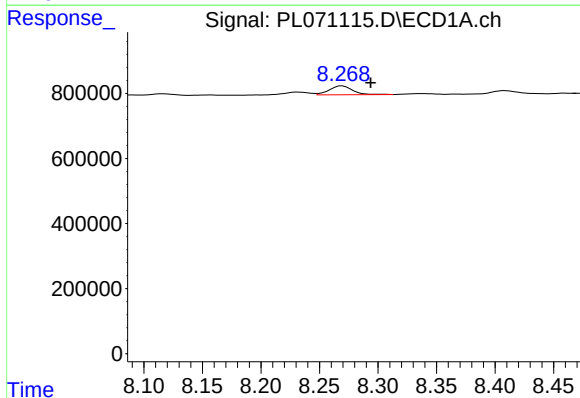


#15 Endosulfan II

R.T.: 8.270 min  
Delta R.T.: -0.024 min  
Response: 374485  
Conc: 0.62 ng/ml

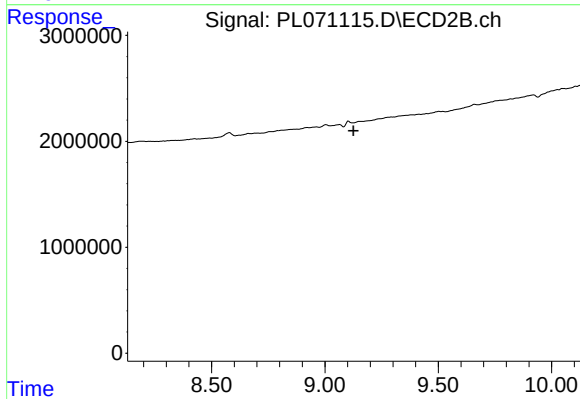

#15 Endosulfan II


R.T.: 0.000 min  
Exp R.T. : 9.126 min  
Response: 0  
Conc: N.D.

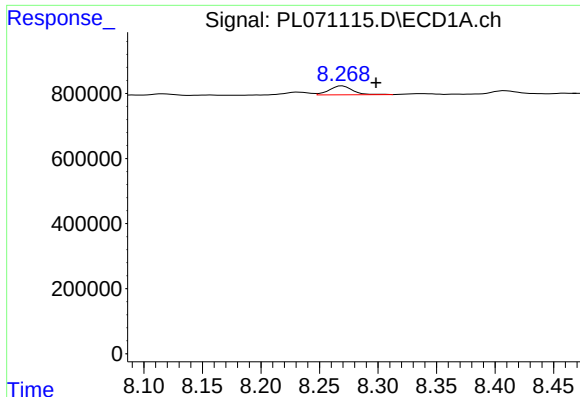

#27 Chlordane-5


R.T.: 8.270 min  
Delta R.T.: -0.029 min  
Response: 374485  
Conc: 16.75 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
I.BLK

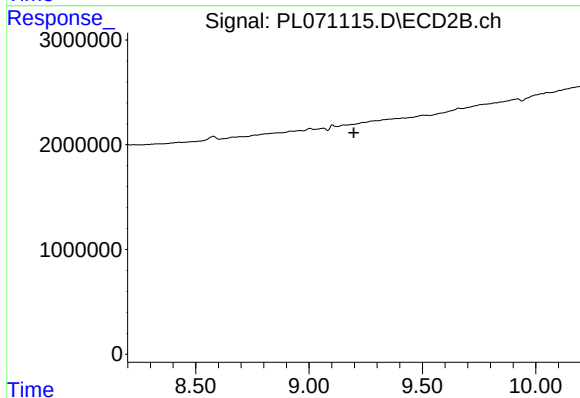


#27 Chlordane-5

R.T.: 0.000 min  
Exp R.T. : 9.197 min  
Response: 0  
Conc: N.D.

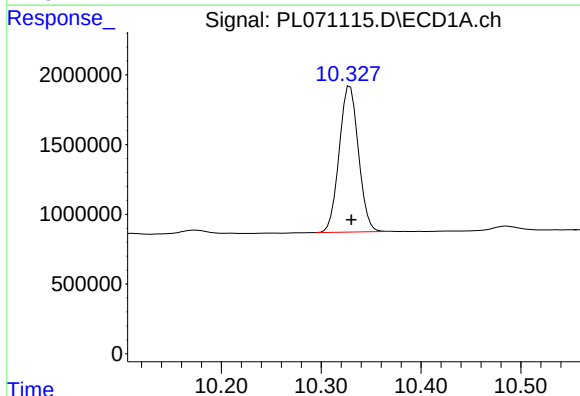

#28 Decachlorobiphenyl

R.T.: 10.329 min  
Delta R.T.: -0.001 min  
Response: 14050545  
Conc: 20.56 ng/ml

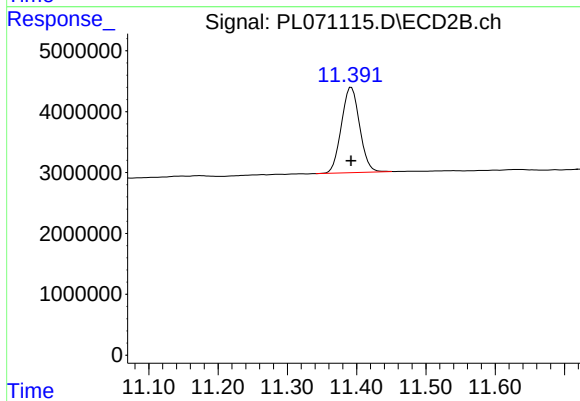

#28 Decachlorobiphenyl

R.T.: 11.392 min  
Delta R.T.: 0.000 min  
Response: 25697934  
Conc: 19.22 ng/ml