

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112221\
 Data File : PL071117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2021 18:09
 Operator : AR\AJ
 Sample : M4796-01 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-03-111921

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/23/2021
 Supervised By : Sohil Jodhani 11/23/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 04:48:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.499	1330469	3319247	2.716m	2.633m
28)	SA Decachlor...	10.329	11.393	2111356	3416507	3.090	2.555

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112221\
Data File : PL071117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2021 18:09
Operator : AR\AJ
Sample : M4796-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-03-111921


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/23/2021
Supervised By : Sohil Jodhani 11/23/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 04:48:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

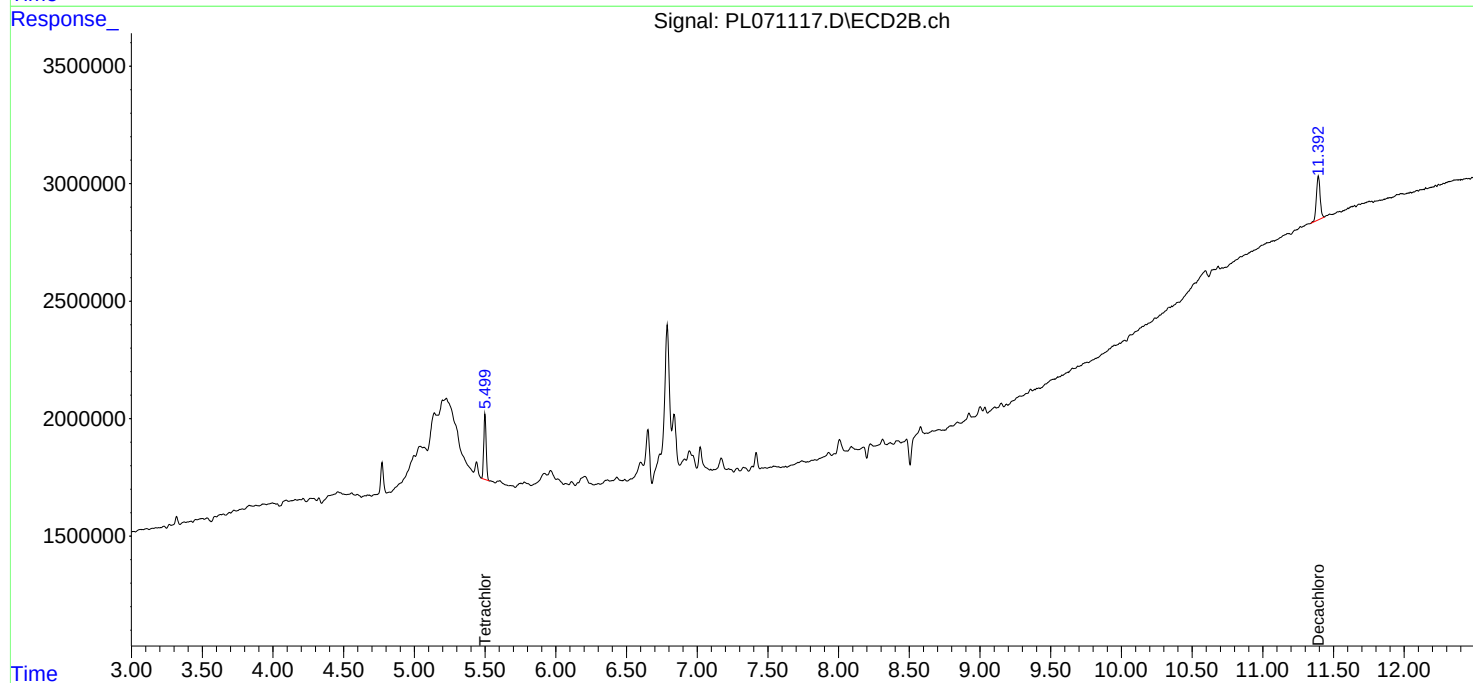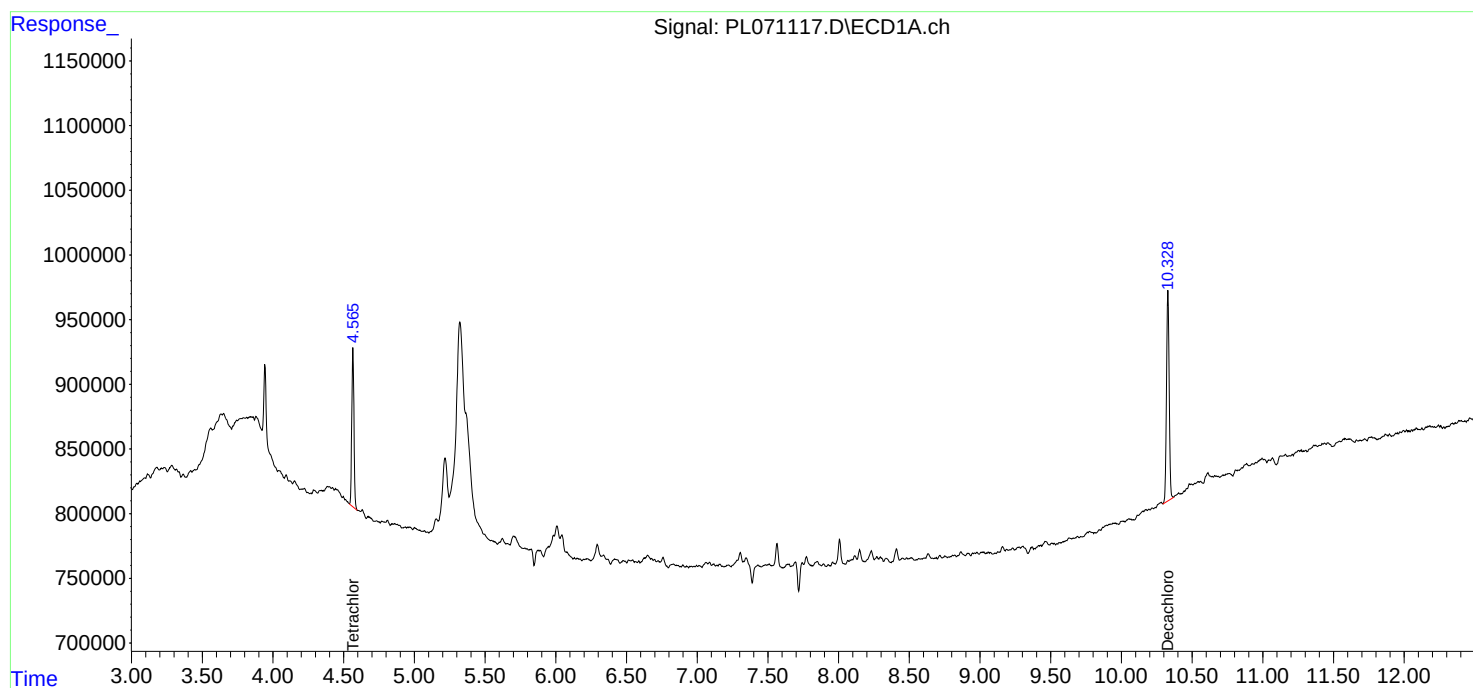

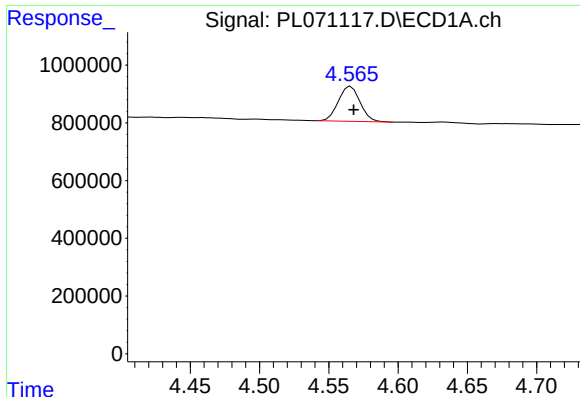


#1 Tetrachloro-m-xylene

R.T.: 4.565 min
Delta R.T.: -0.003 min
Response: 1330469
Conc: 2.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-03-111921


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/23/2021
Supervised By :Sohil Jodhani 11/23/2021

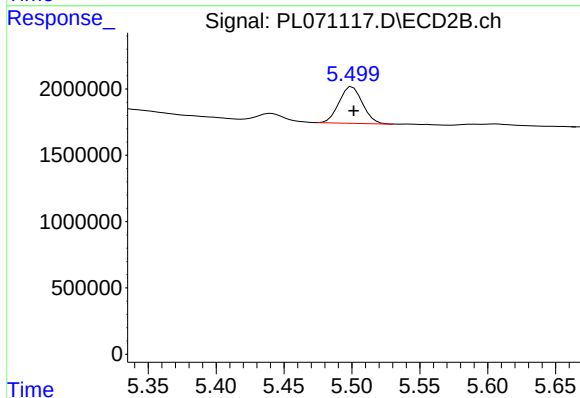


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: -0.003 min
Response: 3319247
Conc: 2.63 ng/ml m

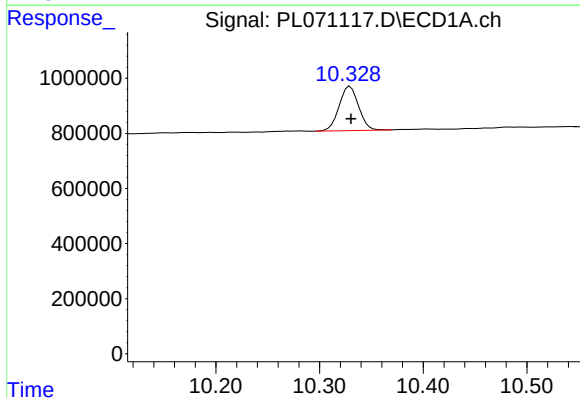

#28 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: 0.000 min
Response: 2111356
Conc: 3.09 ng/ml

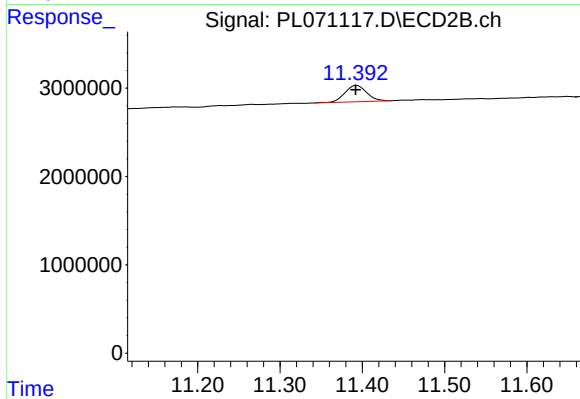

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: 0.002 min
Response: 3416507
Conc: 2.55 ng/ml