

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112222\
 Data File : PL079359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 11:49
 Operator : AR\AJ
 Sample : N5698-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 12:52:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.566	42858081	51771144	20.581	20.327
28)	SA Decachlor...	8.769	7.633	30186784	34842864	18.046	16.796
Target Compounds							
3)	MA gamma-BHC...	4.127	3.401f	310847	234174	0.104	0.066 #
8)	B Heptachlo...	5.461	4.463	5363276	839073	2.269	0.270 #
9)	A Endosulfan I	5.835	0.000	5254360	0	2.188	N.D. #
10)	B gamma-Chl...	5.712	0.000	3804844	0	1.489	N.D. #
12)	B 4,4'-DDE	5.969	0.000	281960	0	0.123	N.D. #
13)	MA Dieldrin	0.000	5.092	0	3442683	N.D.	1.120 #
14)	MA Endrin	0.000	5.388f	0	1834032	N.D.	0.702 #
20)	A Methoxychlor	7.311f	0.000	198379	0	0.186	N.D. #
24)	Chlordane-2	0.000	4.097	0	959485	N.D.	9.035 #
25)	Chlordane-3	5.712	0.000	3804844	0	9.878	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112222\
Data File : PL079359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 11:49
Operator : AR\AJ
Sample : N5698-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 12:52:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

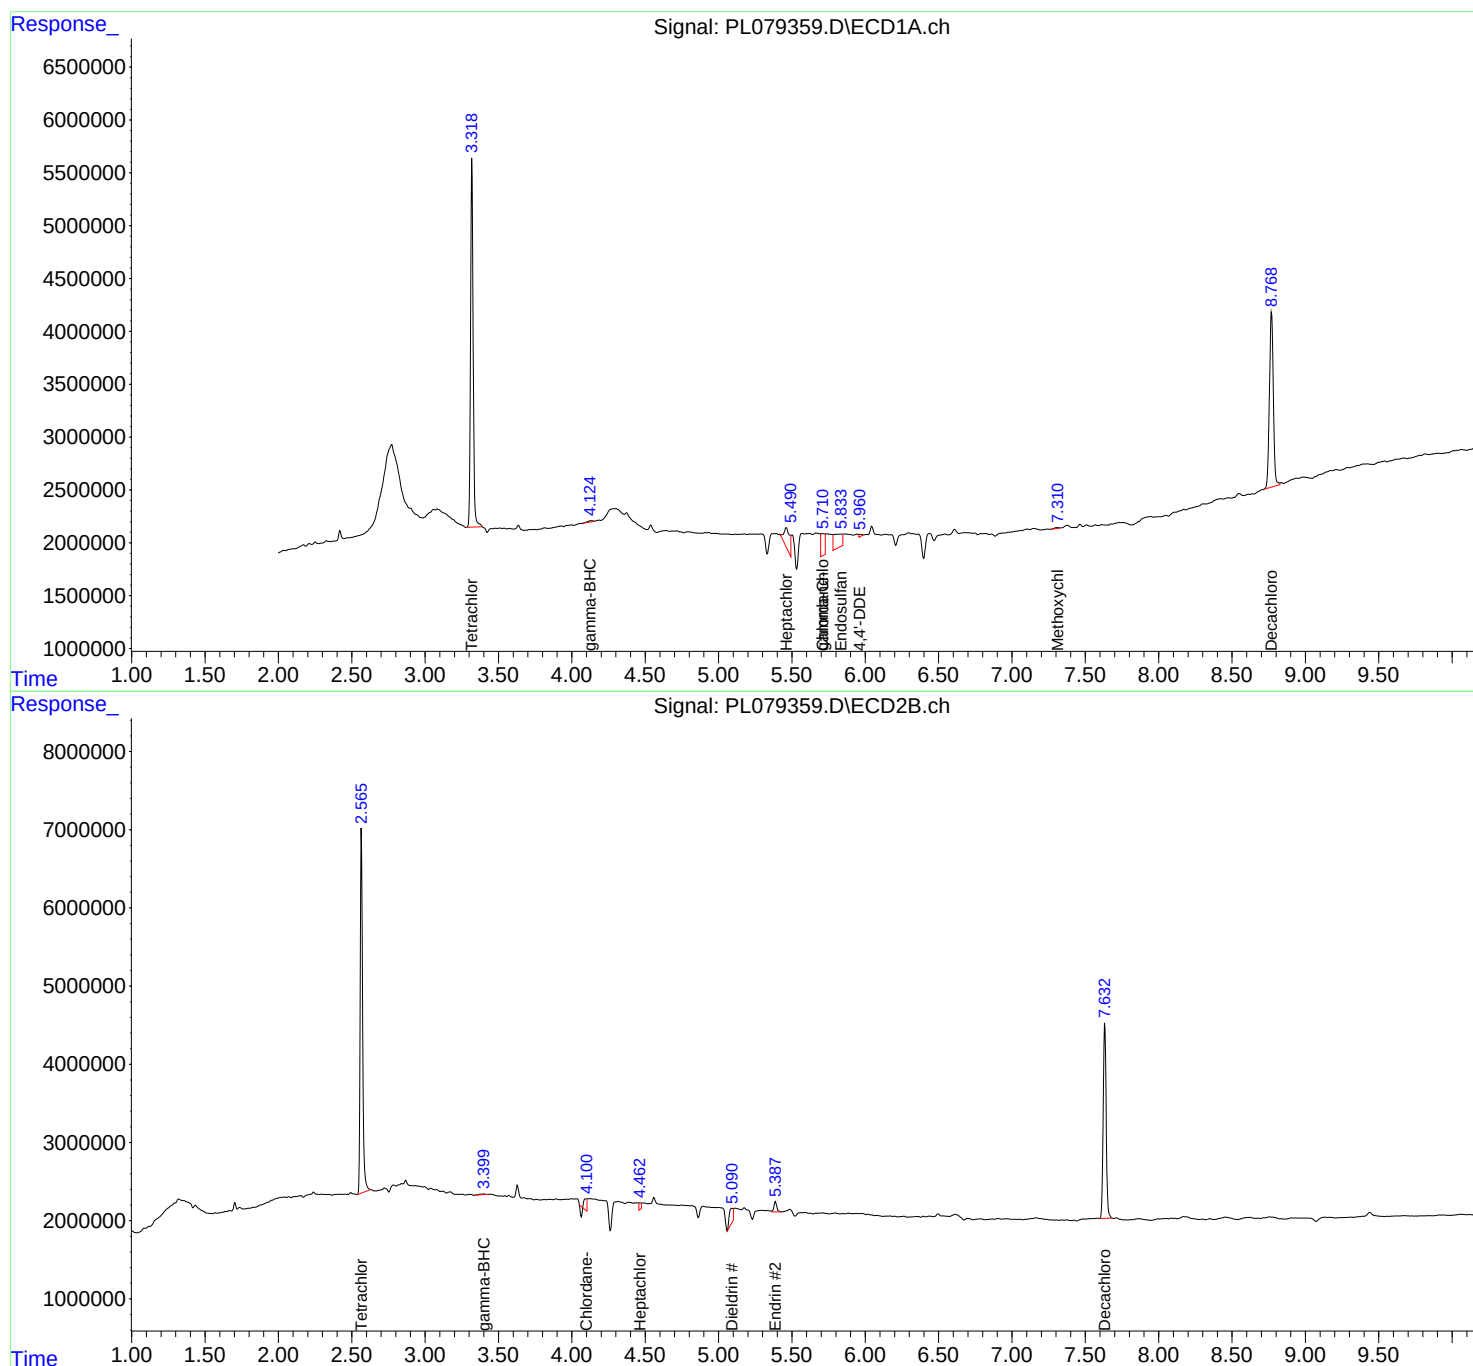


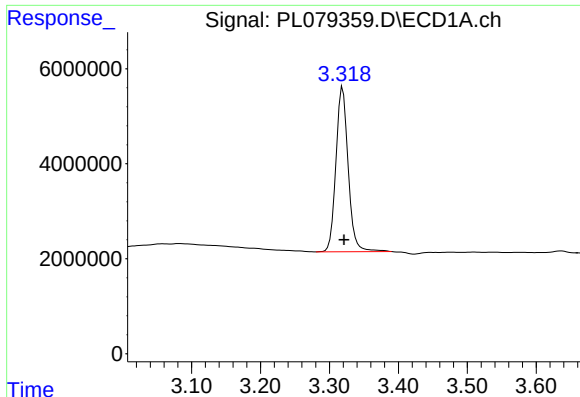

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 42858081
Conc: 20.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

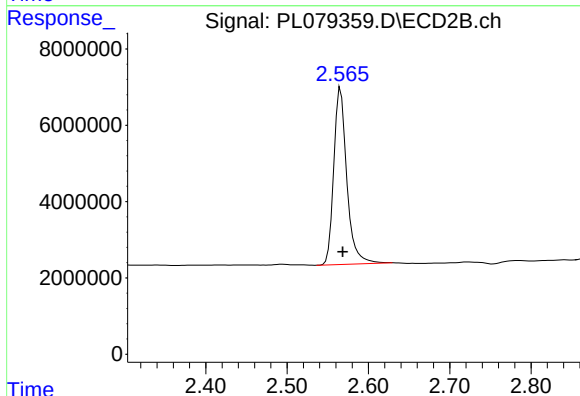


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: -0.003 min
Response: 51771144
Conc: 20.33 ng/ml

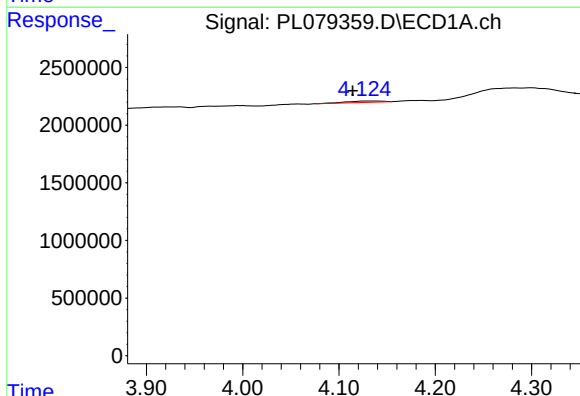


#3 gamma-BHC (Lindane)

R.T.: 4.127 min
Delta R.T.: 0.013 min
Response: 310847
Conc: 0.10 ng/ml

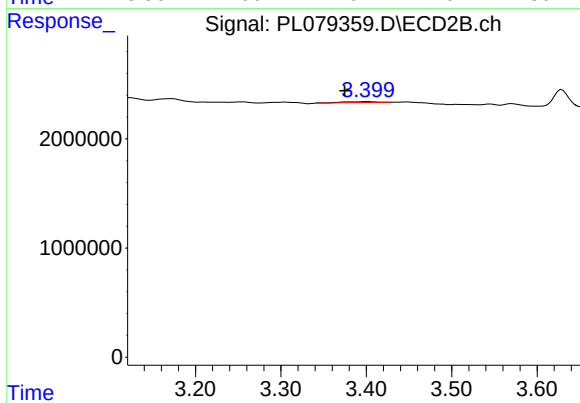

#3 gamma-BHC (Lindane)


R.T.: 3.401 min
Delta R.T.: 0.026 min
Response: 234174
Conc: 0.07 ng/ml

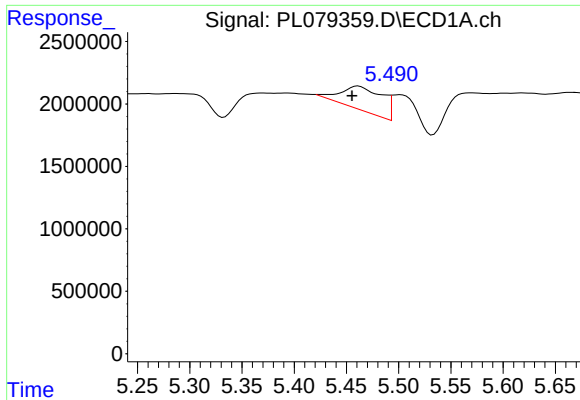

#8 Heptachlor epoxide


R.T.: 5.461 min
Delta R.T.: 0.006 min
Response: 5363276
Conc: 2.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

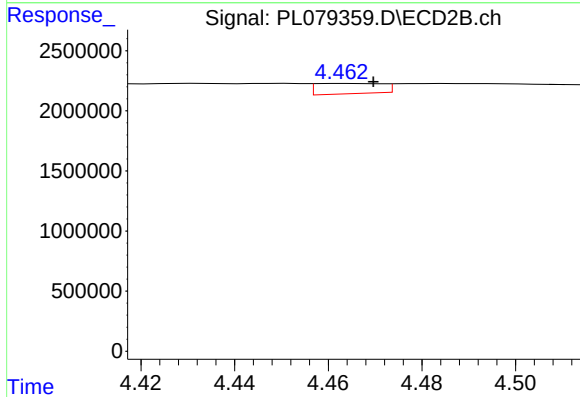


#8 Heptachlor epoxide

R.T.: 4.463 min
Delta R.T.: -0.006 min
Response: 839073
Conc: 0.27 ng/ml

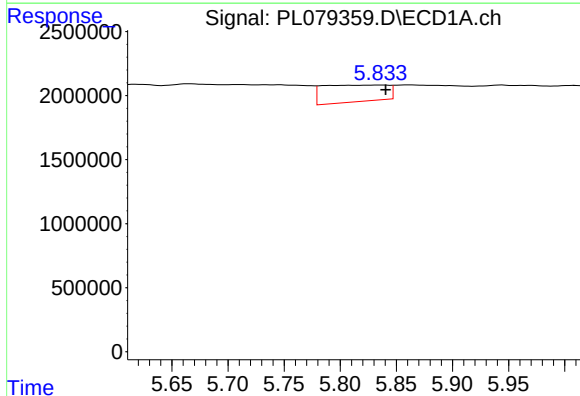


#9 Endosulfan I

R.T.: 5.835 min
Delta R.T.: -0.006 min
Response: 5254360
Conc: 2.19 ng/ml

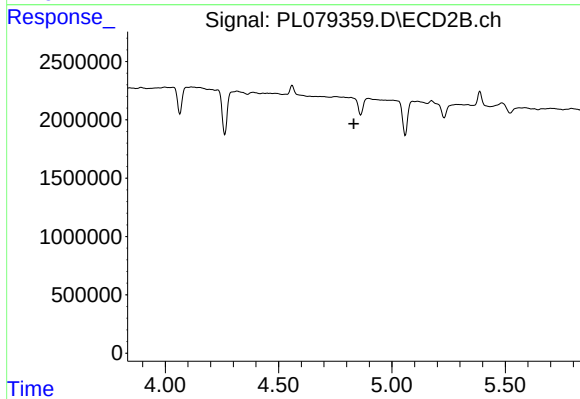

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 4.832 min
Response: 0
Conc: N.D.

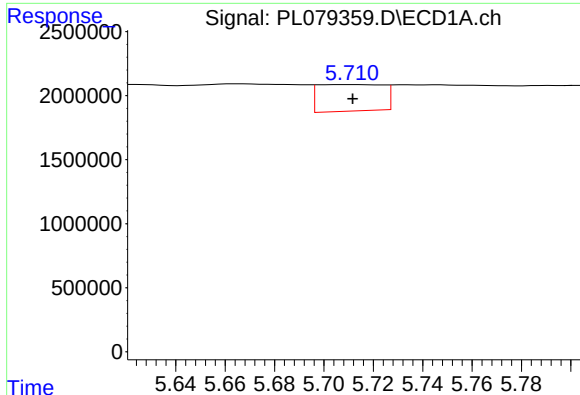

#10 gamma-Chlordane


R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 3804844
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

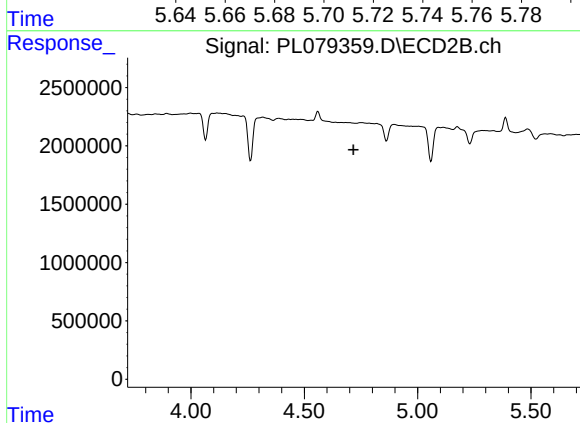


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.718 min
Response: 0
Conc: N.D.

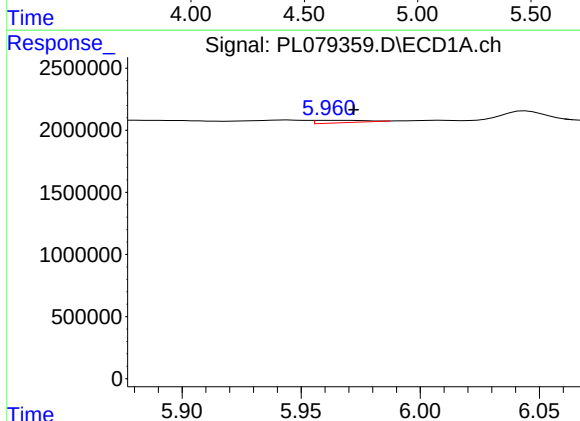


#12 4,4'-DDE

R.T.: 5.969 min
Delta R.T.: -0.003 min
Response: 281960
Conc: 0.12 ng/ml

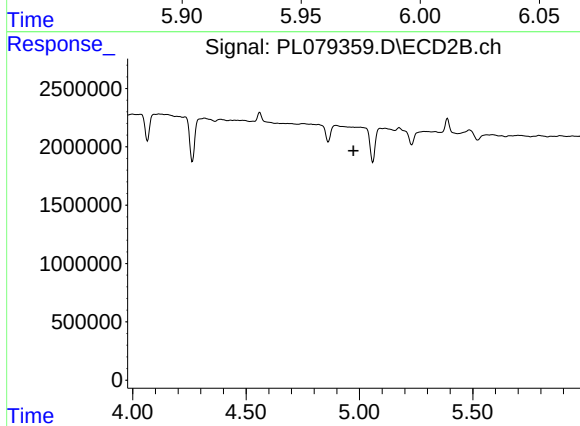

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

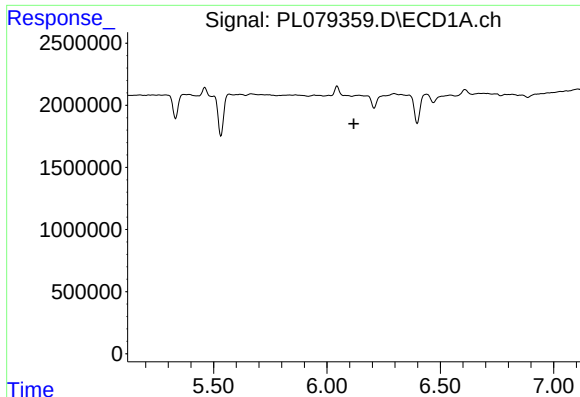

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

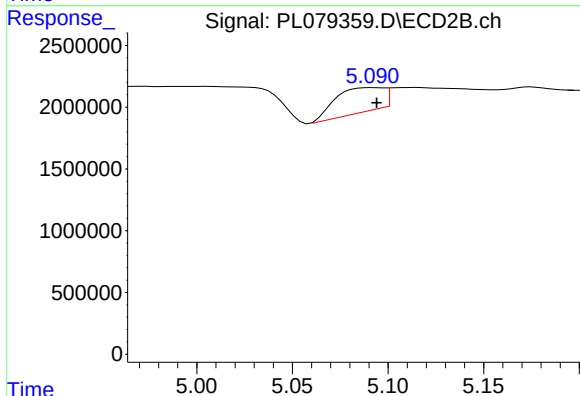


#13 Dieldrin

R.T.: 5.092 min
Delta R.T.: -0.002 min
Response: 3442683
Conc: 1.12 ng/ml

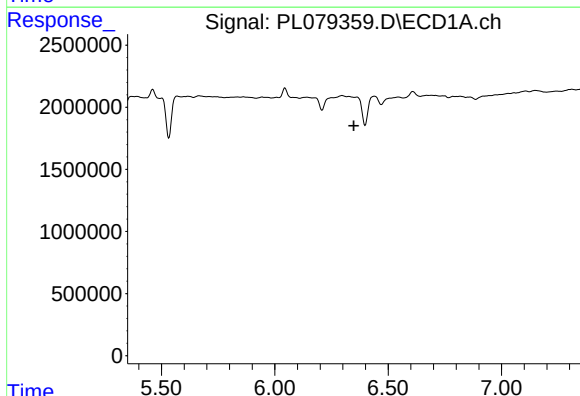


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.349 min
Response: 0
Conc: N.D.

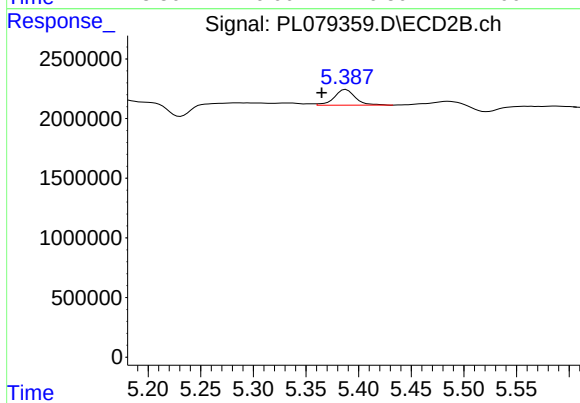

#14 Endrin


R.T.: 5.388 min
Delta R.T.: 0.023 min
Response: 1834032
Conc: 0.70 ng/ml

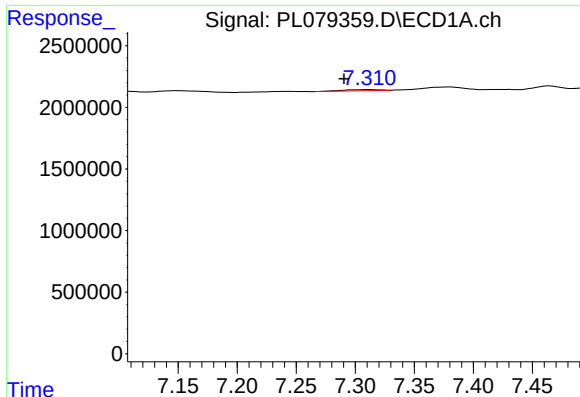

#20 Methoxychlor


R.T.: 7.311 min
Delta R.T.: 0.021 min
Response: 198379
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

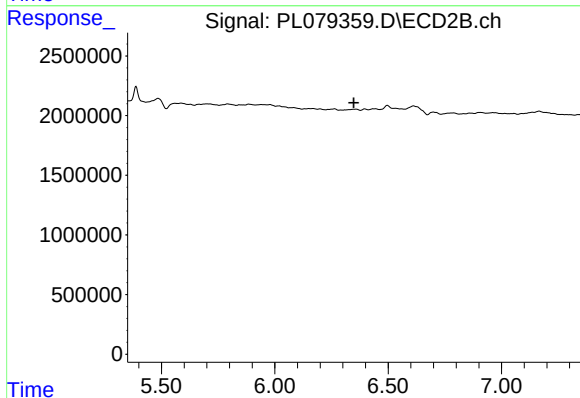


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.349 min
Response: 0
Conc: N.D.

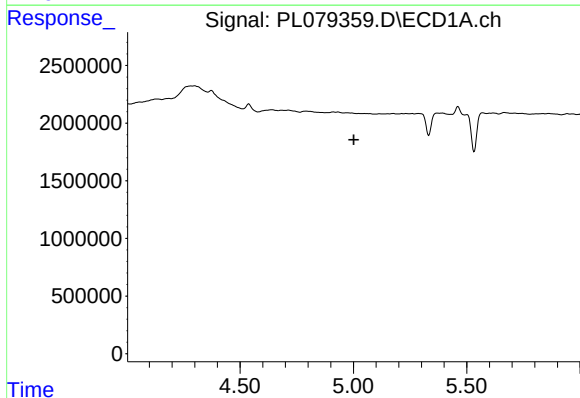


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.002 min
Response: 0
Conc: N.D.

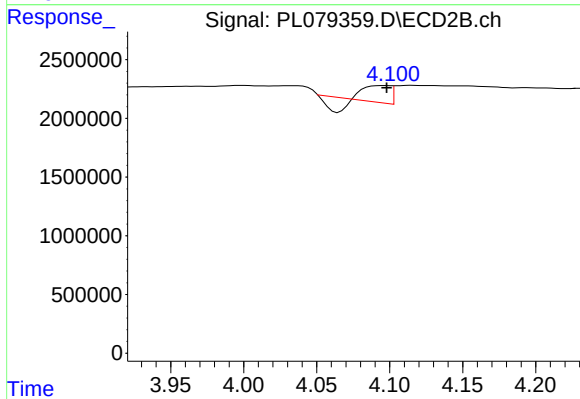

#24 Chlordane-2


R.T.: 4.097 min
Delta R.T.: -0.001 min
Response: 959485
Conc: 9.04 ng/ml

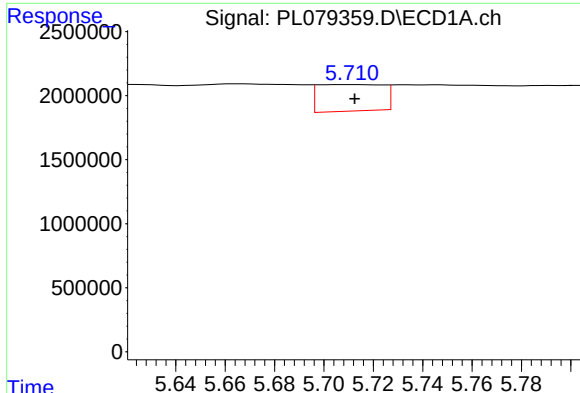

#25 Chlordane-3


R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 3804844
Conc: 9.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

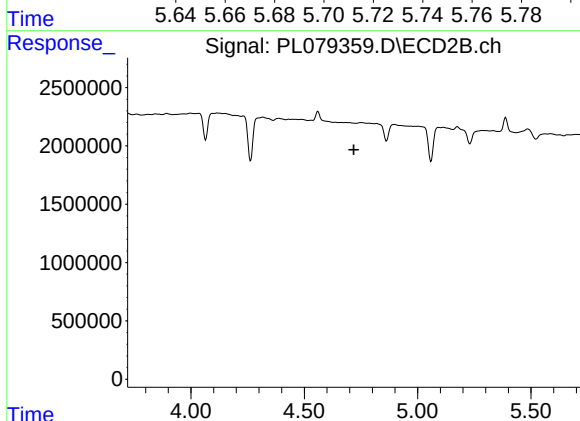


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.718 min
Response: 0
Conc: N.D.

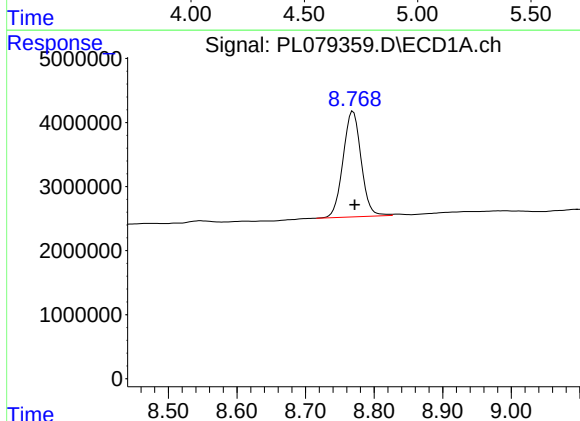

#28 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.002 min
Response: 30186784
Conc: 18.05 ng/ml

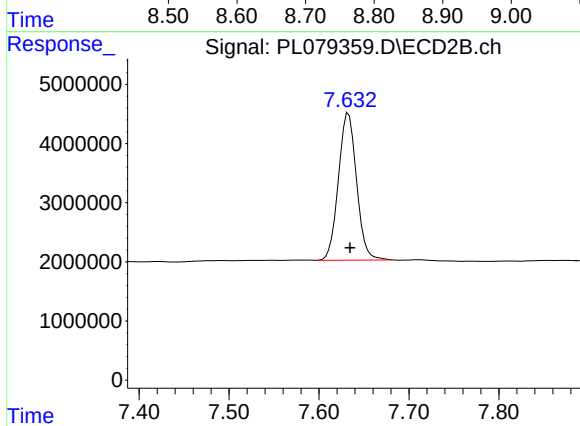

#28 Decachlorobiphenyl

R.T.: 7.633 min
Delta R.T.: -0.002 min
Response: 34842864
Conc: 16.80 ng/ml