

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112222\
 Data File : PL079372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 16:31
 Operator : AR\AJ
 Sample : N5740-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-12

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/23/2022
 Supervised By : Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:52:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.319	2.566	46505648	54886872	22.333	21.551
2) SA Decachlor...	8.766	7.631	32194139	35068459	19.246	16.905
Target Compounds						
13) MA Dieldrin	6.117	5.091	1110005	1456076	0.458m	0.474

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112222\
Data File : PL079372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 16:31
Operator : AR\AJ
Sample : N5740-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MH-12


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/23/2022
Supervised By : Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:52:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

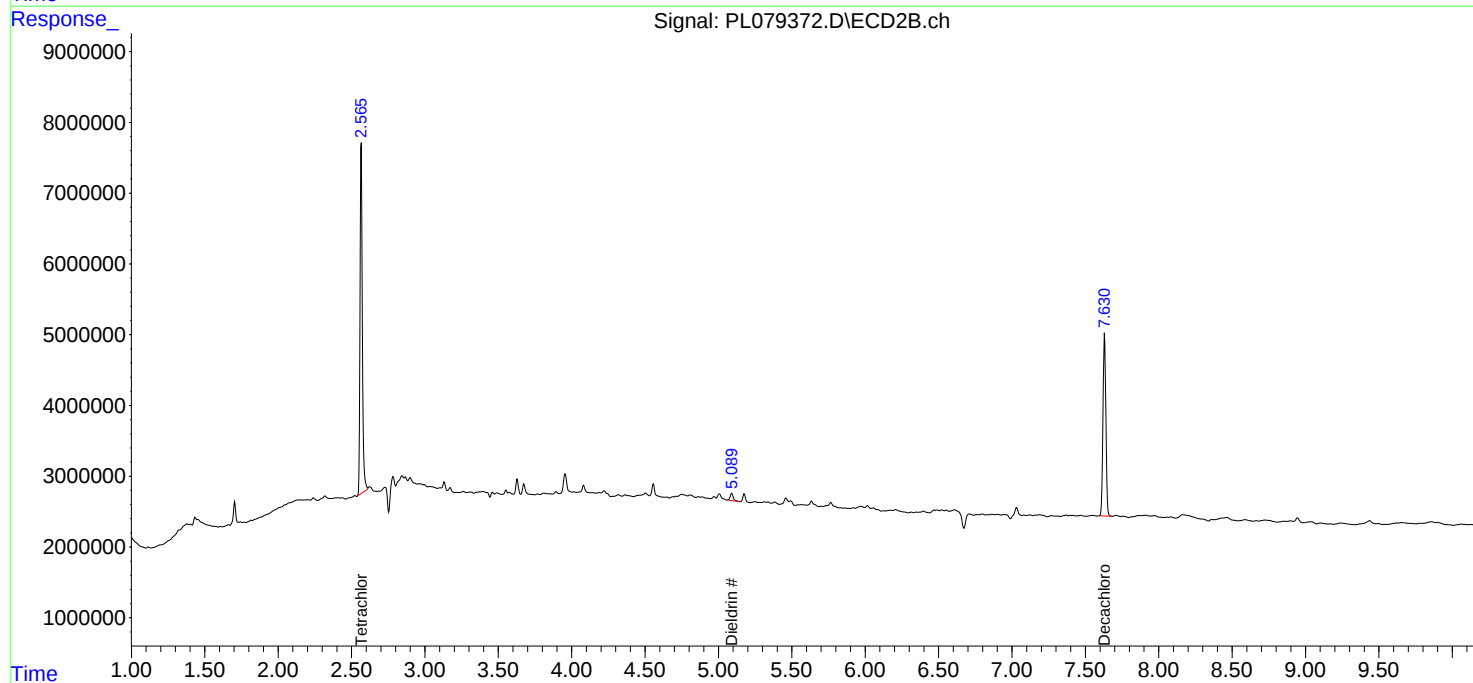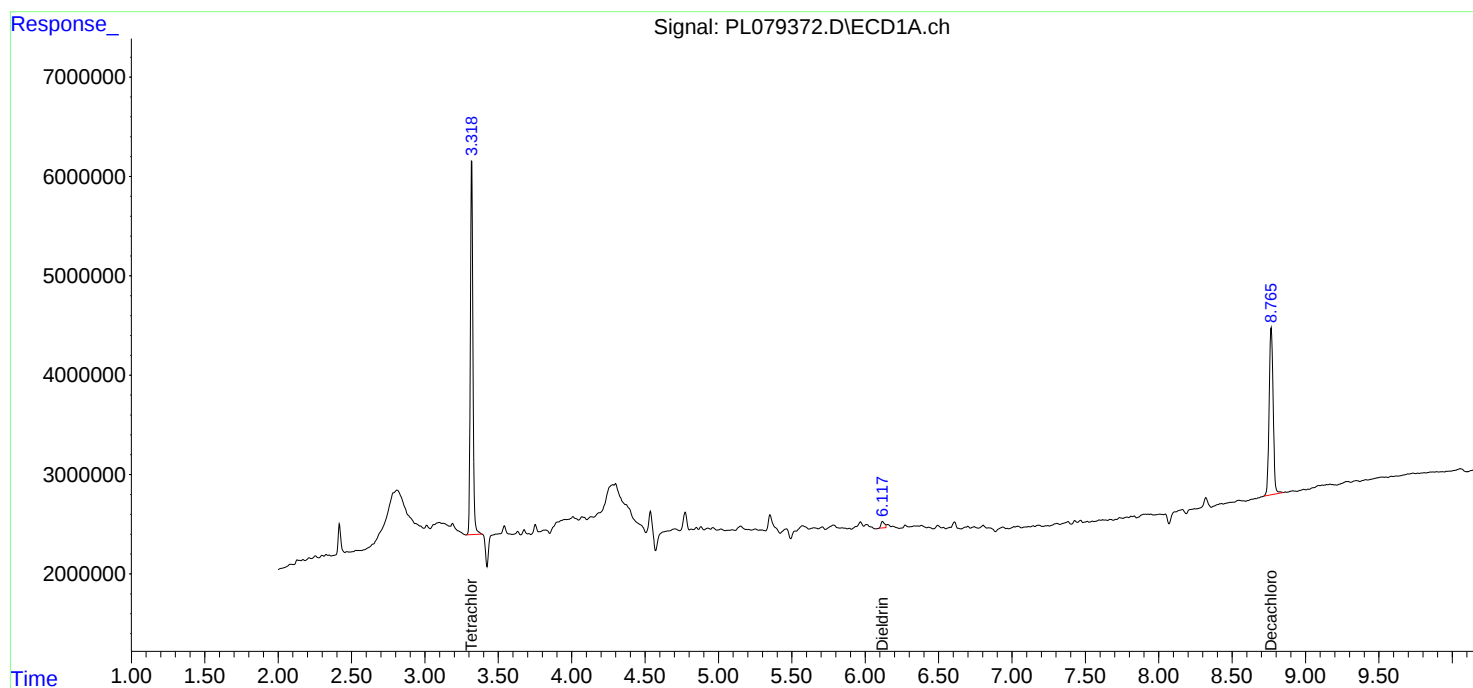

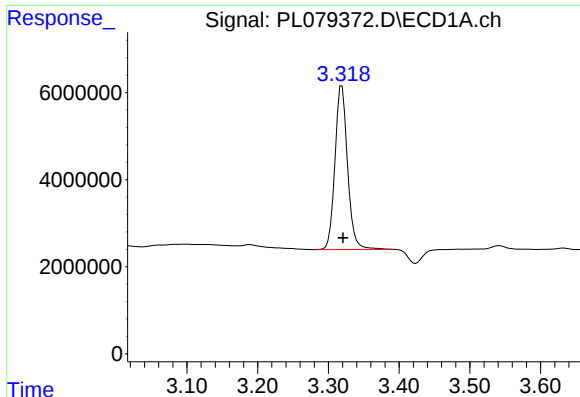


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 46505648
Conc: 22.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-12


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

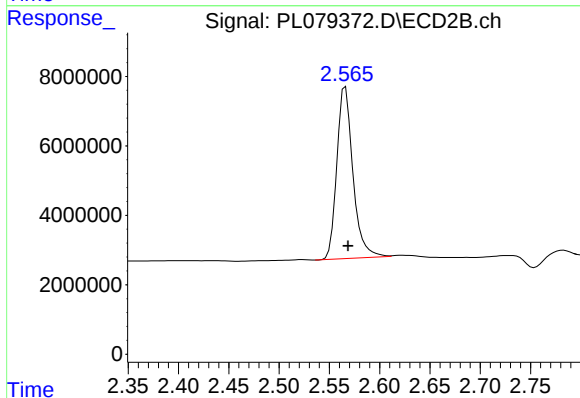


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: -0.003 min
Response: 54886872
Conc: 21.55 ng/ml

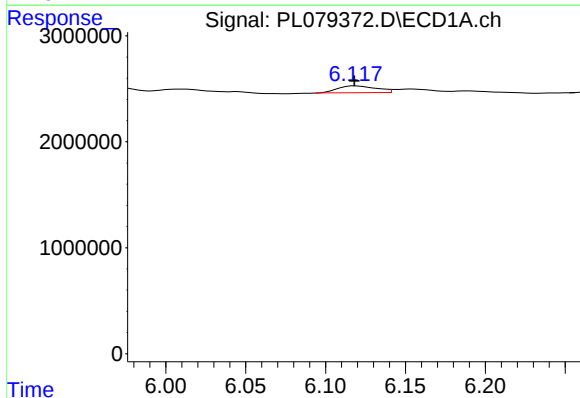


#13 Dieldrin

R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 1110005
Conc: 0.46 ng/ml m

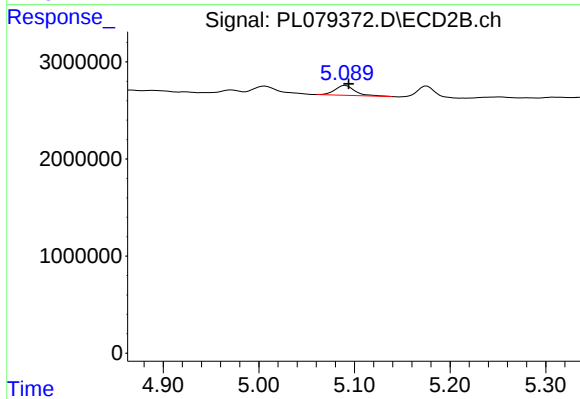

#13 Dieldrin

R.T.: 5.091 min
Delta R.T.: -0.003 min
Response: 1456076
Conc: 0.47 ng/ml

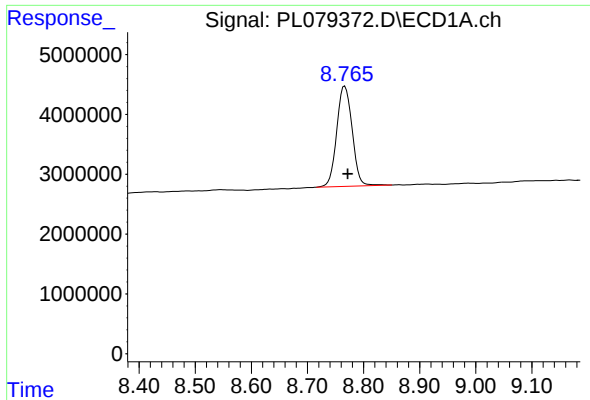


#28 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.005 min
Response: 32194139
Conc: 19.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-12

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

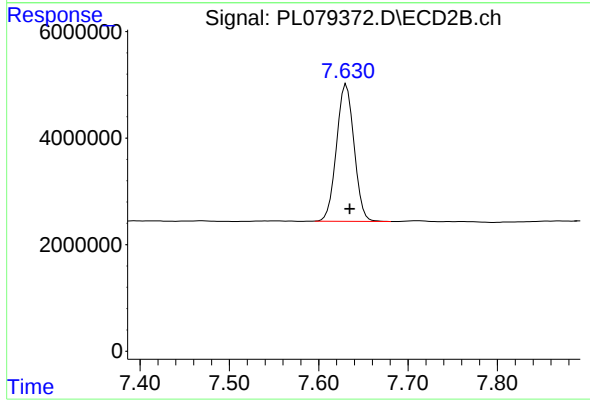

#28 Decachlorobiphenyl

R.T.: 7.631 min
Delta R.T.: -0.004 min
Response: 35068459
Conc: 16.90 ng/ml