

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112222\
 Data File : PL079387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 21:02
 Operator : AR\AJ
 Sample : N5655-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/23/2022
 Supervised By :Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 03:50:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.310	2.573	20004692	10078351	9.607m	3.957m#
2) SA Decachlor...	8.766	7.630	10523152	15743350	6.291m	7.589

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112222\
Data File : PL079387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 21:02
Operator : AR\AJ
Sample : N5655-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/23/2022
Supervised By : Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 03:50:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

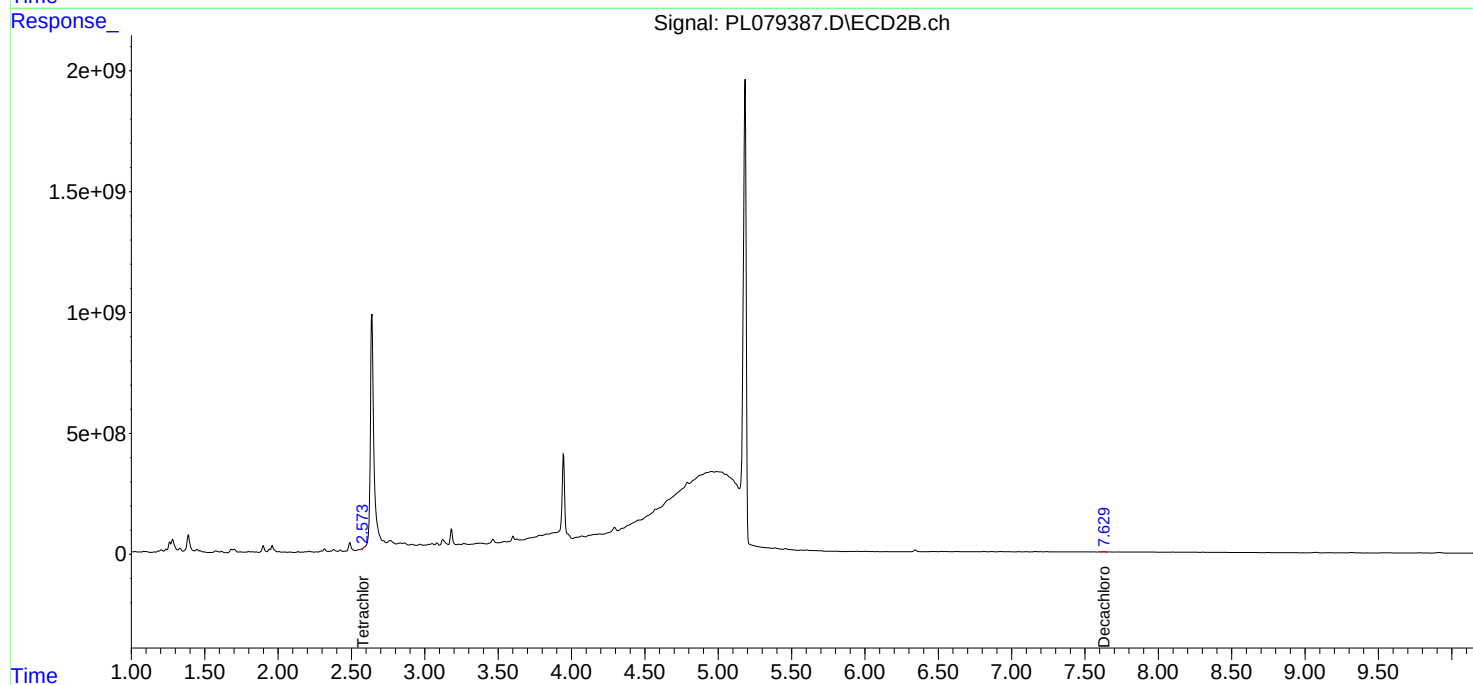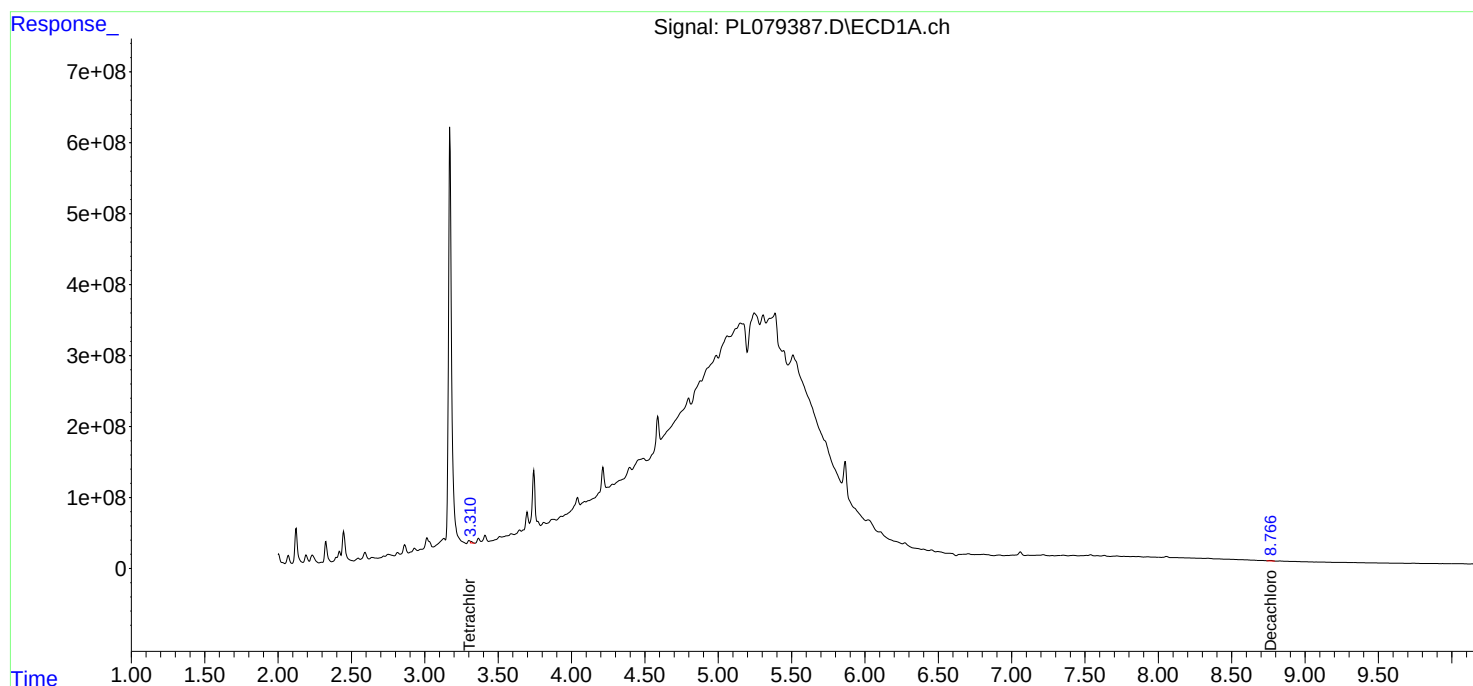

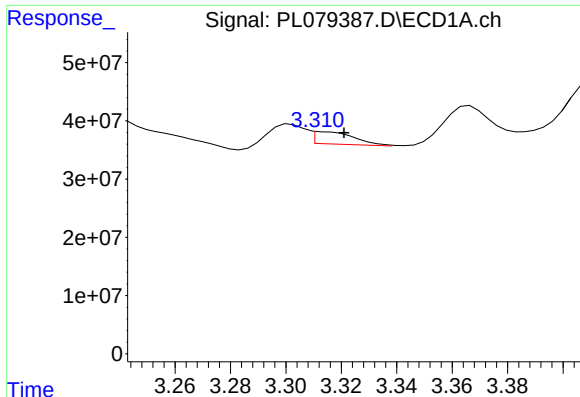


#1 Tetrachloro-m-xylene

R.T.: 3.310 min
Delta R.T.: -0.011 min
Response: 20004692
Conc: 9.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

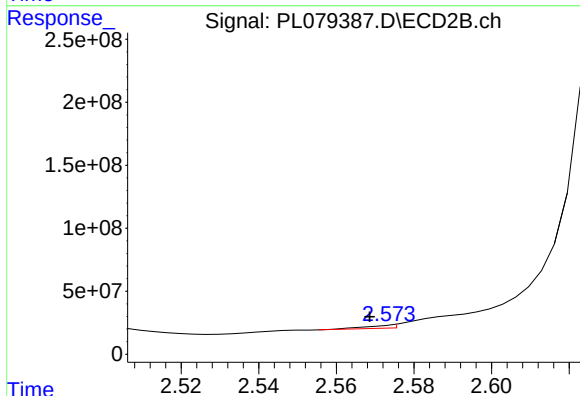


#1 Tetrachloro-m-xylene

R.T.: 2.573 min
Delta R.T.: 0.004 min
Response: 10078351
Conc: 3.96 ng/ml m

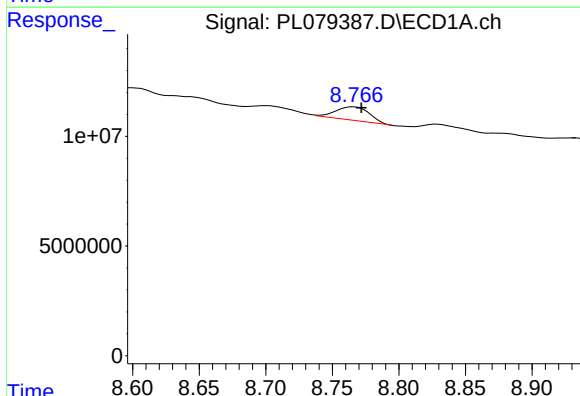

#28 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.005 min
Response: 10523152
Conc: 6.29 ng/ml m

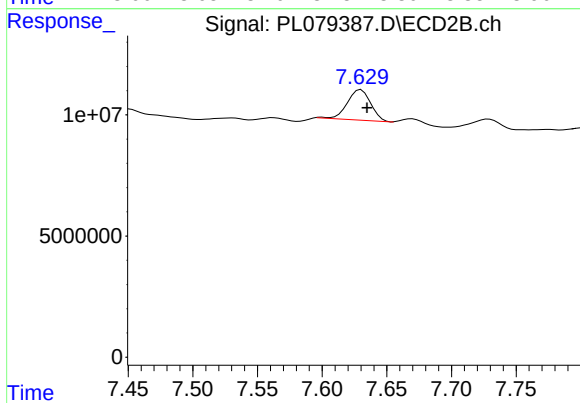

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: -0.005 min
Response: 15743350
Conc: 7.59 ng/ml