

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112223\
 Data File : PL086796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2023 08:35
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:32:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.617	64890237	19655556	19.984	19.962
2)	SA Decachlor...	8.856	7.768	54874718	24586525	18.747	20.360
Target Compounds							
2)	A alpha-BHC	3.806	3.115	45505857	12341959	9.460	9.259
3)	MA gamma-BHC...	4.138	3.442	43941127	12066254	9.340	9.092
5)	MB Aldrin	0.000	4.071f	0	188586	N.D.	0.145 #
6)	B beta-BHC	4.342	3.745	22172870	6776730	10.963	11.370
9)	A Endosulfan I	0.000	4.939	0	401458	N.D.	0.349 #
11)	B alpha-Chl...	0.000	4.887	0	1101630	N.D.	0.881 #
12)	B 4,4'-DDE	6.015	5.074	1085318	156731	0.313	0.153 #
14)	MA Endrin	6.384	5.466	140.8E6	50138127	40.892	45.774
15)	B Endosulfa...	6.605	5.750f	3184872	85203	0.896	0.078 #
16)	A 4,4'-DDD	6.535	5.630	6638552	2256387	2.493	2.648
17)	MA 4,4'-DDT	6.850	5.881	277.8E6	105.0E6	93.728	107.442
18)	B Endrin al...	6.739	5.946	6216440	4674195	2.345	4.990 #
19)	B Endosulfa...	6.959	6.173	543859	-48466	0.162	N.D. #
20)	A Methoxychlor	7.337	6.466	352.3E6	144.1E6	220.785	240.841
21)	B Endrin ke...	7.457	6.672	9773125	5125046	2.868	4.000 #
22)	Mirex	0.000	6.837	0	38338	N.D.	0.034 #
23)	Chlordane-1	0.000	3.580f	0	11024	N.D.	0.315 #
24)	Chlordane-2	0.000	4.166f	0	106620	N.D.	2.361 #
26)	Chlordane-4	0.000	4.887	0	1101630	N.D.	8.628 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112223\
Data File : PL086796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2023 08:35
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:32:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

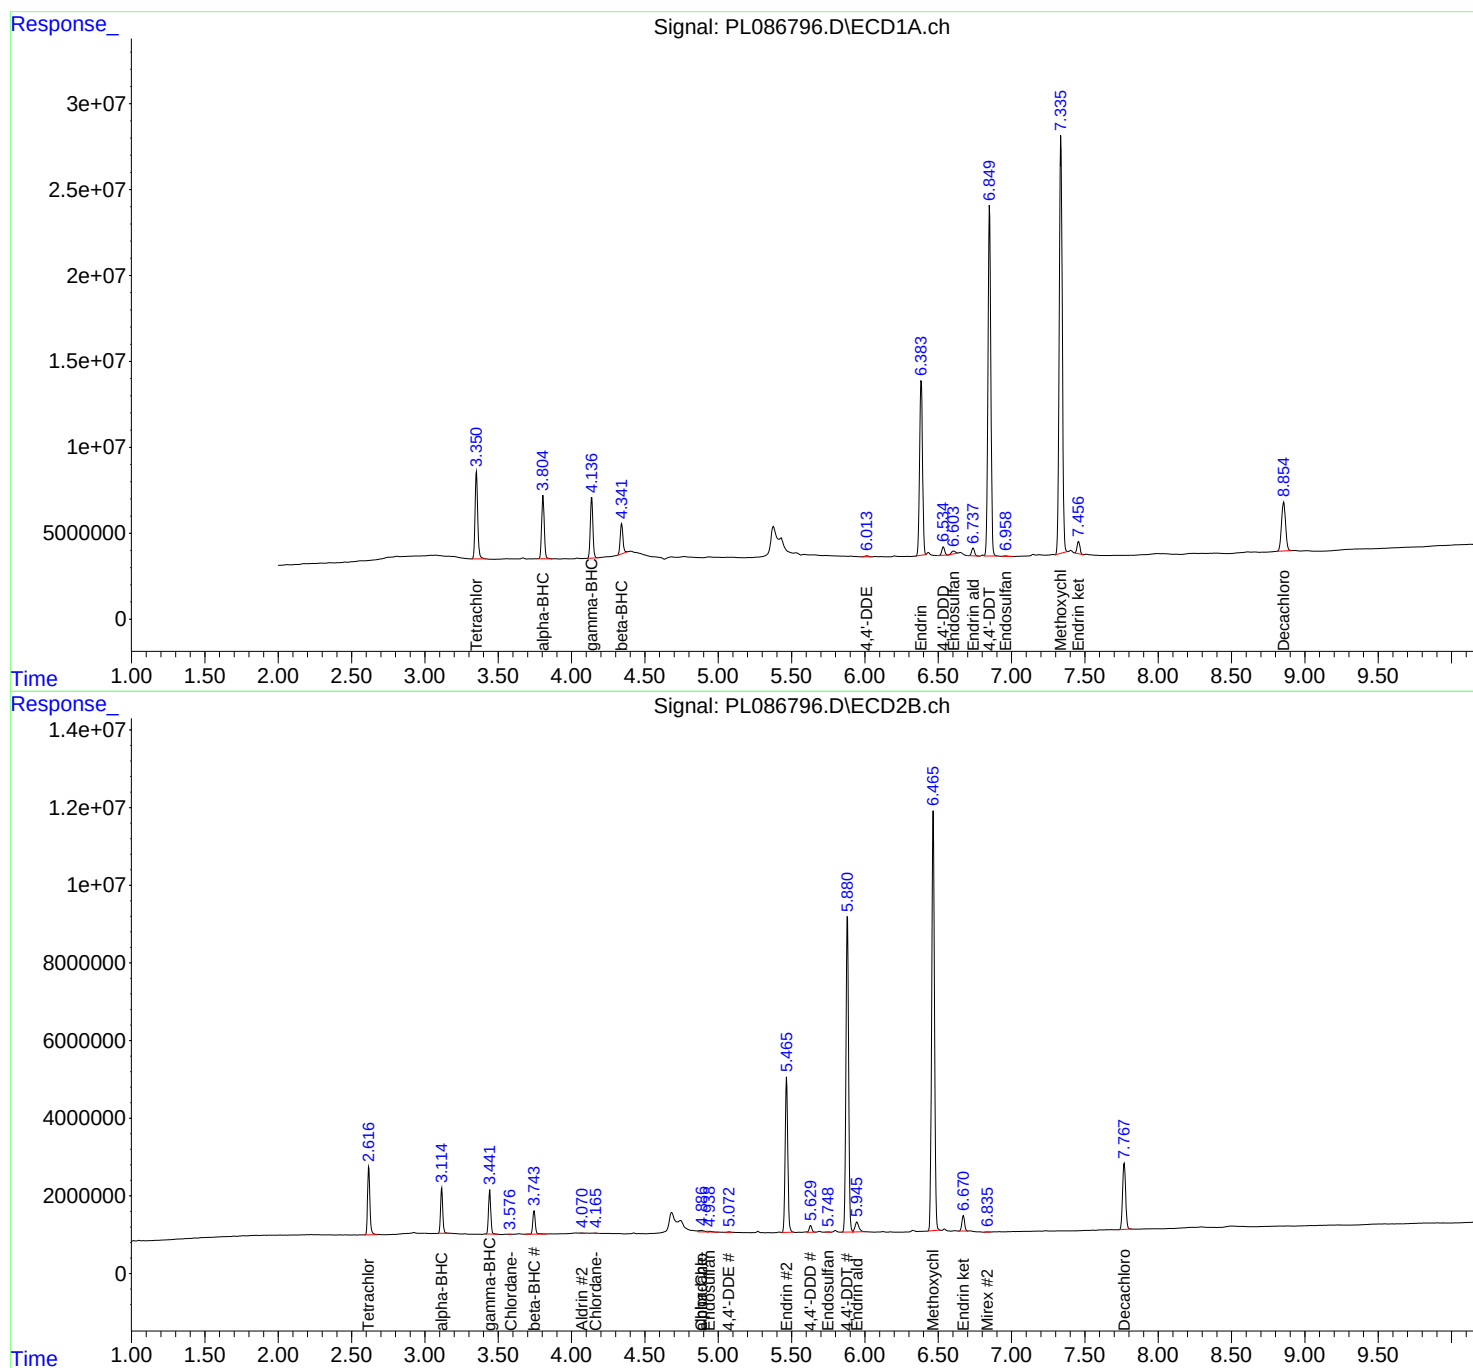


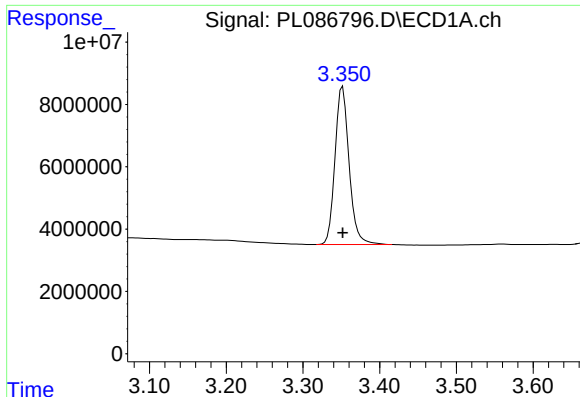

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 64890237
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

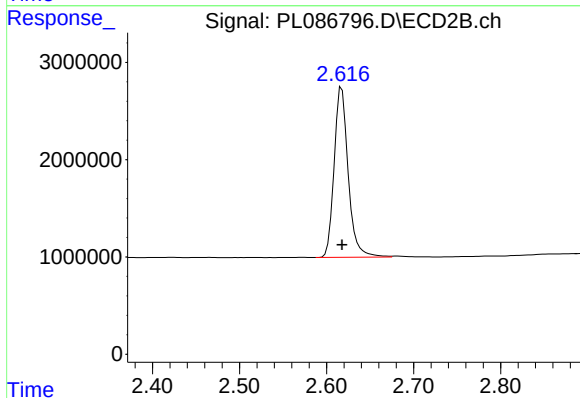


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 19655556
Conc: 19.96 ng/ml

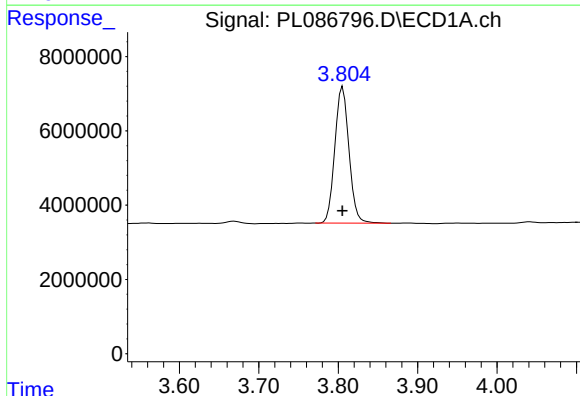


#2 alpha-BHC

R.T.: 3.806 min
Delta R.T.: 0.000 min
Response: 45505857
Conc: 9.46 ng/ml

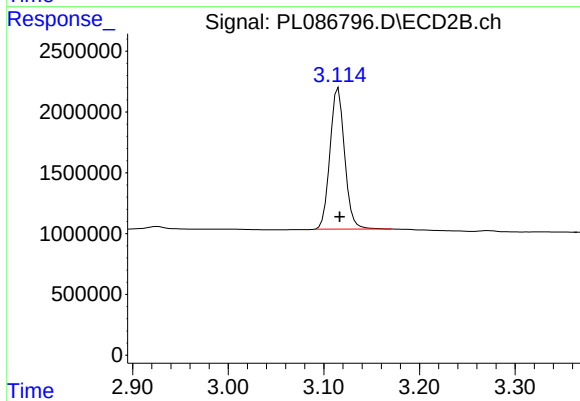

#2 alpha-BHC


R.T.: 3.115 min
Delta R.T.: -0.001 min
Response: 12341959
Conc: 9.26 ng/ml

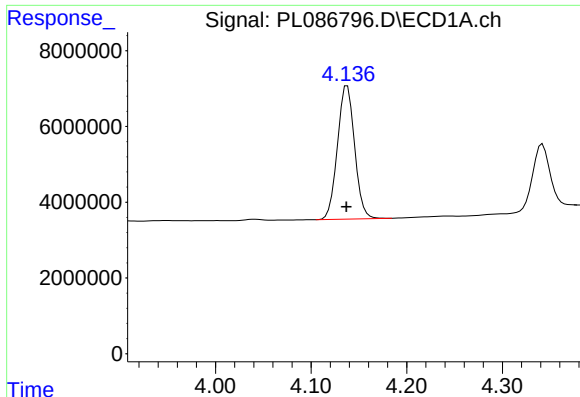

#3 gamma-BHC (Lindane)


R.T.: 4.138 min
Delta R.T.: 0.000 min
Response: 43941127
Conc: 9.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

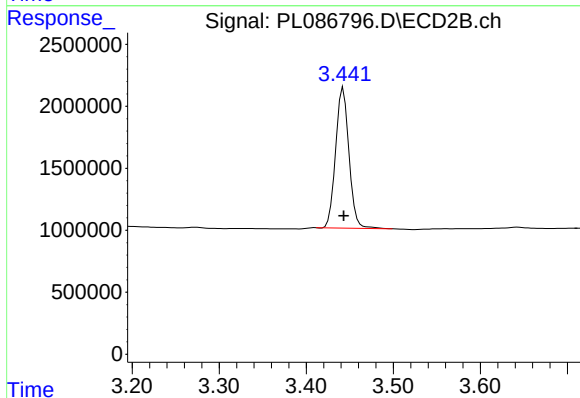


#3 gamma-BHC (Lindane)

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 12066254
Conc: 9.09 ng/ml

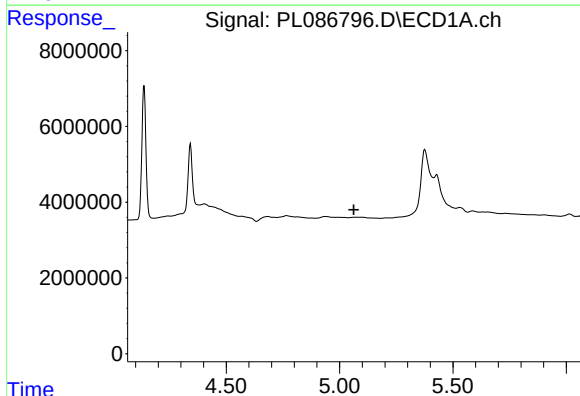


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

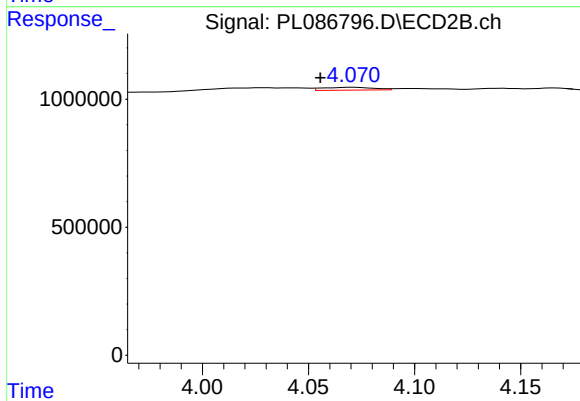

#5 Aldrin


R.T.: 4.071 min
Delta R.T.: 0.016 min
Response: 188586
Conc: 0.14 ng/ml

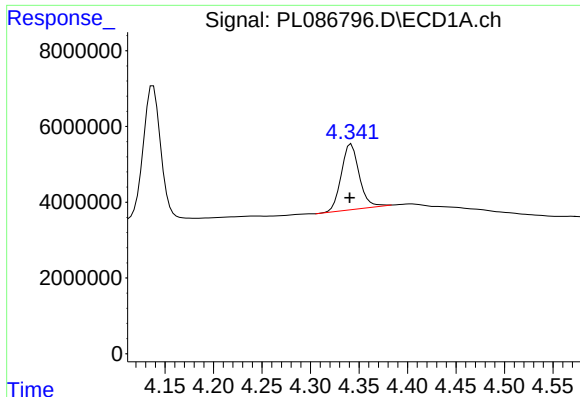

#6 beta-BHC


R.T.: 4.342 min
Delta R.T.: 0.002 min
Response: 22172870
Conc: 10.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

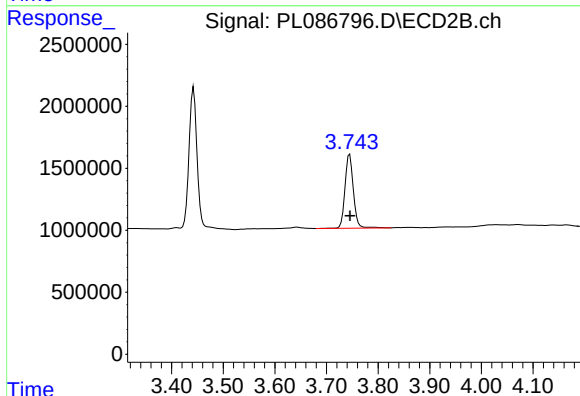


#6 beta-BHC

R.T.: 3.745 min
Delta R.T.: 0.000 min
Response: 6776730
Conc: 11.37 ng/ml

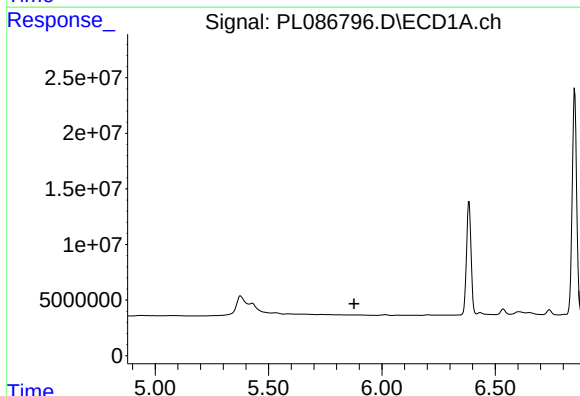


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.877 min
Response: 0
Conc: N.D.

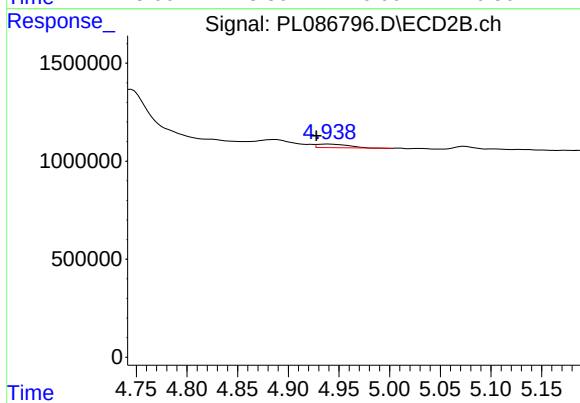

#9 Endosulfan I


R.T.: 4.939 min
Delta R.T.: 0.012 min
Response: 401458
Conc: 0.35 ng/ml

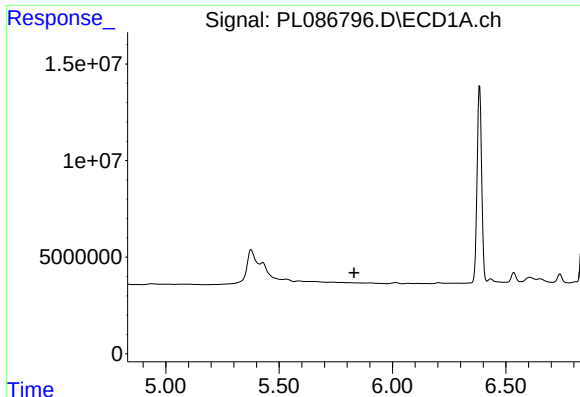

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.831 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

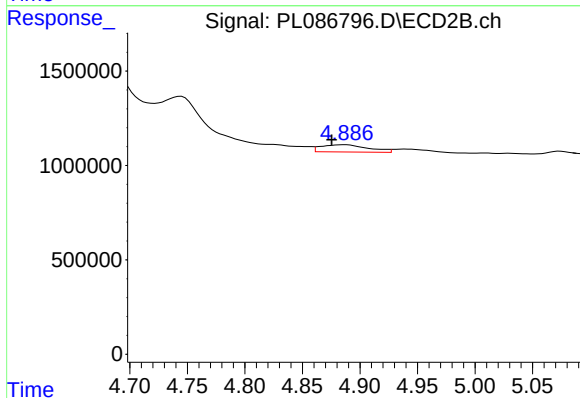


#11 alpha-Chlordane

R.T.: 4.887 min
Delta R.T.: 0.012 min
Response: 1101630
Conc: 0.88 ng/ml

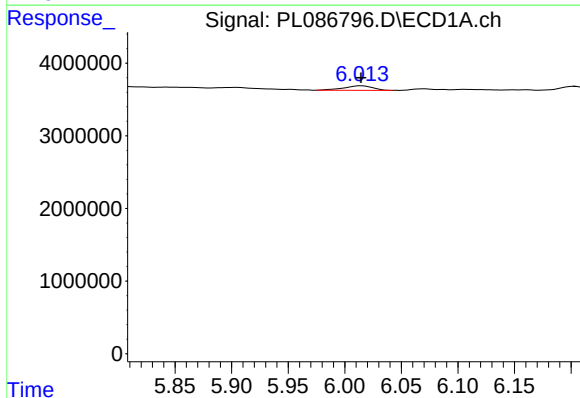


#12 4,4'-DDE

R.T.: 6.015 min
Delta R.T.: 0.000 min
Response: 1085318
Conc: 0.31 ng/ml

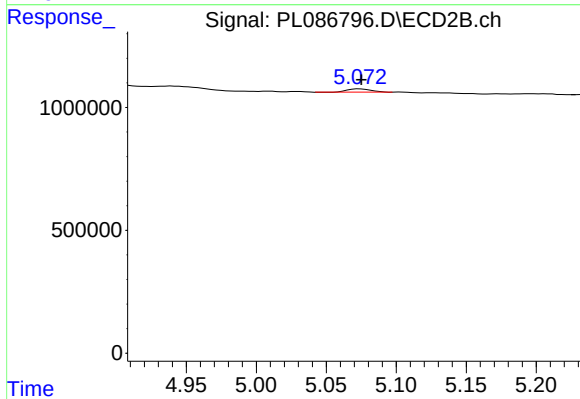

#12 4,4'-DDE


R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 156731
Conc: 0.15 ng/ml

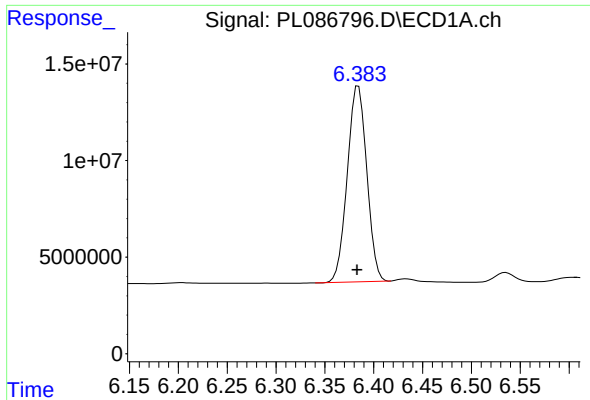

#14 Endrin


R.T.: 6.384 min
Delta R.T.: 0.001 min
Response: 140847468
Conc: 40.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

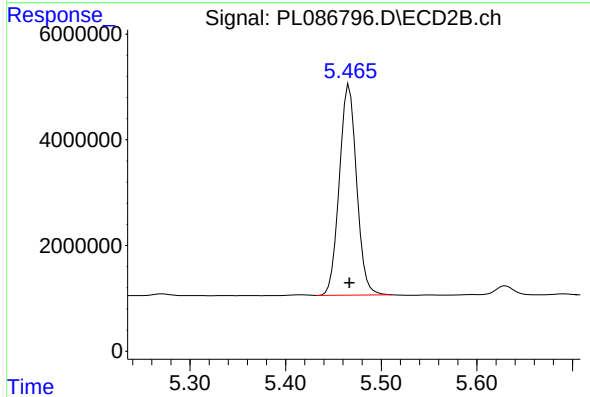


#14 Endrin

R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 50138127
Conc: 45.77 ng/ml

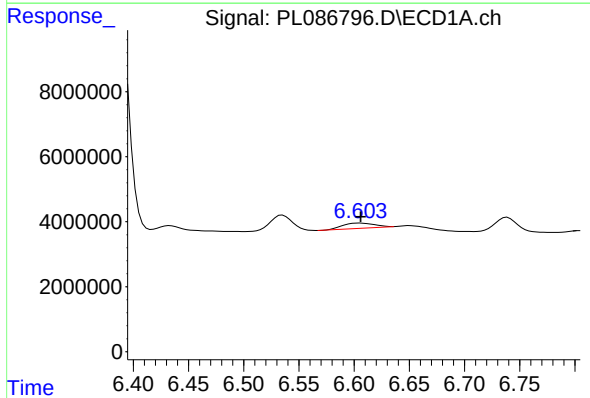


#15 Endosulfan II

R.T.: 6.605 min
Delta R.T.: -0.001 min
Response: 3184872
Conc: 0.90 ng/ml

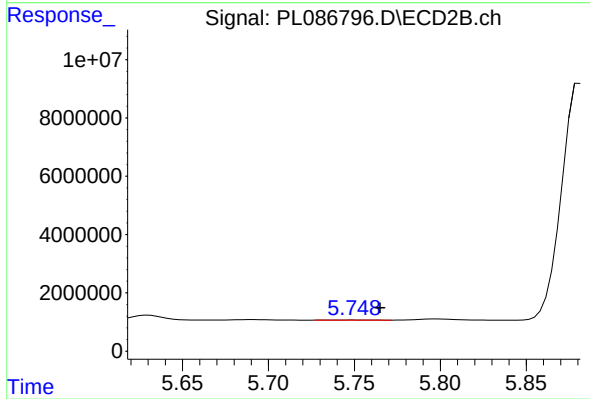

#15 Endosulfan II


R.T.: 5.750 min
Delta R.T.: -0.015 min
Response: 85203
Conc: 0.08 ng/ml

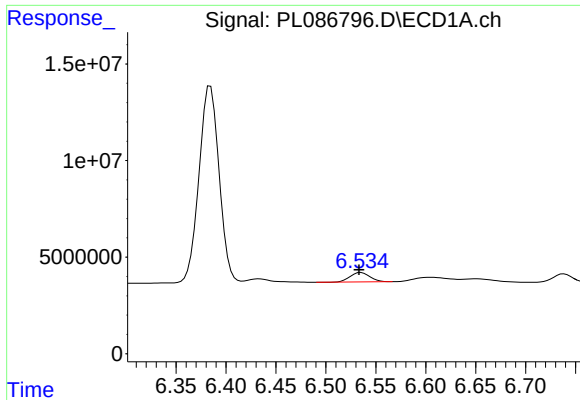

#16 4,4'-DDD


R.T.: 6.535 min
Delta R.T.: 0.002 min
Response: 6638552
Conc: 2.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

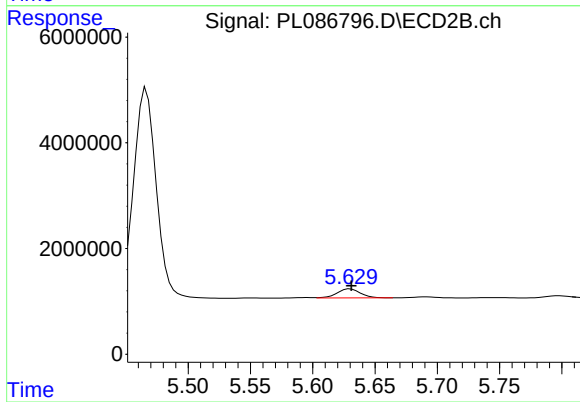


#16 4,4'-DDD

R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 2256387
Conc: 2.65 ng/ml

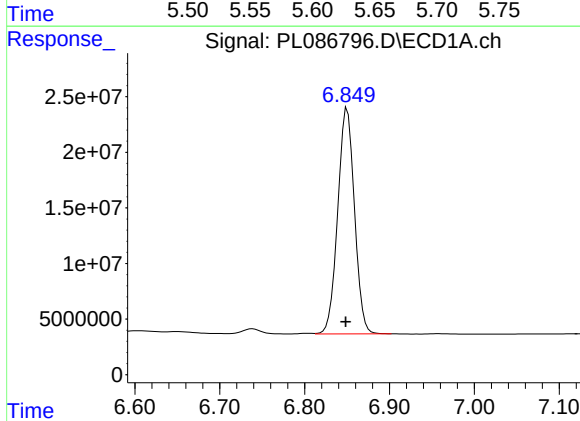


#17 4,4'-DDT

R.T.: 6.850 min
Delta R.T.: 0.002 min
Response: 277840333
Conc: 93.73 ng/ml

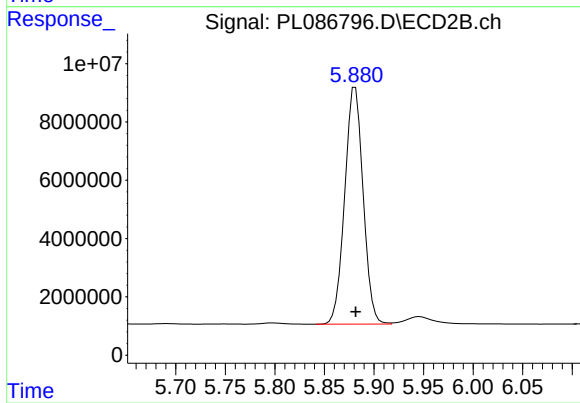

#17 4,4'-DDT


R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 105032217
Conc: 107.44 ng/ml

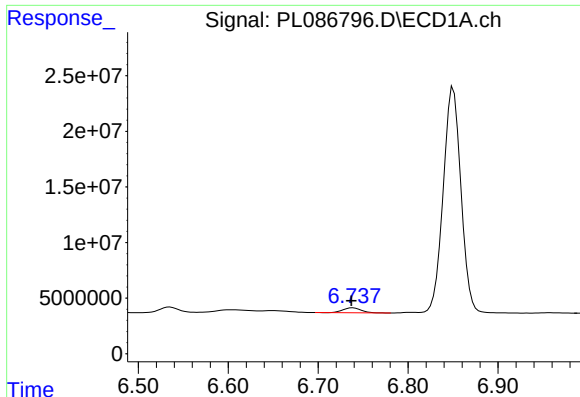

#18 Endrin aldehyde


R.T.: 6.739 min
Delta R.T.: 0.002 min
Response: 6216440
Conc: 2.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

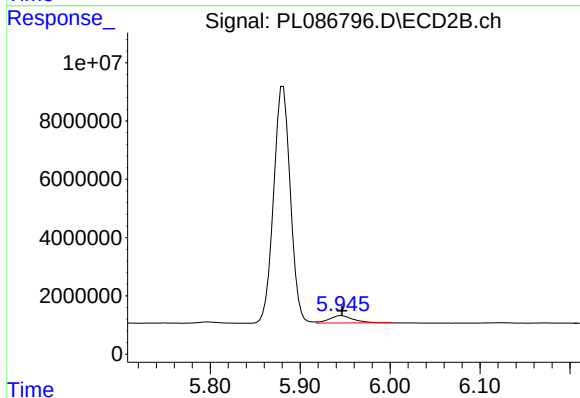


#18 Endrin aldehyde

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 4674195
Conc: 4.99 ng/ml

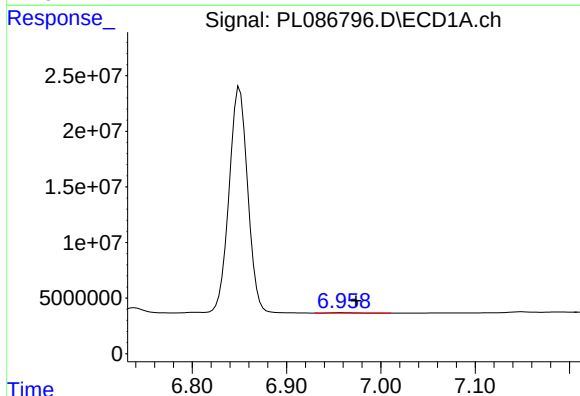


#19 Endosulfan Sulfate

R.T.: 6.959 min
Delta R.T.: -0.014 min
Response: 543859
Conc: 0.16 ng/ml

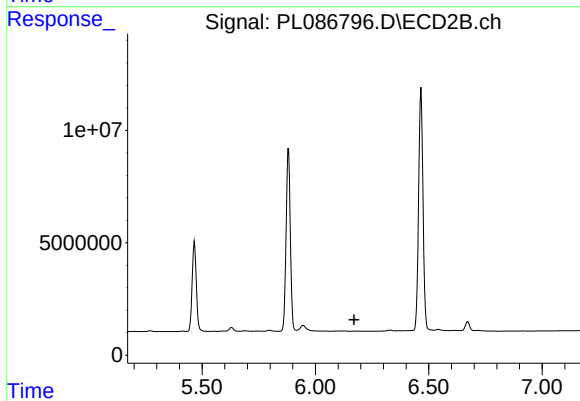

#19 Endosulfan Sulfate


R.T.: 6.173 min
Delta R.T.: 0.002 min
Response: -48466
Conc: N.D.

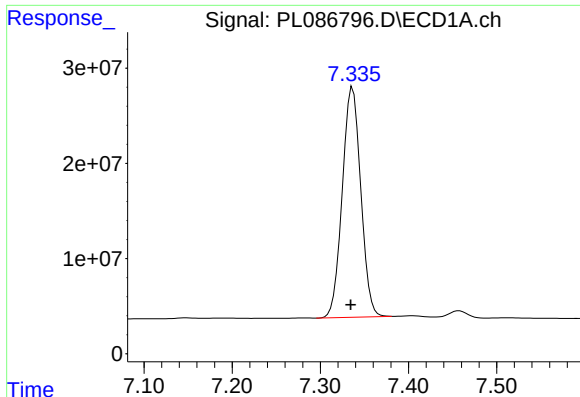

#20 Methoxychlor


R.T.: 7.337 min
Delta R.T.: 0.002 min
Response: 352344698
Conc: 220.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

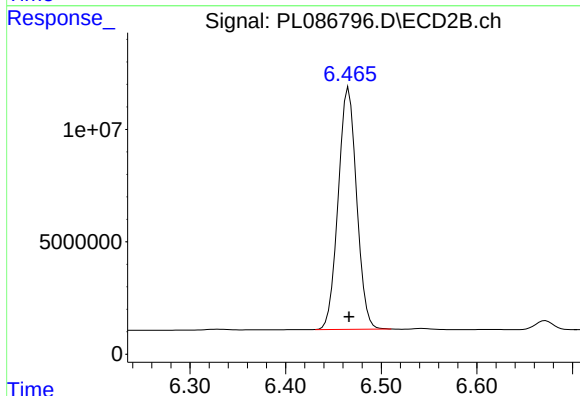


#20 Methoxychlor

R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 144063785
Conc: 240.84 ng/ml

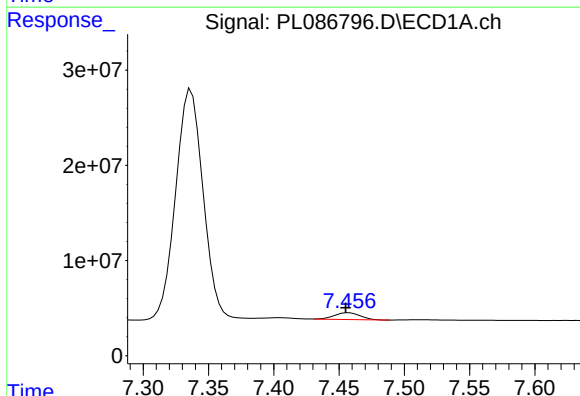


#21 Endrin ketone

R.T.: 7.457 min
Delta R.T.: 0.002 min
Response: 9773125
Conc: 2.87 ng/ml

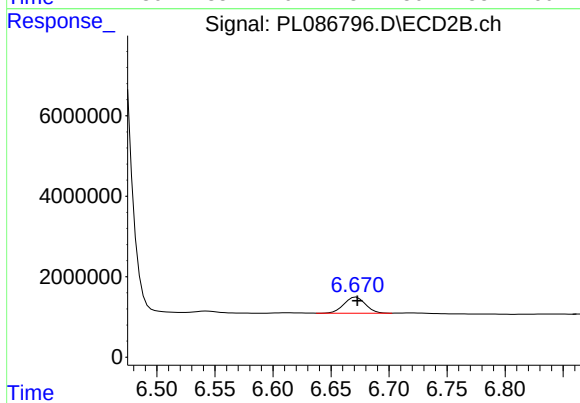

#21 Endrin ketone


R.T.: 6.672 min
Delta R.T.: 0.000 min
Response: 5125046
Conc: 4.00 ng/ml

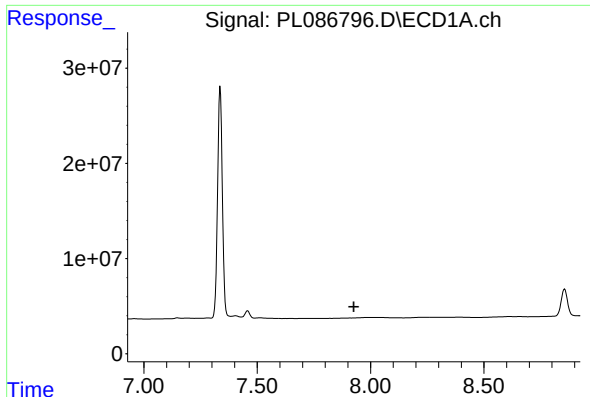

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.926 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

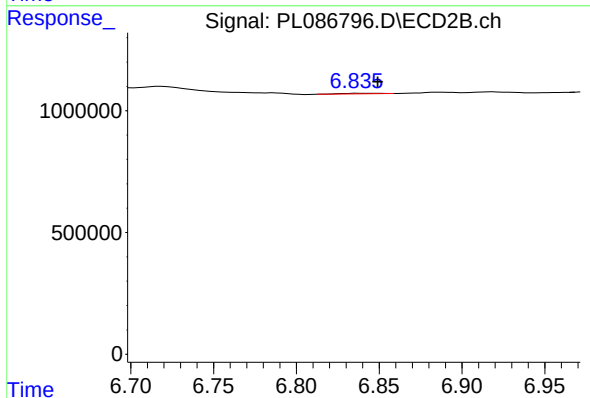


#22 Mirex

R.T.: 6.837 min
Delta R.T.: -0.012 min
Response: 38338
Conc: 0.03 ng/ml

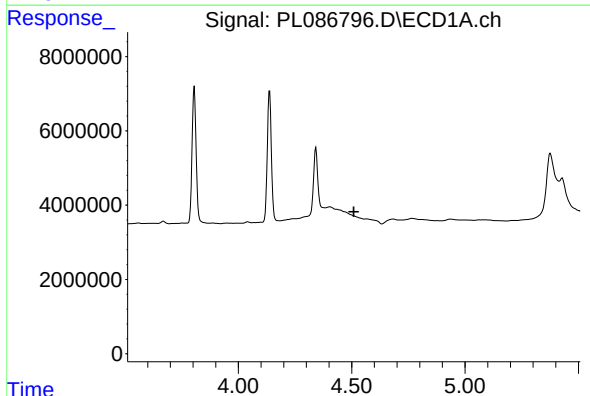


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.509 min
Response: 0
Conc: N.D.

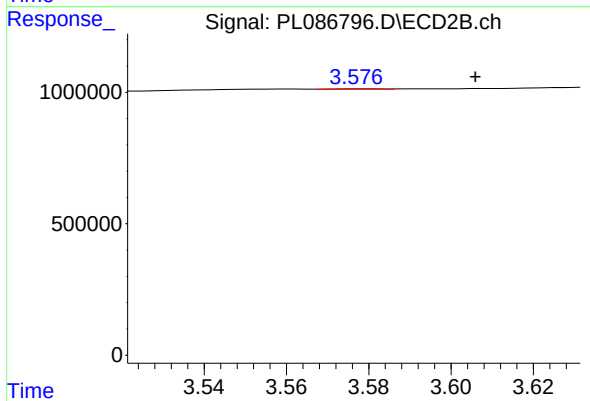

#23 Chlordane-1


R.T.: 3.580 min
Delta R.T.: -0.026 min
Response: 11024
Conc: 0.31 ng/ml

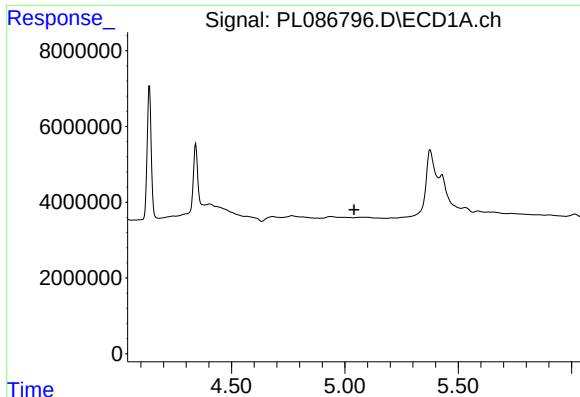

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

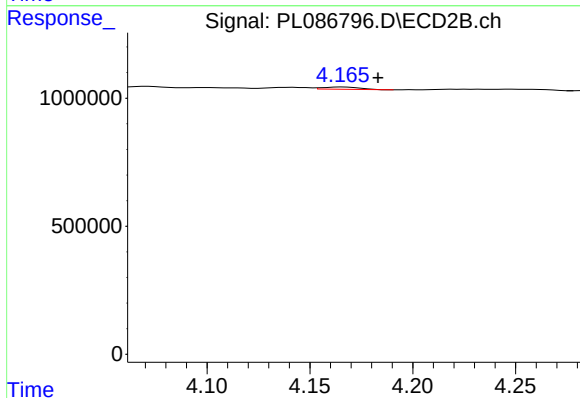


#24 Chlordane-2

R.T.: 4.166 min
Delta R.T.: -0.017 min
Response: 106620
Conc: 2.36 ng/ml

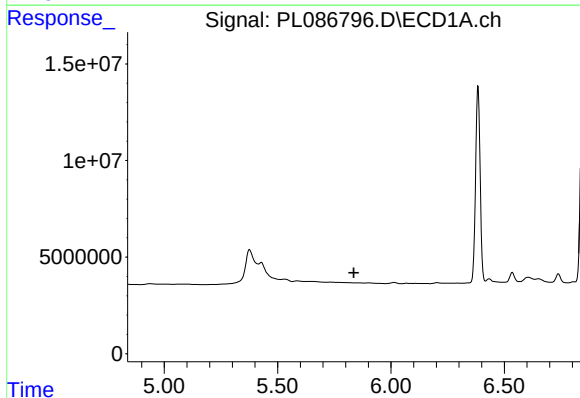


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.836 min
Response: 0
Conc: N.D.

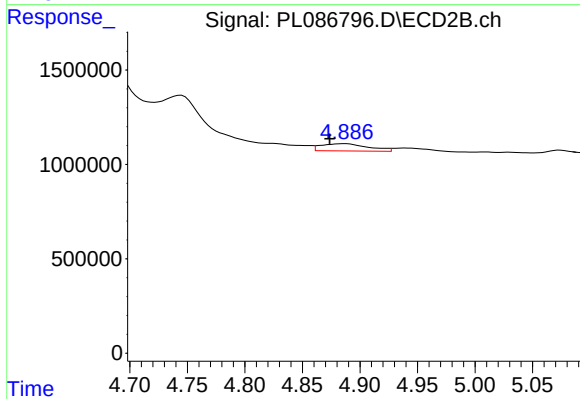

#26 Chlordane-4


R.T.: 4.887 min
Delta R.T.: 0.013 min
Response: 1101630
Conc: 8.63 ng/ml

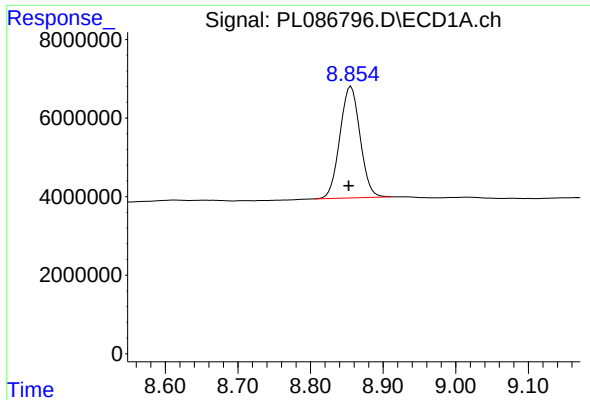

#28 Decachlorobiphenyl

R.T.: 8.856 min
Delta R.T.: 0.003 min
Response: 54874718
Conc: 18.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

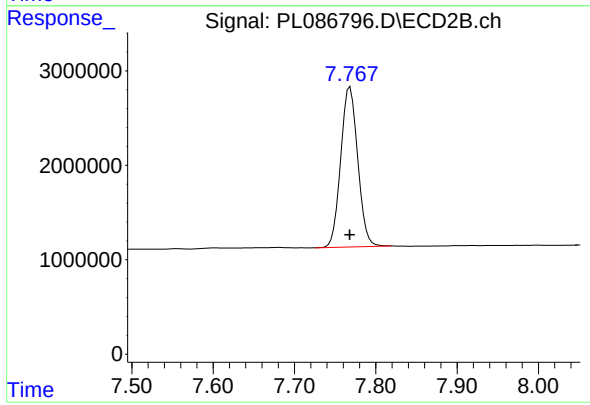

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 24586525
Conc: 20.36 ng/ml