

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112223\
 Data File : PL086807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2023 14:32
 Operator : AR\AJ
 Sample : 05517-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-D

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/24/2023
 Supervised By :Ankita Jodhani 11/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:44:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.351	2.617	70220746	21906144	21.626	22.248
2) SA Decachlor...	8.854	7.768	52221558	23400951	17.840	19.378
Target Compounds						
11) B alpha-Chl...	5.834	4.873	5290244	999723	1.303m	0.799m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112223\
Data File : PL086807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2023 14:32
Operator : AR\AJ
Sample : 05517-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-D


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/24/2023
Supervised By :Ankita Jodhani 11/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:44:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

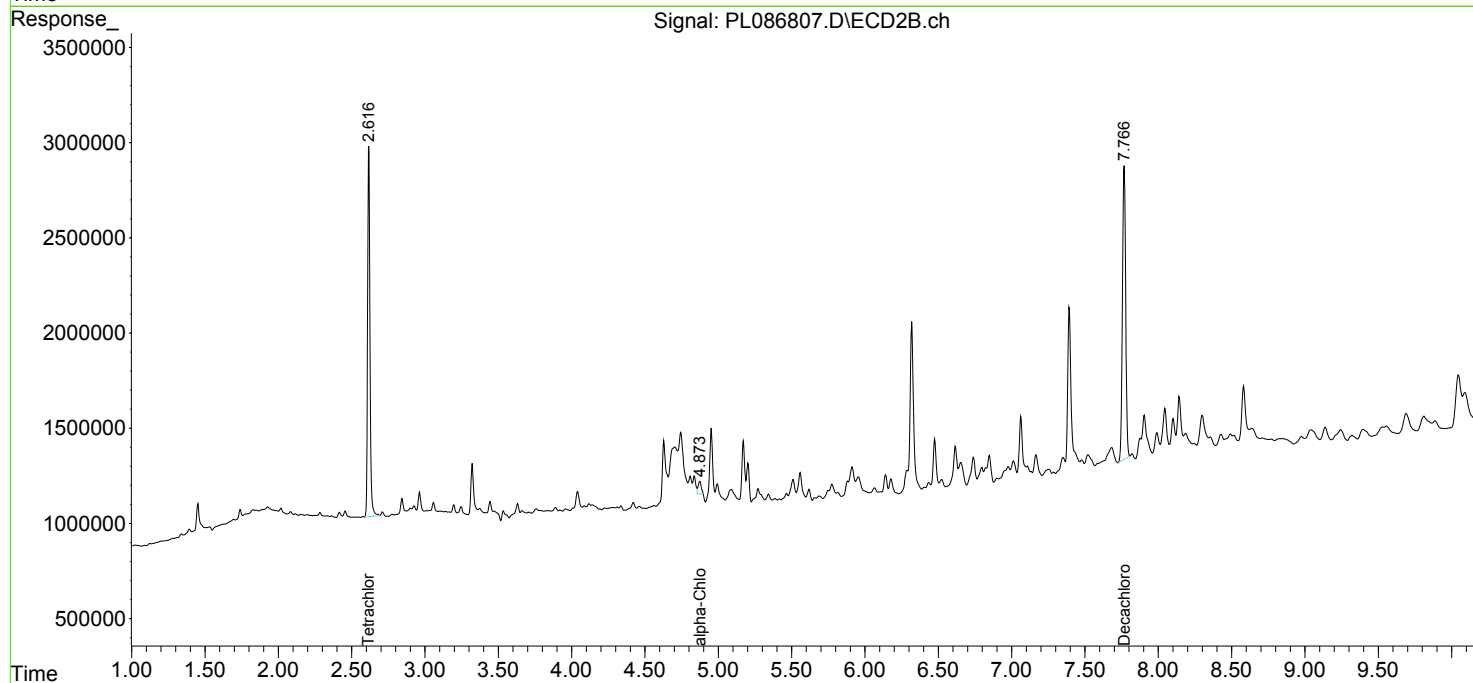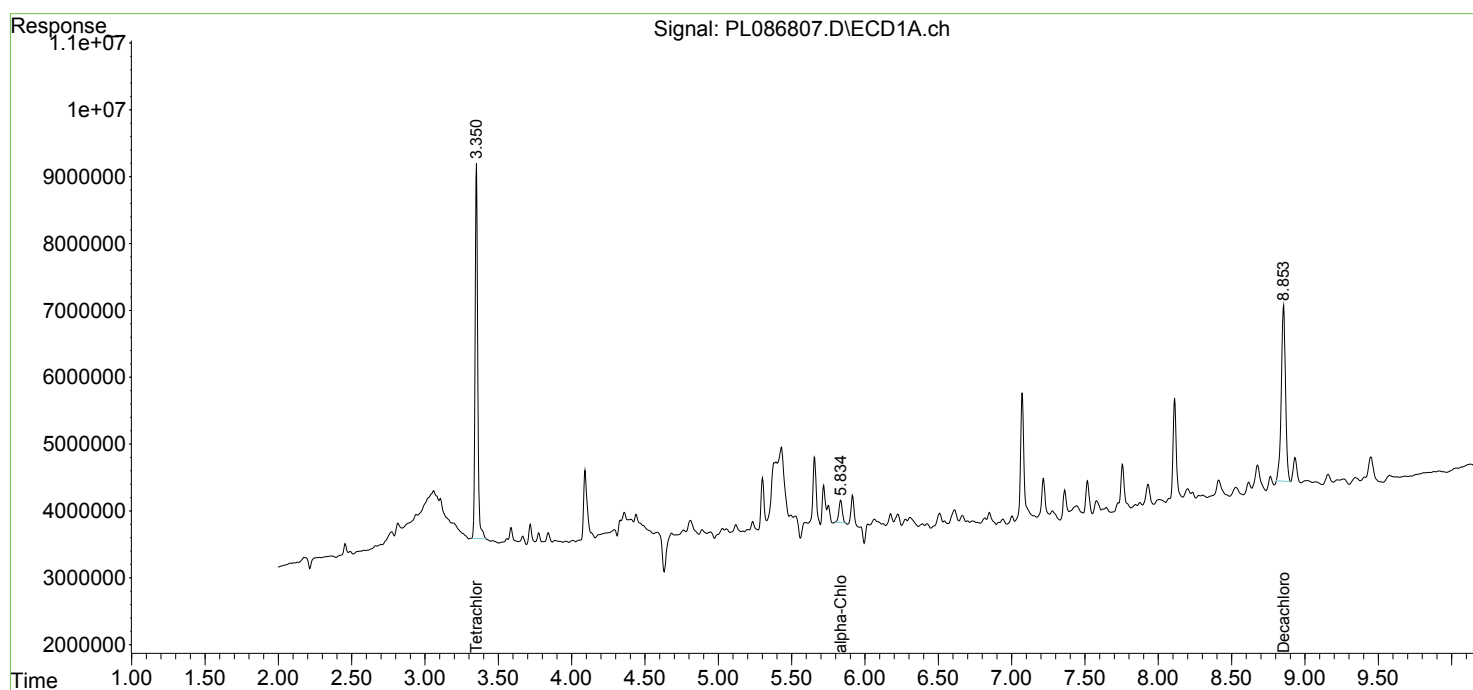

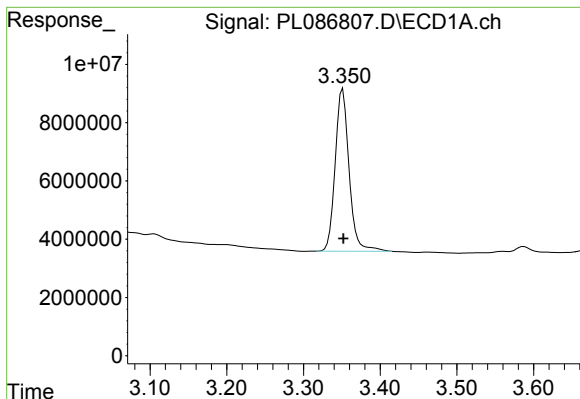


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 70220746
Conc: 21.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-D


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/24/2023
Supervised By :Ankita Jodhani 11/27/2023

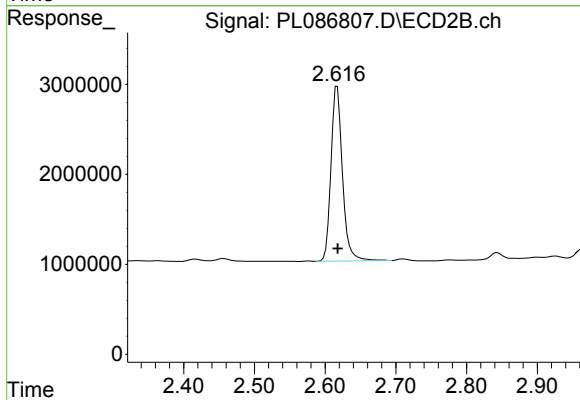


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 21906144
Conc: 22.25 ng/ml

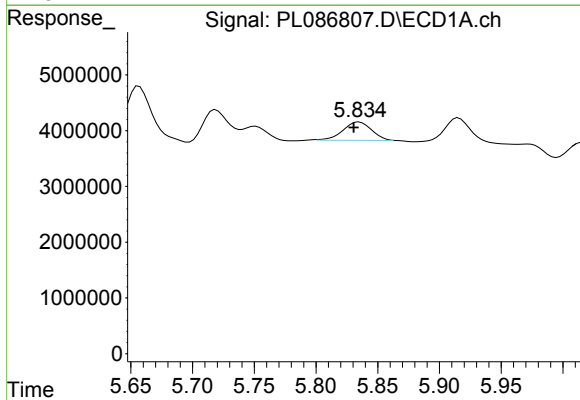


#11 alpha-Chlordane

R.T.: 5.834 min
Delta R.T.: 0.003 min
Response: 5290244
Conc: 1.30 ng/ml m

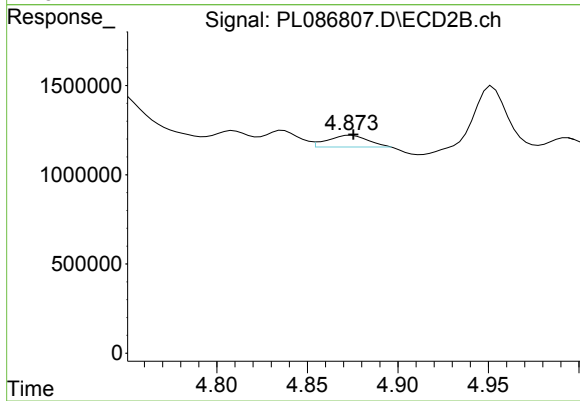

#11 alpha-Chlordane

R.T.: 4.873 min
Delta R.T.: -0.003 min
Response: 999723
Conc: 0.80 ng/ml m

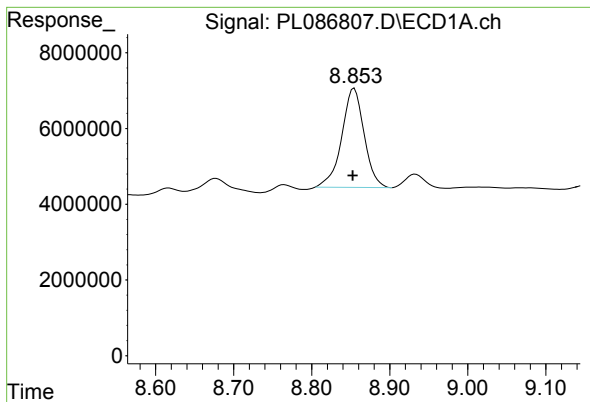


#28 Decachlorobiphenyl

R.T.: 8.854 min
Delta R.T.: 0.002 min
Response: 52221558
Conc: 17.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-D

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/24/2023
Supervised By :Ankita Jodhani 11/27/2023

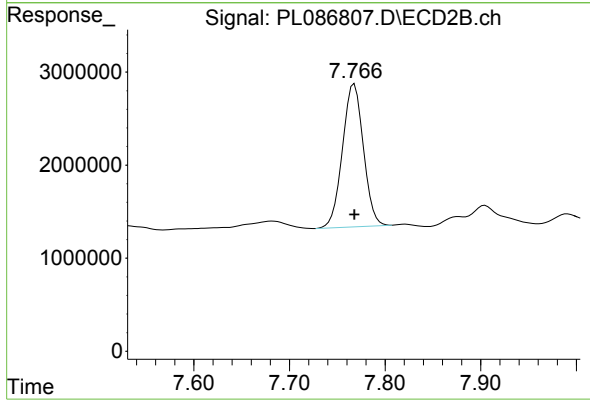

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 23400951
Conc: 19.38 ng/ml