

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112320\
 Data File : PL063153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 19:32
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 01:36:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:36:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.951	94227171	159.5E6	50.000	50.000
28)	SA Decachlor...	8.126	8.990	89703224	116.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.268	4.937	24944511	55189027	500.000	500.000
24)	Chlordane-2	4.764	5.403	27797296	58815311	500.000	500.000
25)	Chlordane-3	5.328	6.047	78499527	221.7E6	500.000	500.000
26)	Chlordane-4	5.385	6.122	65729062	268.2E6	500.000	500.000
27)	Chlordane-5	6.213	6.924	29110379	42918896	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112320\
Data File : PL063153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 19:32
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 01:36:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:36:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

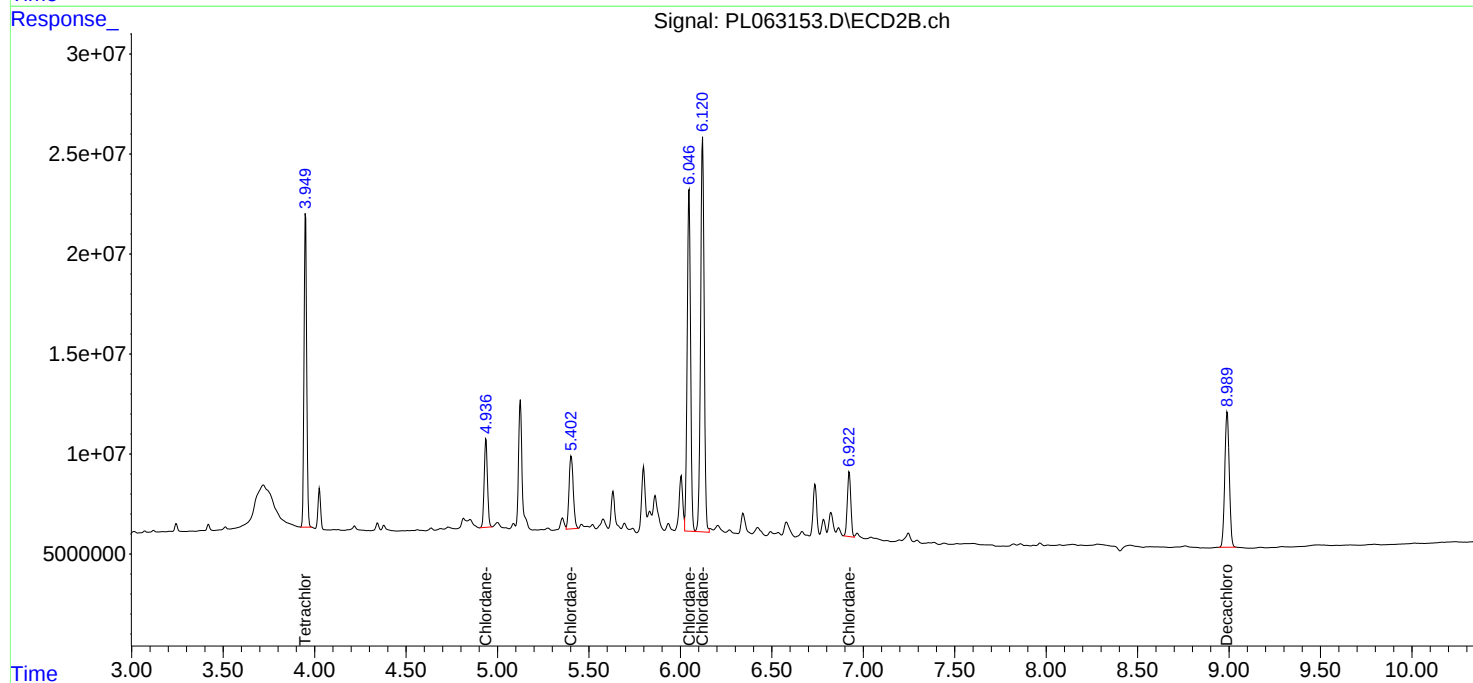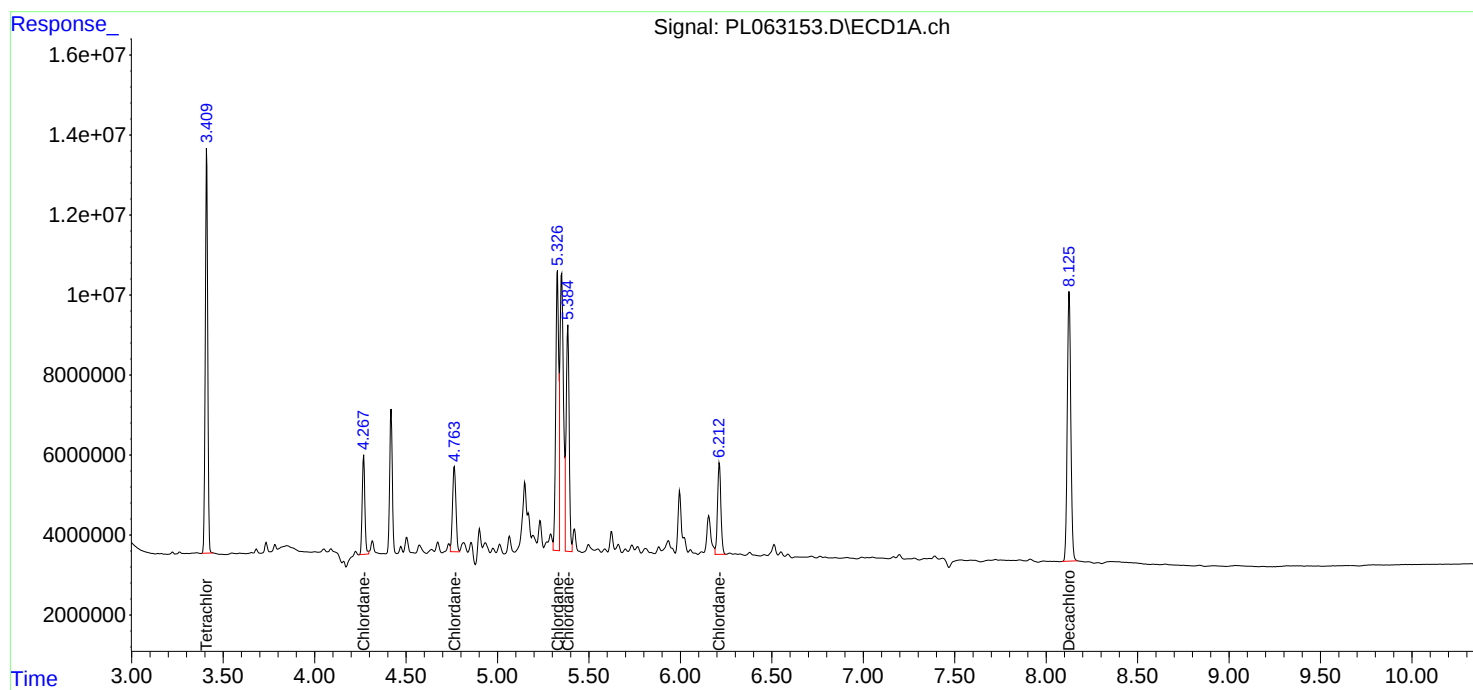


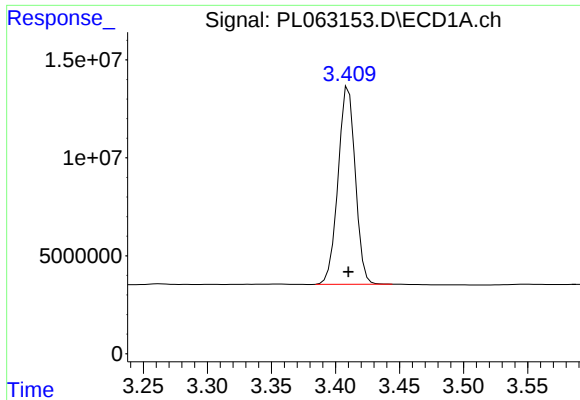

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 94227171
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

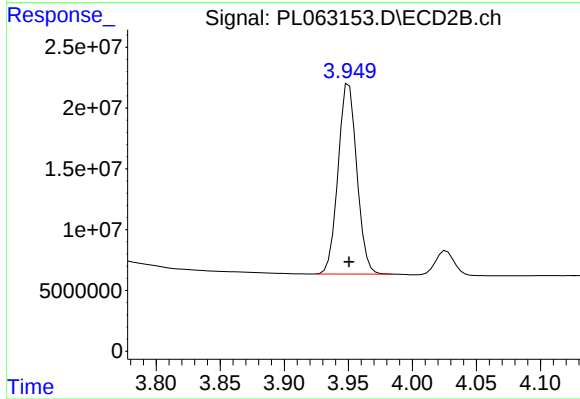


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 159543674
Conc: 50.00 ng/ml

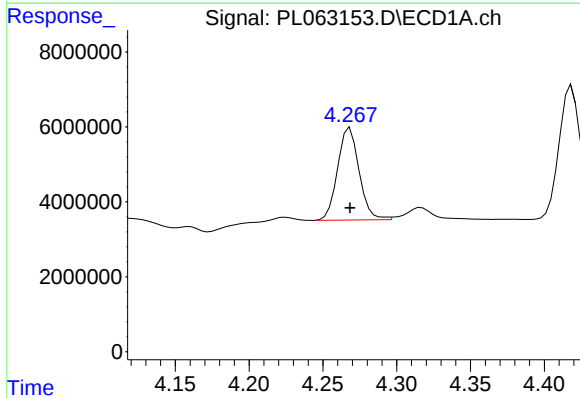


#23 Chlordane-1

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 24944511
Conc: 500.00 ng/ml

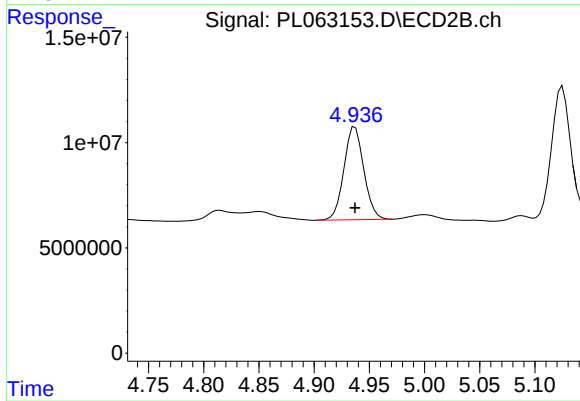

#23 Chlordane-1


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 55189027
Conc: 500.00 ng/ml

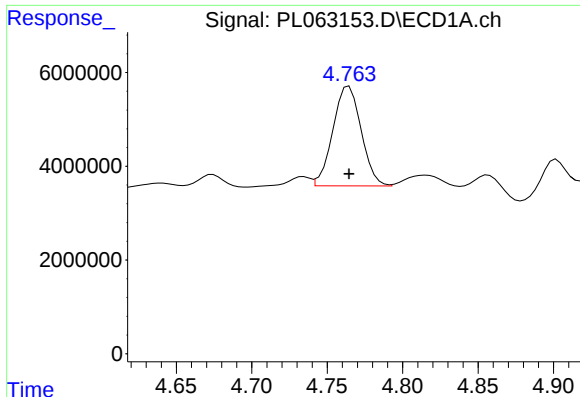

#24 Chlordane-2


R.T.: 4.764 min
Delta R.T.: 0.000 min
Response: 27797296
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

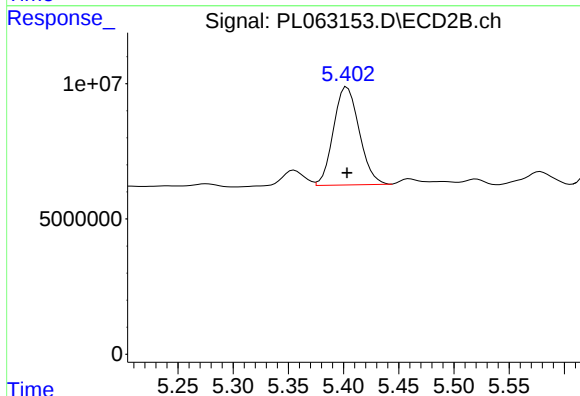


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 58815311
Conc: 500.00 ng/ml

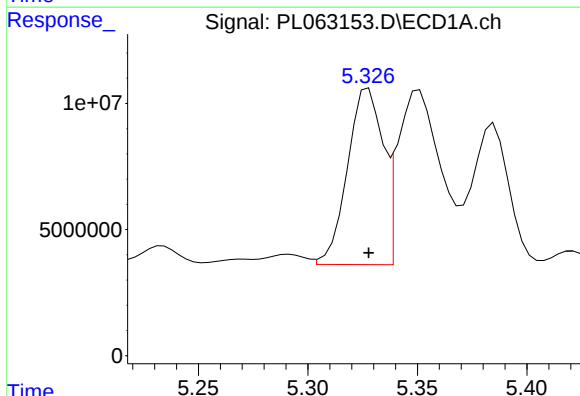


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 78499527
Conc: 500.00 ng/ml

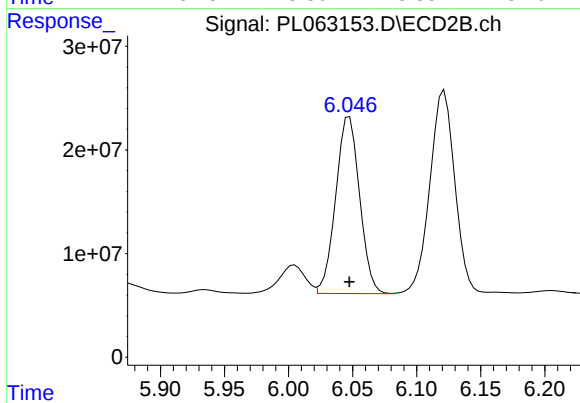

#25 Chlordane-3


R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 221740116
Conc: 500.00 ng/ml

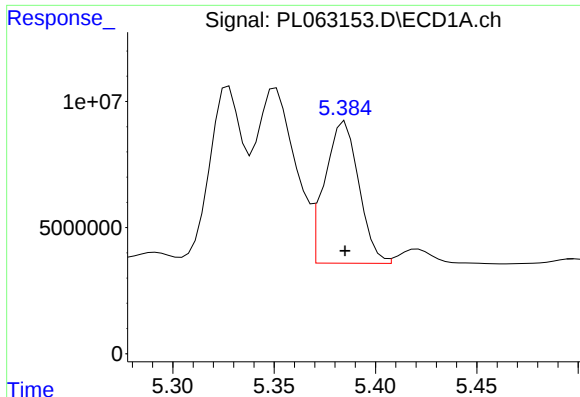

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 65729062
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

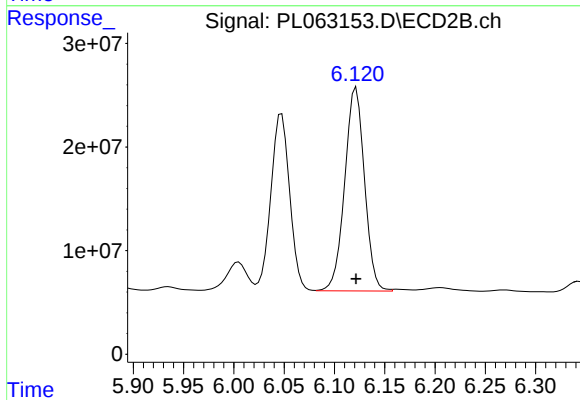


#26 Chlordane-4

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 268171736
Conc: 500.00 ng/ml

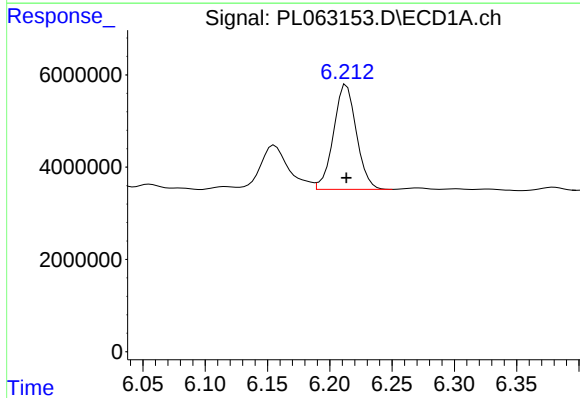


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 29110379
Conc: 500.00 ng/ml

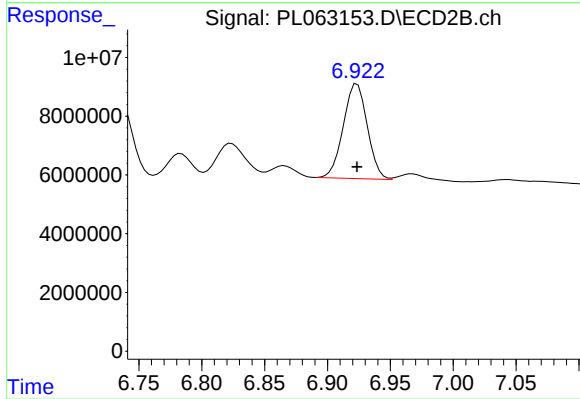

#27 Chlordane-5


R.T.: 6.924 min
Delta R.T.: 0.000 min
Response: 42918896
Conc: 500.00 ng/ml

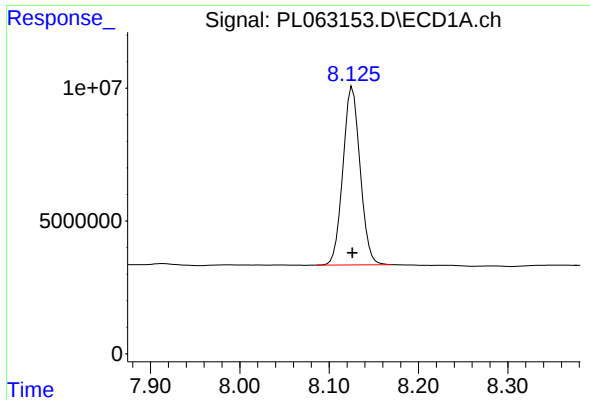

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 89703224
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

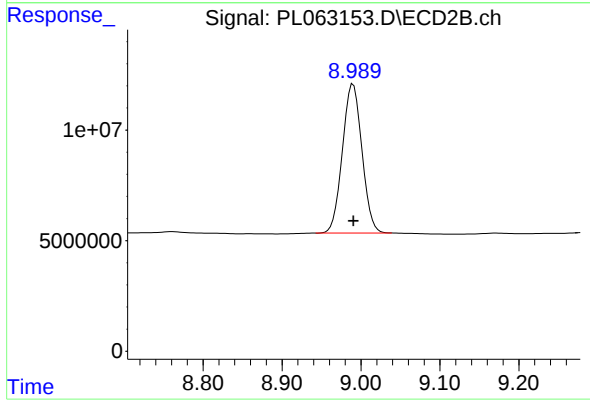

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 115969320
Conc: 50.00 ng/ml