

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112321\
 Data File : PL071134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2021 15:00
 Operator : AR\AJ
 Sample : M4808-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 02:53:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.569	5.499	4681354	11045895	9.558	8.761
28)	SA Decachlor...	10.331	11.393	10221728	19221116	14.959	14.372
Target Compounds							
10)	B gamma-Chl...	7.270	0.000	461082	0	0.695	N.D. #
13)	MA Dieldrin	0.000	8.652	0	1478495	N.D.	1.015 #
14)	MA Endrin	8.006f	0.000	448511	0	0.791	N.D. #
16)	A 4,4'-DDD	0.000	9.040	0	2049274	N.D.	1.703 #
17)	MA 4,4'-DDT	8.406	0.000	816764	0	1.485	N.D. #
18)	B Endrin al...	8.510f	0.000	294658	0	0.649	N.D. #
19)	B Endosulfa...	8.716	0.000	639676	0	1.037	N.D. #
20)	A Methoxychlor	8.981f	0.000	1529365	0	4.180	N.D. #
23)	Chlordane-1	0.000	6.903f	0	1119665	N.D.	23.058 #
25)	Chlordane-3	7.270	0.000	461082	0	7.552	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112321\
Data File : PL071134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2021 15:00
Operator : AR\AJ
Sample : M4808-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 02:53:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

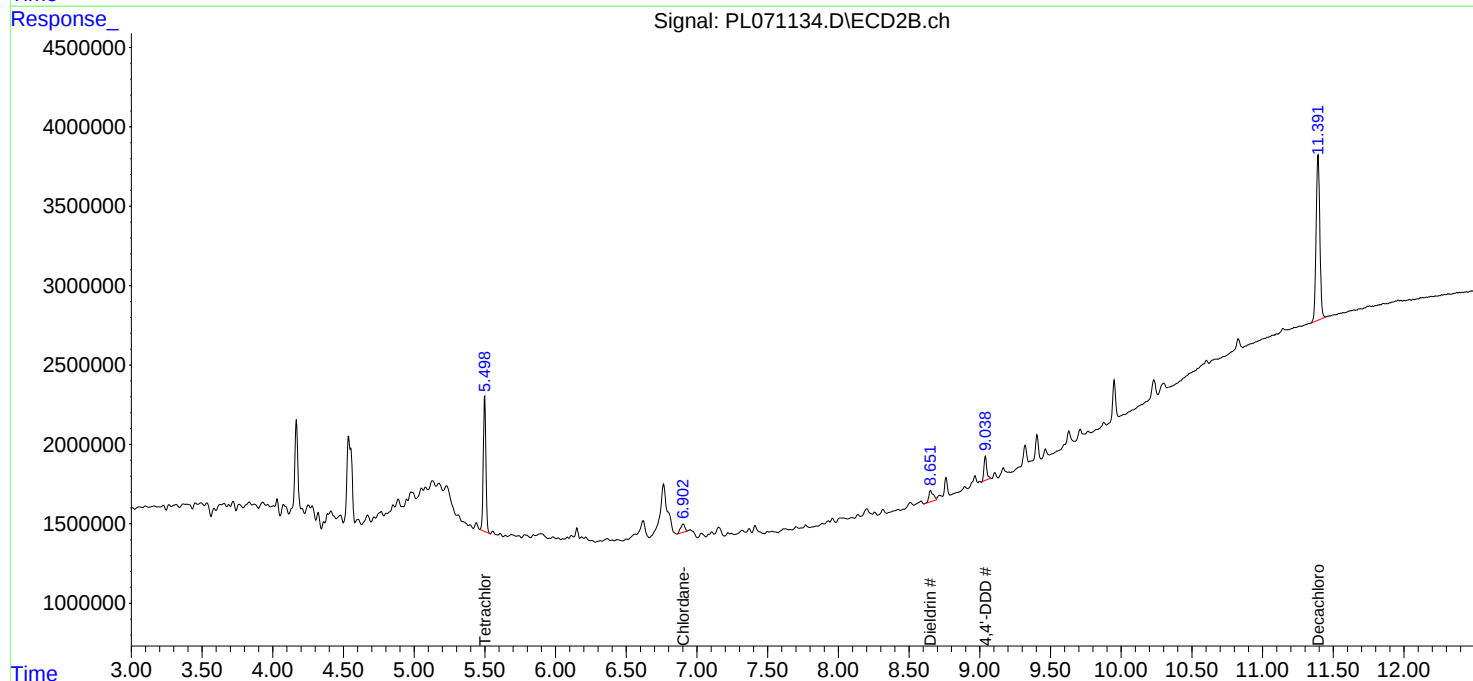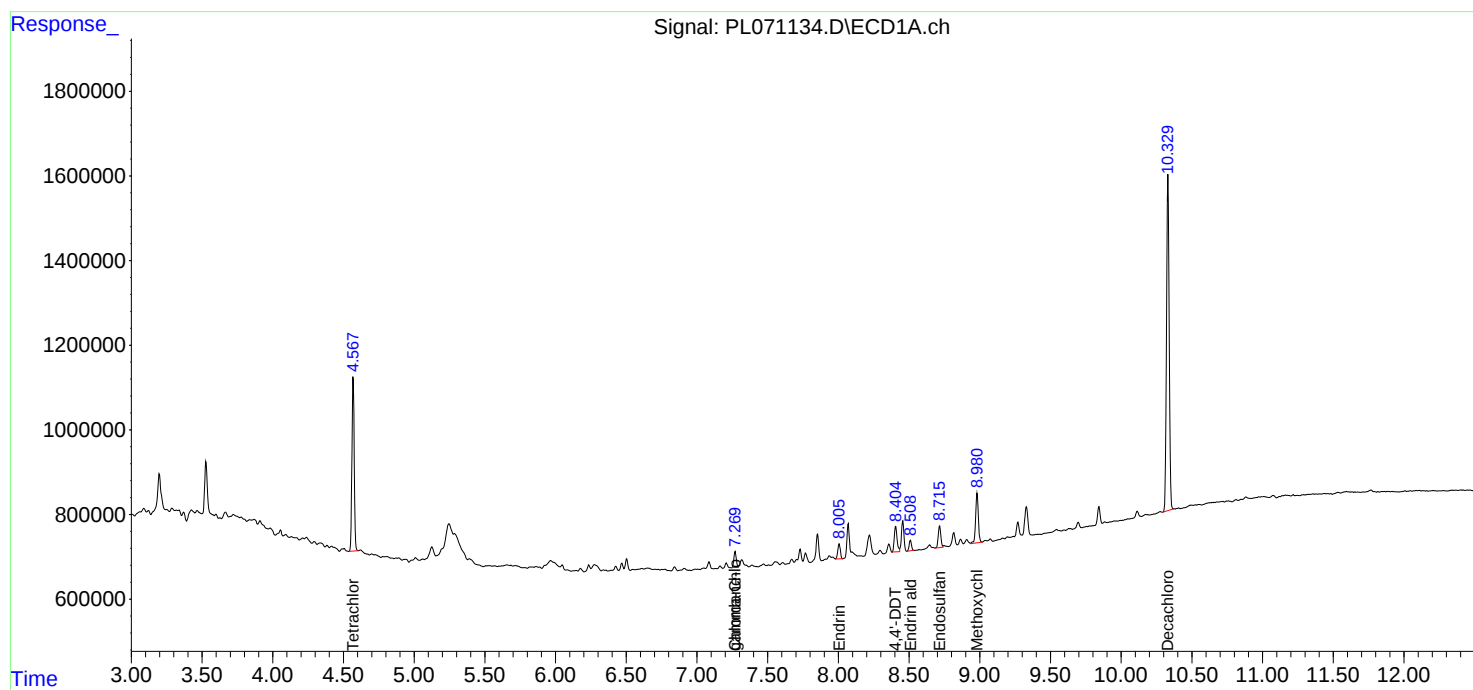


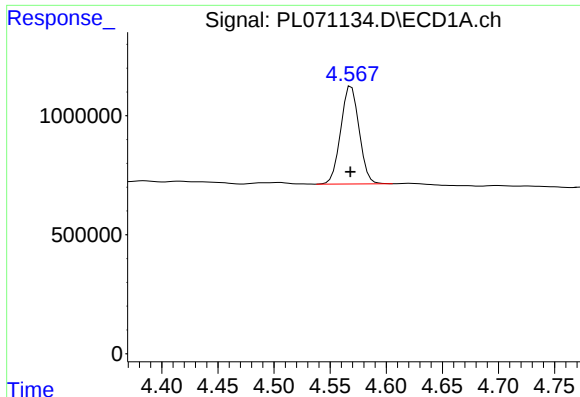

#1 Tetrachloro-m-xylene


R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 4681354
Conc: 9.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

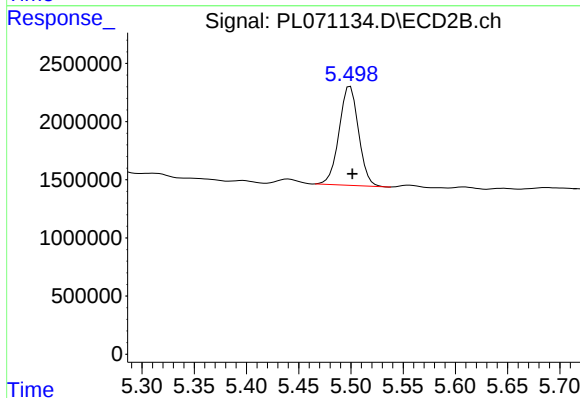


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: -0.002 min
Response: 11045895
Conc: 8.76 ng/ml

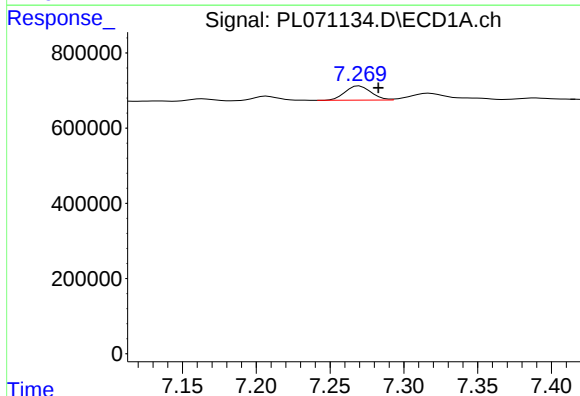


#10 gamma-Chlordane

R.T.: 7.270 min
Delta R.T.: -0.013 min
Response: 461082
Conc: 0.69 ng/ml

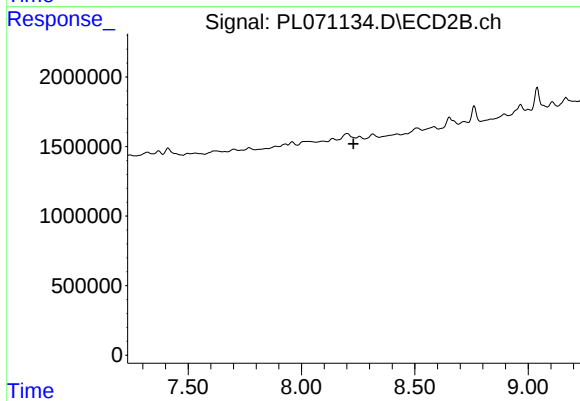

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.230 min
Response: 0
Conc: N.D.

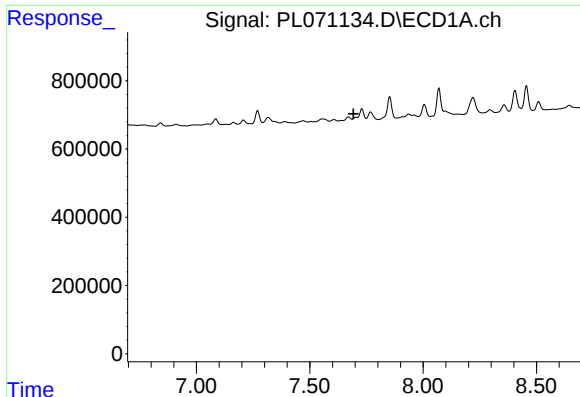

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

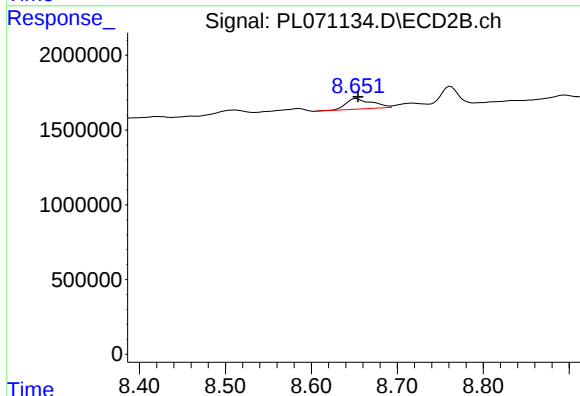


#13 Dieldrin

R.T.: 8.652 min
Delta R.T.: -0.002 min
Response: 1478495
Conc: 1.01 ng/ml

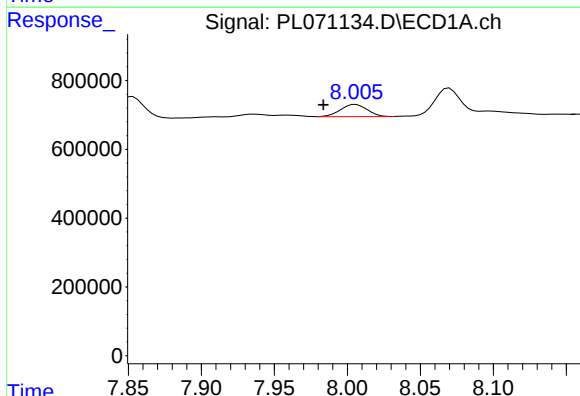


#14 Endrin

R.T.: 8.006 min
Delta R.T.: 0.022 min
Response: 448511
Conc: 0.79 ng/ml

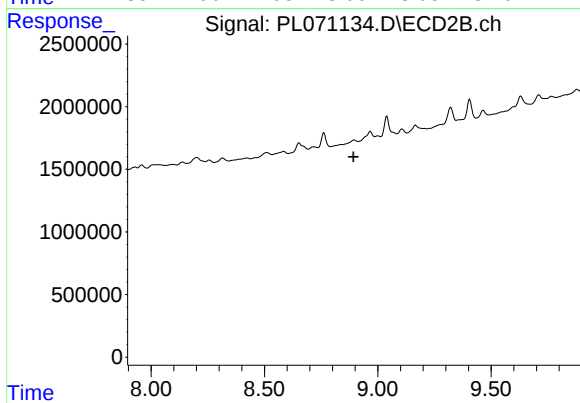

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

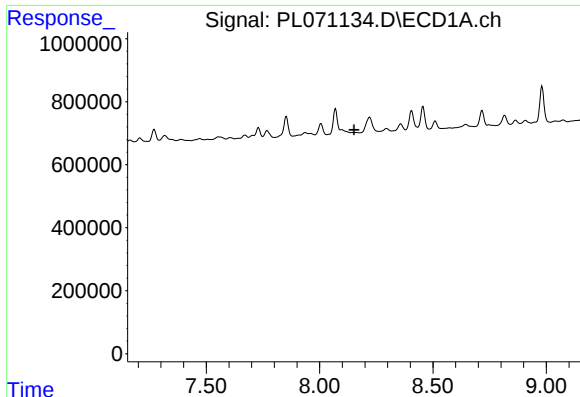

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

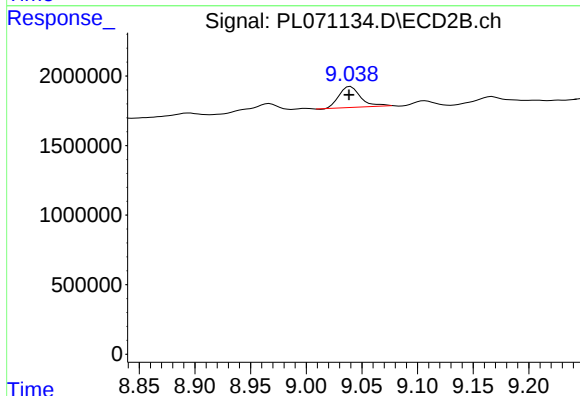


#16 4,4'-DDD

R.T.: 9.040 min
Delta R.T.: 0.001 min
Response: 2049274
Conc: 1.70 ng/ml

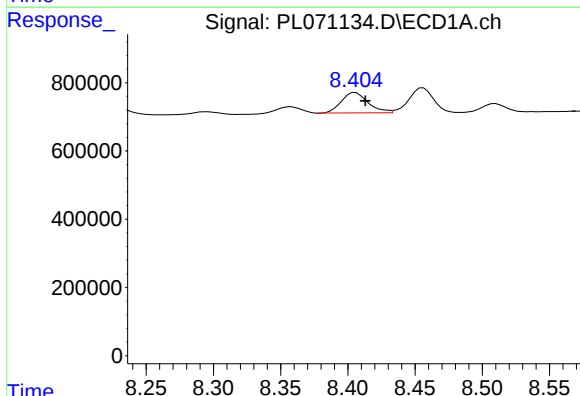


#17 4,4'-DDT

R.T.: 8.406 min
Delta R.T.: -0.007 min
Response: 816764
Conc: 1.49 ng/ml

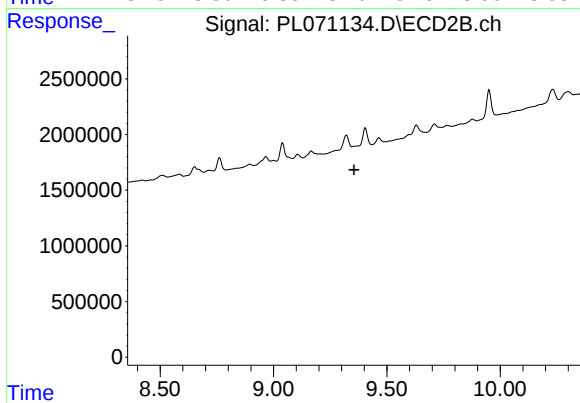

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.356 min
Response: 0
Conc: N.D.

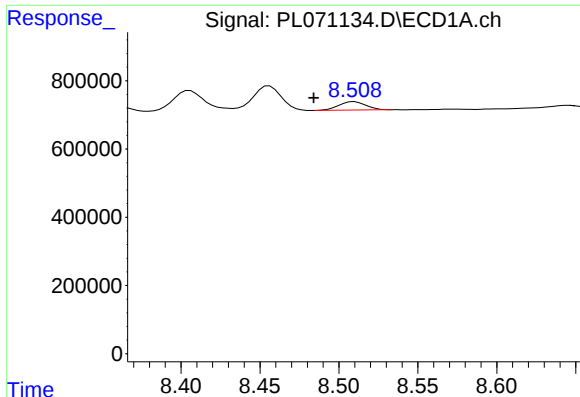

#18 Endrin aldehyde


R.T.: 8.510 min
Delta R.T.: 0.026 min
Response: 294658
Conc: 0.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

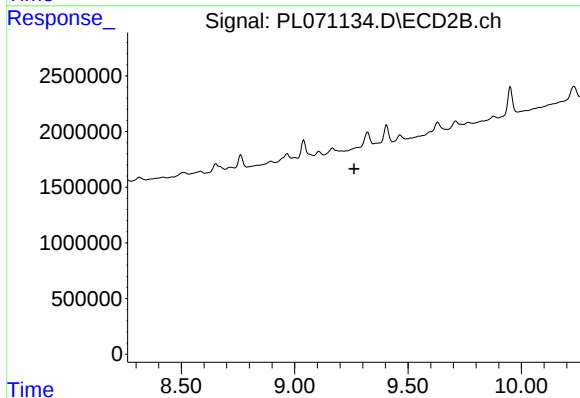


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.262 min
Response: 0
Conc: N.D.

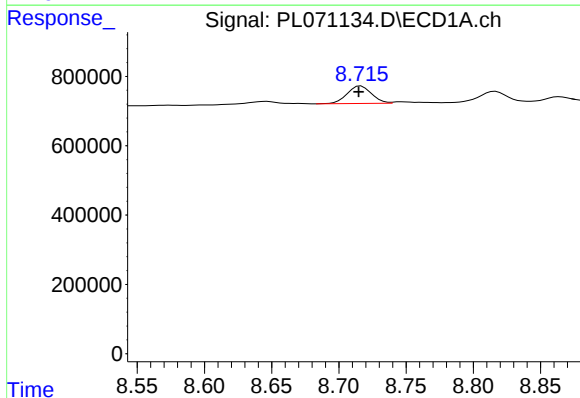


#19 Endosulfan Sulfate

R.T.: 8.716 min
Delta R.T.: 0.002 min
Response: 639676
Conc: 1.04 ng/ml

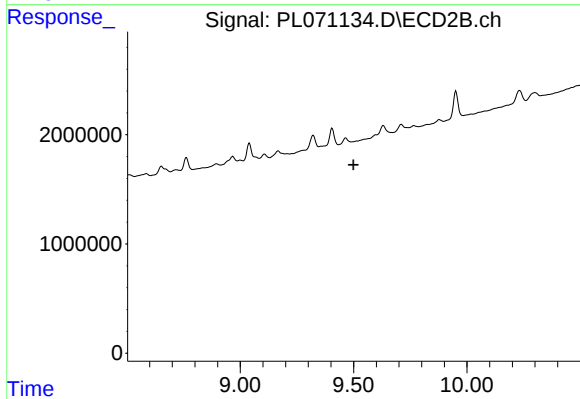

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.500 min
Response: 0
Conc: N.D.

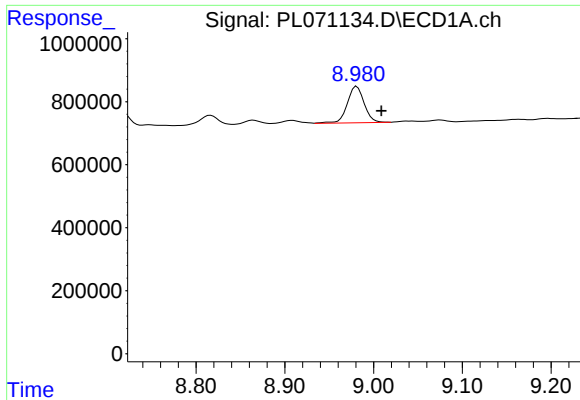

#20 Methoxychlor


R.T.: 8.981 min
Delta R.T.: -0.028 min
Response: 1529365
Conc: 4.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

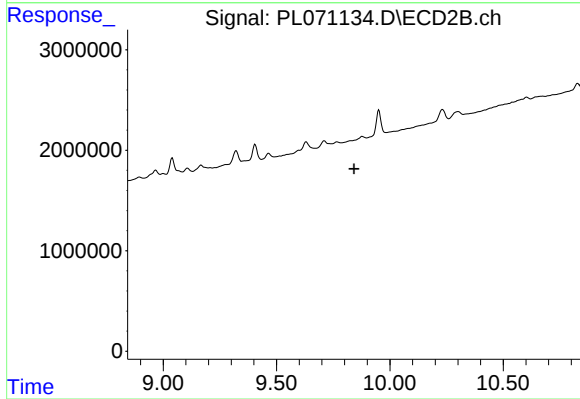


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.842 min
Response: 0
Conc: N.D.

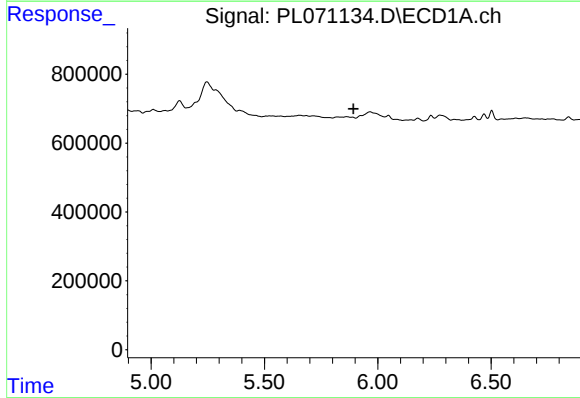


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.893 min
Response: 0
Conc: N.D.

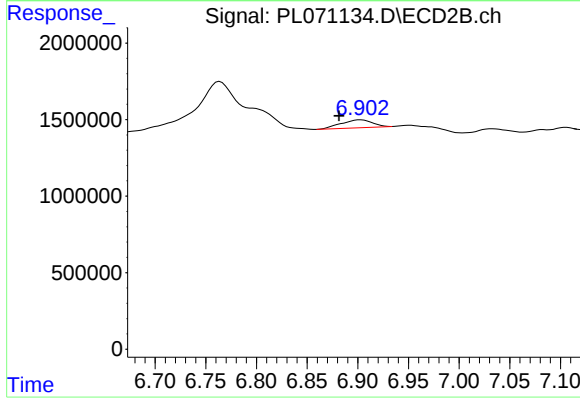

#23 Chlordane-1


R.T.: 6.903 min
Delta R.T.: 0.022 min
Response: 1119665
Conc: 23.06 ng/ml

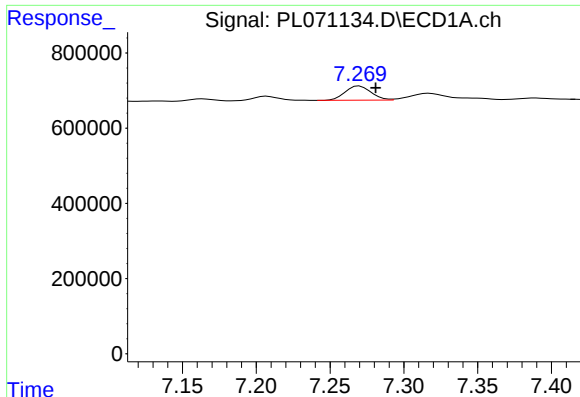

#25 Chlordane-3


R.T.: 7.270 min
Delta R.T.: -0.011 min
Response: 461082
Conc: 7.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

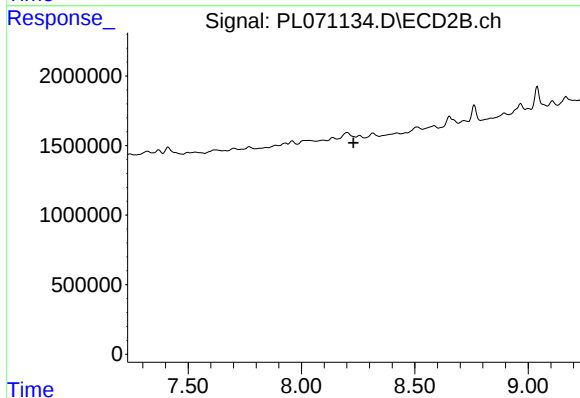


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

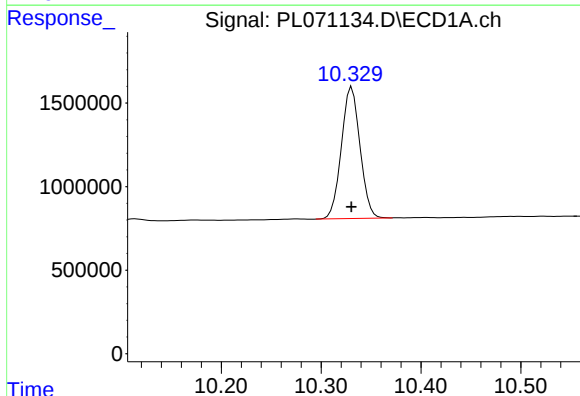

#28 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.000 min
Response: 10221728
Conc: 14.96 ng/ml

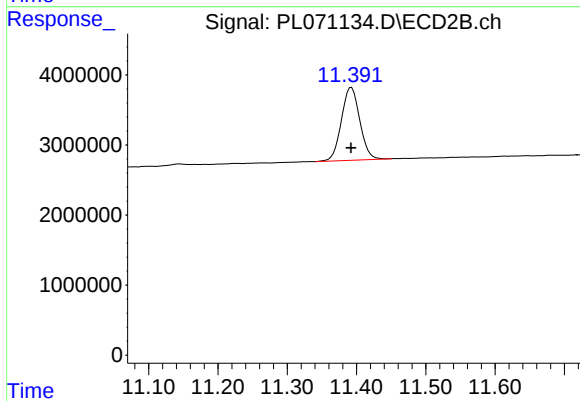

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: 0.000 min
Response: 19221116
Conc: 14.37 ng/ml