

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
 Data File : PL079399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 20:08
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 23:16:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 23 23:13:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.563	235.5E6	336.8E6	101.732	100.713
28)	SA Decachlor...	8.764	7.630	189.6E6	226.5E6	98.586	98.043
Target Compounds							
23)	Chlordane-1	4.466	3.528	101.4E6	106.5E6	1015.222	998.759
24)	Chlordane-2	4.999	4.094	104.5E6	114.5E6	989.593	981.517
25)	Chlordane-3	5.708	4.714	447.2E6	343.3E6	1024.922	1003.531
26)	Chlordane-4	5.786	4.773	536.8E6	367.7E6	1016.217	1001.236
27)	Chlordane-5	6.641	5.434	87824998	93108560	1017.376	994.482



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
Data File : PL079399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 20:08
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 23:16:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Wed Nov 23 23:13:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

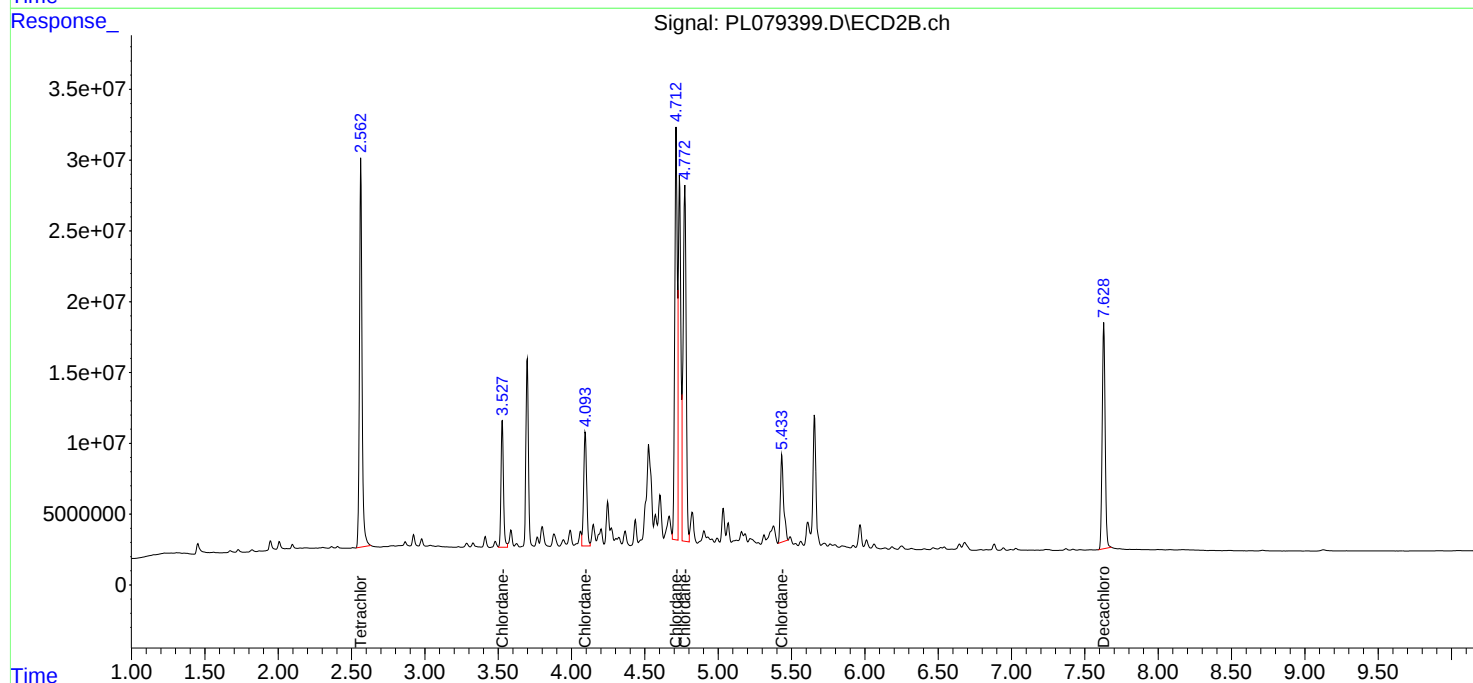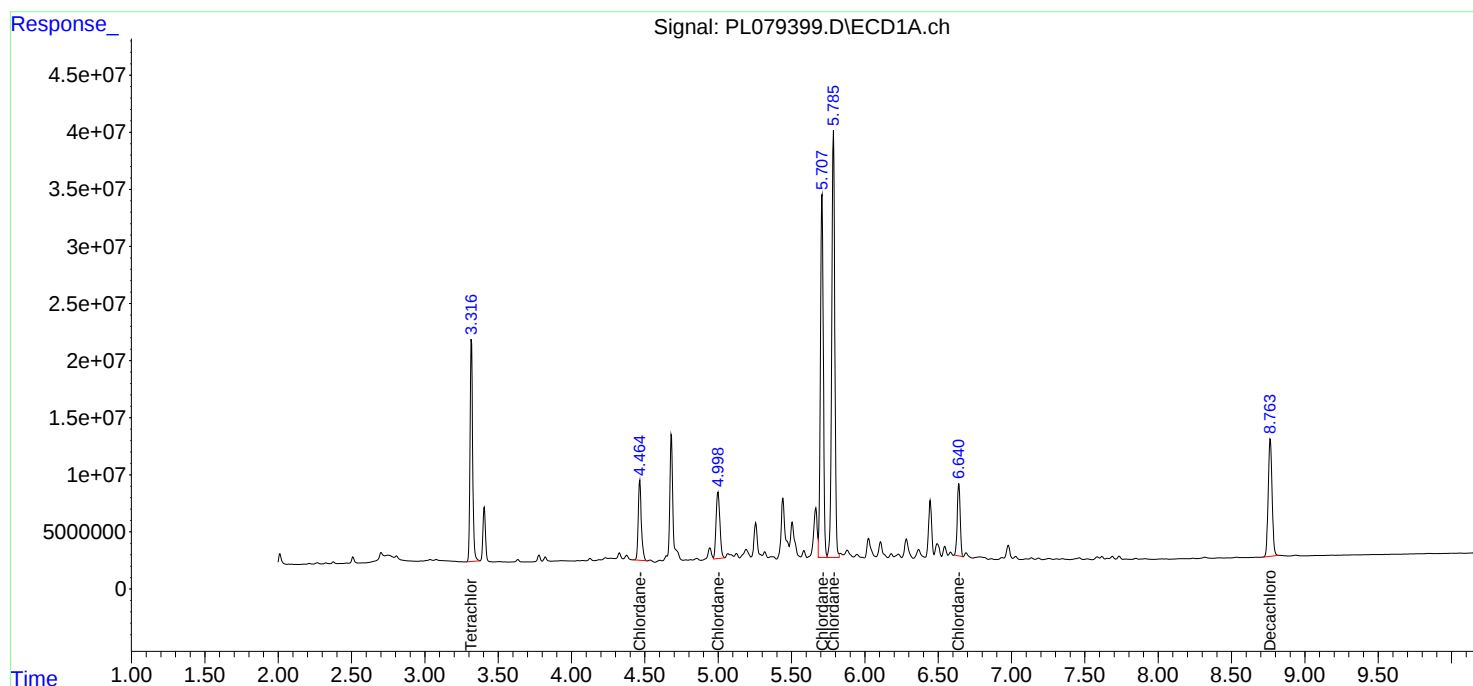


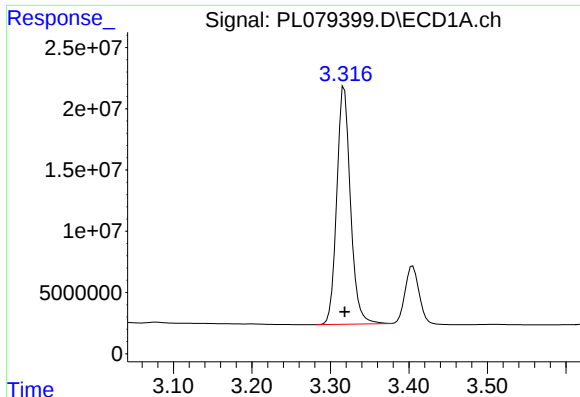

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 235541601
Conc: 101.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

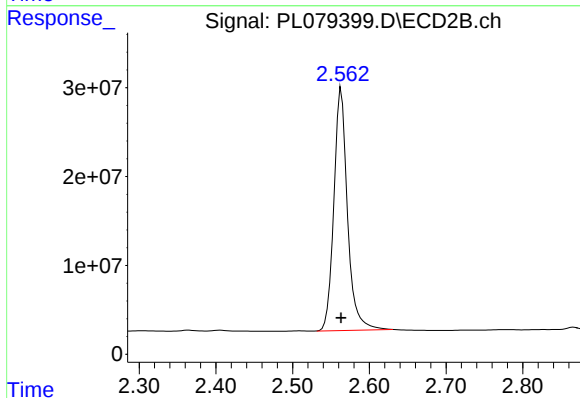


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 336807865
Conc: 100.71 ng/ml

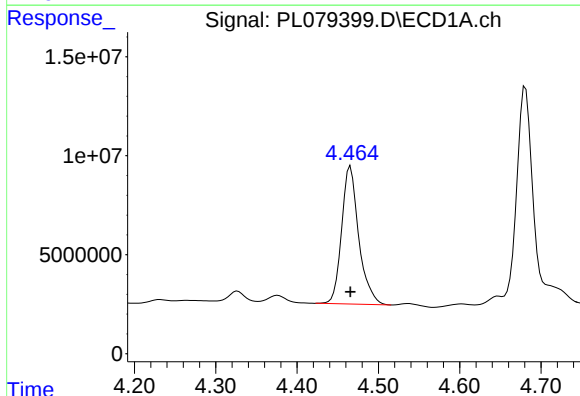


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 101423272
Conc: 1015.22 ng/ml

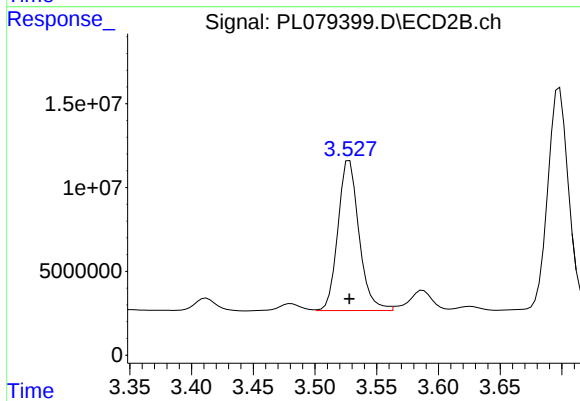

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 106475315
Conc: 998.76 ng/ml

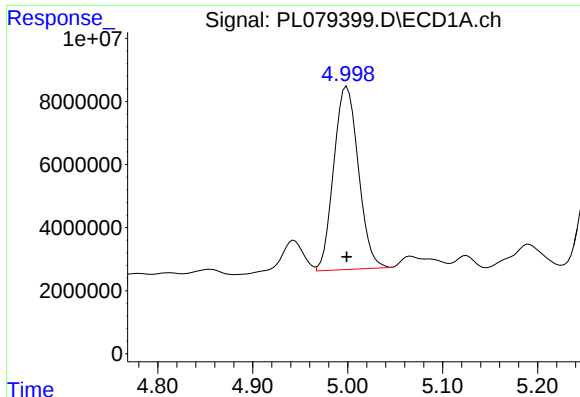

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 104543140
Conc: 989.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

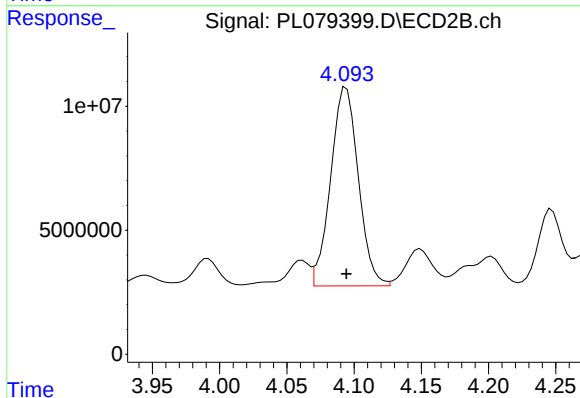


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 114519858
Conc: 981.52 ng/ml

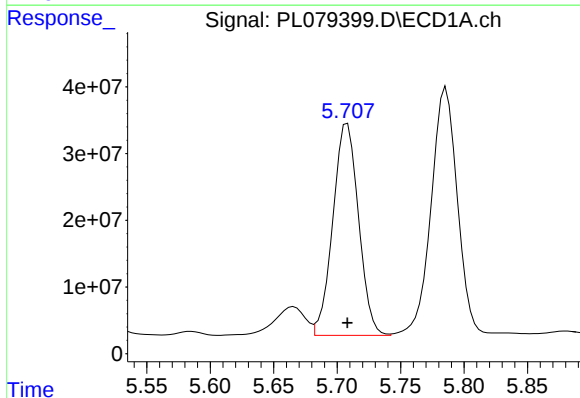


#25 Chlordane-3

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 447245160
Conc: 1024.92 ng/ml

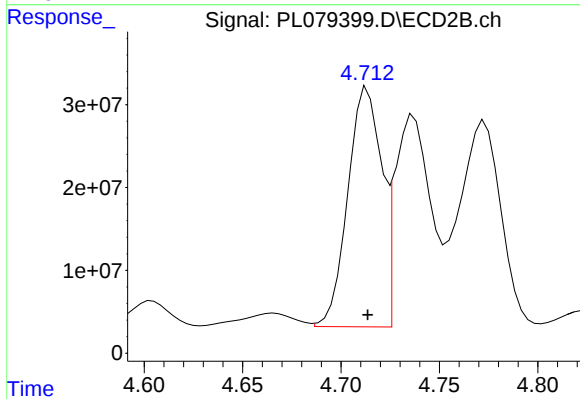

#25 Chlordane-3


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 343293361
Conc: 1003.53 ng/ml

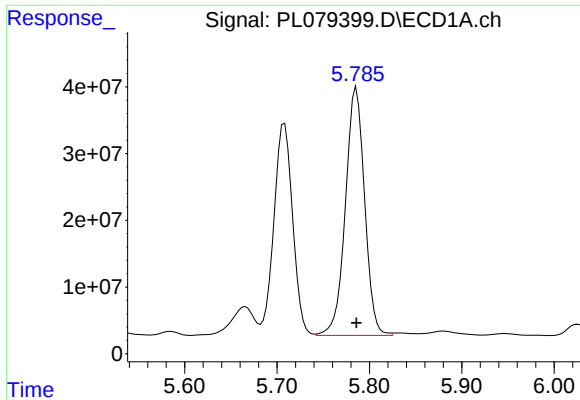

#26 Chlordane-4


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 536801606
Conc: 1016.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

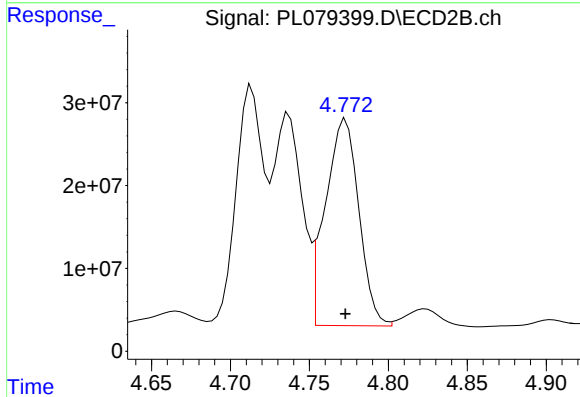


#26 Chlordane-4

R.T.: 4.773 min
Delta R.T.: 0.000 min
Response: 367744701
Conc: 1001.24 ng/ml

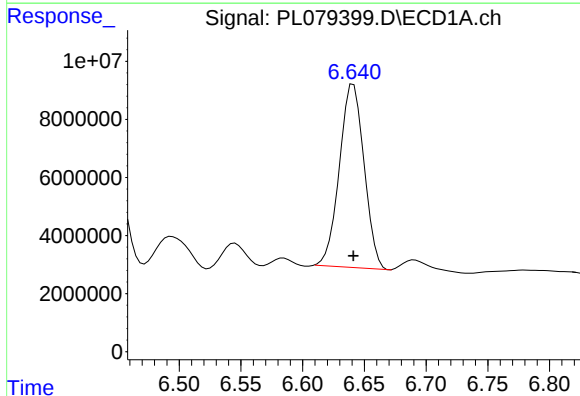


#27 Chlordane-5

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 87824998
Conc: 1017.38 ng/ml

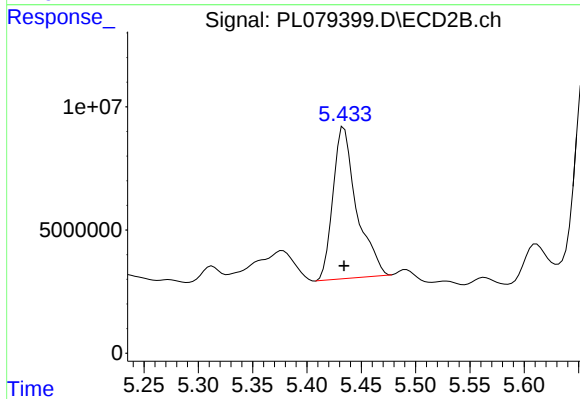

#27 Chlordane-5


R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 93108560
Conc: 994.48 ng/ml

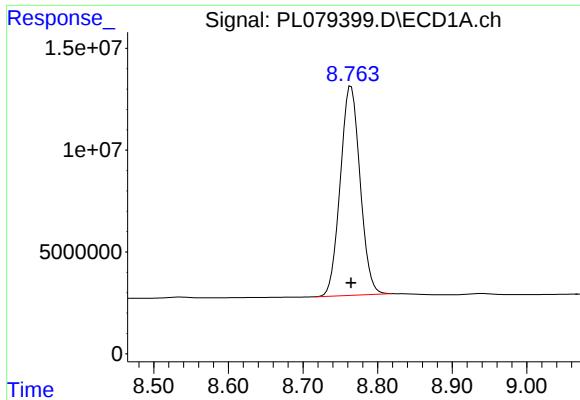

#28 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 189560549
Conc: 98.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

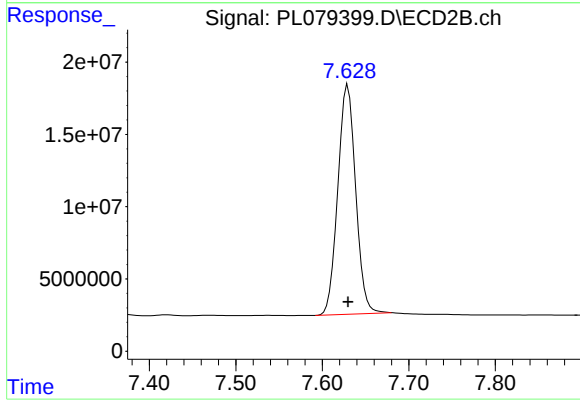

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 226460011
Conc: 98.04 ng/ml